

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
 Data File : PS005794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2019 18:10
 Operator : SM\AJ
 Sample : K4044-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 01:52:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.560	5.280	240.1E6	178.6E6	165.482	179.544
Target Compounds							
2) T	3,5-DICHL...	0.000	4.598	0 70026623		N.D.	53.978
5) T	DICAMBA	5.781	0.000	24919596	0	4.172	N.D. #
7) T	MCPA	0.000	5.612	0 128.6E6		N.D.	30.562
10) T	Pentachlo...	0.000	6.539	0 20771312		N.D.	1.600
11) T	2,4,5-TP ...	0.000	7.007	0 22775106		N.D.	4.391



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
Data File : PS005794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2019 18:10
Operator : SM\AJ
Sample : K4044-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 01:52:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

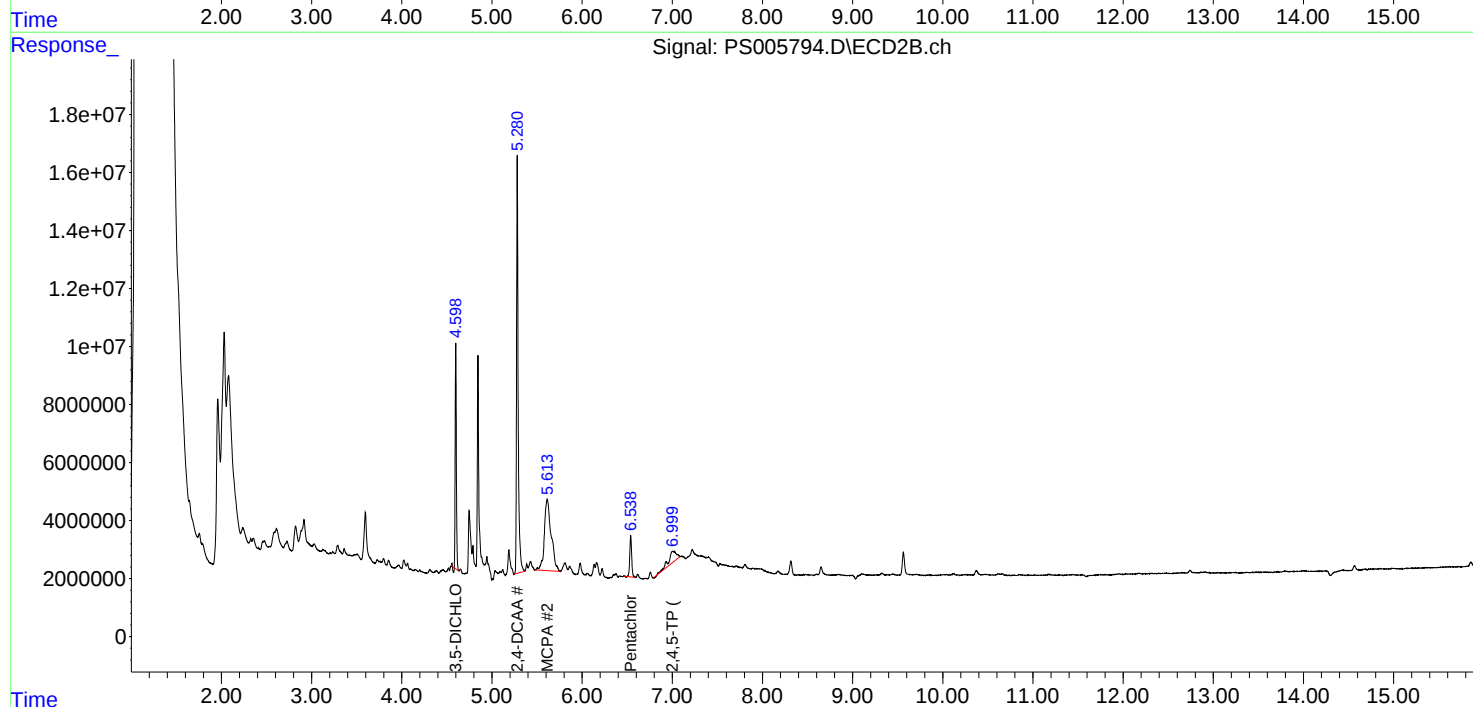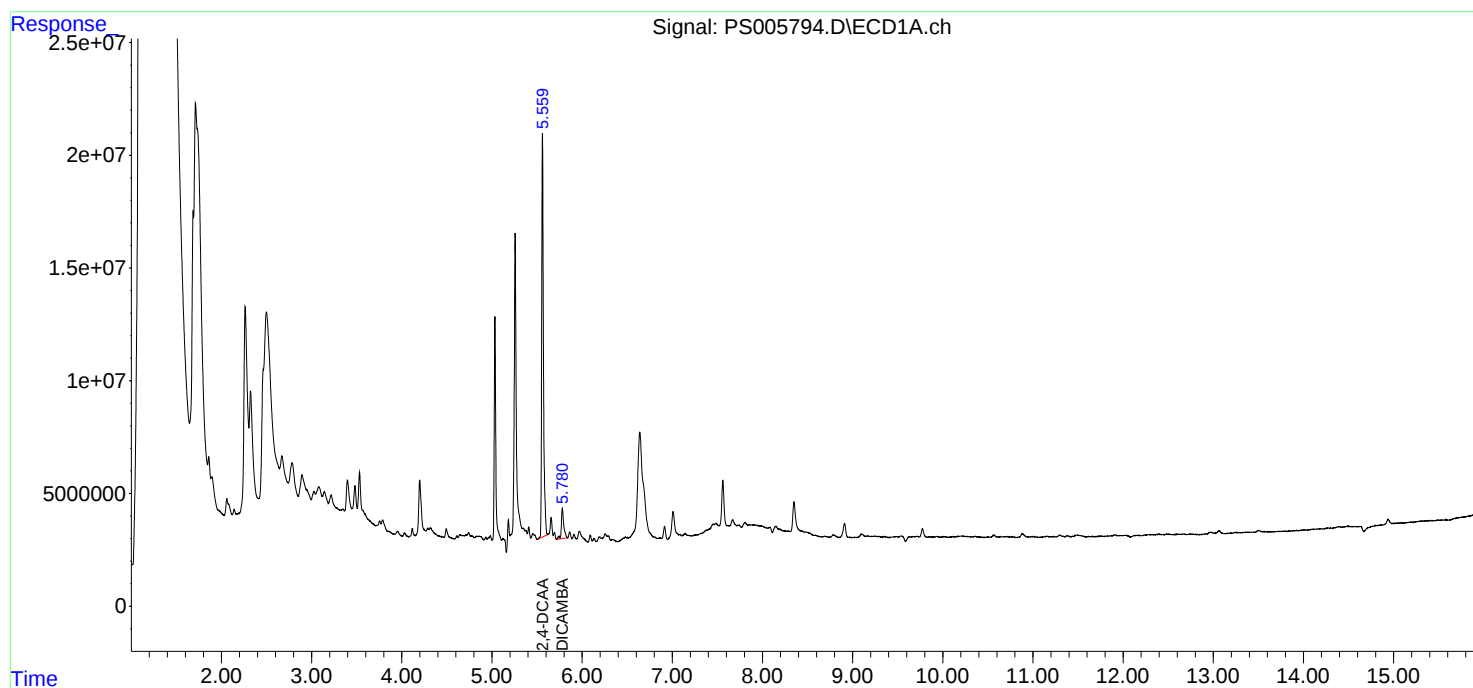


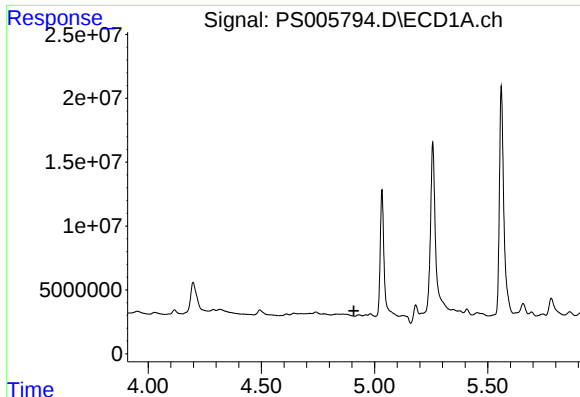

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

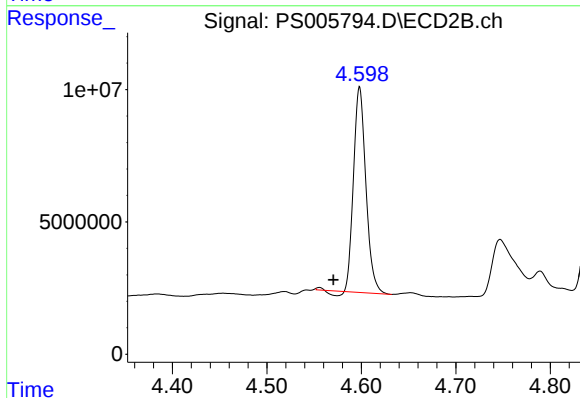


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.598 min
Delta R.T.: 0.028 min
Response: 70026623
Conc: 53.98 ng/ml

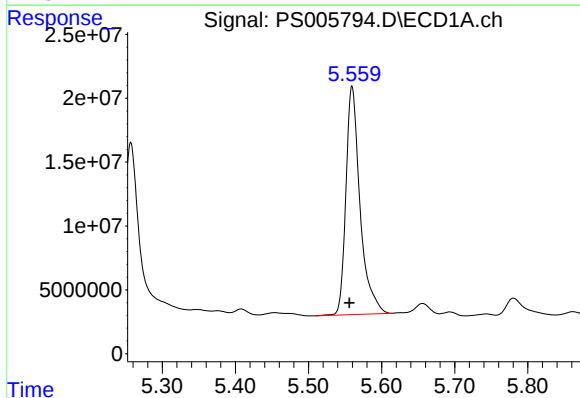


#4 2,4-DCAA

R.T.: 5.560 min
Delta R.T.: 0.004 min
Response: 240084264
Conc: 165.48 ng/ml

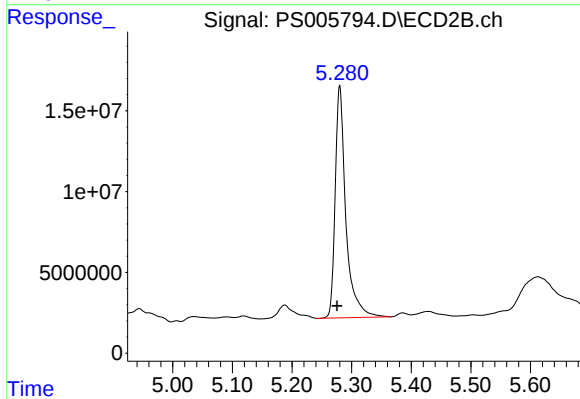

#4 2,4-DCAA


R.T.: 5.280 min
Delta R.T.: 0.004 min
Response: 178588435
Conc: 179.54 ng/ml

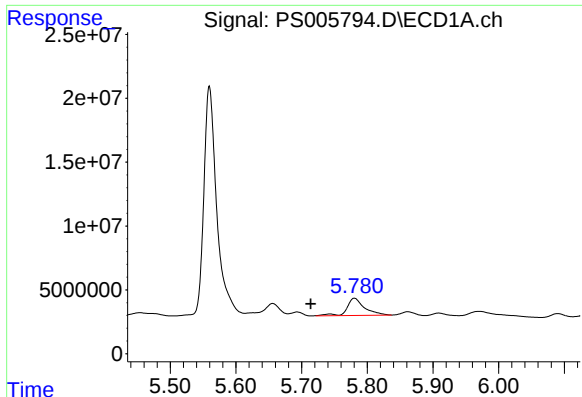

#5 DICAMBA


R.T.: 5.781 min
Delta R.T.: 0.066 min
Response: 24919596
Conc: 4.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

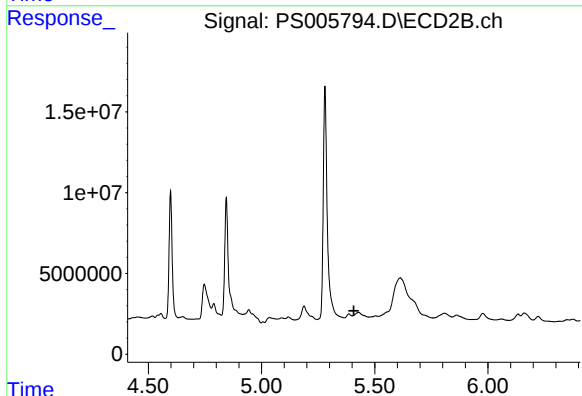


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

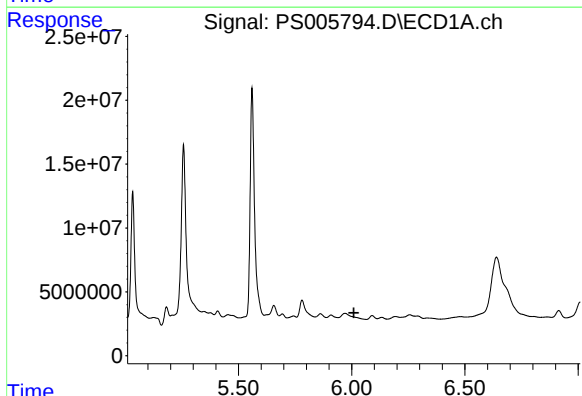


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.009 min
Response: 0
Conc: N.D.

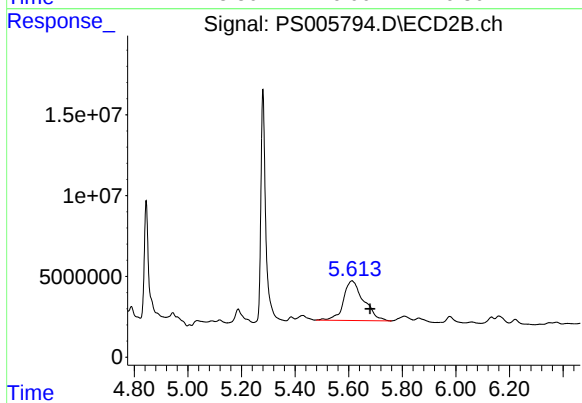

#7 MCPA


R.T.: 5.612 min
Delta R.T.: -0.068 min
Response: 128636242
Conc: 30.56 ug/ml

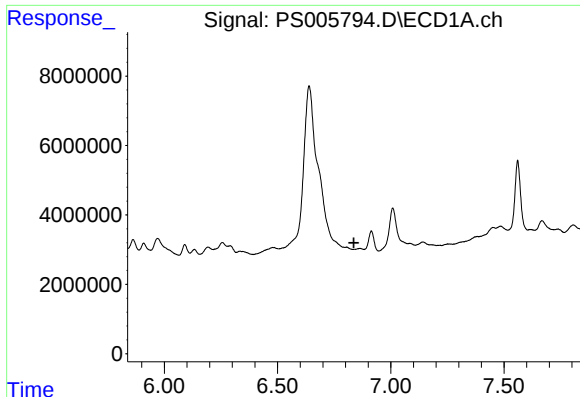

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

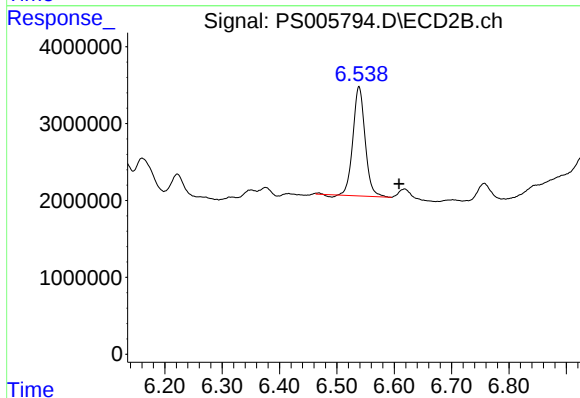


#10 Pentachlorophenol

R.T.: 6.539 min
Delta R.T.: -0.070 min
Response: 20771312
Conc: 1.60 ng/ml

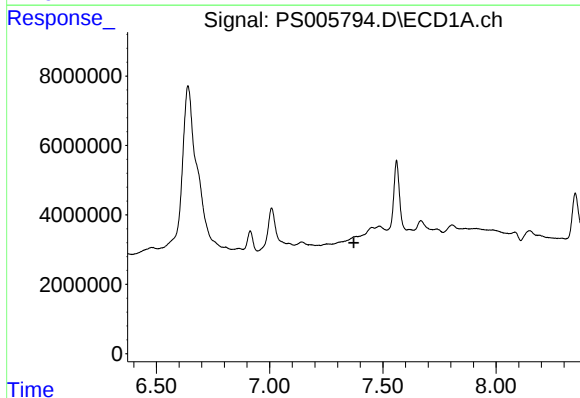

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

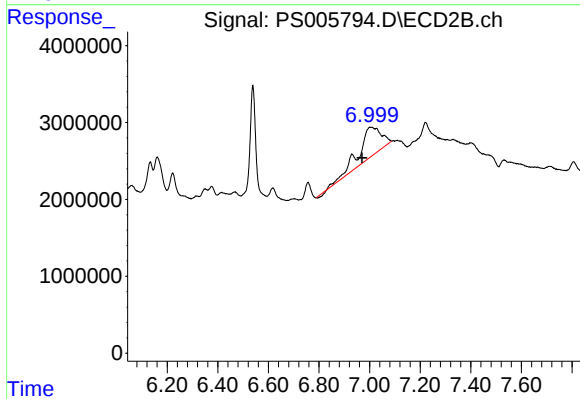

#11 2,4,5-TP (SILVEX)

R.T.: 7.007 min
Delta R.T.: 0.037 min
Response: 22775106
Conc: 4.39 ng/ml