

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
 Data File : PS005795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2019 18:32
 Operator : SM\AJ
 Sample : K4044-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 01:53:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.576	5.296	231.6E6	169.4E6	159.631	170.290
Target Compounds							
2) T	3,5-DICHL...	0.000	4.614	0	76606194	N.D.	59.050
7) T	MCPA	0.000	5.630	0	122.2E6	N.D.	29.040
10) T	Pentachlo...	0.000	6.554	0	20634584	N.D.	1.589
12) T	2,4,5-T	7.577	0.000	31962796	0	3.829	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
Data File : PS005795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2019 18:32
Operator : SM\AJ
Sample : K4044-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 01:53:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

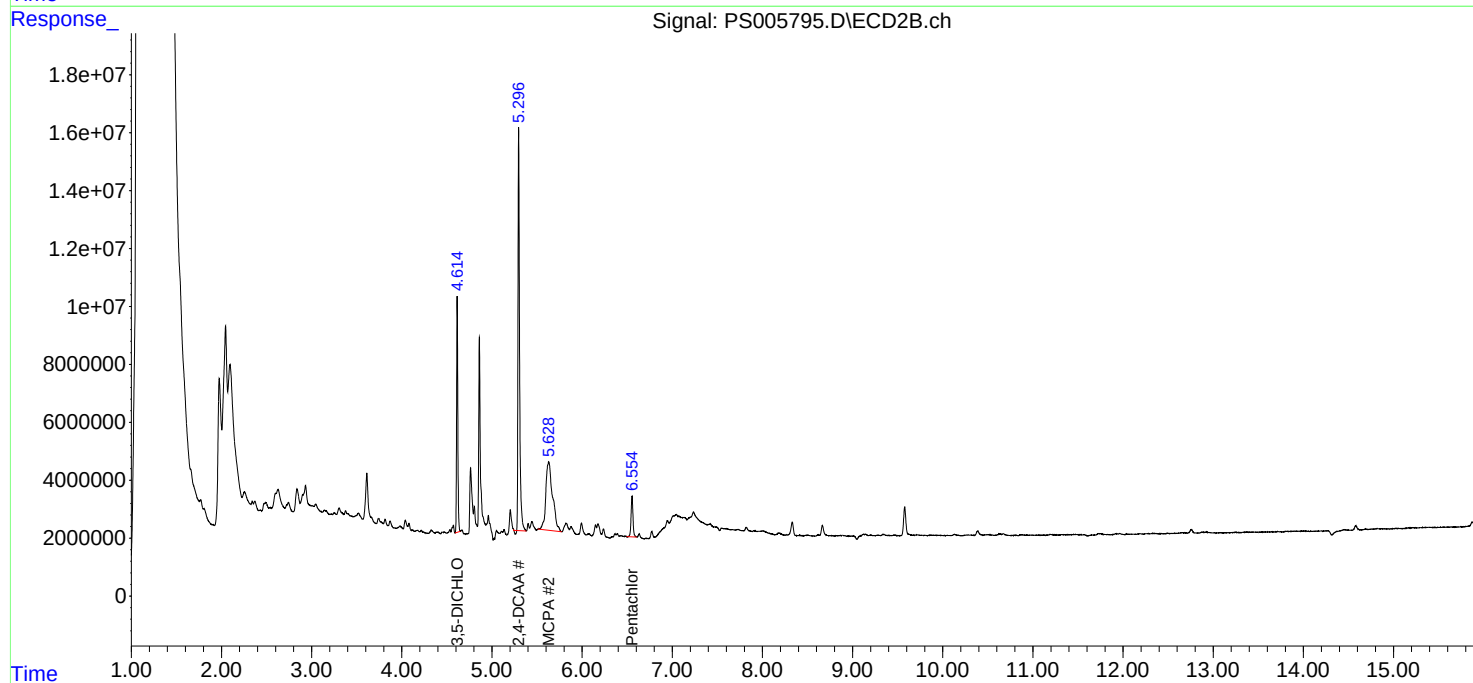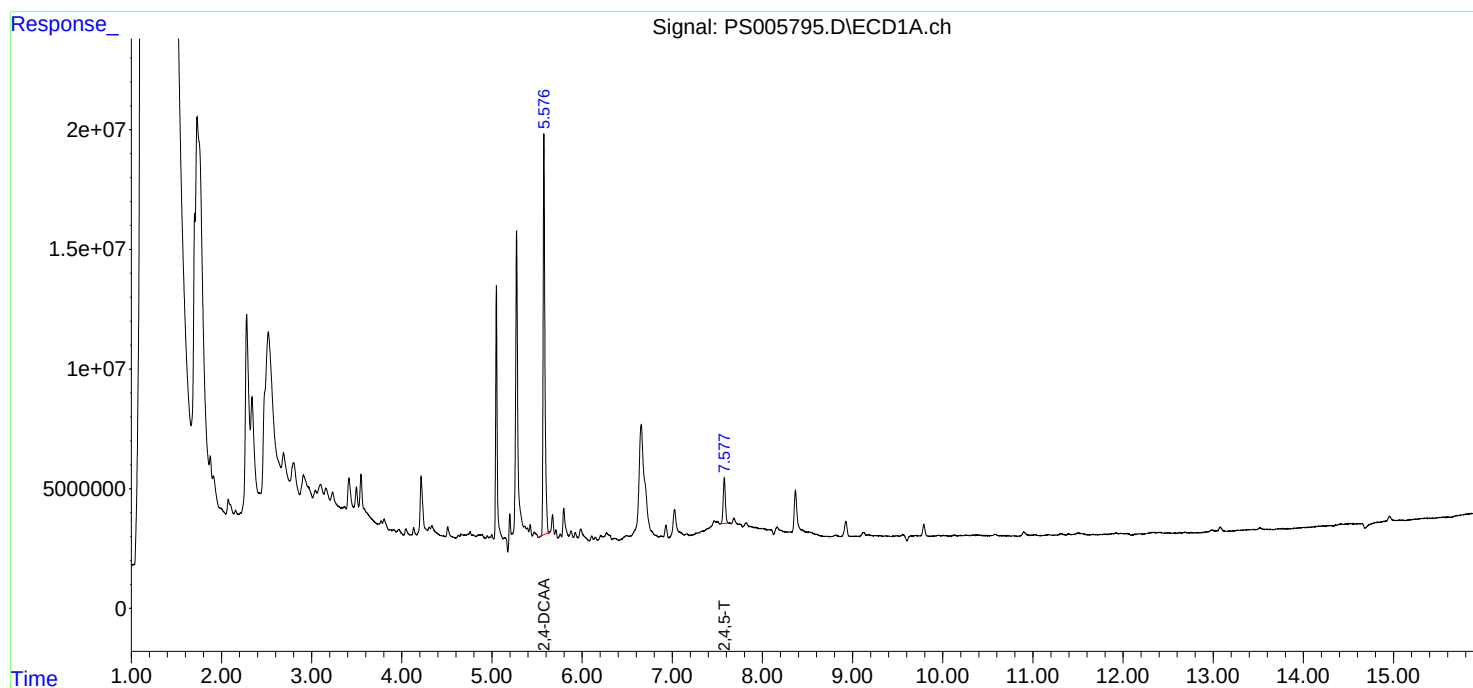


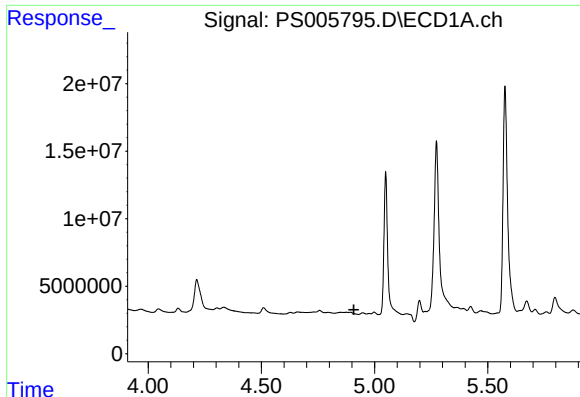

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6

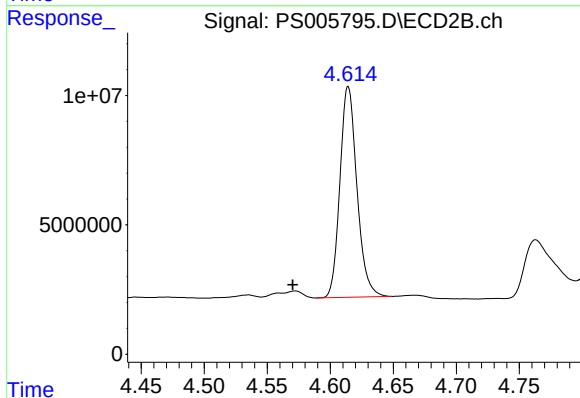


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.614 min
Delta R.T.: 0.044 min
Response: 76606194
Conc: 59.05 ng/ml

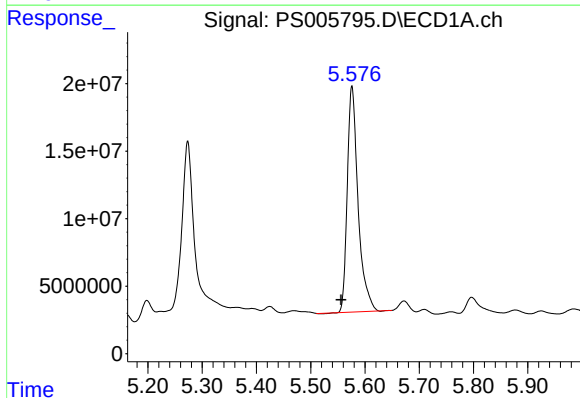


#4 2,4-DCAA

R.T.: 5.576 min
Delta R.T.: 0.020 min
Response: 231594968
Conc: 159.63 ng/ml

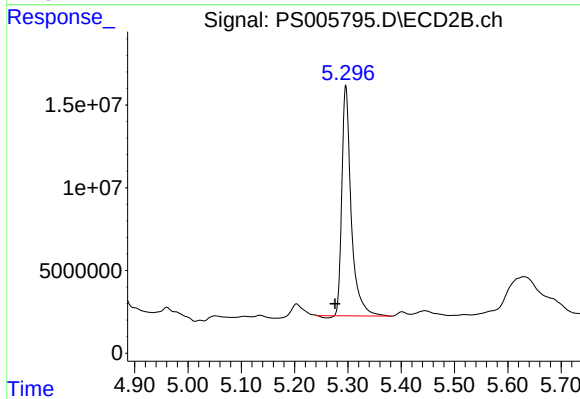

#4 2,4-DCAA


R.T.: 5.296 min
Delta R.T.: 0.021 min
Response: 169384109
Conc: 170.29 ng/ml

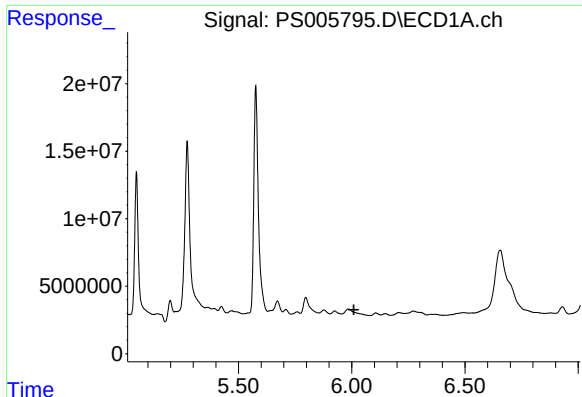

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6

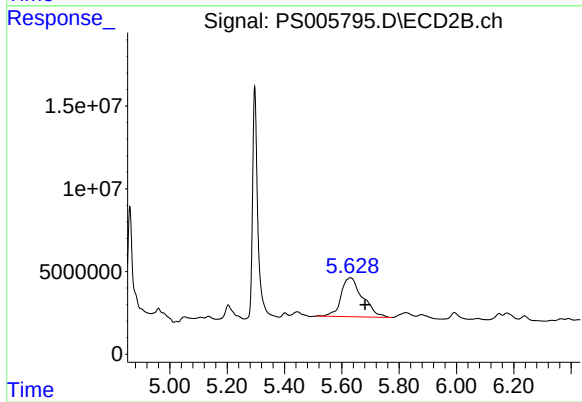


#7 MCPA

R.T.: 5.630 min
Delta R.T.: -0.051 min
Response: 122228521
Conc: 29.04 ug/ml

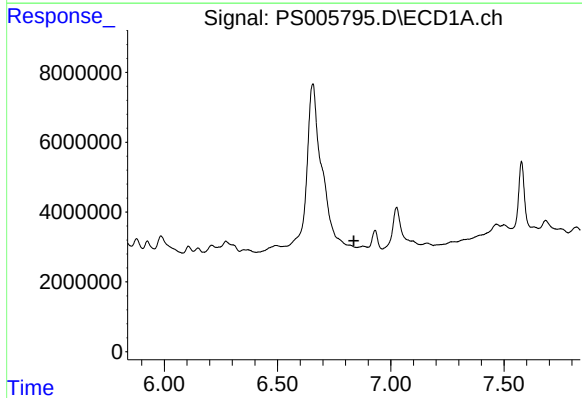


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

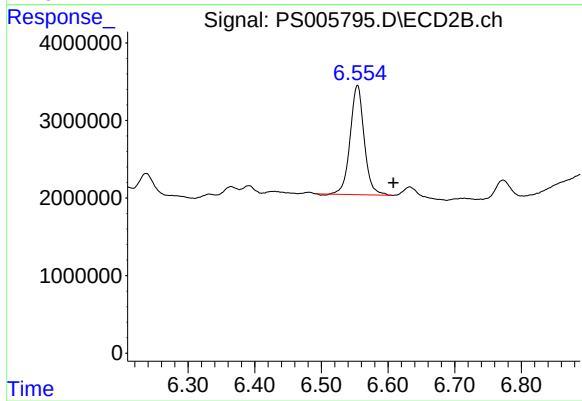

#10 Pentachlorophenol


R.T.: 6.554 min
Delta R.T.: -0.054 min
Response: 20634584
Conc: 1.59 ng/ml

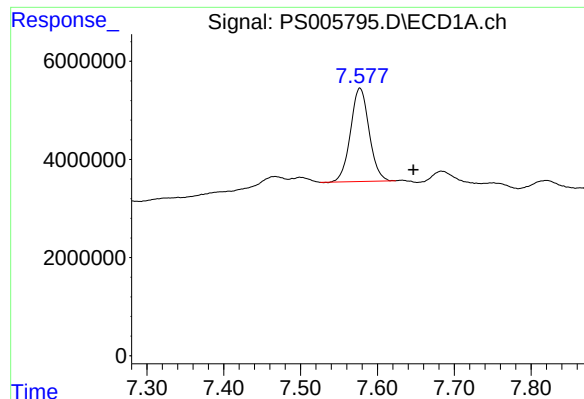

#12 2,4,5-T

R.T.: 7.577 min
Delta R.T.: -0.070 min
Response: 31962796
Conc: 3.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6

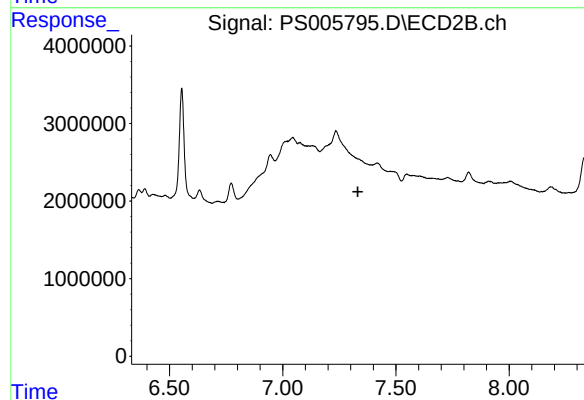

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.332 min
Response: 0
Conc: N.D.