

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
 Data File : PS005799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2019 20:01
 Operator : SM\AJ
 Sample : K4024-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 01:54:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.555	5.275	304.8E6	225.4E6	210.089	226.639
Target Compounds							
1) T	Dalapon	2.055	0.000	20390692	0	11.002	N.D. #
2) T	3,5-DICHL...	0.000	4.594	0	72183072	N.D.	55.640
5) T	DICAMBA	5.776	0.000	28662941	0	4.799	N.D. #
9) T	2,4-D	6.635	0.000	199.2E6	0	132.932	N.D. #
10) T	Pentachlo...	6.836	0.000	19135524	0	<MDL	N.D. #
12) T	2,4,5-T	0.000	7.379	0	66628870	N.D.	14.016
15) T	Picloram	9.124	9.083	275.1E6	218.1E6	23.501	29.037
16) T	DCPA	0.000	9.083	0	218.1E6	N.D.	33.080



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
Data File : PS005799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2019 20:01
Operator : SM\AJ
Sample : K4024-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
TP-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 01:54:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

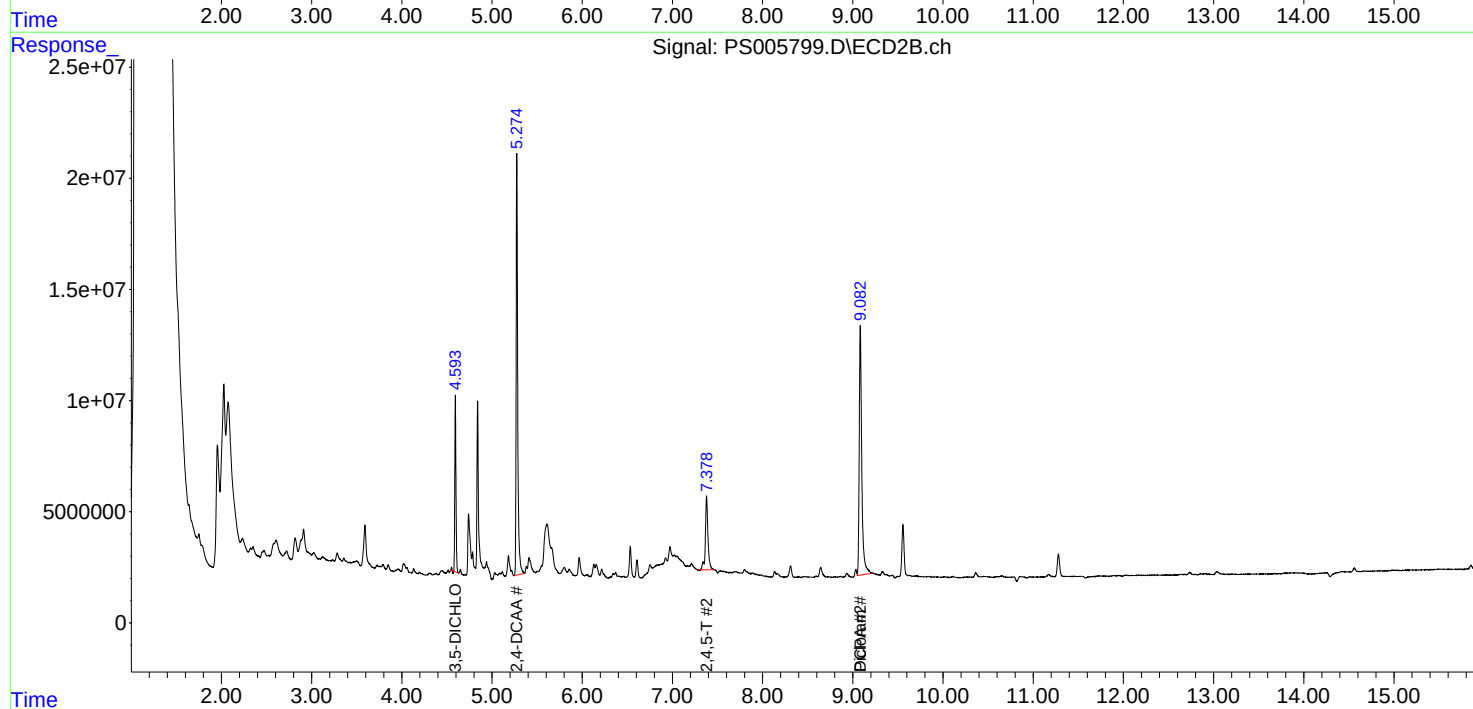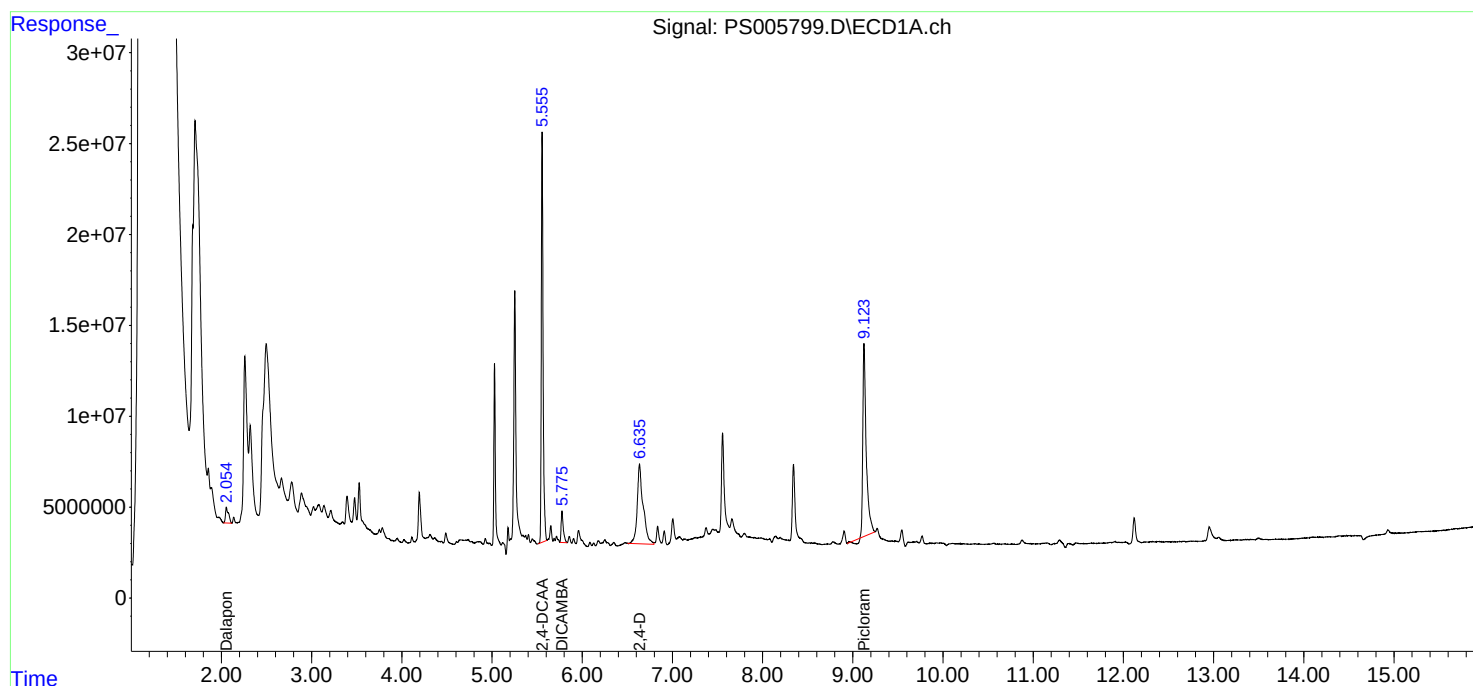


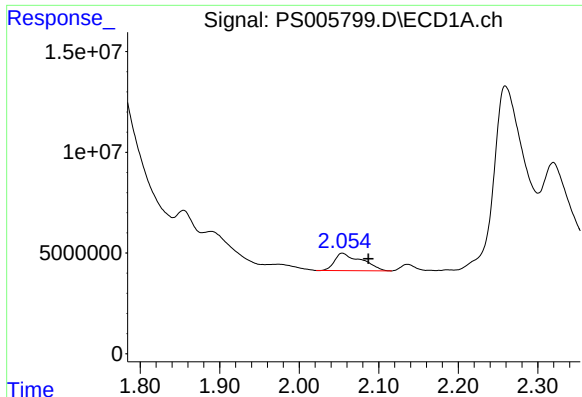

#1 Dalapon


R.T.: 2.055 min
Delta R.T.: -0.032 min
Response: 20390692
Conc: 11.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-8

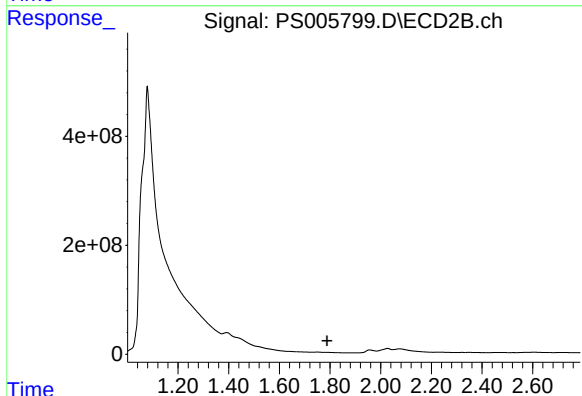


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

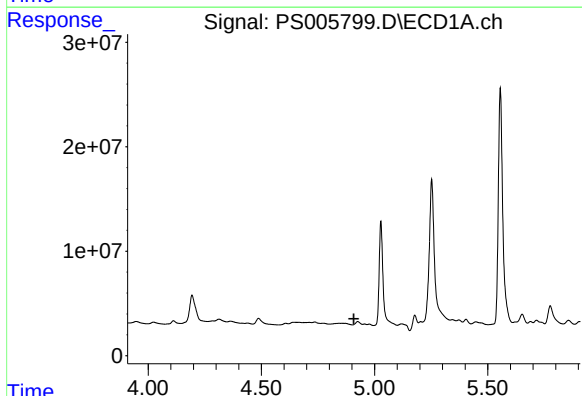


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

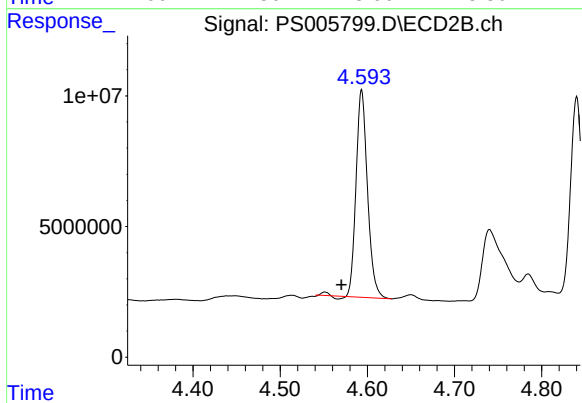

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.594 min
Delta R.T.: 0.023 min
Response: 72183072
Conc: 55.64 ng/ml

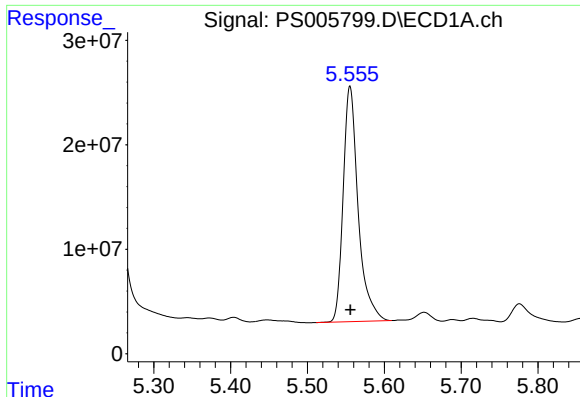

#4 2,4-DCAA


R.T.: 5.555 min
Delta R.T.: 0.000 min
Response: 304800654
Conc: 210.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-8

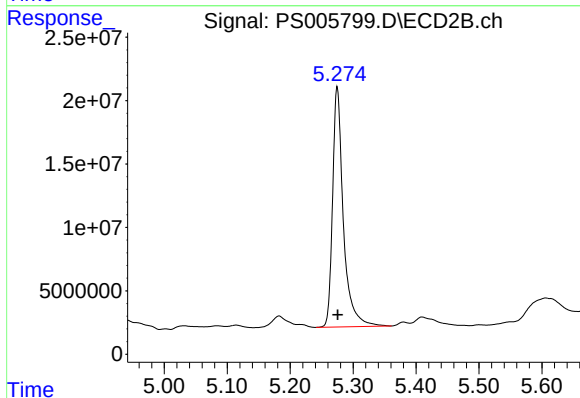


#4 2,4-DCAA

R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 225432606
Conc: 226.64 ng/ml

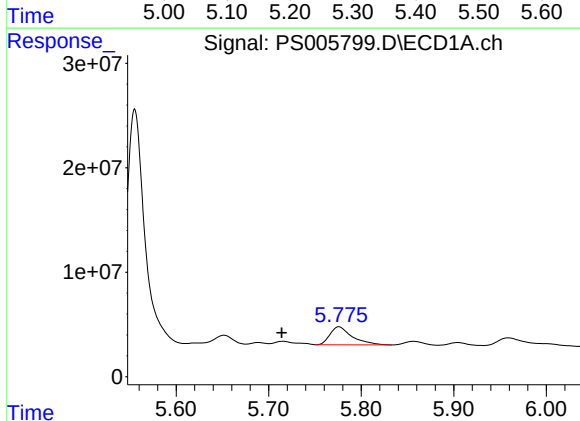


#5 DICAMBA

R.T.: 5.776 min
Delta R.T.: 0.062 min
Response: 28662941
Conc: 4.80 ng/ml

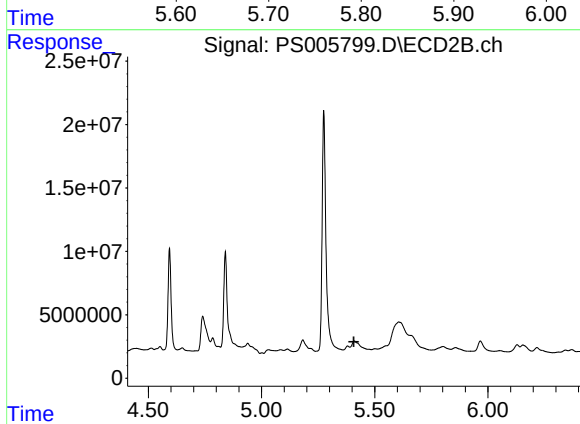

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.408 min
Response: 0
Conc: N.D.

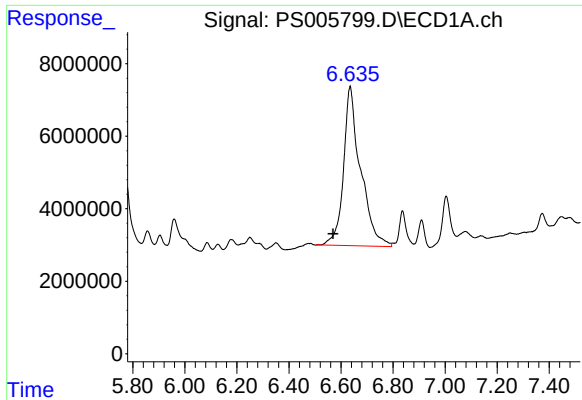

#9 2,4-D


R.T.: 6.635 min
Delta R.T.: 0.066 min
Response: 199221583
Conc: 132.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-8

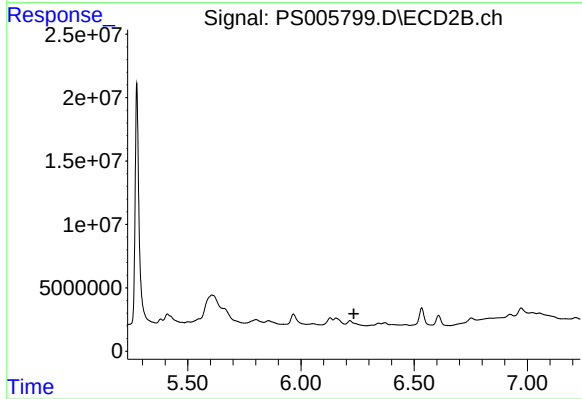


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

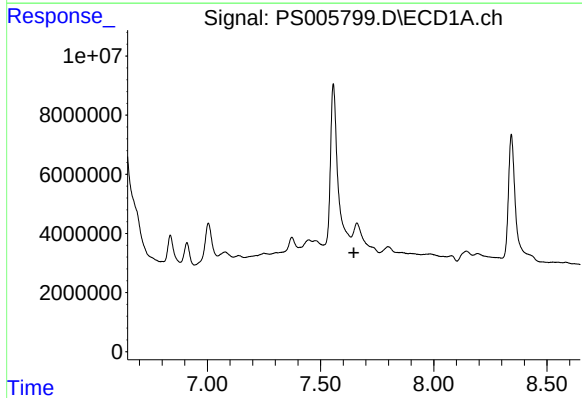


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.647 min
Response: 0
Conc: N.D.

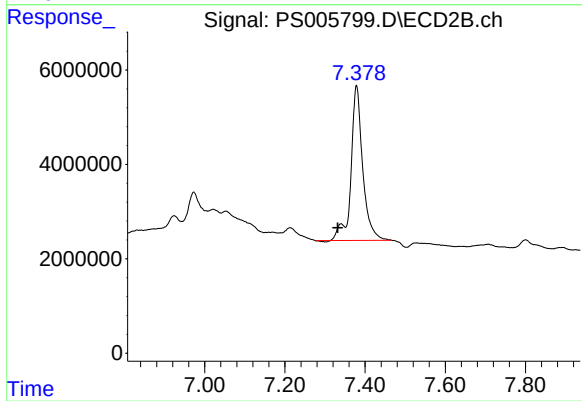

#12 2,4,5-T


R.T.: 7.379 min
Delta R.T.: 0.047 min
Response: 66628870
Conc: 14.02 ng/ml

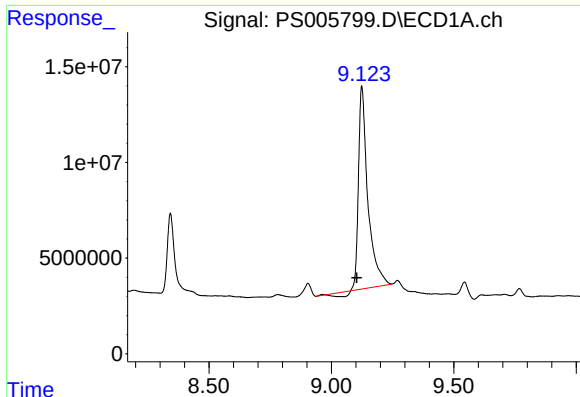

#15 Picloram


R.T.: 9.124 min
Delta R.T.: 0.020 min
Response: 275075478
Conc: 23.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-8

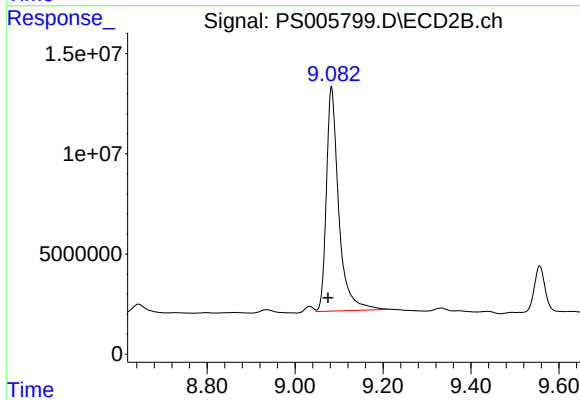


#15 Picloram

R.T.: 9.083 min
Delta R.T.: 0.008 min
Response: 218132278
Conc: 29.04 ng/ml

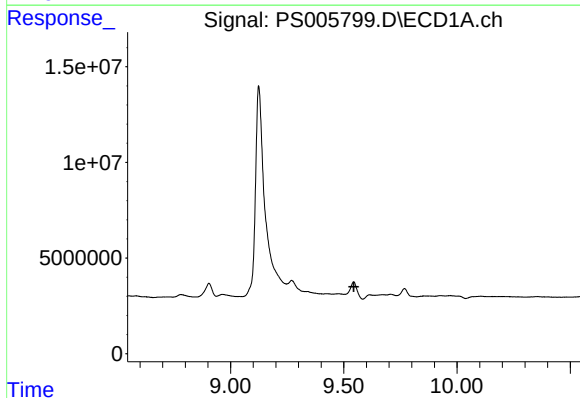

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.545 min
Response: 0
Conc: N.D.

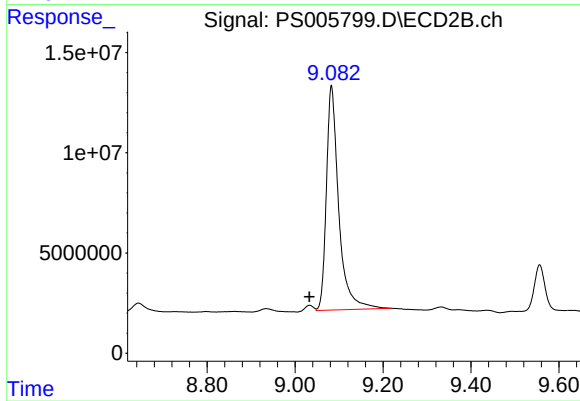

#16 DCPA

R.T.: 9.083 min
Delta R.T.: 0.050 min
Response: 218132278
Conc: 33.08 ng/ml