

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
 Data File : PS005800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2019 20:23
 Operator : SM\AJ
 Sample : K4021-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 01:54:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.577	5.296	265.4E6	190.9E6	182.926	191.943
Target Compounds							
2) T	3,5-DICHL...	0.000	4.615	0	64996223	N.D.	50.101
7) T	MCPA	5.982	5.630	26535509	108.8E6	4.066	25.844 #
10) T	Pentachlo...	0.000	6.554	0	27781408	N.D.	2.140
12) T	2,4,5-T	7.578	0.000	46341189	0	5.552	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
Data File : PS005800.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2019 20:23
Operator : SM\AJ
Sample : K4021-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 01:54:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

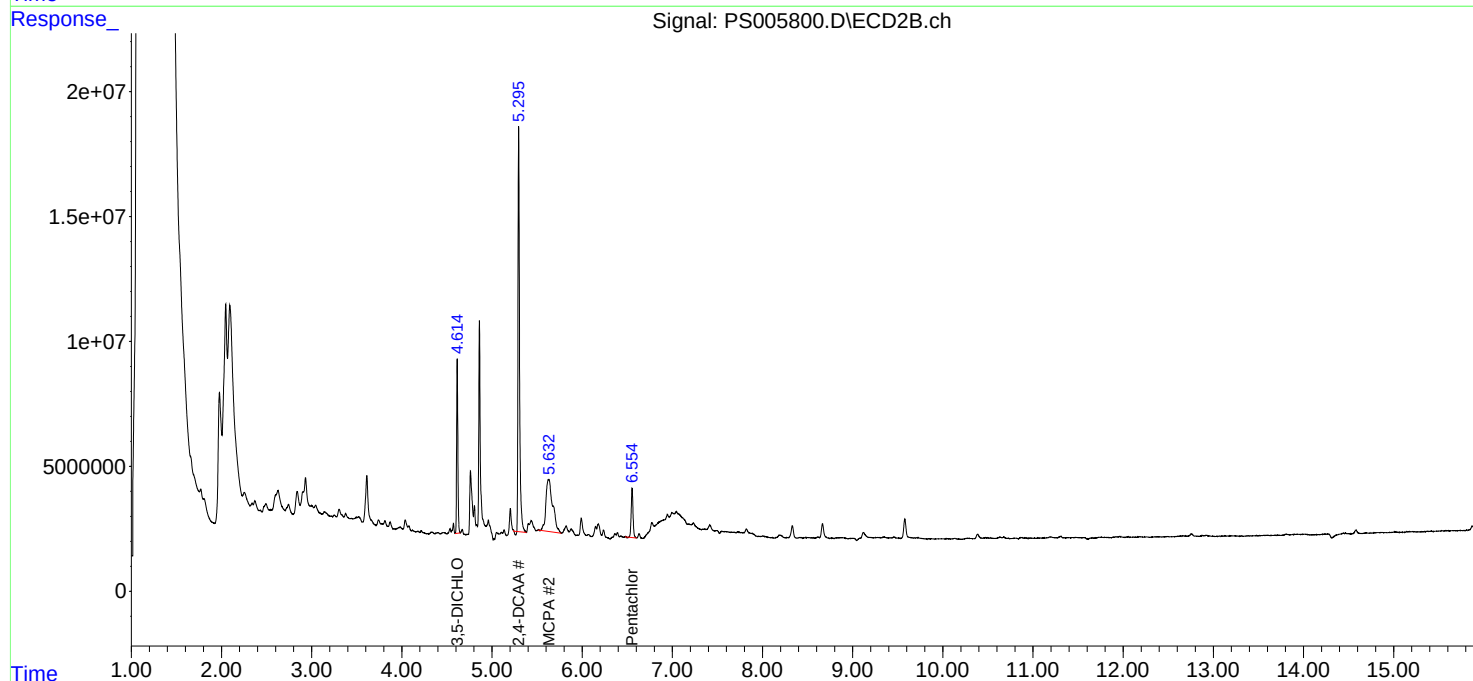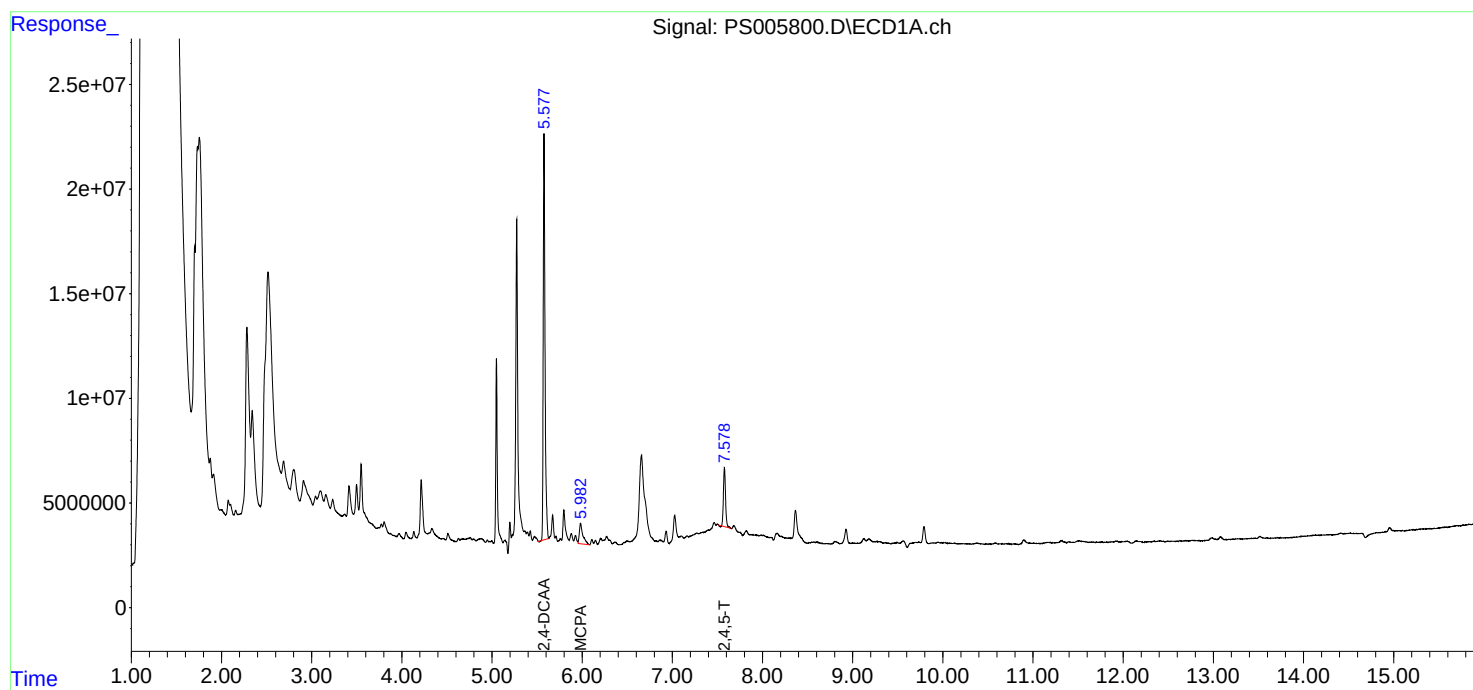


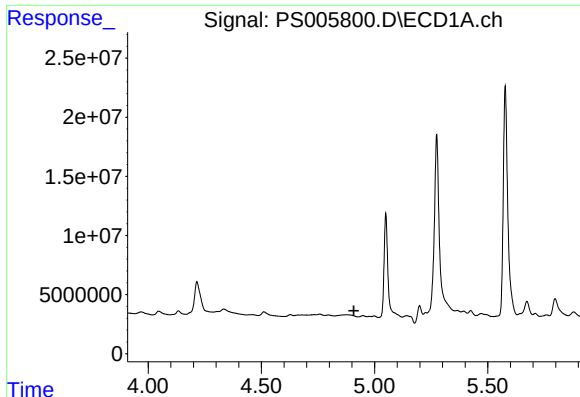

#2 3,5-DICHLORO BENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

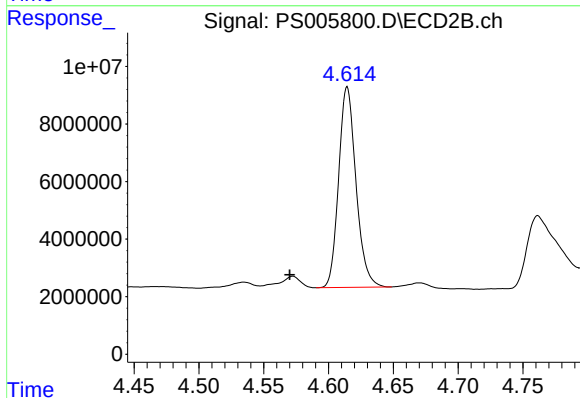


#2 3,5-DICHLORO BENZOIC ACID

R.T.: 4.615 min
Delta R.T.: 0.044 min
Response: 64996223
Conc: 50.10 ng/ml

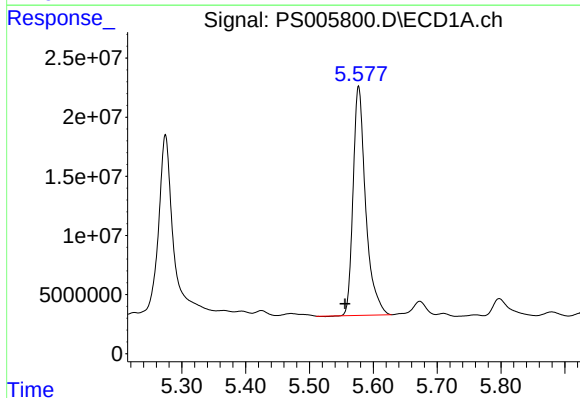


#4 2,4-DCAA

R.T.: 5.577 min
Delta R.T.: 0.021 min
Response: 265392823
Conc: 182.93 ng/ml

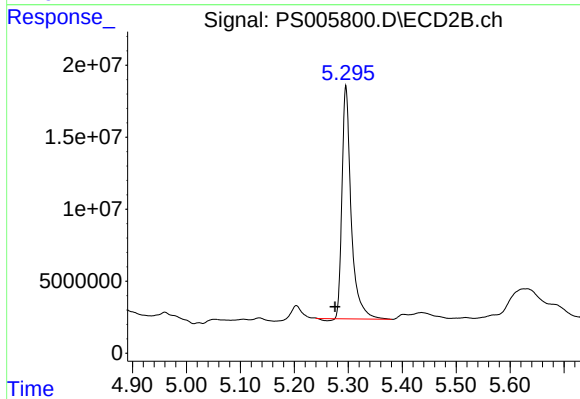

#4 2,4-DCAA


R.T.: 5.296 min
Delta R.T.: 0.020 min
Response: 190921284
Conc: 191.94 ng/ml

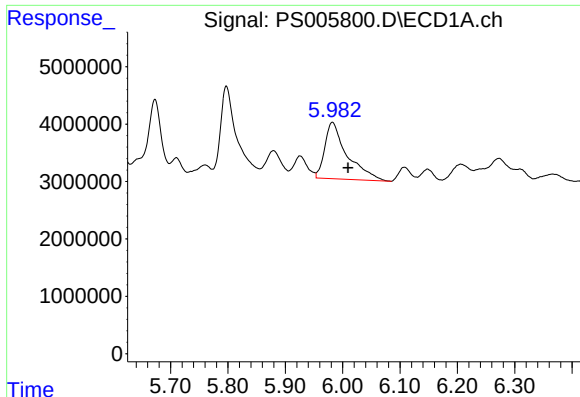

#7 MCPA


R.T.: 5.982 min
Delta R.T.: -0.027 min
Response: 26535509
Conc: 4.07 ug/ml

Instrument :
ECD_S
ClientSampleId :

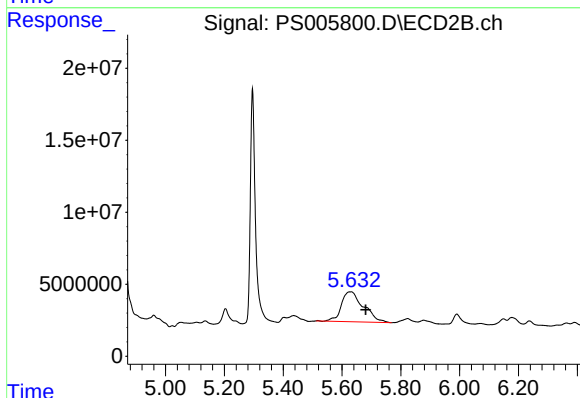


#7 MCPA

R.T.: 5.630 min
Delta R.T.: -0.051 min
Response: 108776553
Conc: 25.84 ug/ml

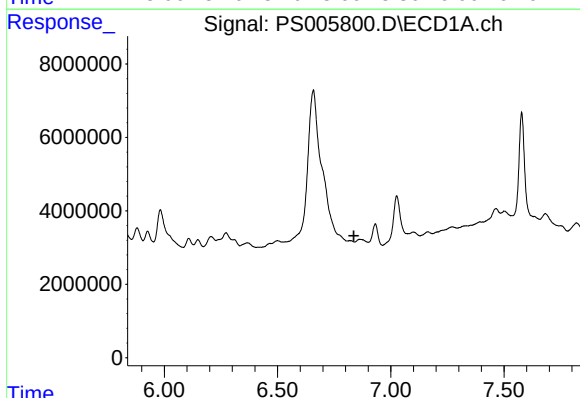


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

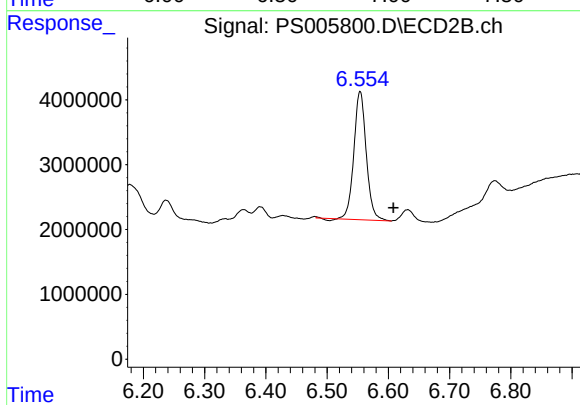

#10 Pentachlorophenol


R.T.: 6.554 min
Delta R.T.: -0.054 min
Response: 27781408
Conc: 2.14 ng/ml

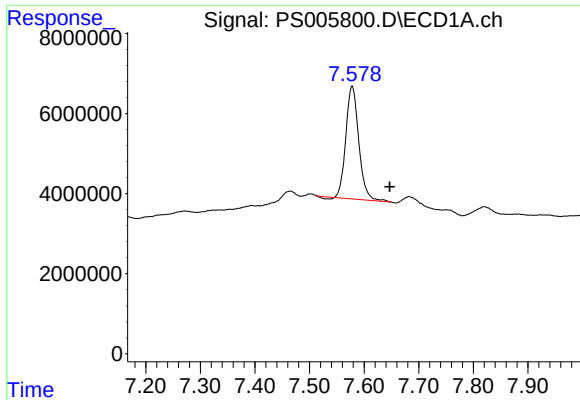

#12 2,4,5-T

R.T.: 7.578 min
Delta R.T.: -0.069 min
Response: 46341189
Conc: 5.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

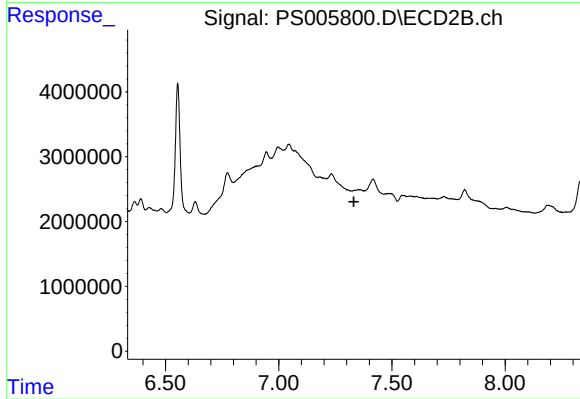

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.332 min
Response: 0
Conc: N.D.