

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
 Data File : PS005795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2019 18:32
 Operator : SM\AJ
 Sample : K4044-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-6

Manual Integrations
 APPROVED

mohammad
 8/1/2019 3:13:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 01:53:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	5.576	5.296	231.6E6	174.7E6	159.631	175.667m
------	----------	-------	-------	---------	---------	---------	----------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073119\
Data File : PS005795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2019 18:32
Operator : SM\AJ
Sample : K4044-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-6


Manual Integrations
APPROVED

mohammad
8/1/2019 3:13:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 01:53:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

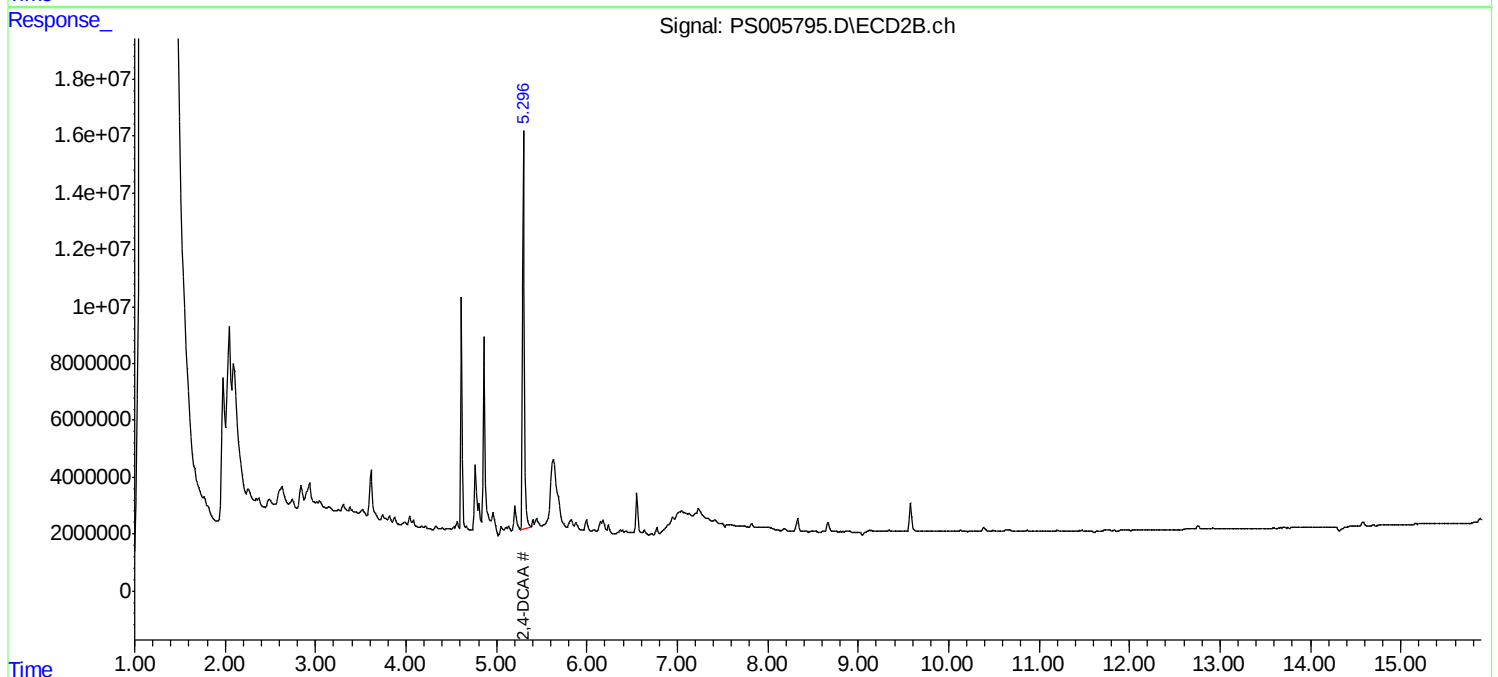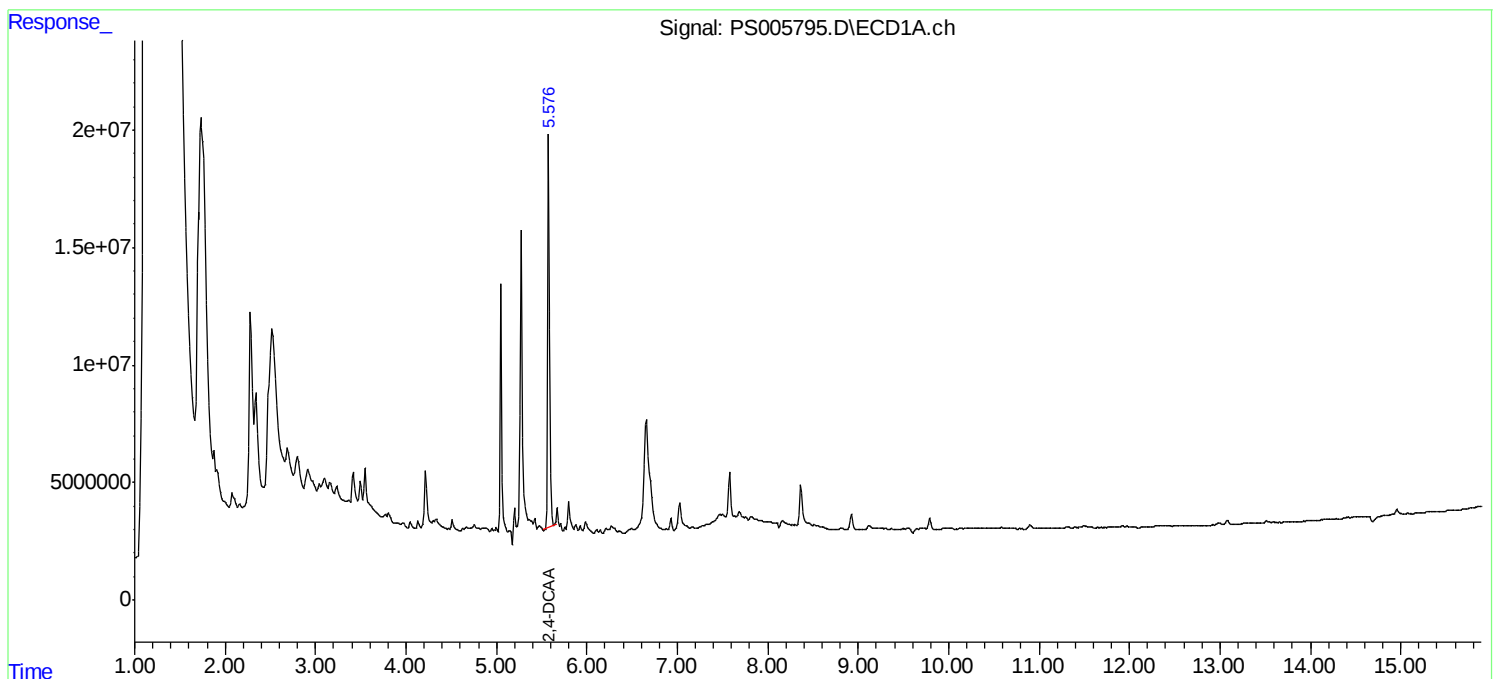

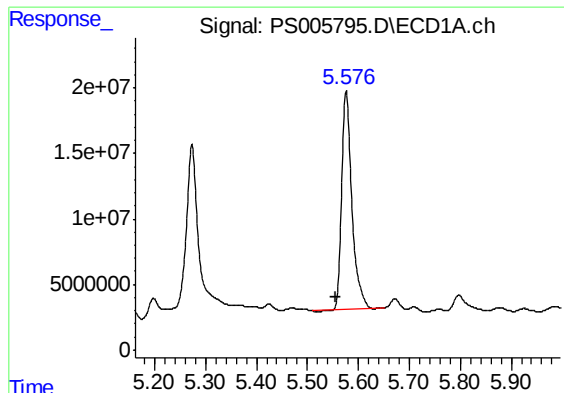


#4 2,4-DCAA

R.T.: 5.576 min
Delta R.T.: 0.020 min
Response: 231594968
Conc: 159.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6

Manual Integrations
APPROVED

mohammad
8/1/2019 3:13:04 PM

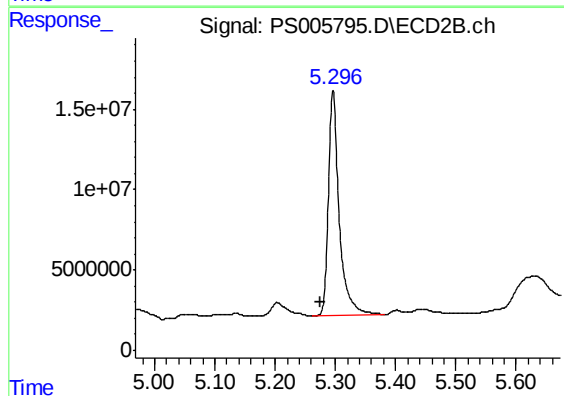

#4 2,4-DCAA

R.T.: 5.296 min
Delta R.T.: 0.020 min
Response: 174731773
Conc: 175.67 ng/ml m