

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073120\
 Data File : PS011535.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2020 09:11
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 11:51:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.481	0.000	201.6E6	0	150.686	N.D. #
5) T	DICAMBA	0.000	7.151	0	136.5E6	N.D.	59.612
6) T	MCPD	0.000	7.151	0	136.5E6	N.D.	71.542
7) T	MCPA	7.687	0.000	9401355	0	2.204	N.D. #
8) T	DICHLORPROP	0.000	7.749	0	10705265	N.D.	17.785
9) T	2,4-D	0.000	7.957	0	3641247	N.D.	4.857
12) T	2,4,5-T	0.000	9.188	0	1625220	N.D.	<MDL
15) T	Picloram	11.033	11.010	137.0E6	145.3E6	21.706	33.234 #
16) T	DCPA	0.000	11.010	0	145.3E6	N.D.	38.431



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073120\
Data File : PS011535.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2020 09:11
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 11:51:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

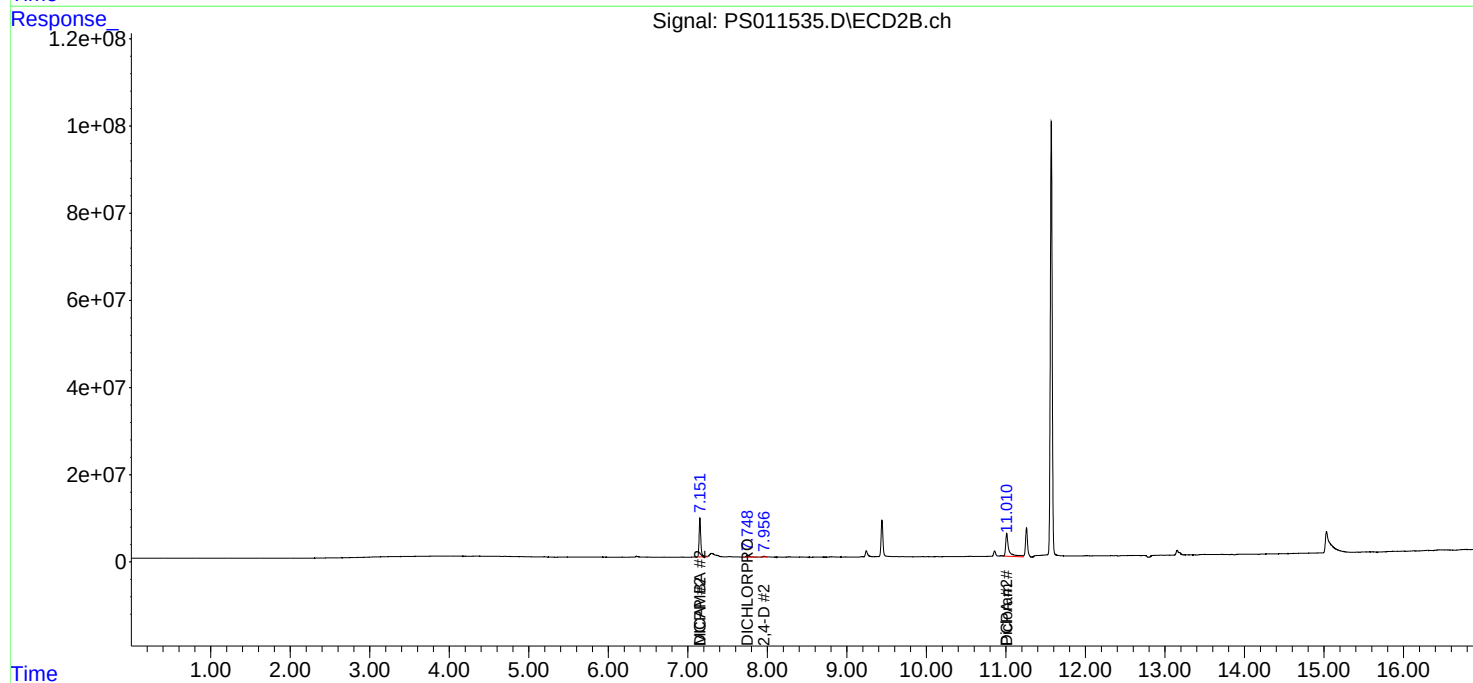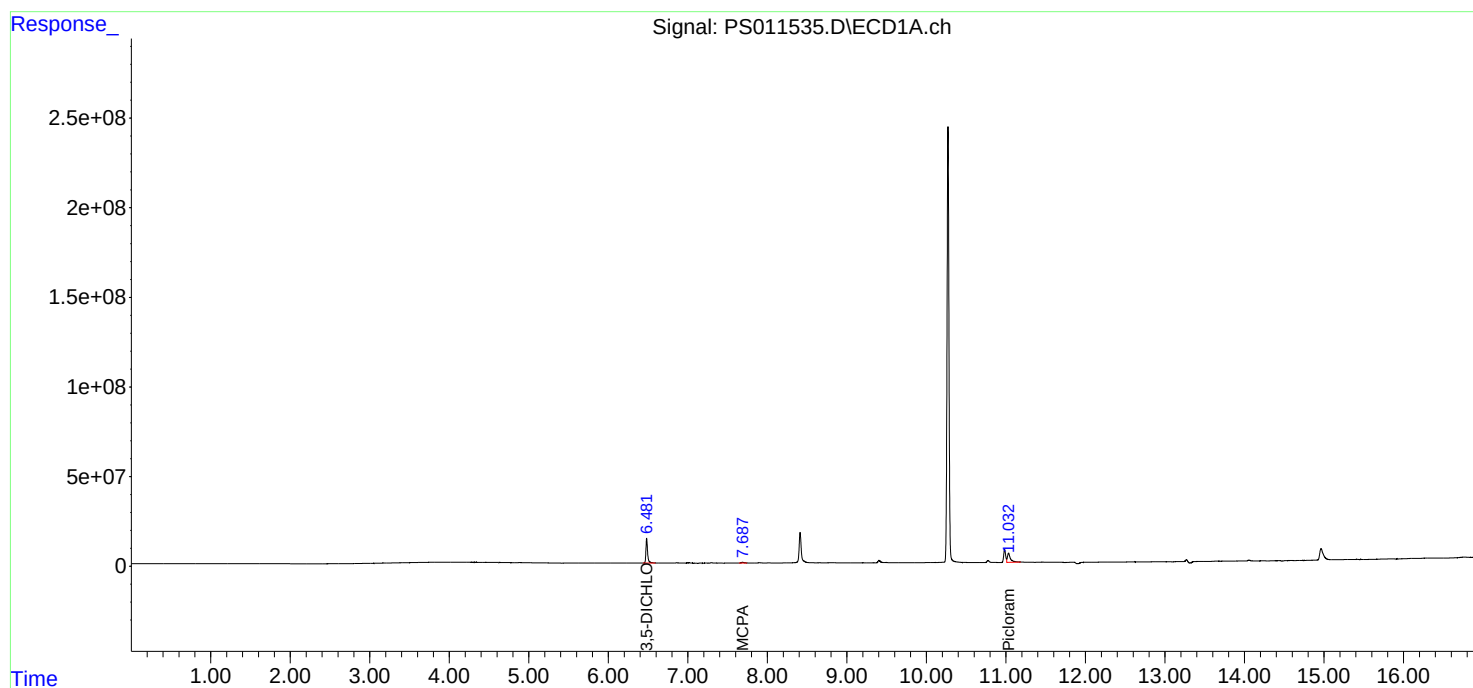


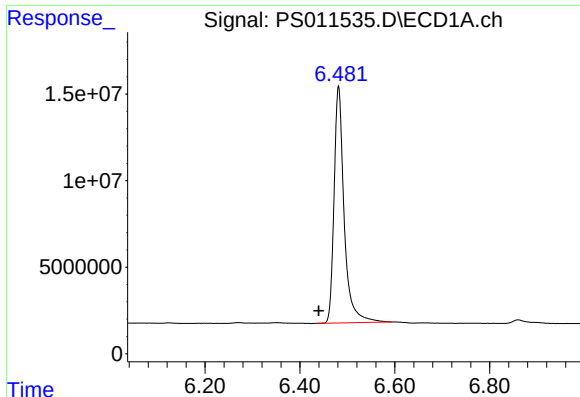

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.481 min
Delta R.T.: 0.042 min
Response: 201642094
Conc: 150.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

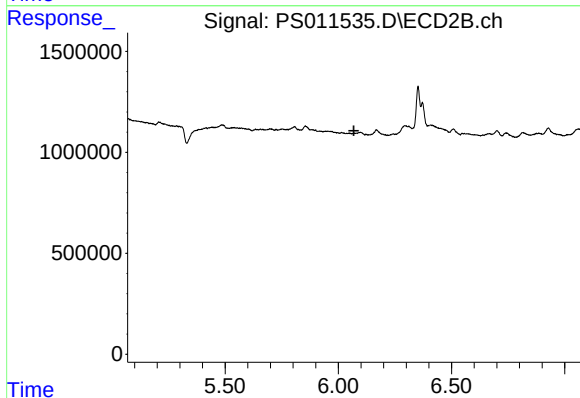


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.069 min
Response: 0
Conc: N.D.

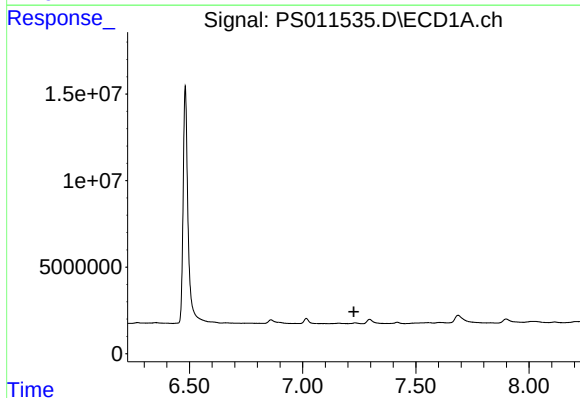


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.226 min
Response: 0
Conc: N.D.

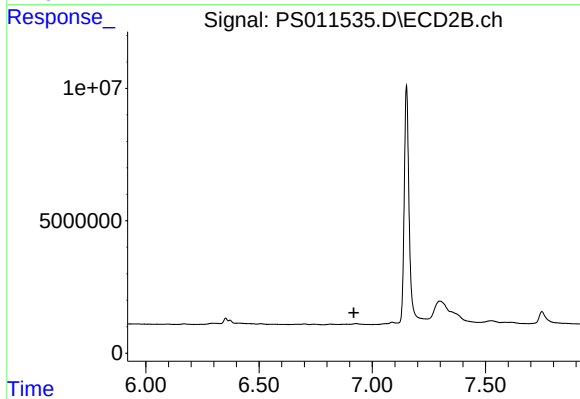

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.918 min
Response: 0
Conc: N.D.

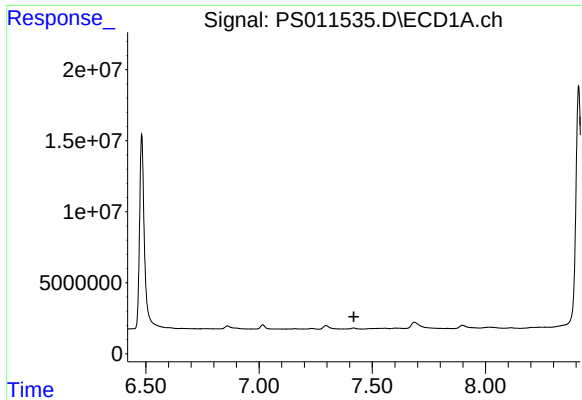

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

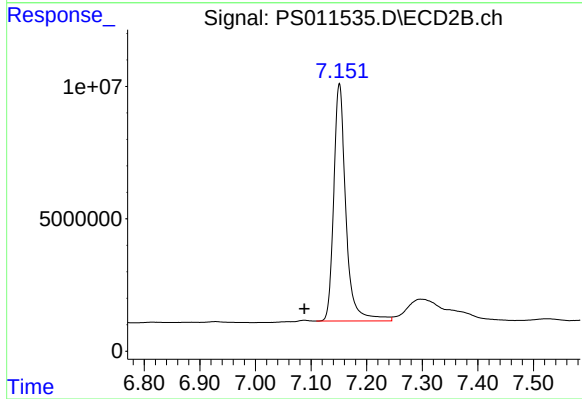


#5 DICAMBA

R.T.: 7.151 min
Delta R.T.: 0.063 min
Response: 136509151
Conc: 59.61 ng/ml

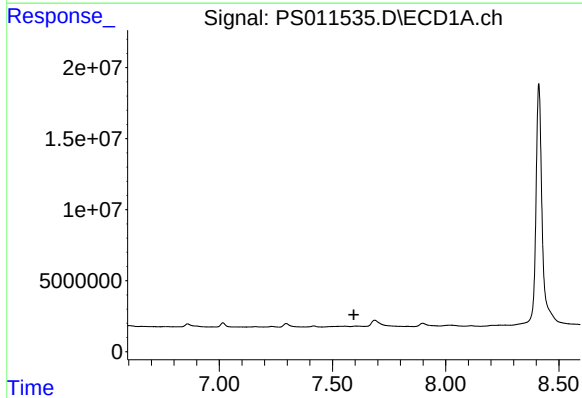


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.594 min
Response: 0
Conc: N.D.

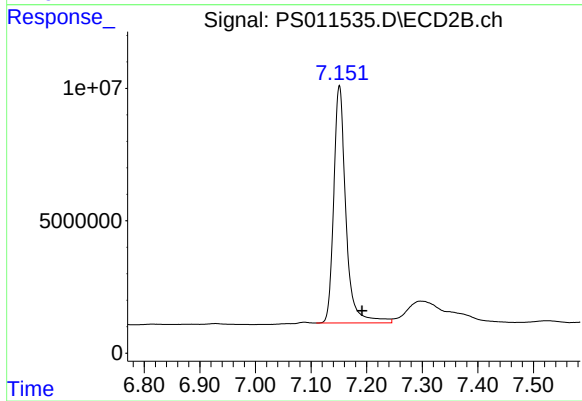

#6 MCP


R.T.: 7.151 min
Delta R.T.: -0.041 min
Response: 136509151
Conc: 71.54 ug/ml

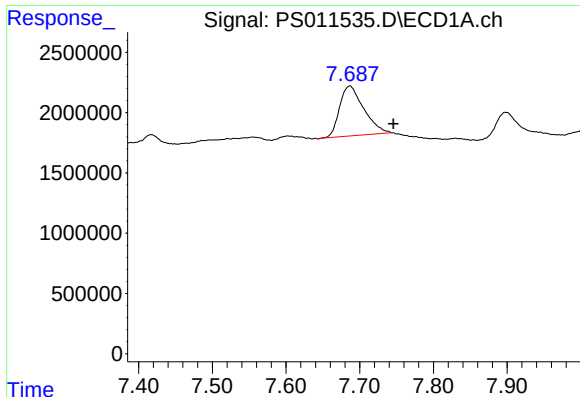

#7 MCPA


R.T.: 7.687 min
Delta R.T.: -0.059 min
Response: 9401355
Conc: 2.20 ug/ml

Instrument :
ECD_S
ClientSampleId :

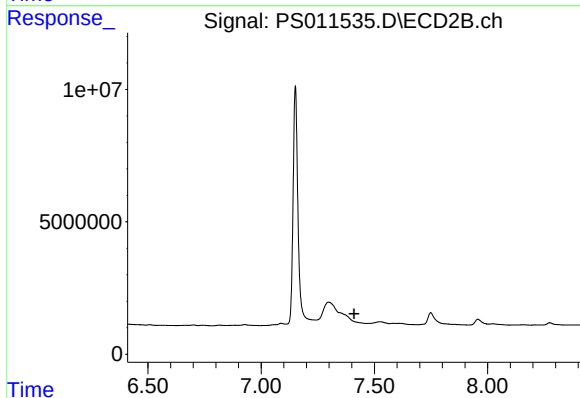


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.410 min
Response: 0
Conc: N.D.

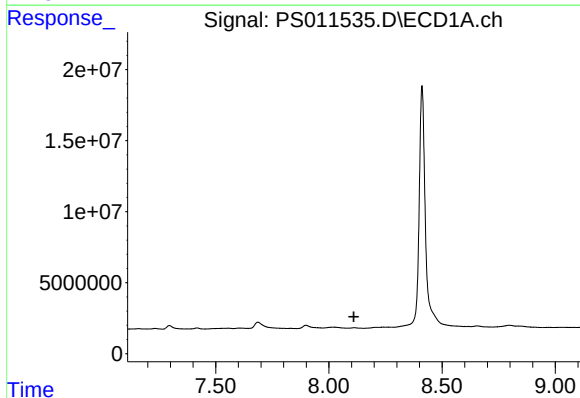


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.110 min
Response: 0
Conc: N.D.

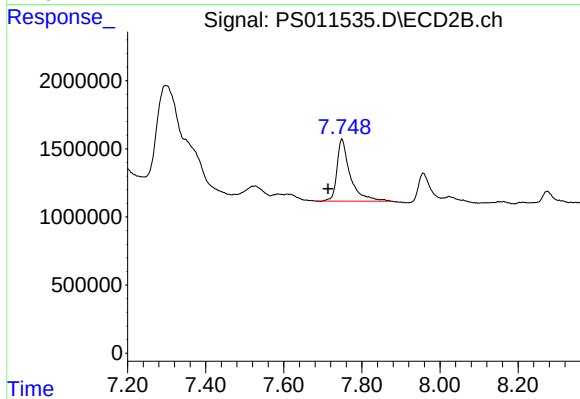

#8 DICHLORPROP


R.T.: 7.749 min
Delta R.T.: 0.036 min
Response: 10705265
Conc: 17.78 ng/ml

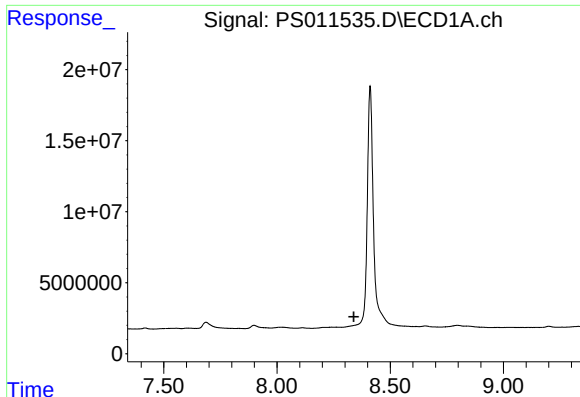

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.339 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

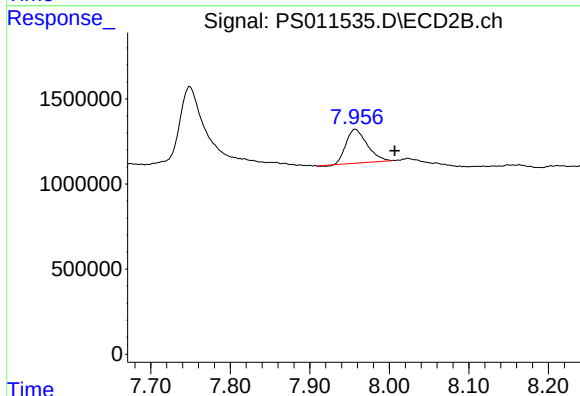


#9 2,4-D

R.T.: 7.957 min
Delta R.T.: -0.050 min
Response: 3641247
Conc: 4.86 ng/ml

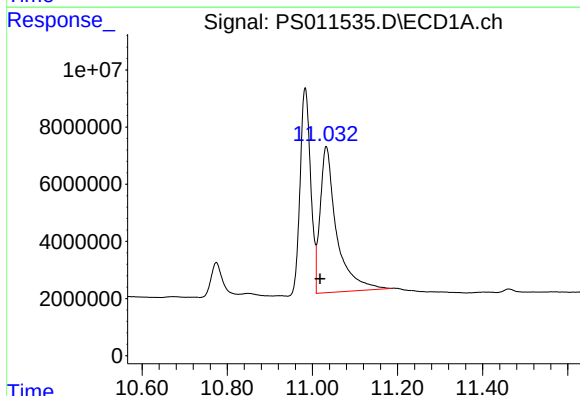


#15 Picloram

R.T.: 11.033 min
Delta R.T.: 0.014 min
Response: 136963352
Conc: 21.71 ng/ml

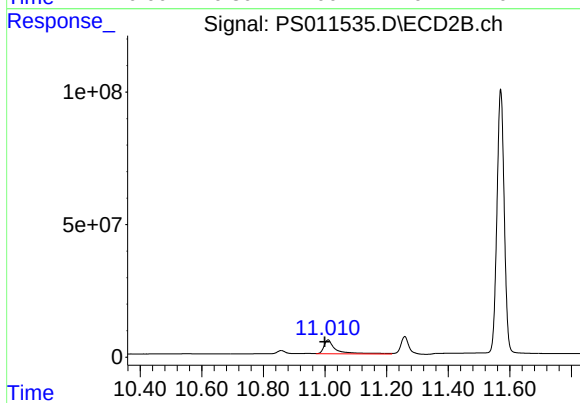

#15 Picloram


R.T.: 11.010 min
Delta R.T.: 0.011 min
Response: 145343607
Conc: 33.23 ng/ml

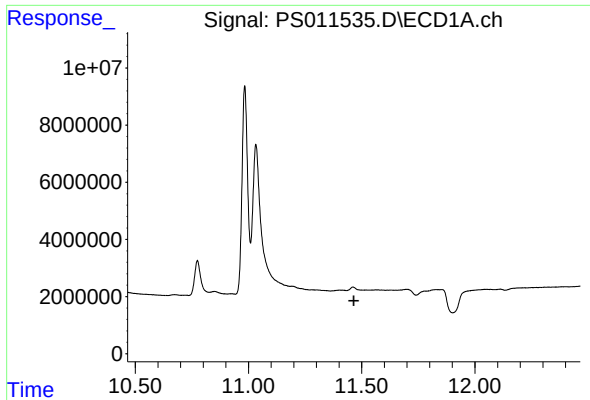

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.466 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

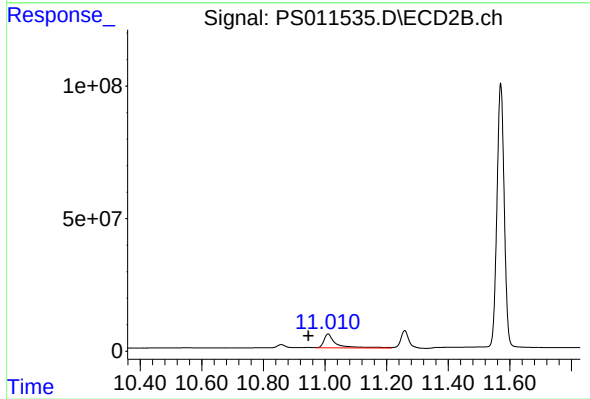

#16 DCPA

R.T.: 11.010 min
Delta R.T.: 0.064 min
Response: 145343607
Conc: 38.43 ng/ml