

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073120\
 Data File : PS011540.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2020 11:24
 Operator : DD\AJ
 Sample : L3478-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 ROLLOFF-VNJ-213

Manual Integrations
 APPROVED

Ankita
 8/3/2020 12:08:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 11:53:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 13 16:10:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.225	6.916	287.9E6	149.0E6	296.715	264.679m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073120\
Data File : PS011540.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2020 11:24
Operator : DD\AJ
Sample : L3478-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
ROLLOFF-VNJ-213


Manual Integrations
APPROVED

Ankita
8/3/2020 12:08:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 11:53:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071320.M
Quant Title : 8080.M
QLast Update : Mon Jul 13 16:10:29 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

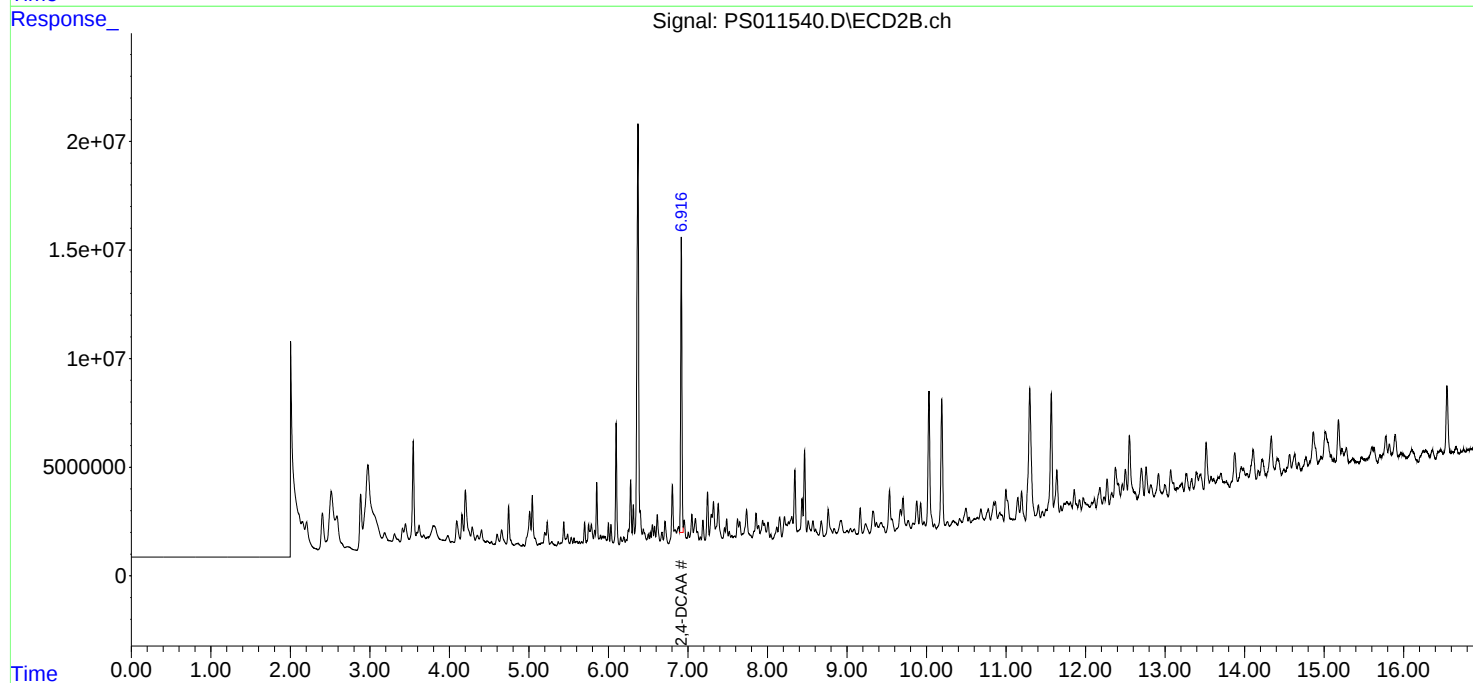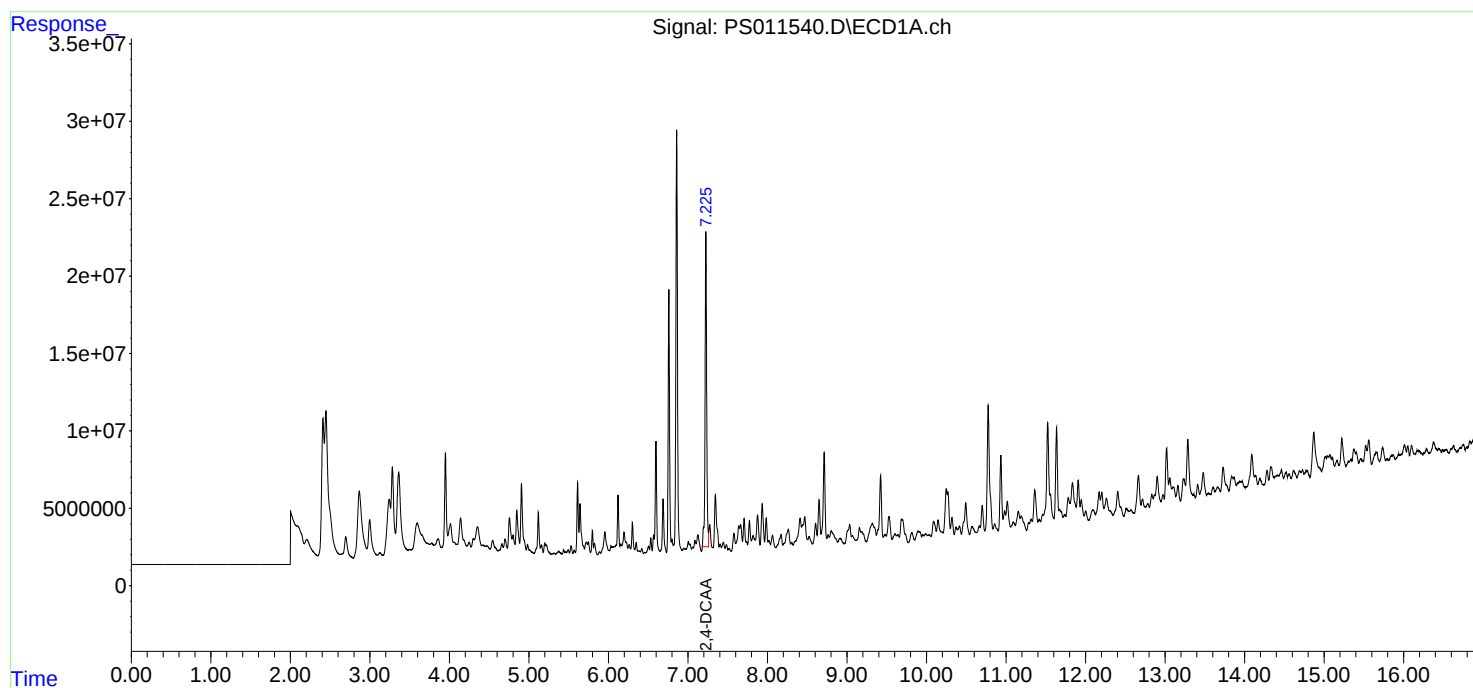

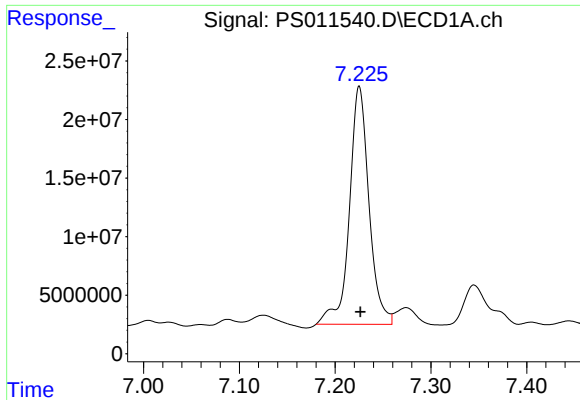


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: -0.001 min
Response: 287914113
Conc: 296.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
ROLLOFF-VNJ-213

Manual Integrations
APPROVED

Ankita
8/3/2020 12:08:42 PM

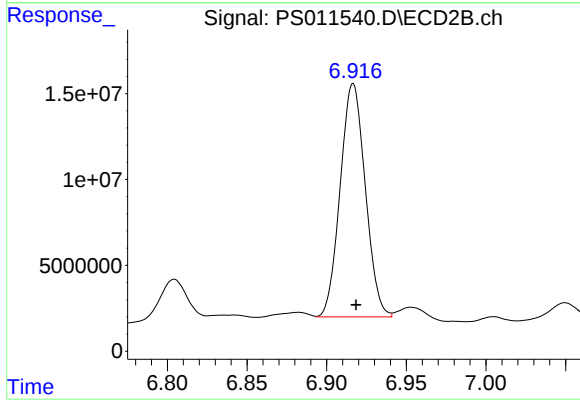

#4 2,4-DCAA

R.T.: 6.916 min
Delta R.T.: -0.002 min
Response: 149020314
Conc: 264.68 ng/ml m