

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073123\
 Data File : PS023876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2023 09:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 20:13:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072023.M
 Quant Title : 8080.M
 QLast Update : Thu Jul 20 19:21:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.371	6.805	984.1E6	324.0E6	496.338	476.436
Target Compounds							
1) T	Dalapon	0.000	2.626f	0	331914	N.D.	<MDL
2) T	3,5-DICHL...	5.725	0.000	904365	0	<MDL	N.D. #
3) T	4-Nitroph...	6.213	0.000	4771553	0	3.838	N.D. #
8) T	DICHLORPROP	7.153f	0.000	900561	0	<MDL	N.D. #
9) T	2,4-D	0.000	7.817f	0	99724	N.D.	<MDL
10) T	Pentachlo...	7.525	0.000	2760804	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.052	0.000	1611215	0	<MDL	N.D. #
12) T	2,4,5-T	8.309	9.072	884090	3759598	<MDL	<MDL #
13) T	2,4-DB	8.764f	0.000	1032974	0	<MDL	N.D. #
14) T	DINOSEB	9.872	0.000	109732	0	<MDL	N.D. #
15) T	Picloram	9.698	10.820	40926313	13459962	2.670	2.219
16) T	DCPA	10.133	10.820	674291	13459962	<MDL	2.831 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS073123\
Data File : PS023876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2023 09:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 20:13:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072023.M
Quant Title : 8080.M
QLast Update : Thu Jul 20 19:21:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

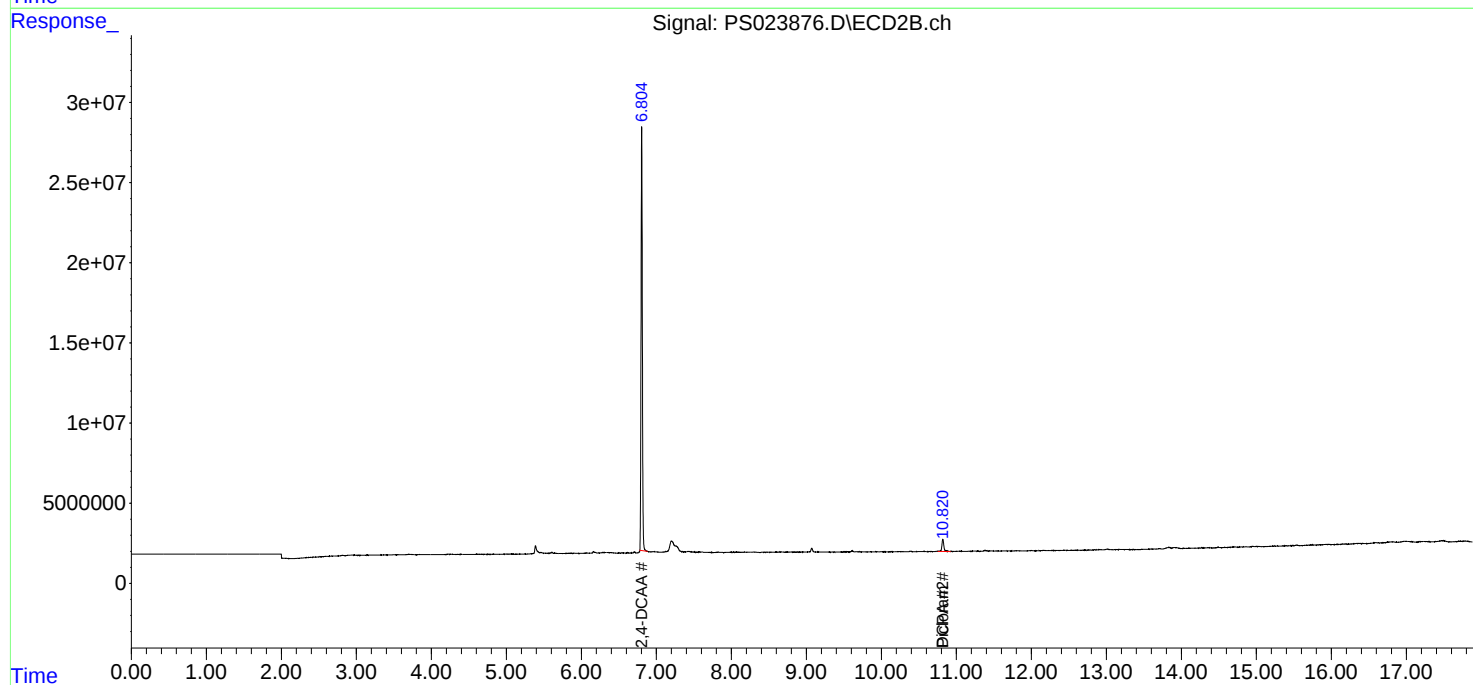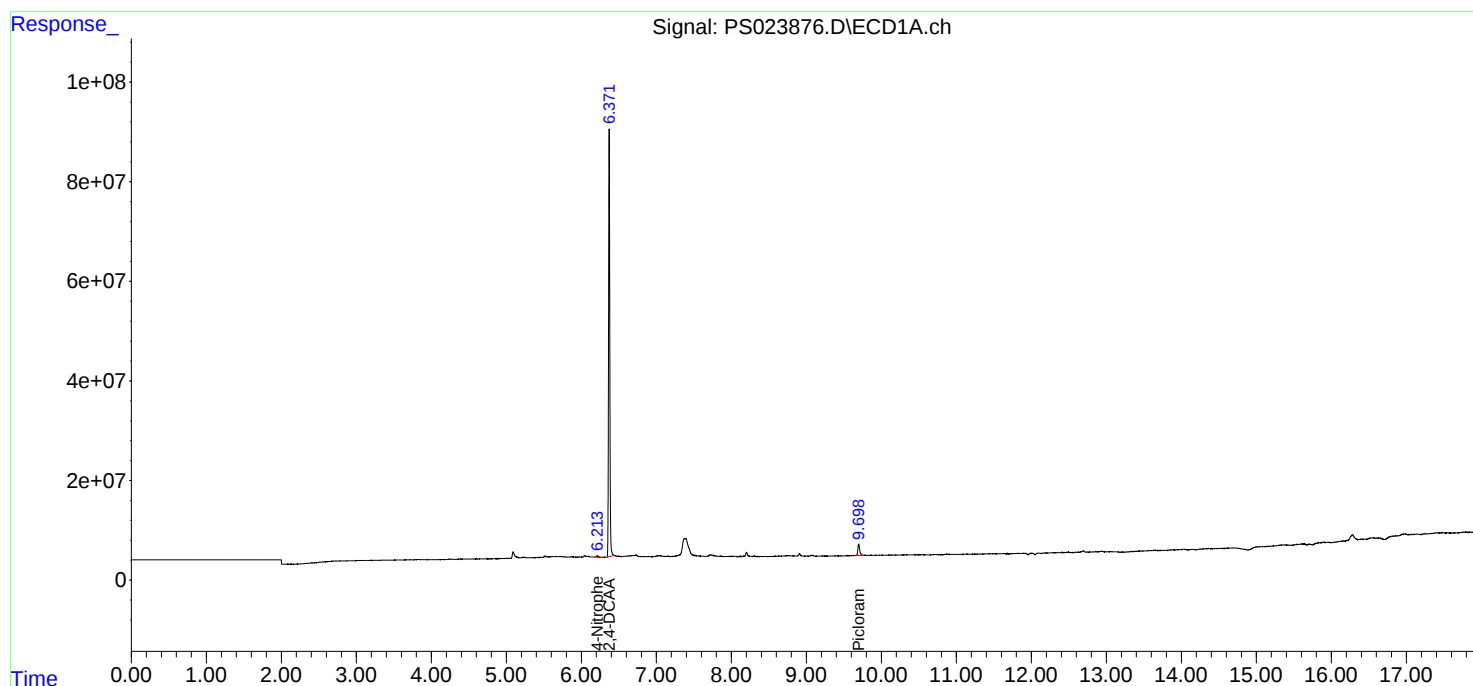


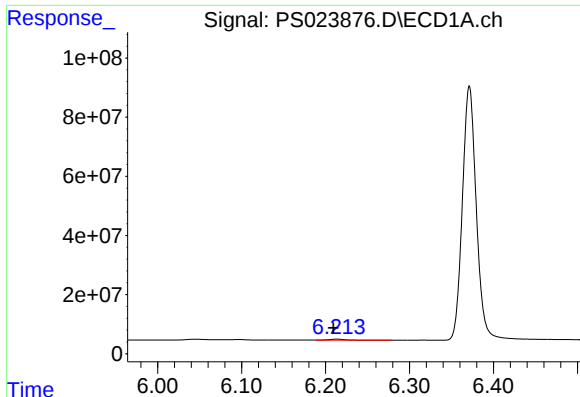

#3 4-Nitrophenol


R.T.: 6.213 min
Delta R.T.: 0.004 min
Response: 4771553
Conc: 3.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

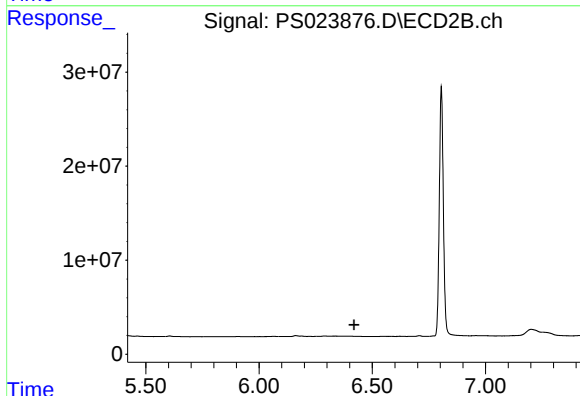


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.419 min
Response: 0
Conc: N.D.

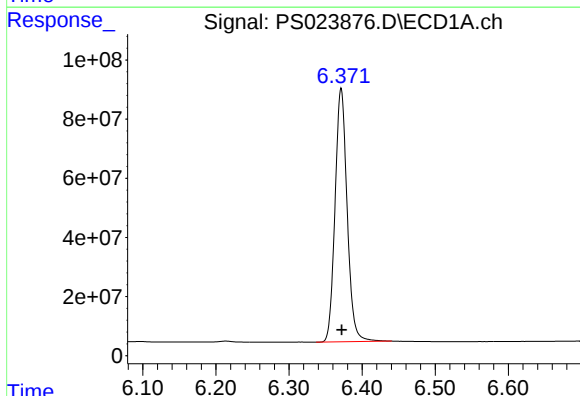


#4 2,4-DCAA

R.T.: 6.371 min
Delta R.T.: 0.000 min
Response: 984057448
Conc: 496.34 ng/ml

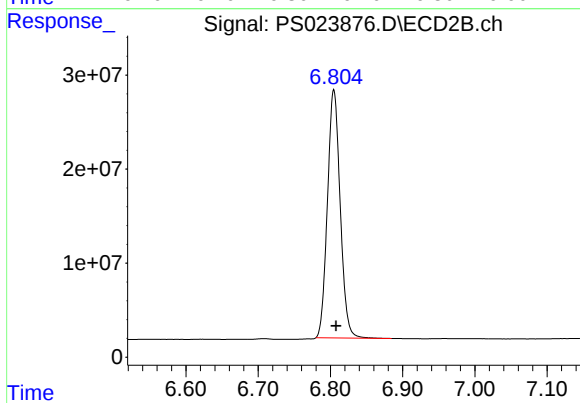

#4 2,4-DCAA


R.T.: 6.805 min
Delta R.T.: -0.003 min
Response: 324023453
Conc: 476.44 ng/ml

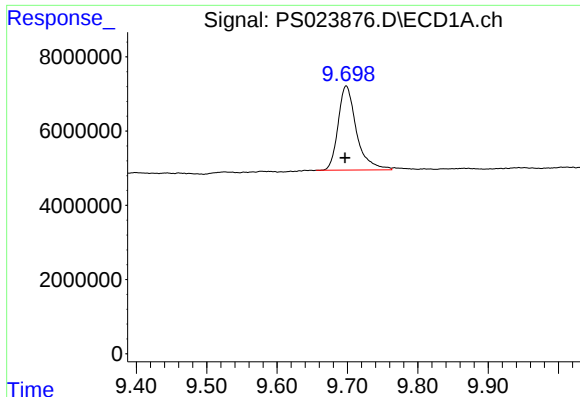

#15 Picloram


R.T.: 9.698 min
Delta R.T.: 0.002 min
Response: 40926313
Conc: 2.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

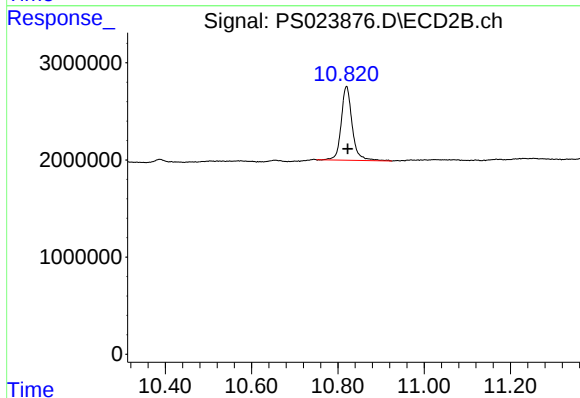


#15 Picloram

R.T.: 10.820 min
Delta R.T.: -0.003 min
Response: 13459962
Conc: 2.22 ng/ml

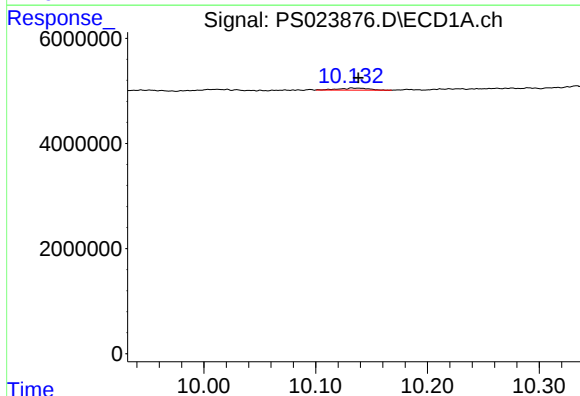

#16 DCPA

R.T.: 10.133 min
Delta R.T.: -0.006 min
Response: 674291
Conc: N.D.

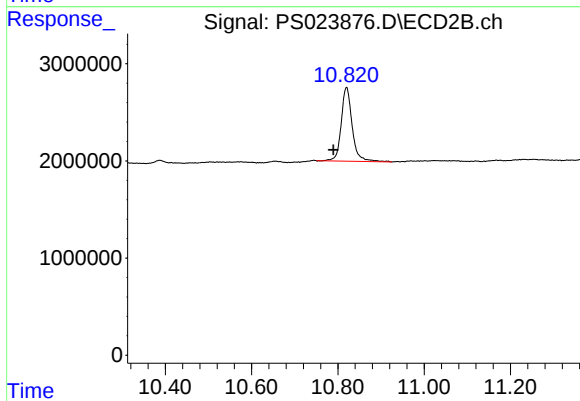

#16 DCPA

R.T.: 10.820 min
Delta R.T.: 0.030 min
Response: 13459962
Conc: 2.83 ng/ml