

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080118\
 Data File : PS001325.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2018 16:59
 Operator : UA
 Sample : PB111622BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.619	11.038	107.5E6	92216118	579.626	507.031
Target Compounds							
1) T	Dalapon	2.962	0.000	976206	0	4.117	N.D. #
5) T	DICAMBA	0.000	11.281	0	4157923	N.D.	6.067 #
6) T	MCPD	12.313	0.000	4857079	0	9.664	N.D. #
7) T	MCPA	12.588	0.000	8379320	0	10.625	N.D. #
14) T	DINOSEB	0.000	15.733	0	10064300	N.D.	14.159 #
15) T	Picloram	0.000	16.978	0	15482959	N.D.	11.232 #
16) T	DCPA	0.000	16.978	0	15482959	N.D.	10.720 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080118\
Data File : PS001325.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2018 16:59
Operator : UA
Sample : PB111622BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 00:47:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

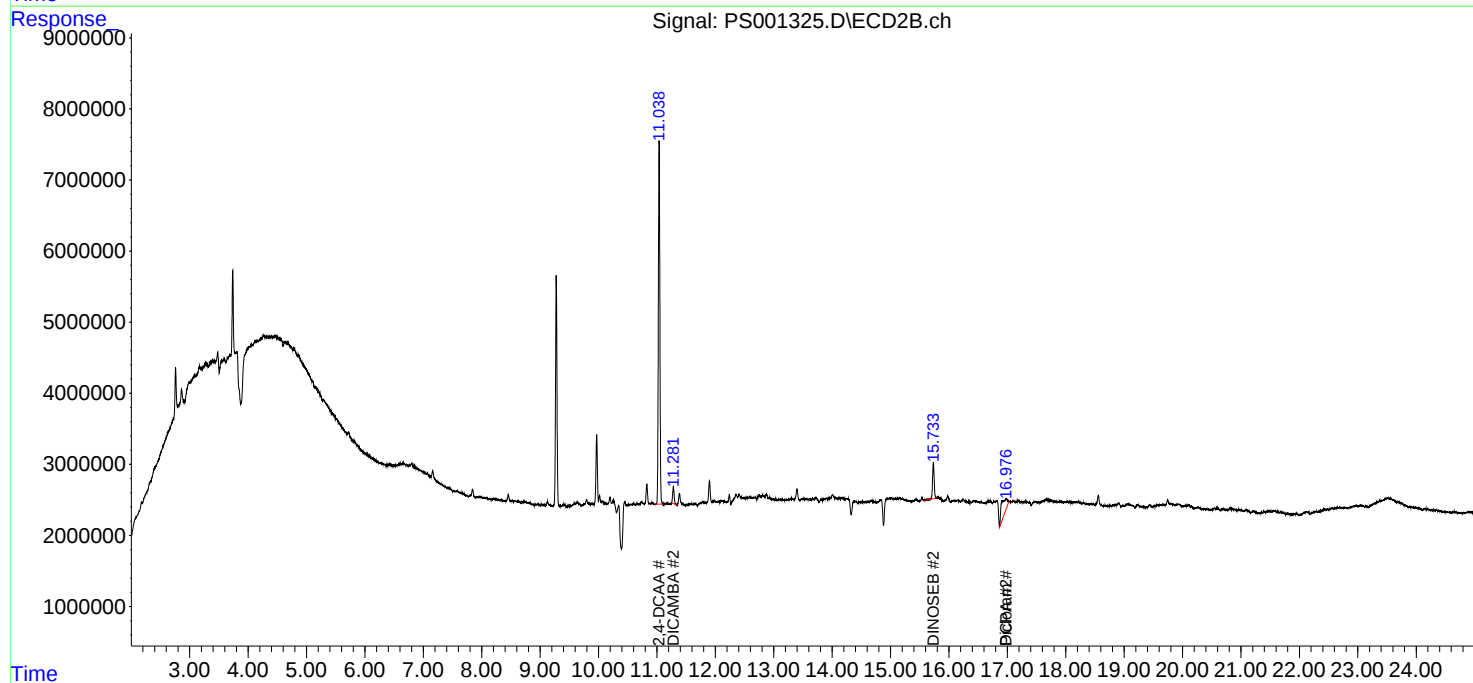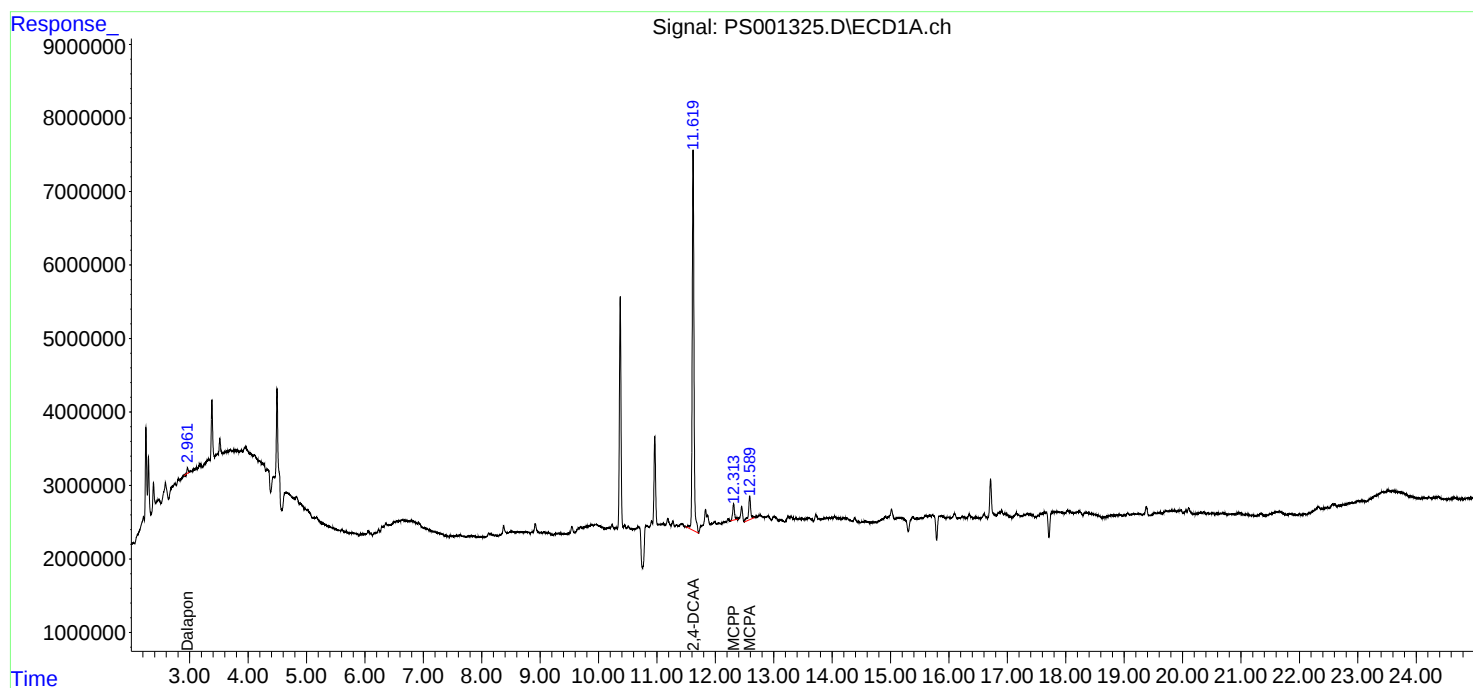


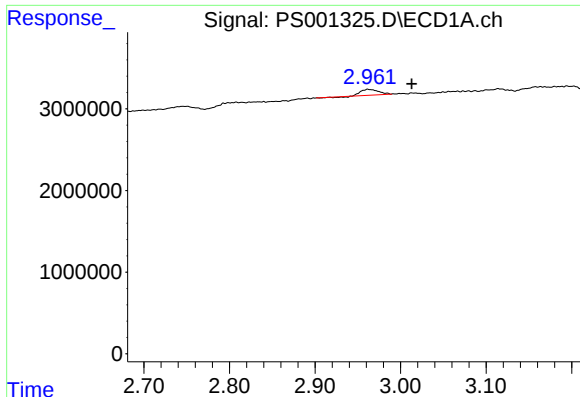

#1 Dalapon


R.T.: 2.962 min
Delta R.T.: -0.051 min
Response: 976206
Conc: 4.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

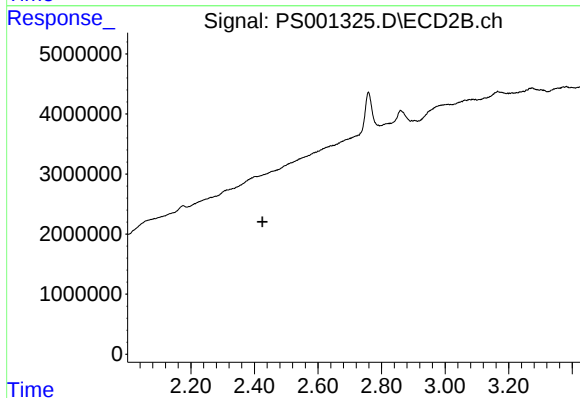


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.426 min
Response: 0
Conc: N.D.

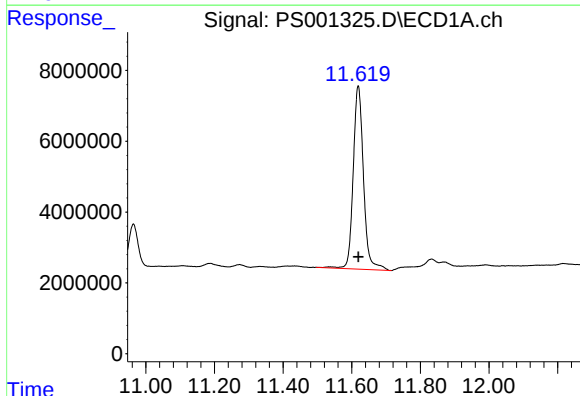


#4 2,4-DCAA

R.T.: 11.619 min
Delta R.T.: 0.000 min
Response: 107549551
Conc: 579.63 ng/ml

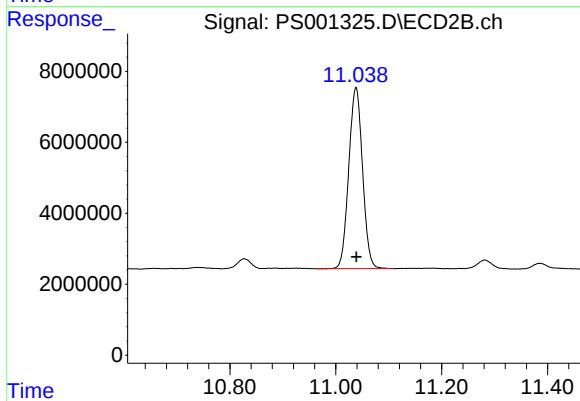

#4 2,4-DCAA


R.T.: 11.038 min
Delta R.T.: 0.000 min
Response: 92216118
Conc: 507.03 ng/ml

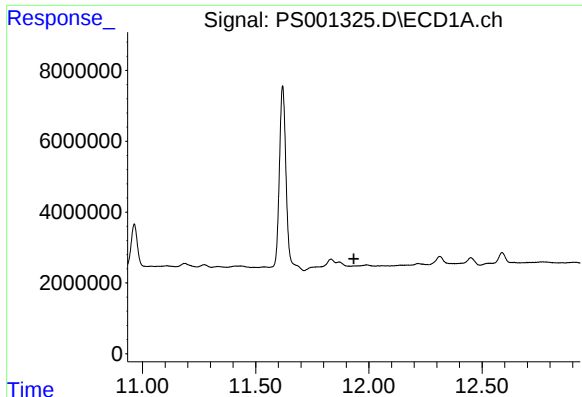

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

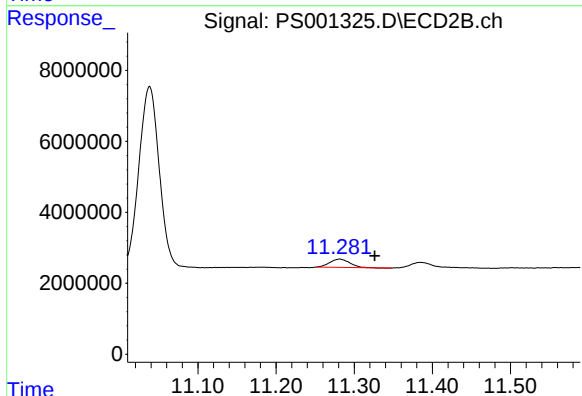


#5 DICAMBA

R.T.: 11.281 min
Delta R.T.: -0.045 min
Response: 4157923
Conc: 6.07 ng/ml

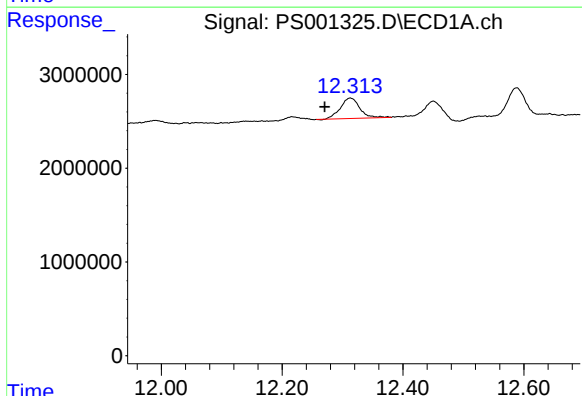


#6 MCP

R.T.: 12.313 min
Delta R.T.: 0.043 min
Response: 4857079
Conc: 9.66 ug/ml

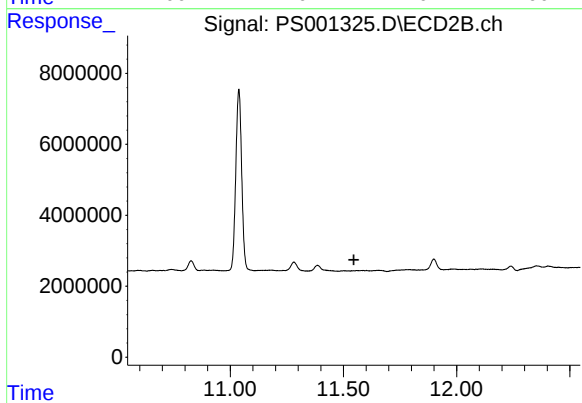

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

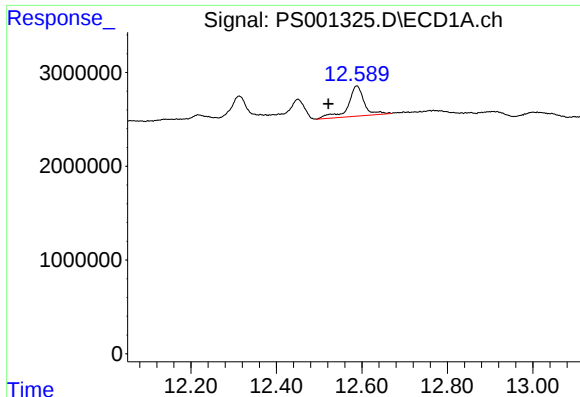

#7 MCPA


R.T.: 12.588 min
Delta R.T.: 0.067 min
Response: 8379320
Conc: 10.63 ug/ml

Instrument :
ECD_S
ClientSampleId :

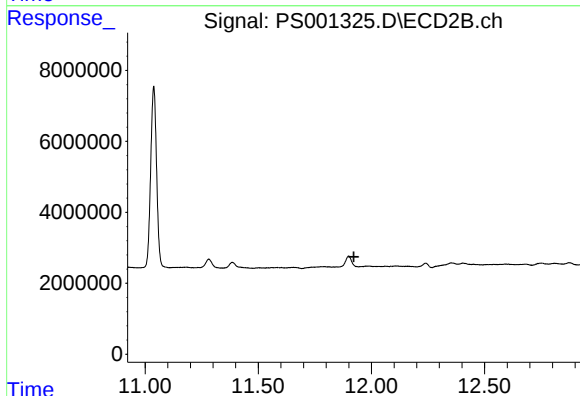


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.922 min
Response: 0
Conc: N.D.

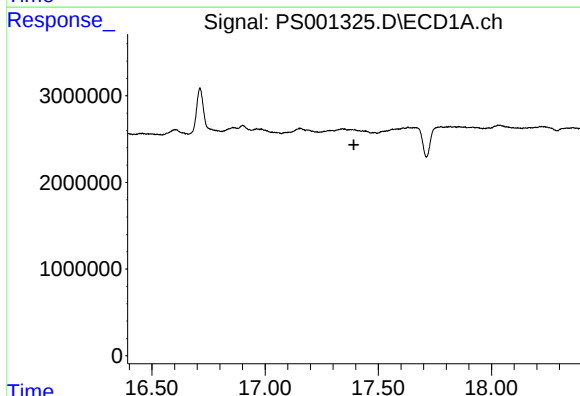


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.392 min
Response: 0
Conc: N.D.

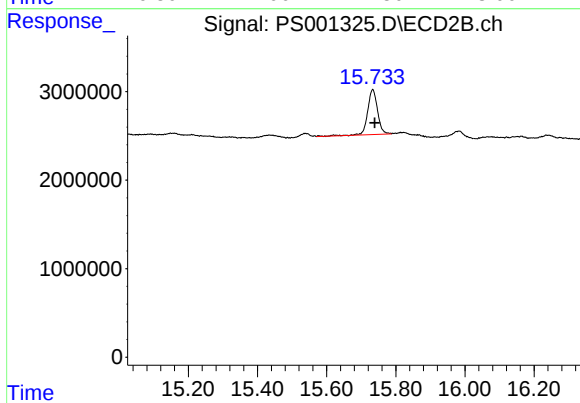

#14 DINOSEB


R.T.: 15.733 min
Delta R.T.: -0.006 min
Response: 10064300
Conc: 14.16 ng/ml

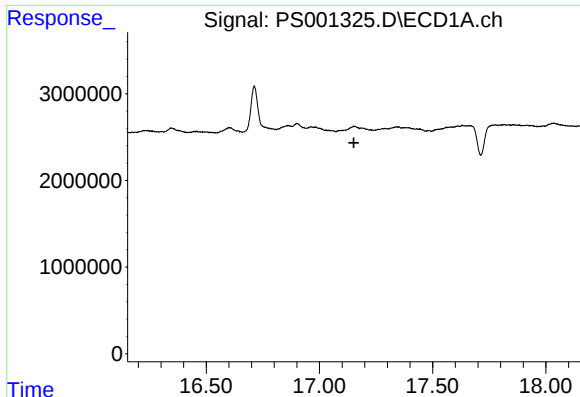

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

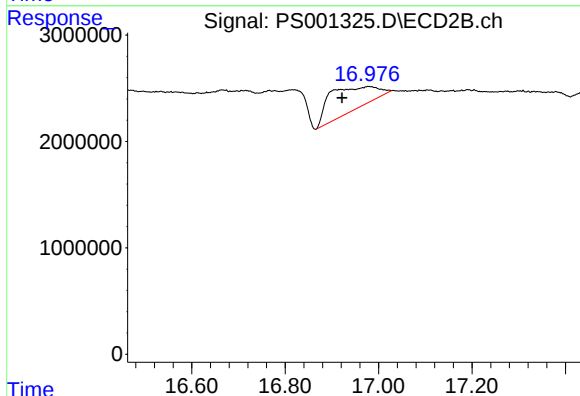


#15 Picloram

R.T.: 16.978 min
Delta R.T.: 0.056 min
Response: 15482959
Conc: 11.23 ng/ml

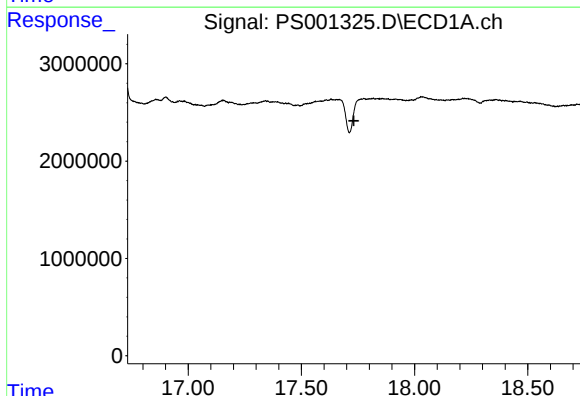

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.732 min
Response: 0
Conc: N.D.

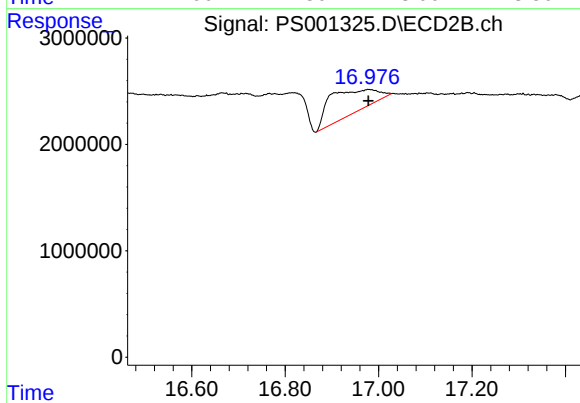

#16 DCPA

R.T.: 16.978 min
Delta R.T.: 0.000 min
Response: 15482959
Conc: 10.72 ng/ml