

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080118\
 Data File : PS001327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2018 18:01
 Operator : UA
 Sample : J4231-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.637	11.056	45413310	40176461	244.750	220.902
Target Compounds							
1) T	Dalapon	2.980	2.439	1843142	2565418	7.773	11.258 #
5) T	DICAMBA	0.000	11.300	0	6317876	N.D.	9.218 #
6) T	MCPD	12.329	0.000	8181174	0	16.277	N.D. #
7) T	MCPA	12.468	0.000	10670172	0	13.530	N.D. #
10) T	Pentachlo...	13.892	13.415	2977099	2532242	1.057	0.920
12) T	2,4,5-T	0.000	14.677	0	2204529	N.D.	2.387 #
13) T	2,4-DB	0.000	15.320	0	36546521	N.D.	274.451 #
14) T	DINOSEB	0.000	15.751	0	17984337	N.D.	25.301 #
15) T	Picloram	0.000	16.930	0	19644161	N.D.	14.250 #
16) T	DCPA	0.000	16.997	0	33793744	N.D.	23.398 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080118\
Data File : PS001327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2018 18:01
Operator : UA
Sample : J4231-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 00:47:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

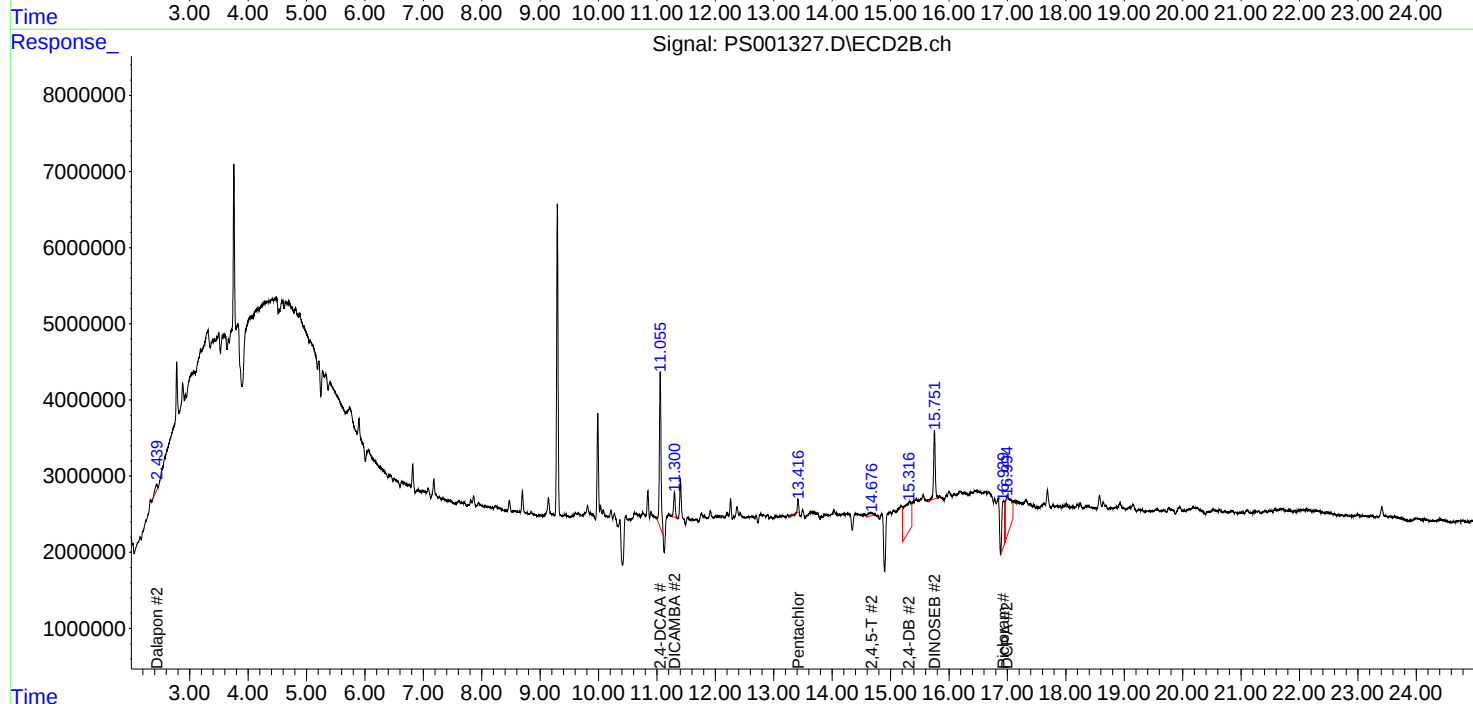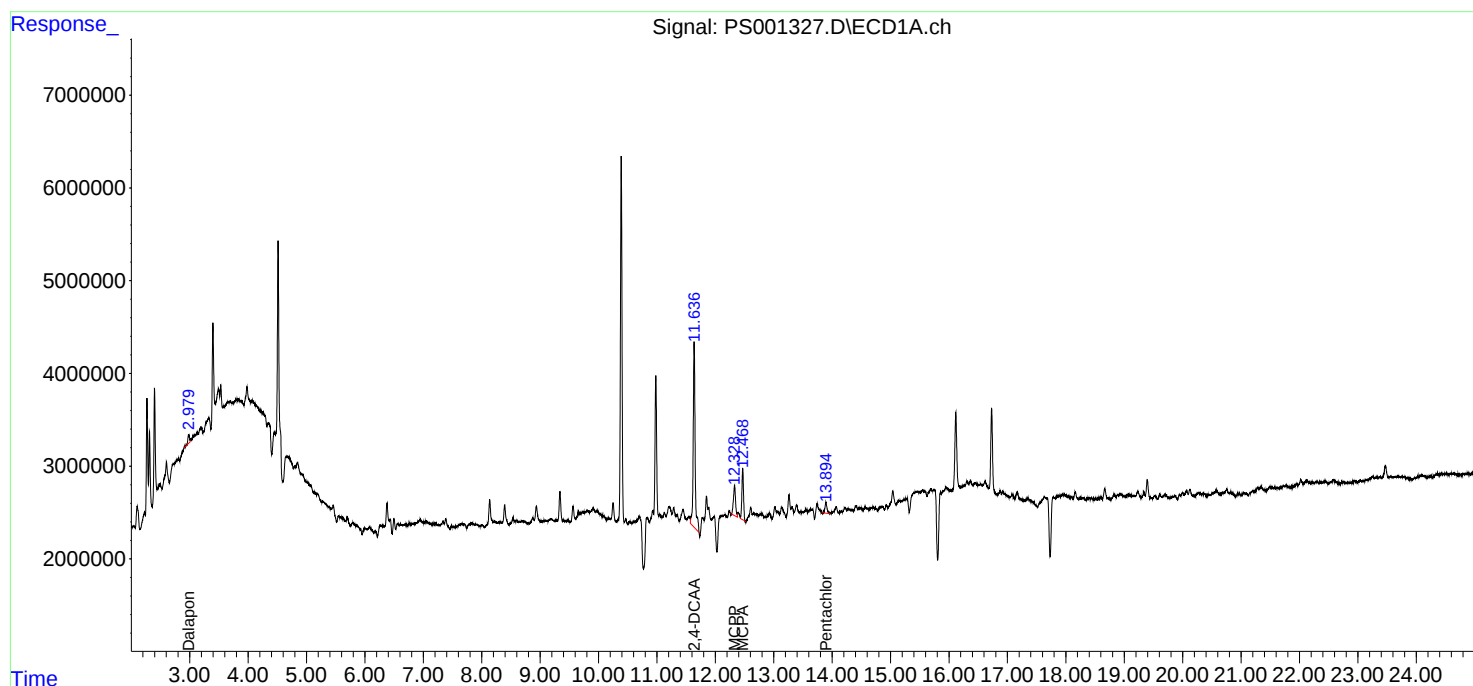


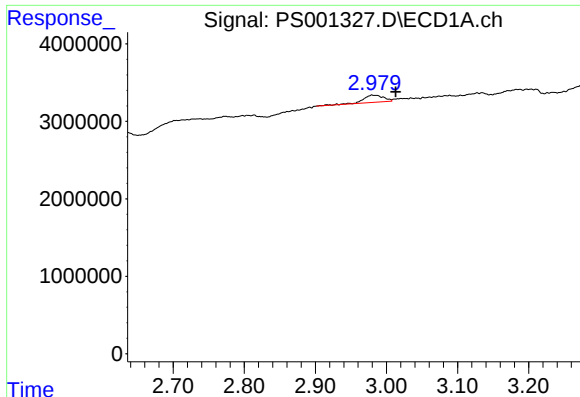

#1 Dalapon


R.T.: 2.980 min
Delta R.T.: -0.033 min
Response: 1843142
Conc: 7.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

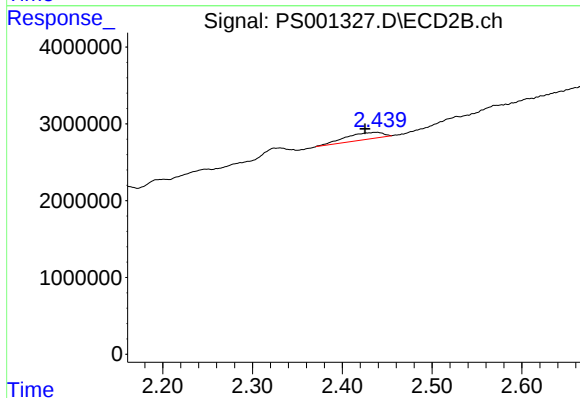


#1 Dalapon

R.T.: 2.439 min
Delta R.T.: 0.014 min
Response: 2565418
Conc: 11.26 ng/ml

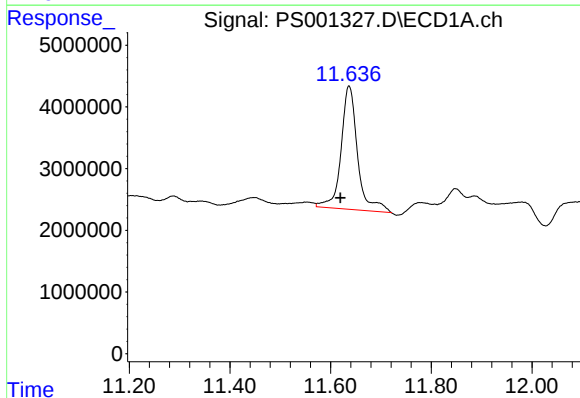


#4 2,4-DCAA

R.T.: 11.637 min
Delta R.T.: 0.017 min
Response: 45413310
Conc: 244.75 ng/ml

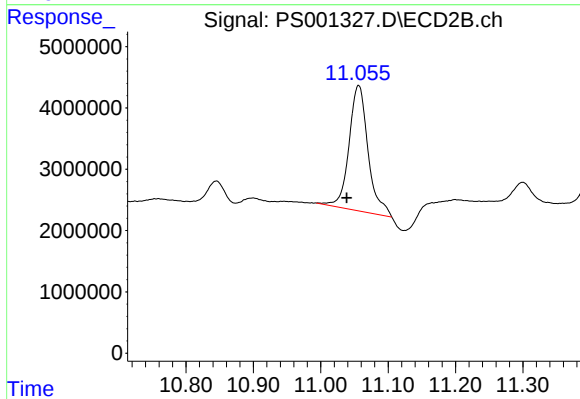

#4 2,4-DCAA


R.T.: 11.056 min
Delta R.T.: 0.018 min
Response: 40176461
Conc: 220.90 ng/ml

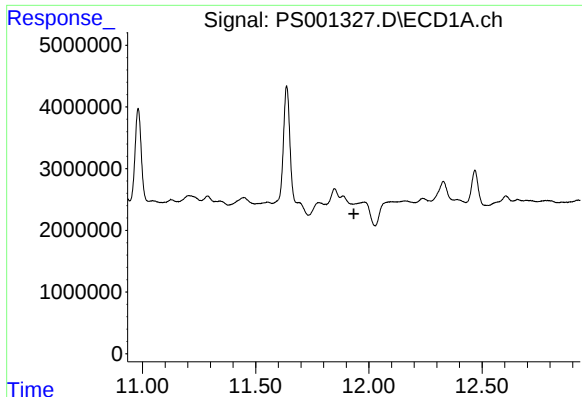

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

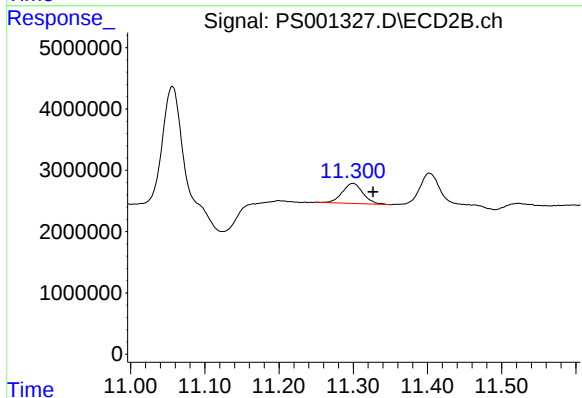


#5 DICAMBA

R.T.: 11.300 min
Delta R.T.: -0.027 min
Response: 6317876
Conc: 9.22 ng/ml

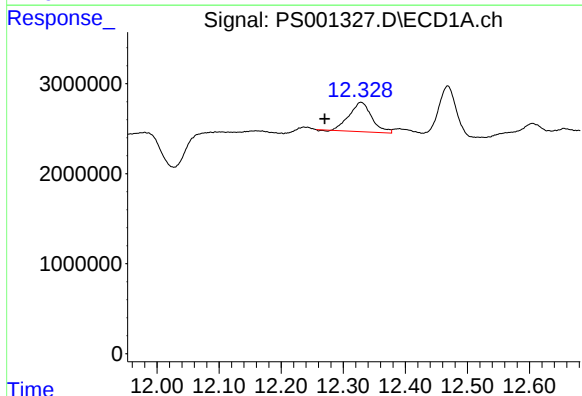


#6 MCP

R.T.: 12.329 min
Delta R.T.: 0.058 min
Response: 8181174
Conc: 16.28 ug/ml

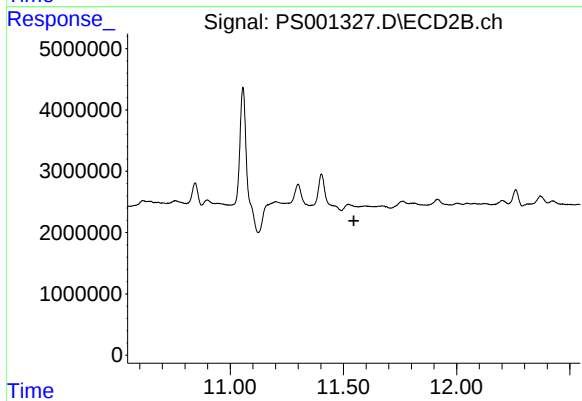

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

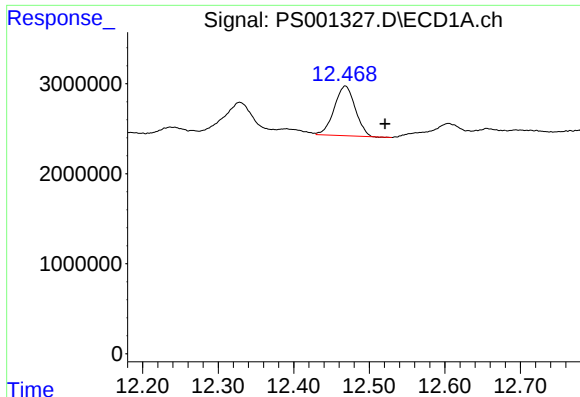

#7 MCPA


R.T.: 12.468 min
Delta R.T.: -0.053 min
Response: 10670172
Conc: 13.53 ug/ml

Instrument :
ECD_S
ClientSampleId :

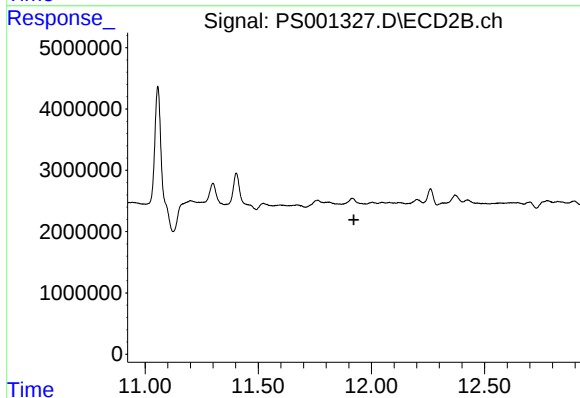


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.922 min
Response: 0
Conc: N.D.

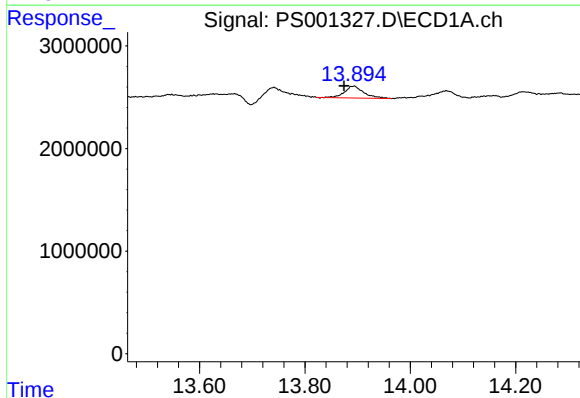


#10 Pentachlorophenol

R.T.: 13.892 min
Delta R.T.: 0.018 min
Response: 2977099
Conc: 1.06 ng/ml

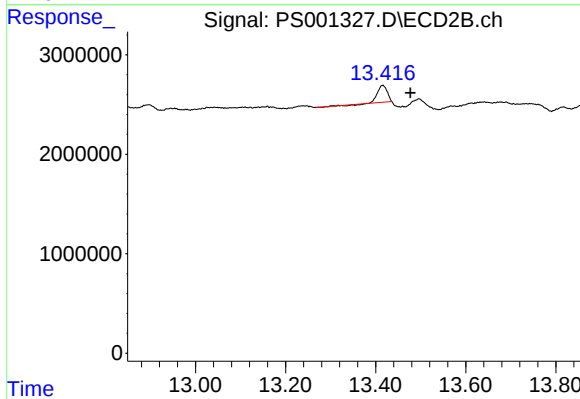

#10 Pentachlorophenol


R.T.: 13.415 min
Delta R.T.: -0.062 min
Response: 2532242
Conc: 0.92 ng/ml

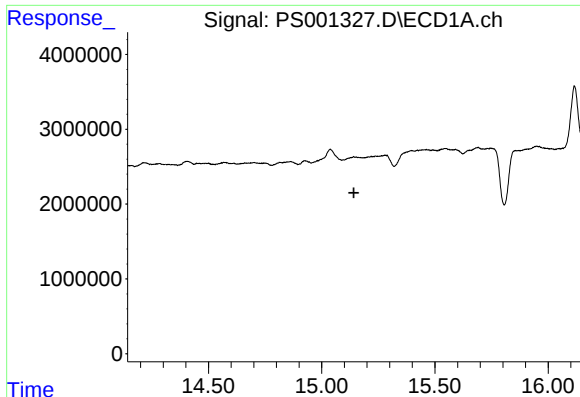

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.142 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

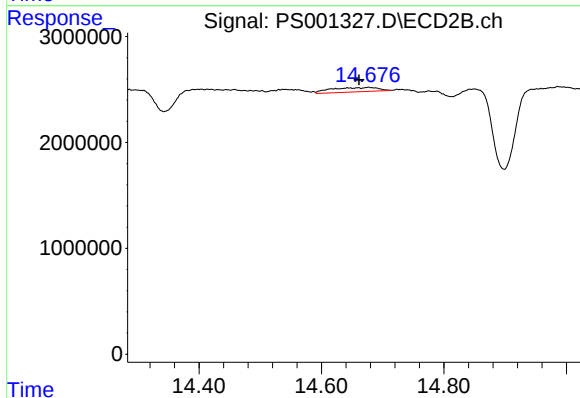


#12 2,4,5-T

R.T.: 14.677 min
Delta R.T.: 0.015 min
Response: 2204529
Conc: 2.39 ng/ml

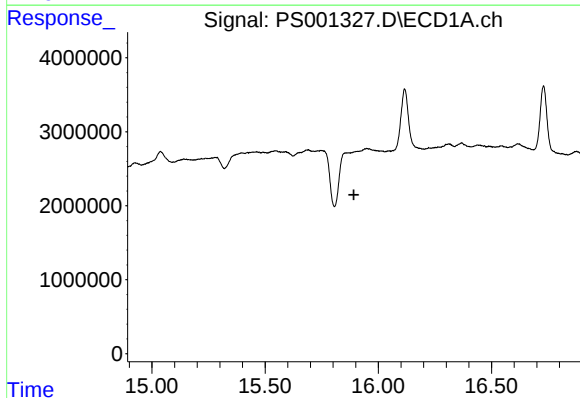


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.892 min
Response: 0
Conc: N.D.

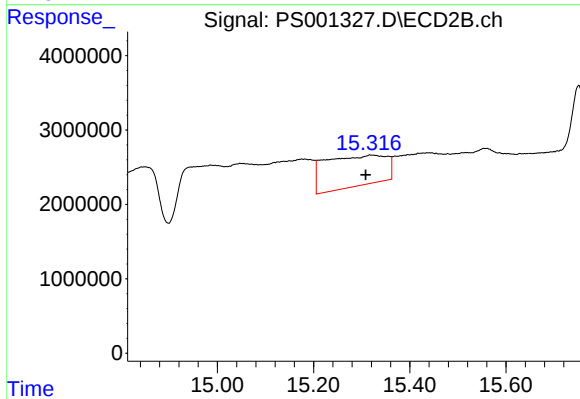

#13 2,4-DB


R.T.: 15.320 min
Delta R.T.: 0.011 min
Response: 36546521
Conc: 274.45 ng/ml

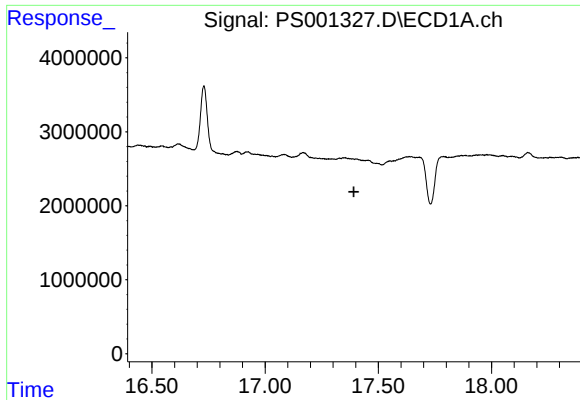

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

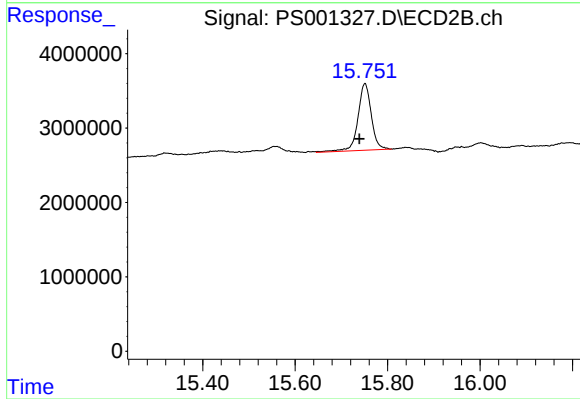


#14 DINOSEB

R.T.: 15.751 min
Delta R.T.: 0.012 min
Response: 17984337
Conc: 25.30 ng/ml

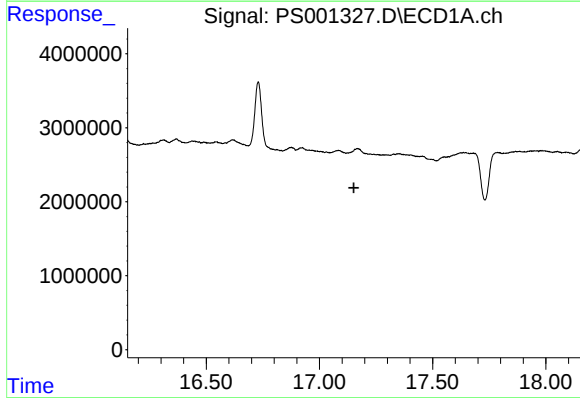


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.152 min
Response: 0
Conc: N.D.

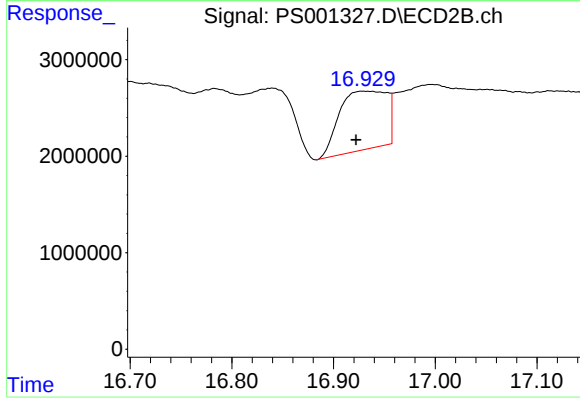

#15 Picloram


R.T.: 16.930 min
Delta R.T.: 0.008 min
Response: 19644161
Conc: 14.25 ng/ml

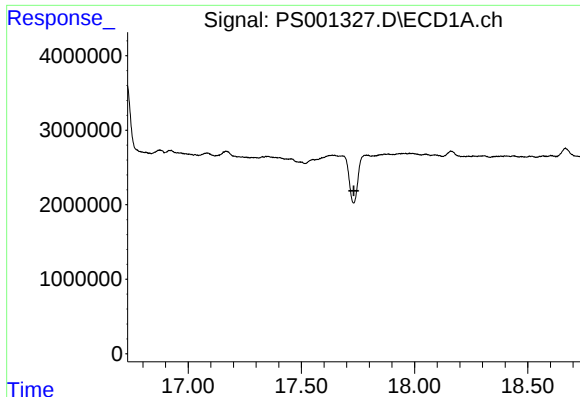

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

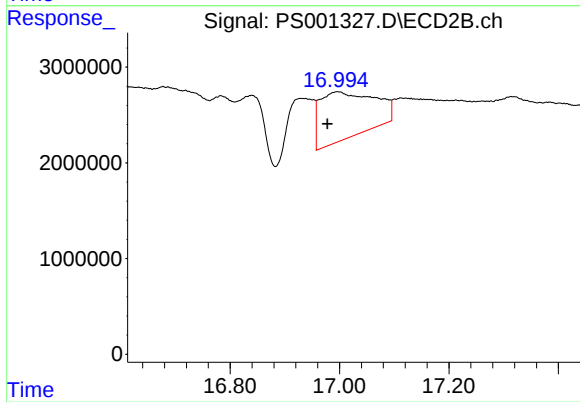

#16 DCPA

R.T.: 16.997 min
Delta R.T.: 0.019 min
Response: 33793744
Conc: 23.40 ng/ml