

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080118\
 Data File : PS001339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2018 00:13
 Operator : UA
 Sample : J4231-21
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:52:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.616	11.037	59001231	45521465	317.980	250.290
Target Compounds							
5) T	DICAMBA	0.000	11.280	0	5881875	N.D.	8.582 #
6) T	MCPD	12.309	0.000	7274480	0	14.473	N.D. #
12) T	2,4,5-T	0.000	14.623	0	8312242	N.D.	8.999 #
14) T	DINOSEB	0.000	15.731	0	24588141	N.D.	34.592 #
15) T	Picloram	0.000	16.976	0	21002013	N.D.	15.235 #
16) T	DCPA	0.000	16.976	0	21002013	N.D.	14.541 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080118\
Data File : PS001339.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2018 00:13
Operator : UA
Sample : J4231-21
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 00:52:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

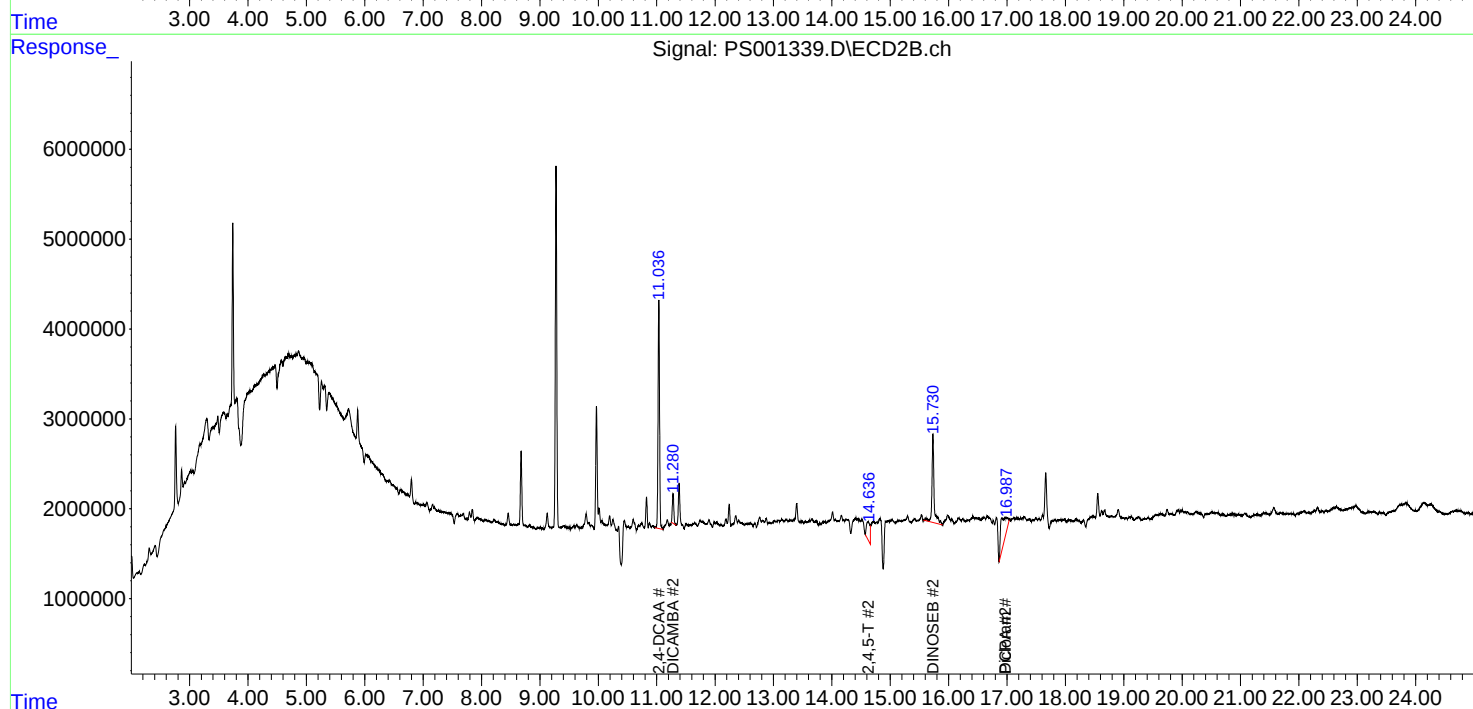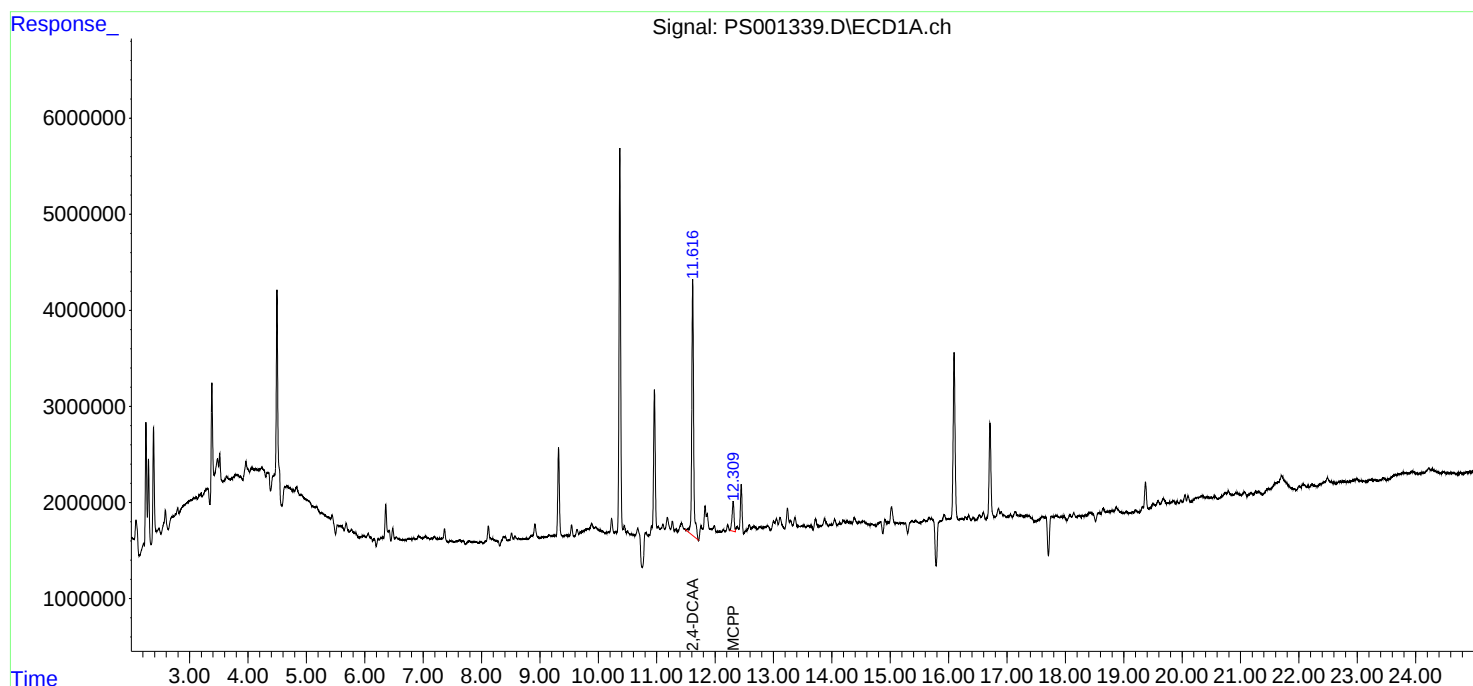


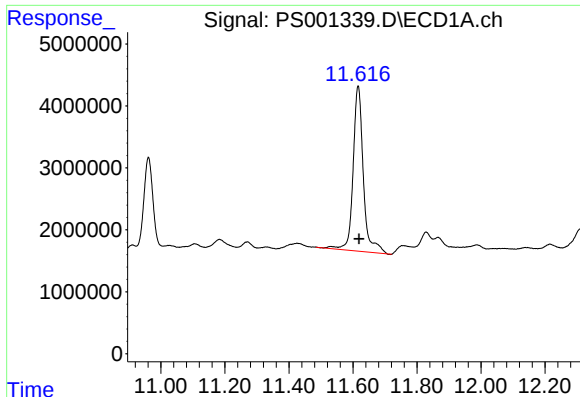

#4 2,4-DCAA


R.T.: 11.616 min
Delta R.T.: -0.003 min
Response: 59001231
Conc: 317.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

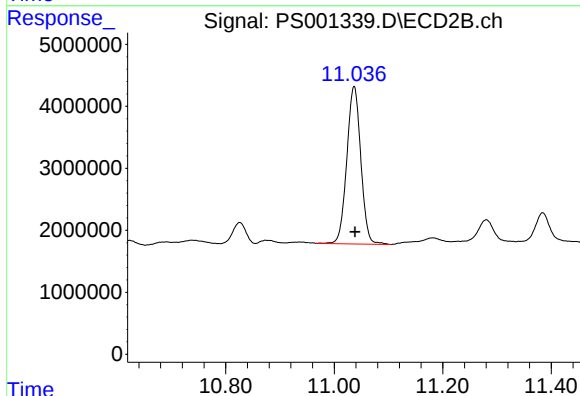


#4 2,4-DCAA

R.T.: 11.037 min
Delta R.T.: -0.002 min
Response: 45521465
Conc: 250.29 ng/ml

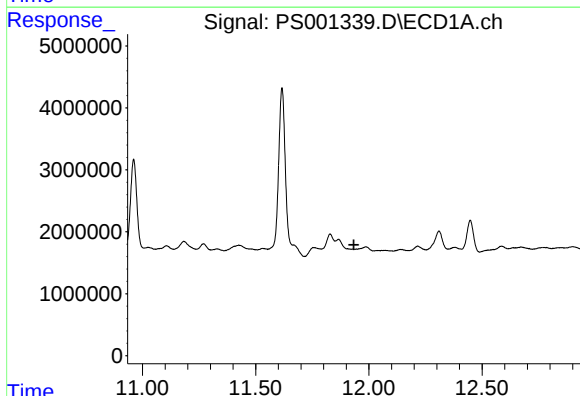


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.934 min
Response: 0
Conc: N.D.

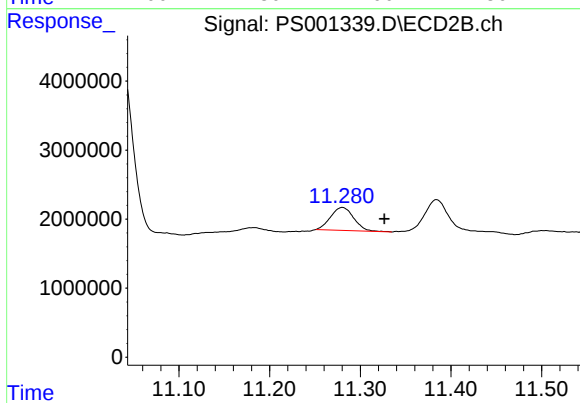

#5 DICAMBA


R.T.: 11.280 min
Delta R.T.: -0.046 min
Response: 5881875
Conc: 8.58 ng/ml

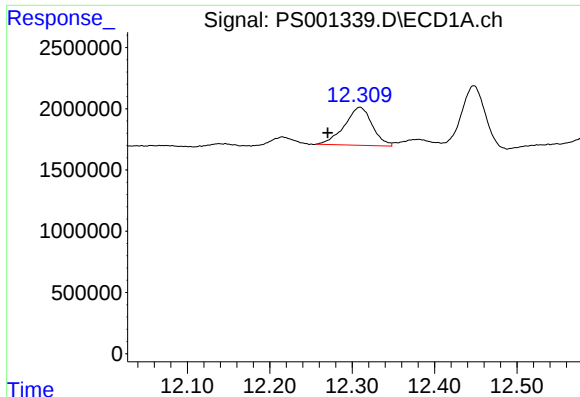

#6 MCP


R.T.: 12.309 min
Delta R.T.: 0.039 min
Response: 7274480
Conc: 14.47 ug/ml

Instrument :
ECD_S
ClientSampleId :

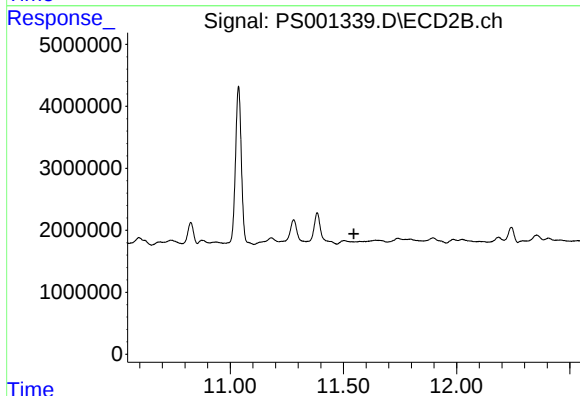


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.546 min
Response: 0
Conc: N.D.

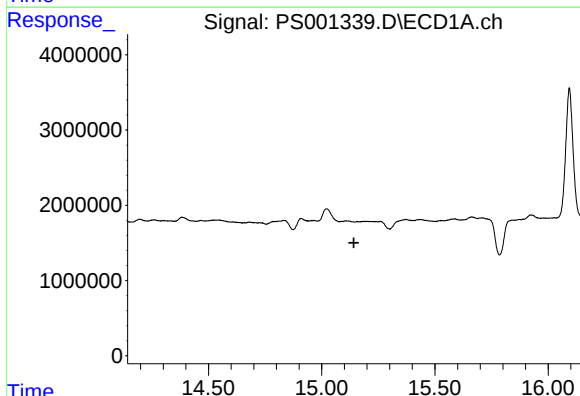


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.142 min
Response: 0
Conc: N.D.

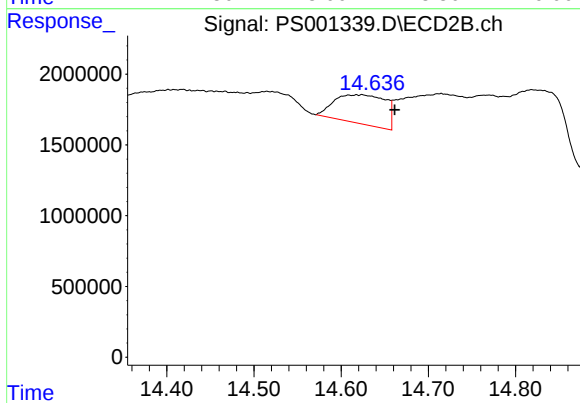

#12 2,4,5-T


R.T.: 14.623 min
Delta R.T.: -0.039 min
Response: 8312242
Conc: 9.00 ng/ml

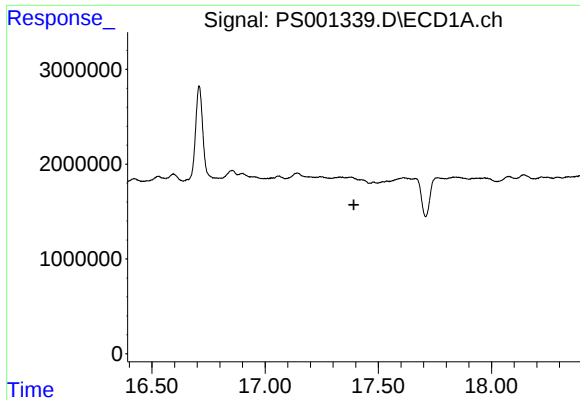

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

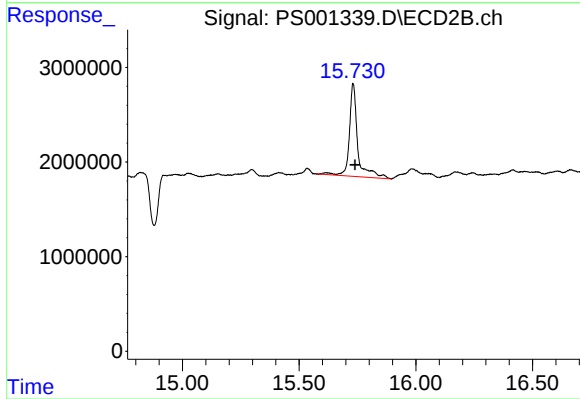


#14 DINOSEB

R.T.: 15.731 min
Delta R.T.: -0.008 min
Response: 24588141
Conc: 34.59 ng/ml

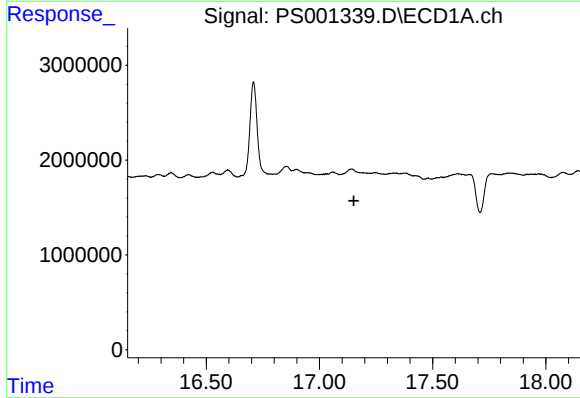


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.152 min
Response: 0
Conc: N.D.

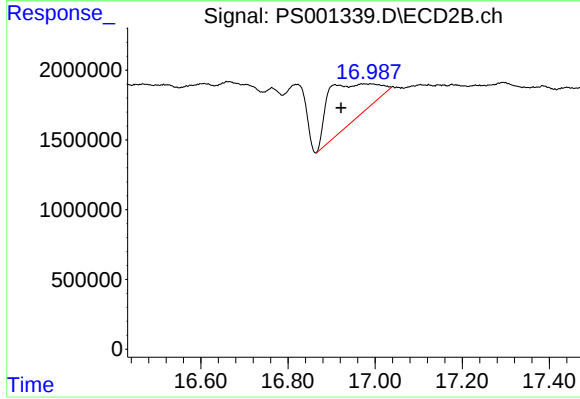

#15 Picloram


R.T.: 16.976 min
Delta R.T.: 0.054 min
Response: 21002013
Conc: 15.24 ng/ml

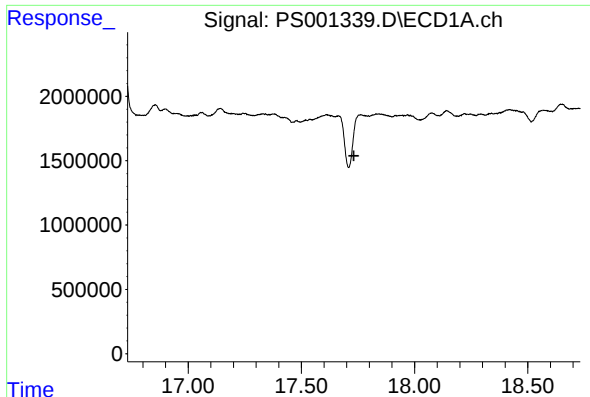

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

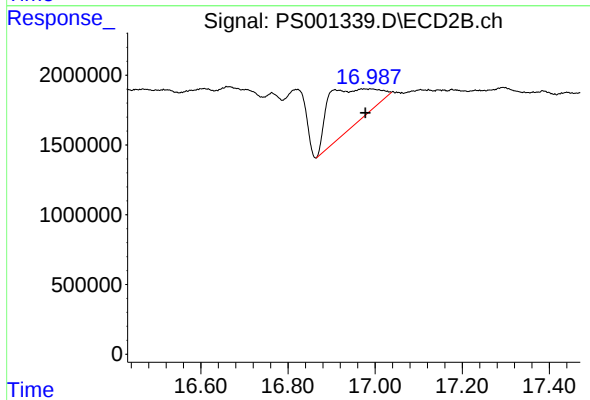

#16 DCPA

R.T.: 16.976 min
Delta R.T.: -0.002 min
Response: 21002013
Conc: 14.54 ng/ml