

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
 Data File : PS005814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2019 10:50
 Operator : SM\AJ
 Sample : K4021-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:06:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.572	5.292	496.7E6	343.5E6	342.383	345.361
Target Compounds							
2) T	3,5-DICHL...	0.000	4.612	0	41196656	N.D.	31.755
7) T	MCPA	0.000	5.624	0	103.0E6	N.D.	24.474
9) T	2,4-D	6.556	0.000	76070730	0	50.759	N.D. #
11) T	2,4,5-TP ...	7.313	6.974	238.2E6	936.4E6	28.829	180.511 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS005814\
Data File : PS005814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2019 10:50
Operator : SM\AJ
Sample : K4021-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:06:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

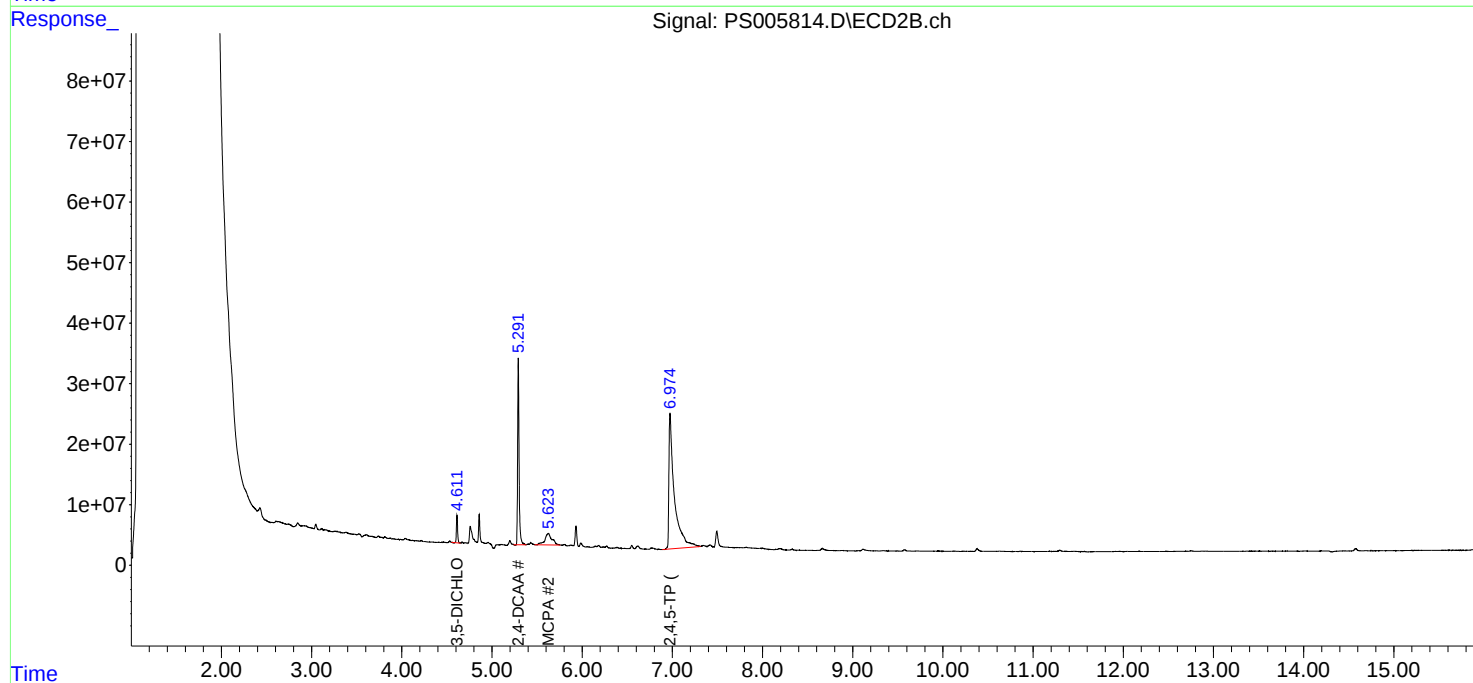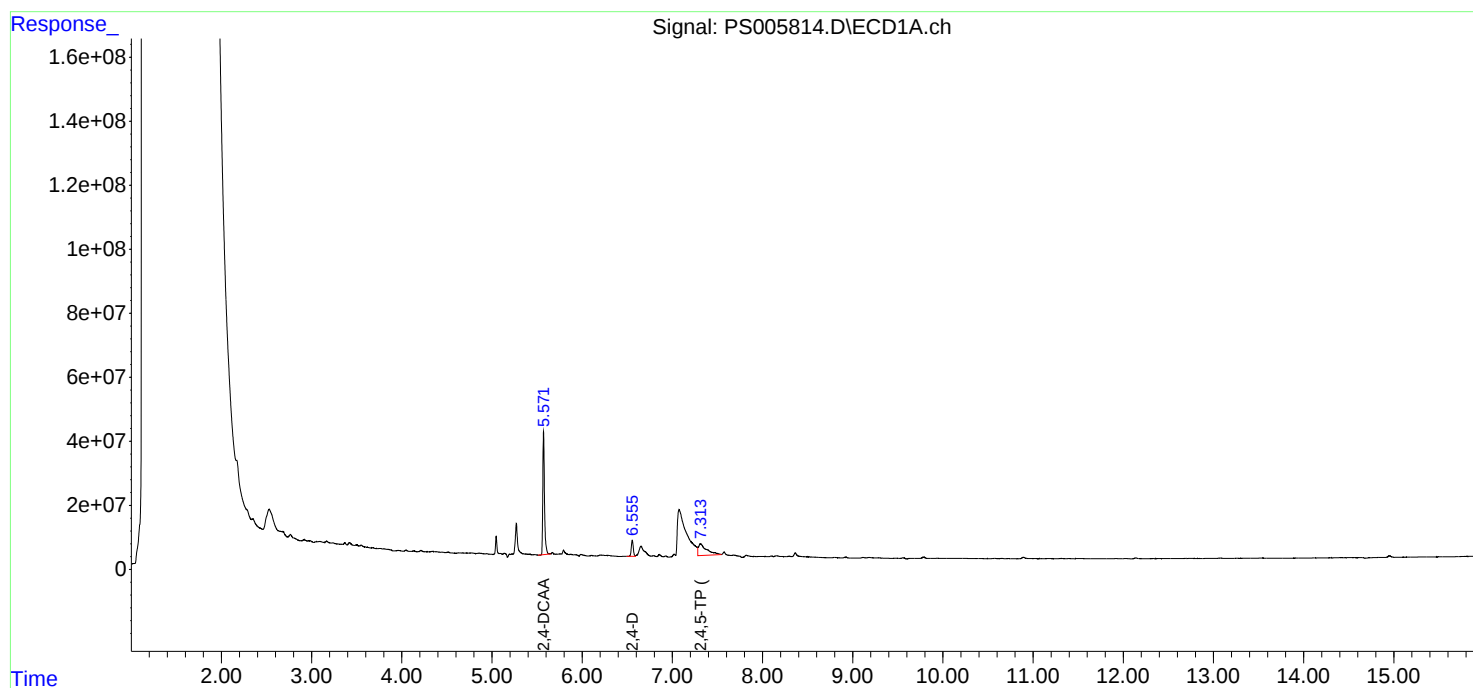


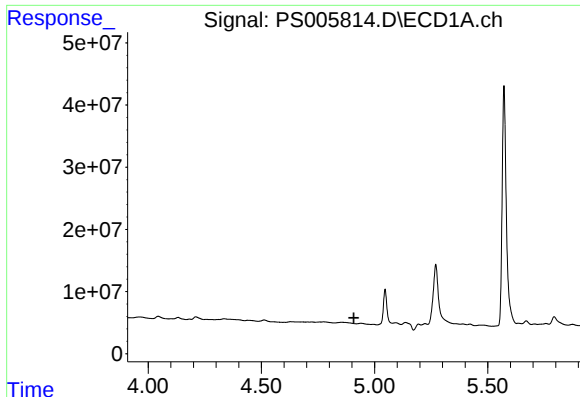

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-9

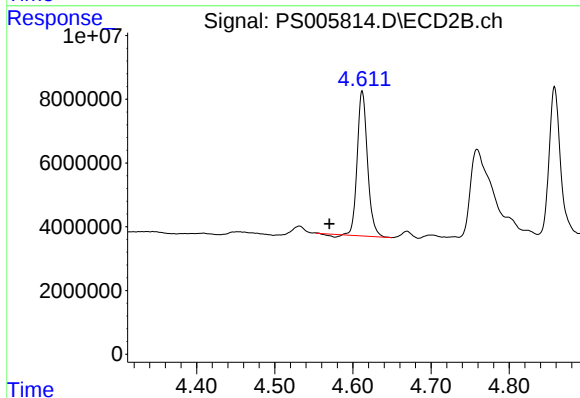


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.612 min
Delta R.T.: 0.042 min
Response: 41196656
Conc: 31.76 ng/ml

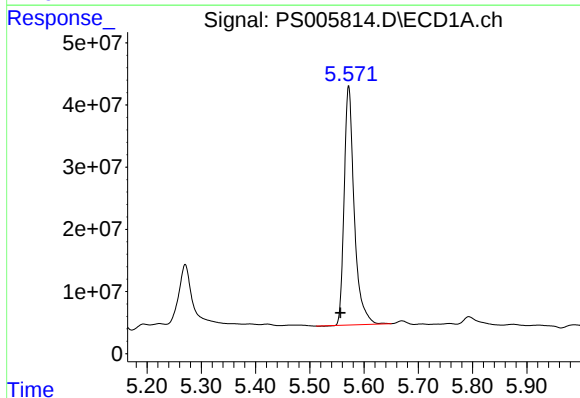


#4 2,4-DCAA

R.T.: 5.572 min
Delta R.T.: 0.016 min
Response: 496735545
Conc: 342.38 ng/ml

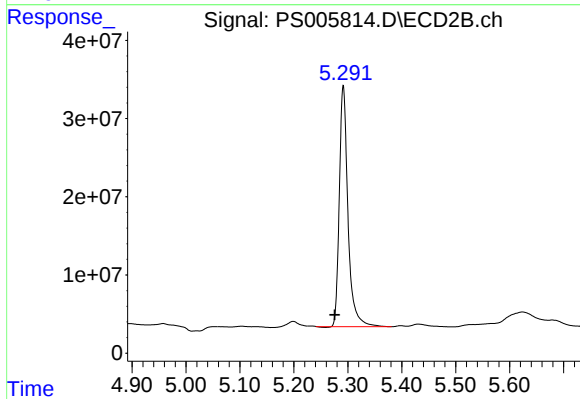

#4 2,4-DCAA


R.T.: 5.292 min
Delta R.T.: 0.016 min
Response: 343523168
Conc: 345.36 ng/ml

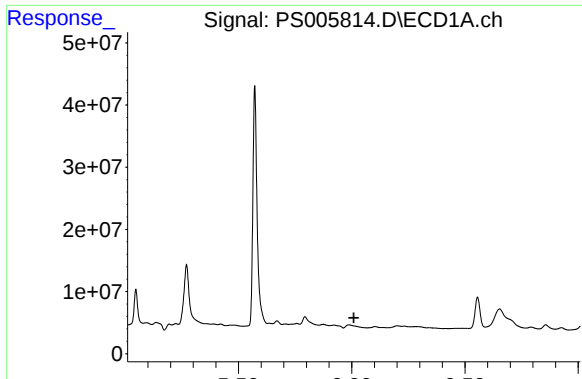

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-9

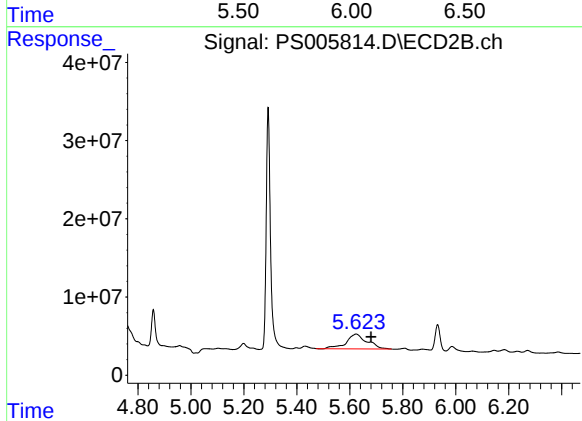


#7 MCPA

R.T.: 5.624 min
Delta R.T.: -0.057 min
Response: 103012304
Conc: 24.47 ug/ml

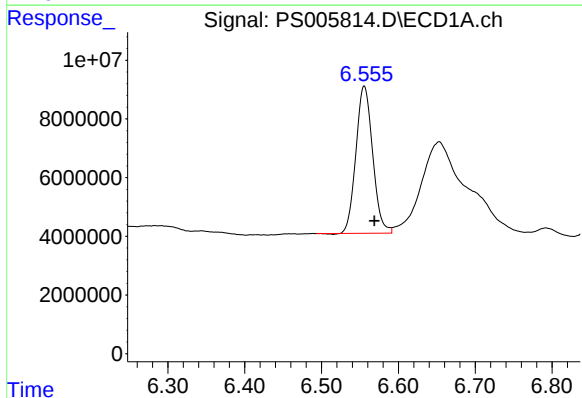


#9 2,4-D

R.T.: 6.556 min
Delta R.T.: -0.013 min
Response: 76070730
Conc: 50.76 ng/ml

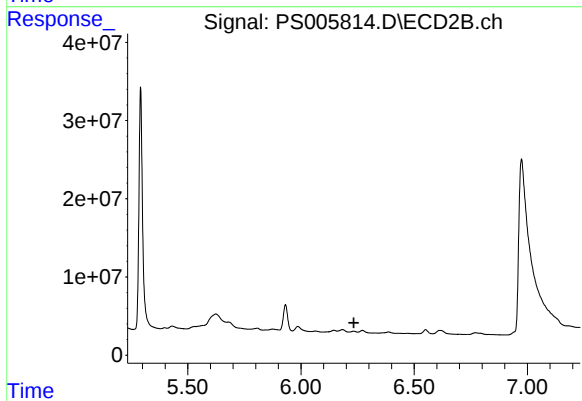

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.234 min
Response: 0
Conc: N.D.

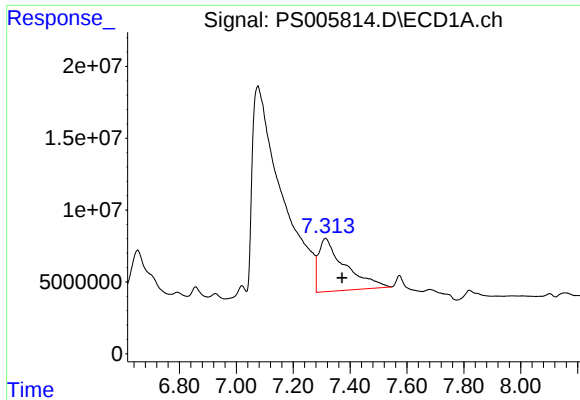

#11 2,4,5-TP (SILVEX)

R.T.: 7.313 min
Delta R.T.: -0.059 min
Response: 238188178
Conc: 28.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-9

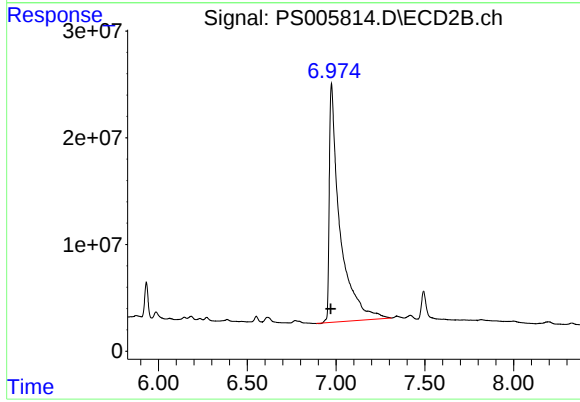

#11 2,4,5-TP (SILVEX)

R.T.: 6.974 min
Delta R.T.: 0.004 min
Response: 936367154
Conc: 180.51 ng/ml