

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
 Data File : PS005815.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2019 11:12
 Operator : SM\AJ
 Sample : K4021-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:06:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.586	5.307	666.8E6	454.1E6	459.595	456.573
Target Compounds							
2) T	3,5-DICHL...	0.000	4.627	0	77907616	N.D.	60.053
6) T	MCP	5.809	0.000	20512105	0	4.427	N.D. #
7) T	MCPA	0.000	5.639	0	102.1E6	N.D.	24.250
8) T	DICHLORPROP	0.000	5.947	0	50866231	N.D.	55.079
9) T	2,4-D	6.570	0.000	93184395	0	62.178	N.D. #
11) T	2,4,5-TP ...	7.326	7.021	84503265	129.3E6	10.228	24.926 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS005815\
Data File : PS005815.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2019 11:12
Operator : SM\AJ
Sample : K4021-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:06:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

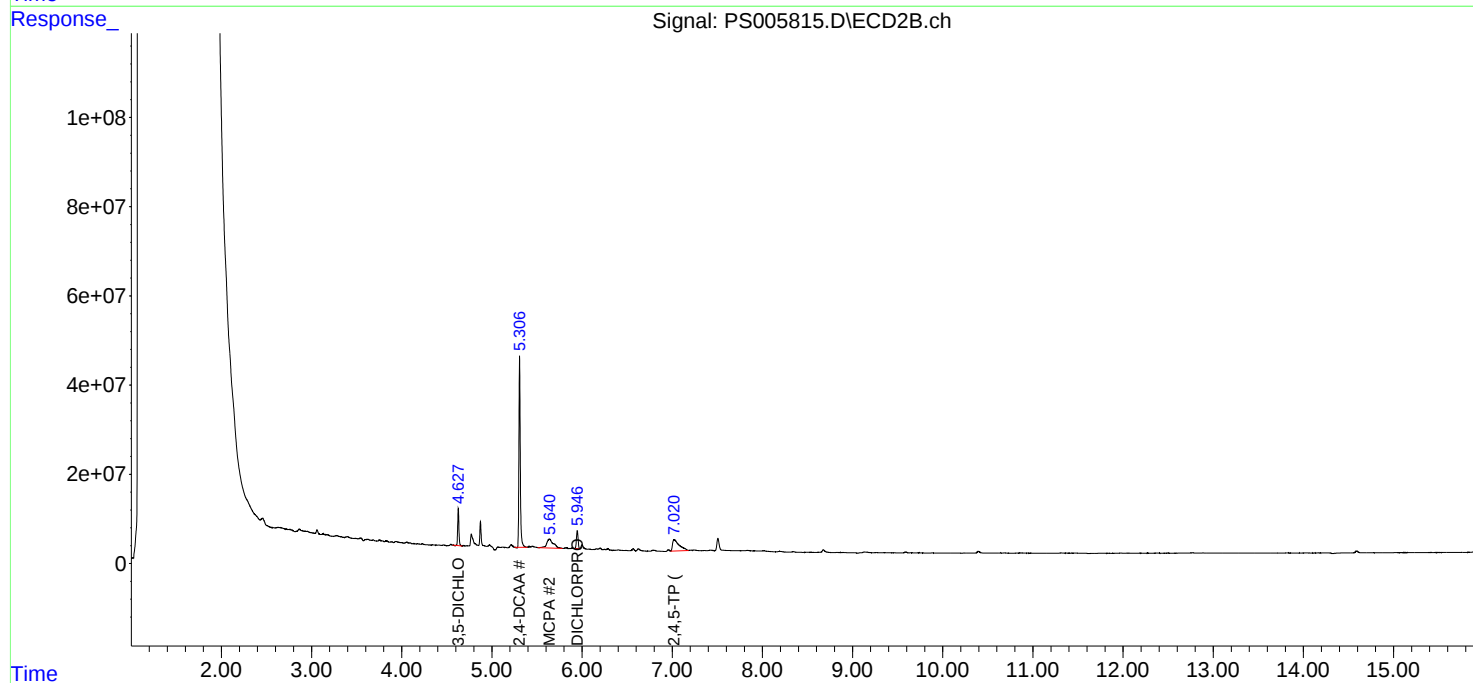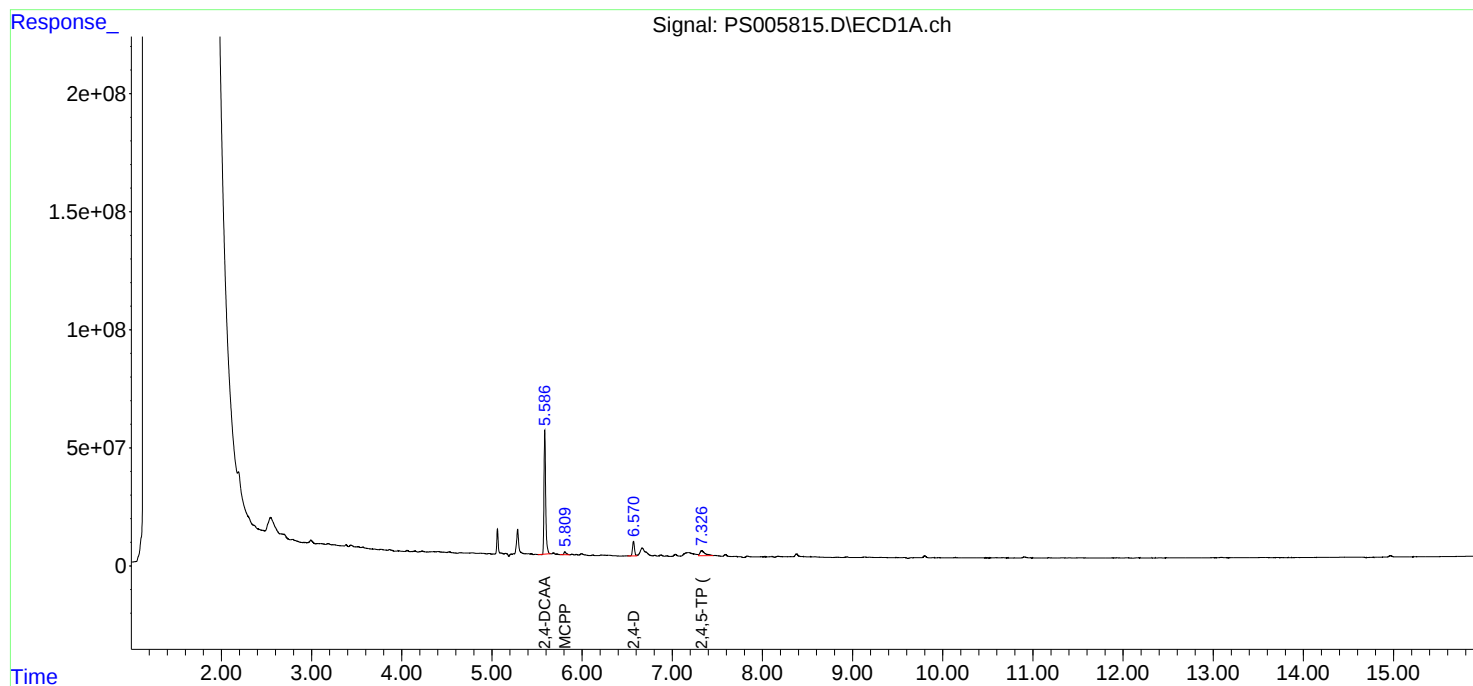


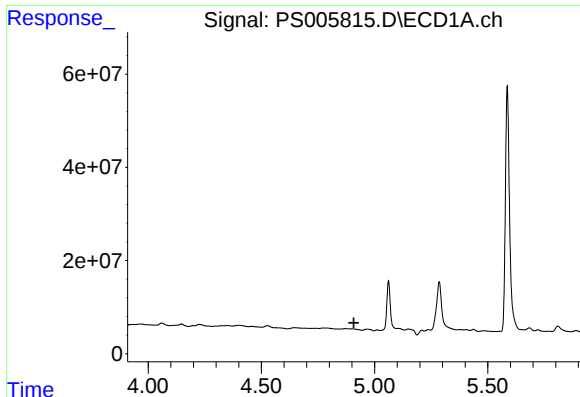

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

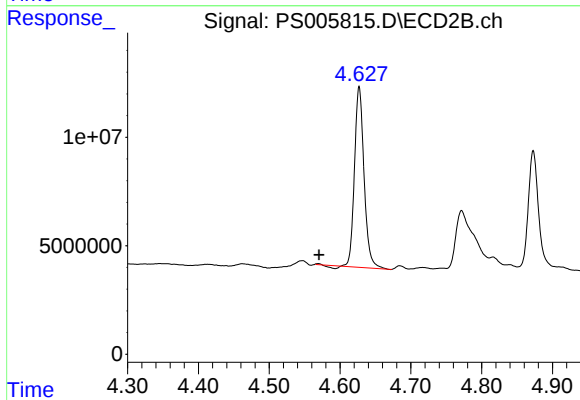


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.627 min
Delta R.T.: 0.057 min
Response: 77907616
Conc: 60.05 ng/ml

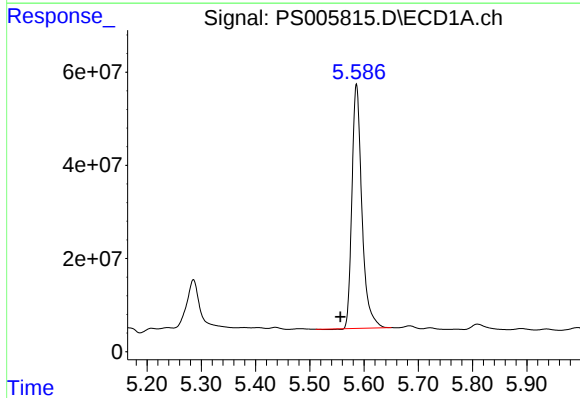


#4 2,4-DCAA

R.T.: 5.586 min
Delta R.T.: 0.030 min
Response: 666788157
Conc: 459.59 ng/ml

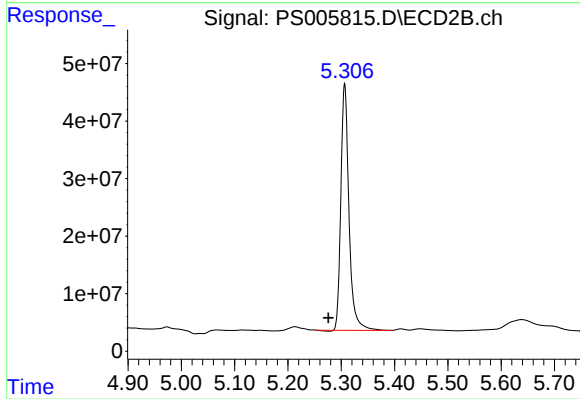

#4 2,4-DCAA


R.T.: 5.307 min
Delta R.T.: 0.031 min
Response: 454143719
Conc: 456.57 ng/ml

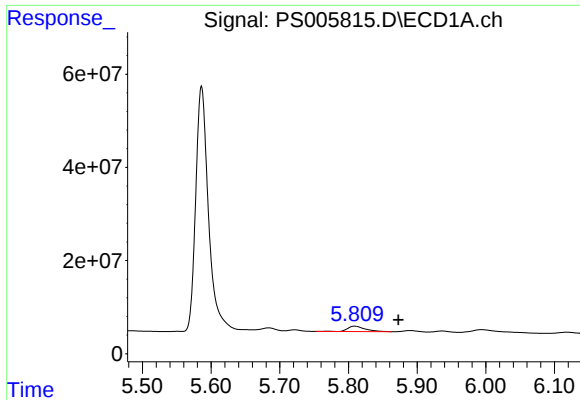

#6 MCPP


R.T.: 5.809 min
Delta R.T.: -0.063 min
Response: 20512105
Conc: 4.43 ug/ml

Instrument :
ECD_S
ClientSampleId :

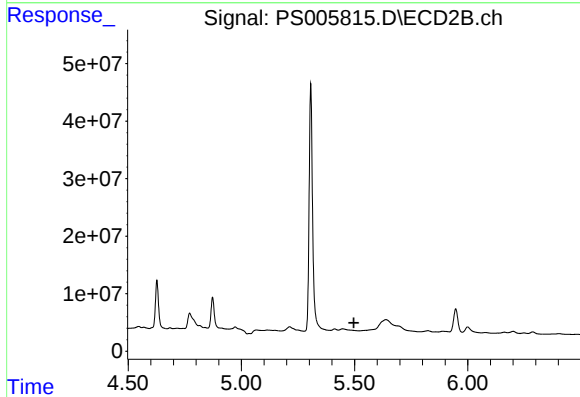


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

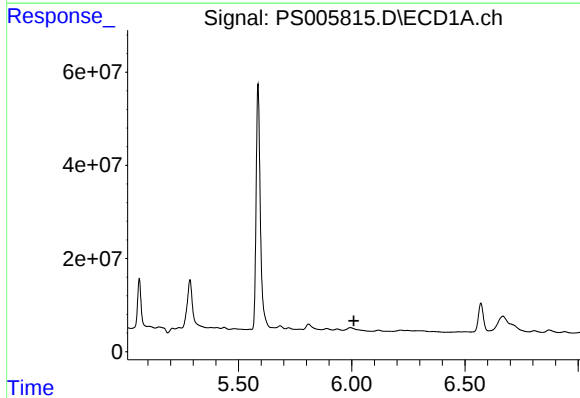


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.009 min
Response: 0
Conc: N.D.

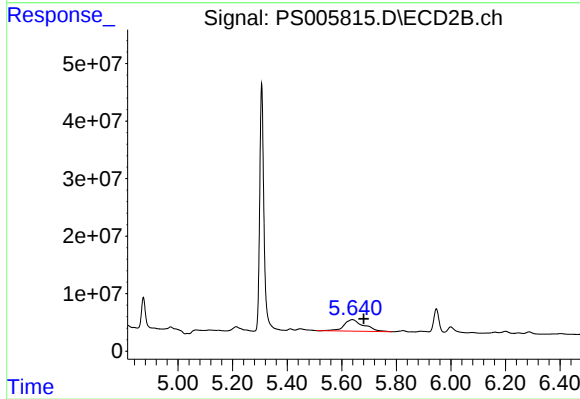

#7 MCPA


R.T.: 5.639 min
Delta R.T.: -0.042 min
Response: 102070527
Conc: 24.25 ug/ml

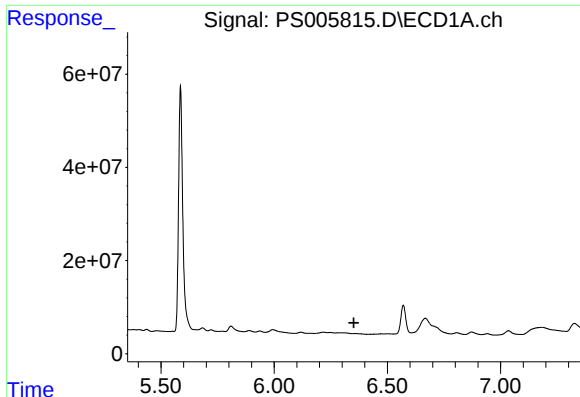

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

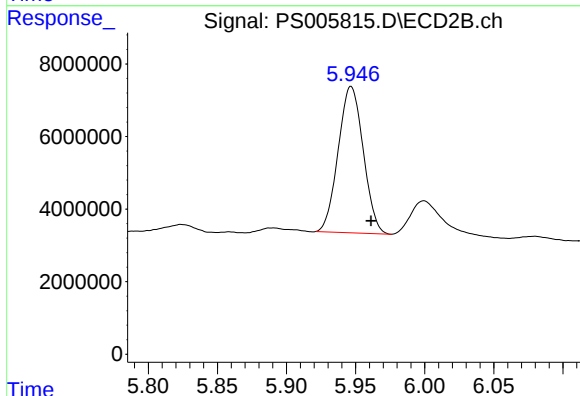


#8 DICHLORPROP

R.T.: 5.947 min
Delta R.T.: -0.015 min
Response: 50866231
Conc: 55.08 ng/ml

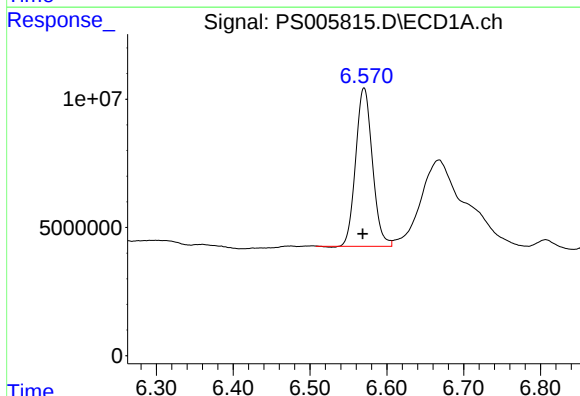


#9 2,4-D

R.T.: 6.570 min
Delta R.T.: 0.001 min
Response: 93184395
Conc: 62.18 ng/ml

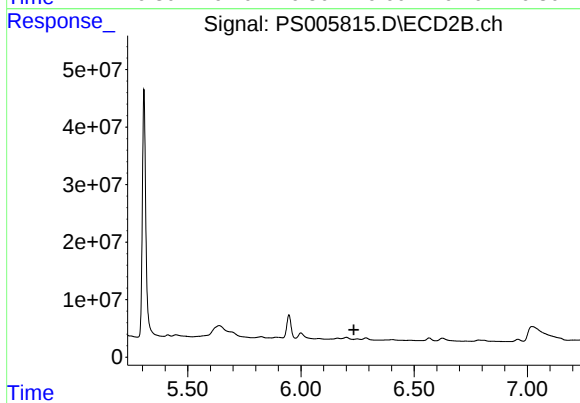

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.234 min
Response: 0
Conc: N.D.

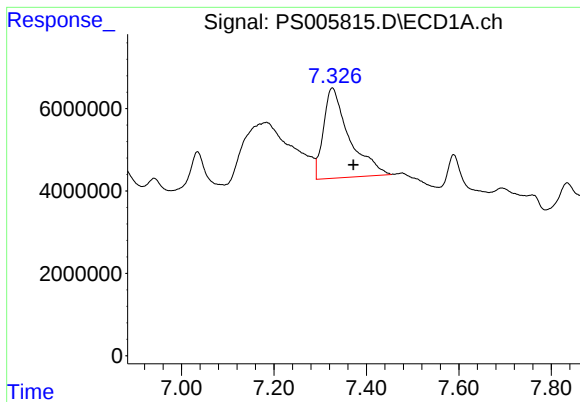

#11 2,4,5-TP (SILVEX)

R.T.: 7.326 min
Delta R.T.: -0.046 min
Response: 84503265
Conc: 10.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

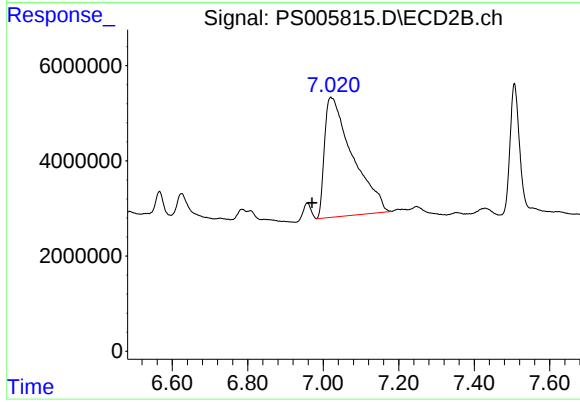

#11 2,4,5-TP (SILVEX)

R.T.: 7.021 min
Delta R.T.: 0.050 min
Response: 129297053
Conc: 24.93 ng/ml