

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
 Data File : PS005816.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2019 11:34
 Operator : SM\AJ
 Sample : K4021-16
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-8-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:06:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.555	5.276	637.2E6	442.1E6	439.202	444.502
Target Compounds							
2) T	3,5-DICHL...	0.000	4.596	0	65718932	N.D.	50.658
5) T	DICAMBA	5.778	0.000	29787160	0	4.987	N.D. #
9) T	2,4-D	6.540	0.000	102.3E6	0	68.229	N.D. #
11) T	2,4,5-TP ...	7.305	0.000	31729219	0	3.840	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
Data File : PS005816.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2019 11:34
Operator : SM\AJ
Sample : K4021-16
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-8-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:06:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

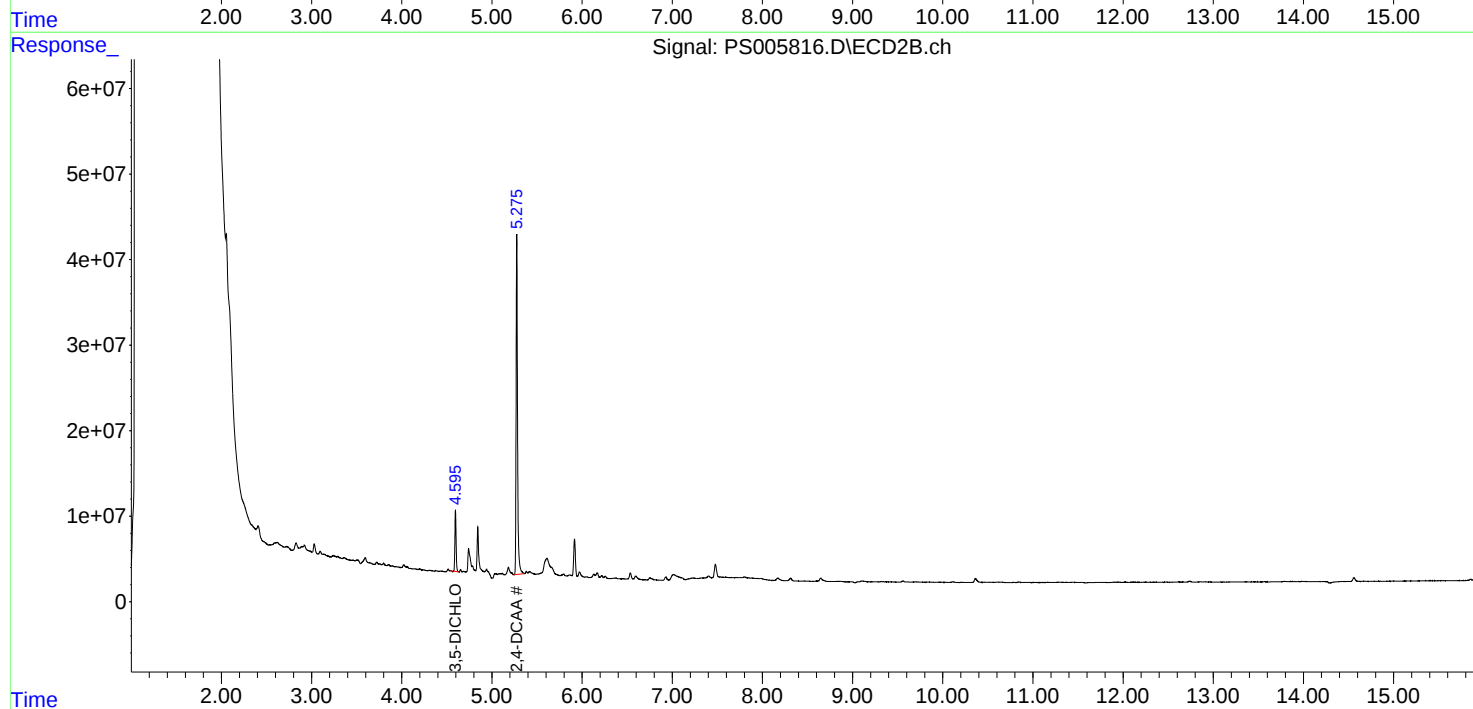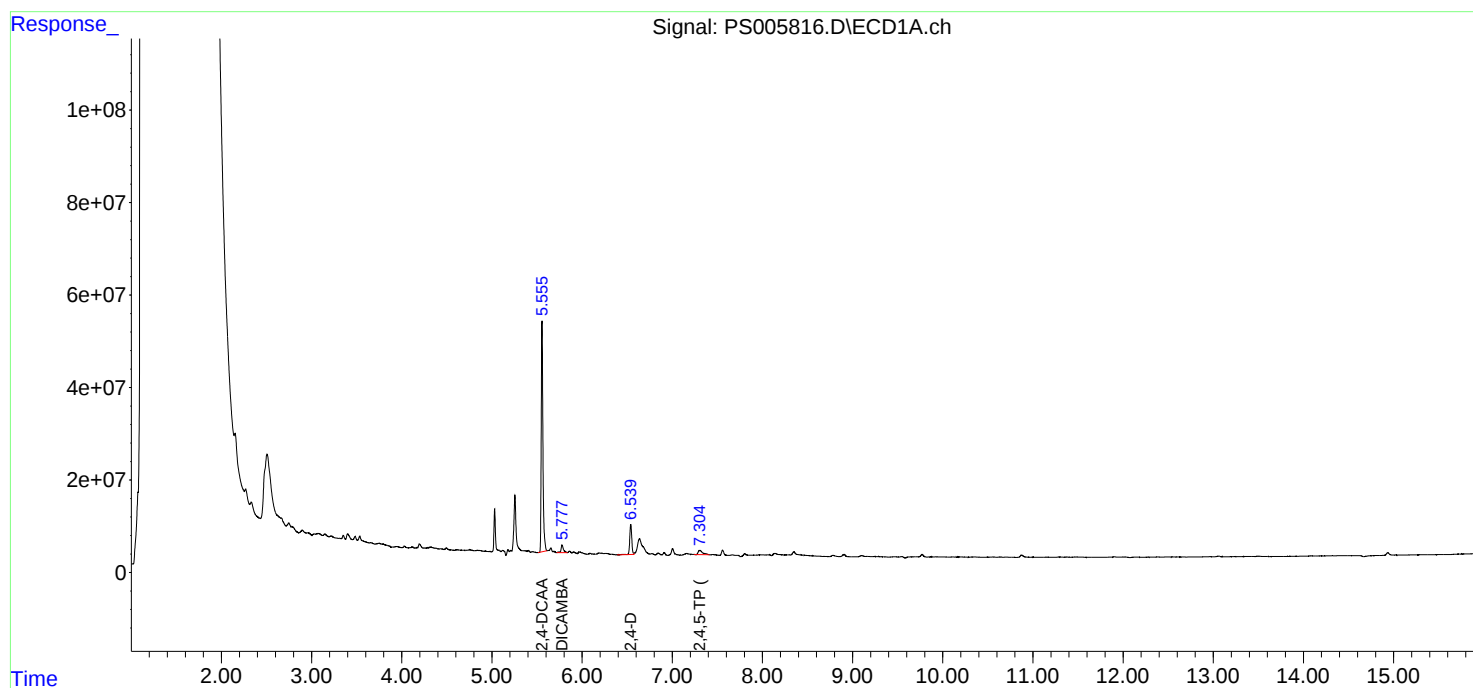


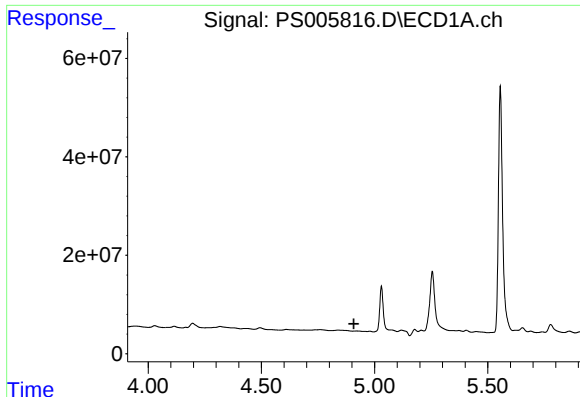

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-8-A

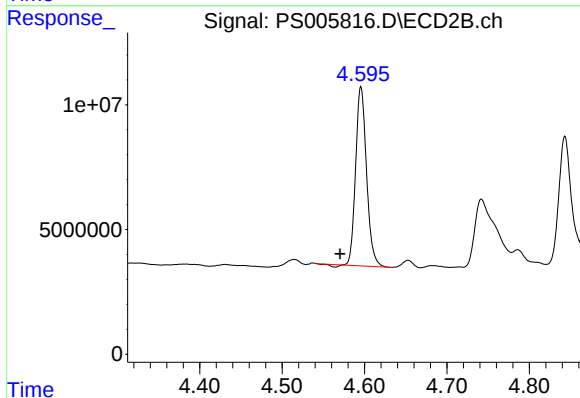


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.596 min
Delta R.T.: 0.026 min
Response: 65718932
Conc: 50.66 ng/ml

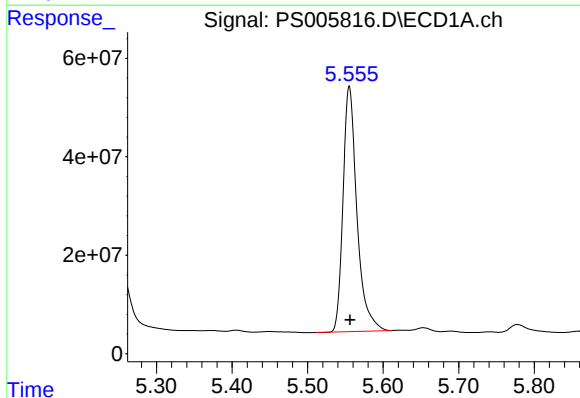


#4 2,4-DCAA

R.T.: 5.555 min
Delta R.T.: 0.000 min
Response: 637202016
Conc: 439.20 ng/ml

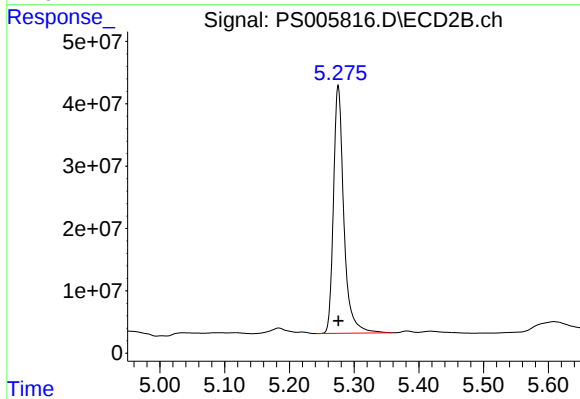

#4 2,4-DCAA


R.T.: 5.276 min
Delta R.T.: 0.000 min
Response: 442136012
Conc: 444.50 ng/ml

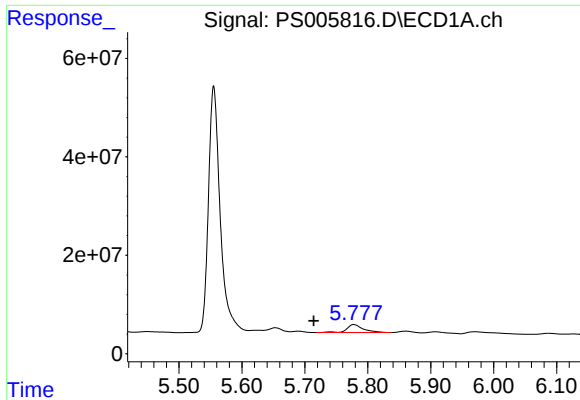

#5 DICAMBA


R.T.: 5.778 min
Delta R.T.: 0.064 min
Response: 29787160
Conc: 4.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-8-A

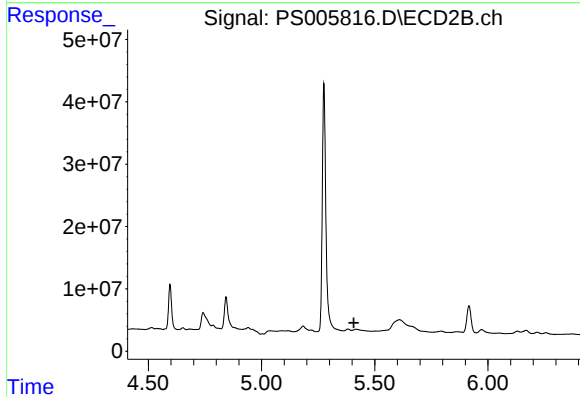


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

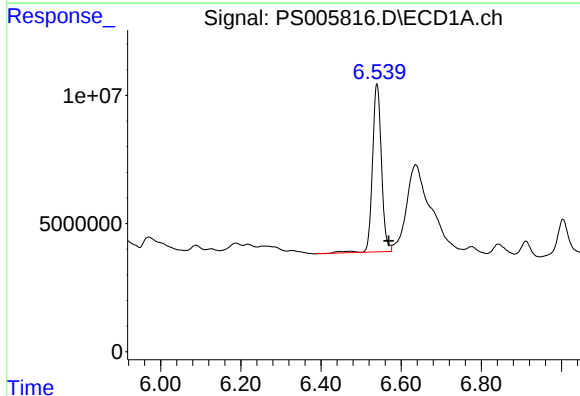


#9 2,4-D

R.T.: 6.540 min
Delta R.T.: -0.029 min
Response: 102252622
Conc: 68.23 ng/ml

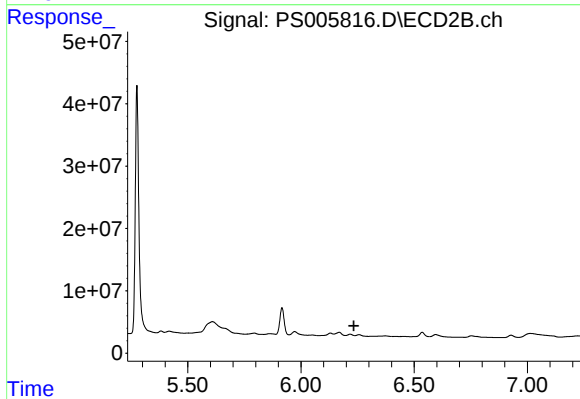

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

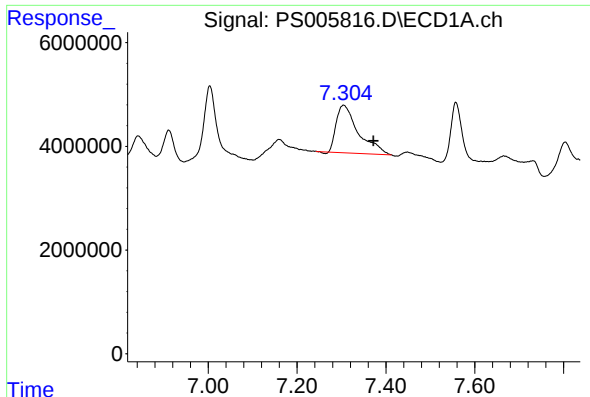

#11 2,4,5-TP (SILVEX)

R.T.: 7.305 min
Delta R.T.: -0.068 min
Response: 31729219
Conc: 3.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-8-A

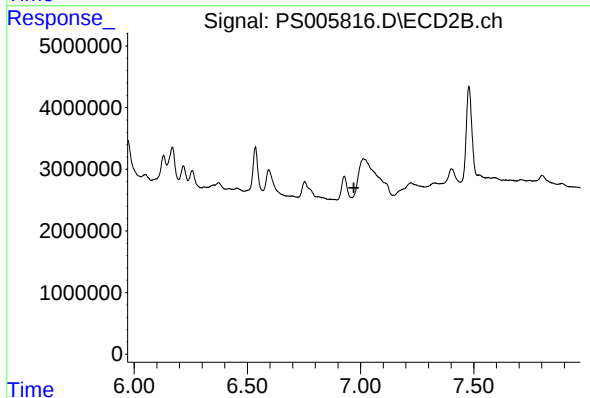

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 6.971 min
Response: 0
Conc: N.D.