

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
 Data File : PS005822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2019 13:49
 Operator : SM\AJ
 Sample : PB121839BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:09:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.558	5.277	861.3E6	580.0E6	593.686	583.142
Target Compounds							
2) T	3,5-DICHL...	0.000	4.598	0	19490053	N.D.	15.023
7) T	MCPA	6.046	5.663	13842608	28086302	2.121	6.673 #
9) T	2,4-D	6.543	0.000	229.6E6	0	153.236	N.D. #
11) T	2,4,5-TP ...	0.000	6.936	0	13422685	N.D.	2.588
12) T	2,4,5-T	7.583	7.394	88724143	79746659	10.630	16.776 #
14) T	DINOSEB	9.275	0.000	88762859	0	13.670	N.D. #
15) T	Picloram	9.163	9.099	223.3E6	216.0E6	19.080	28.753 #
16) T	DCPA	9.548	9.099	98592207	216.0E6	9.696	32.757 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
Data File : PS005822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2019 13:49
Operator : SM\AJ
Sample : PB121839BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:09:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

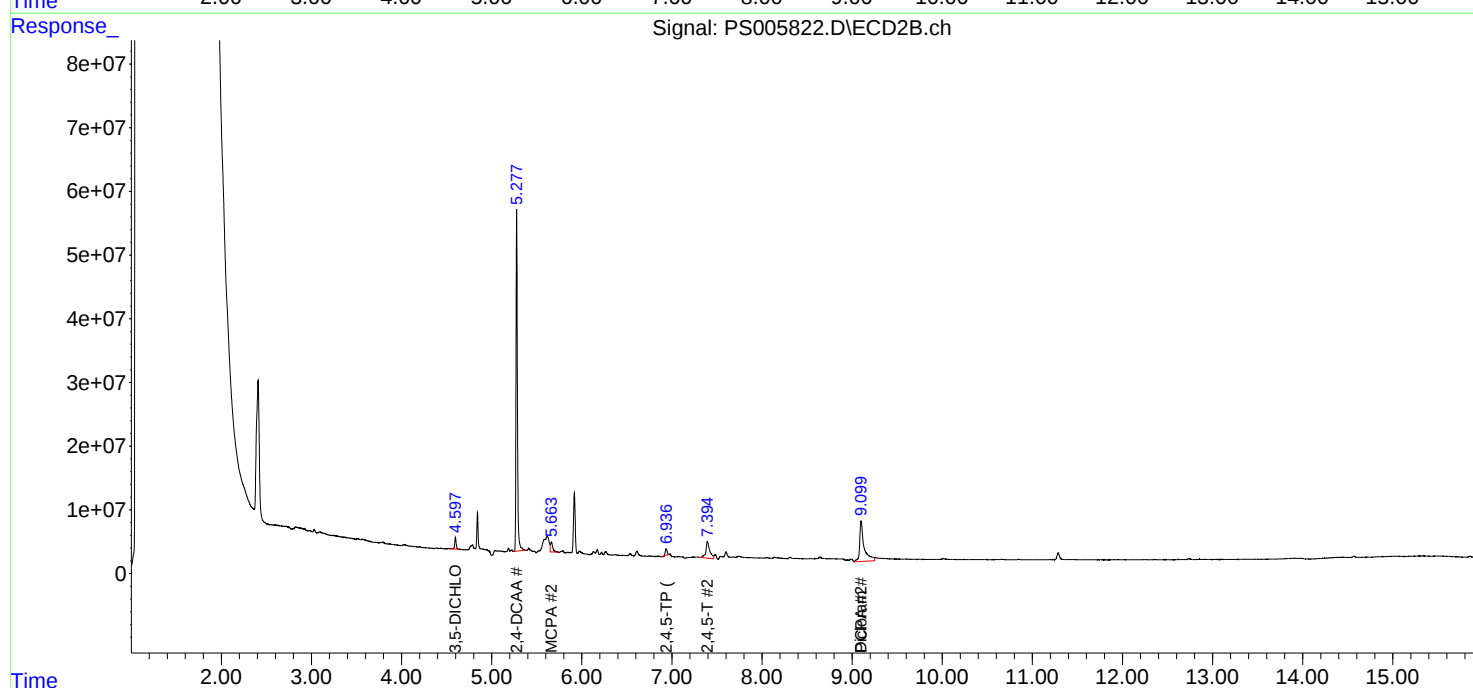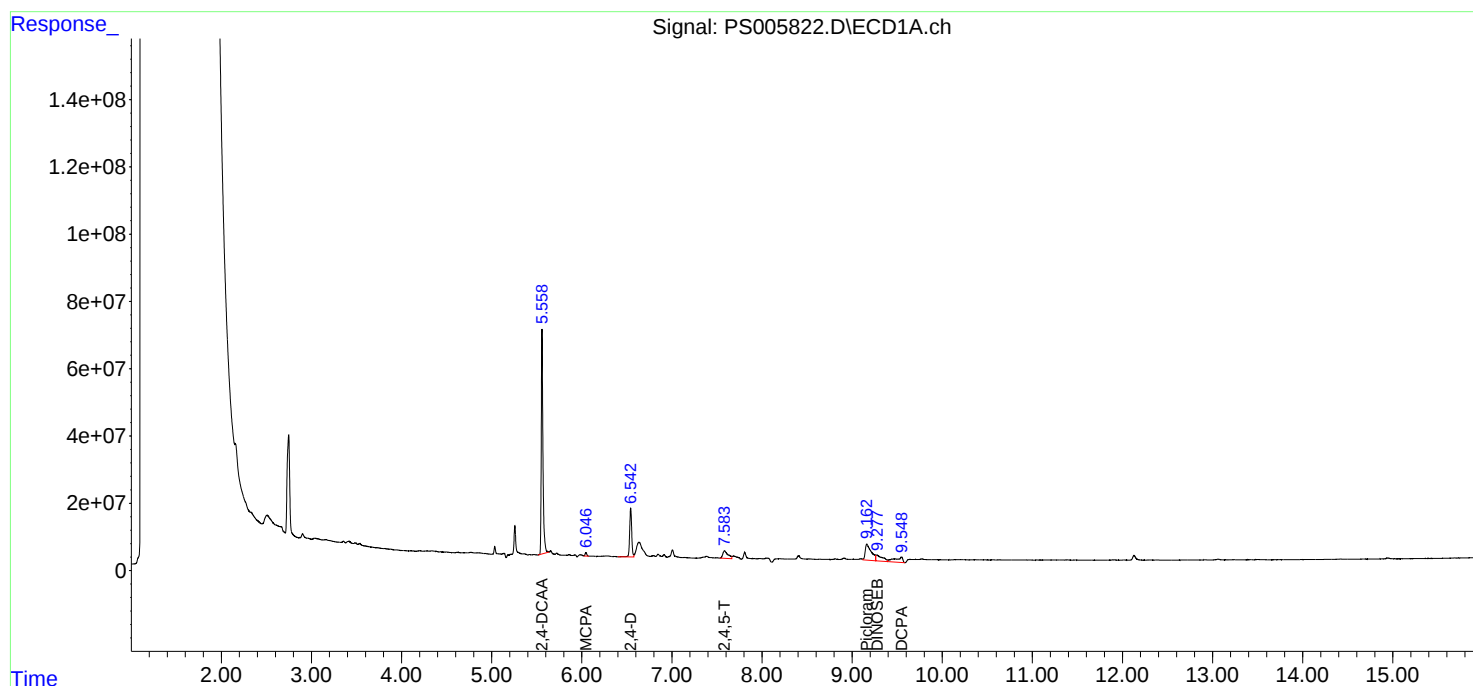


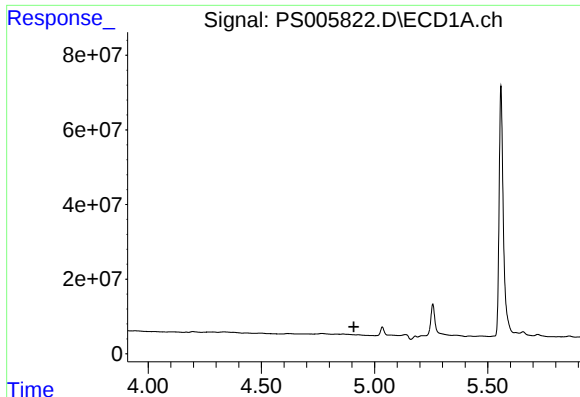

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

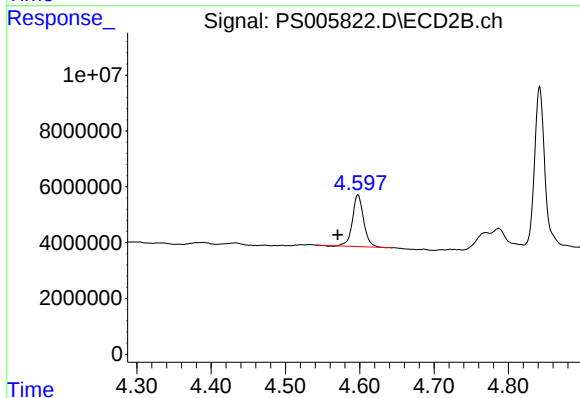


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.598 min
Delta R.T.: 0.027 min
Response: 19490053
Conc: 15.02 ng/ml

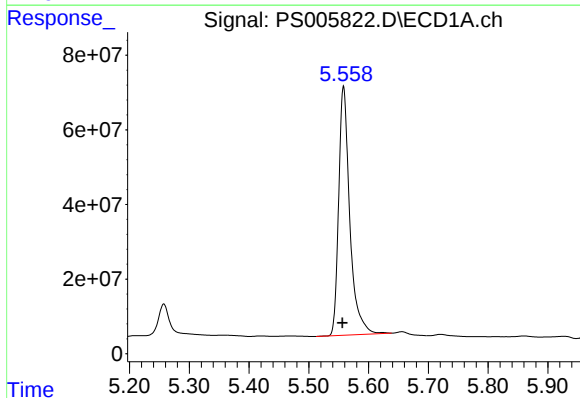


#4 2,4-DCAA

R.T.: 5.558 min
Delta R.T.: 0.002 min
Response: 861329959
Conc: 593.69 ng/ml

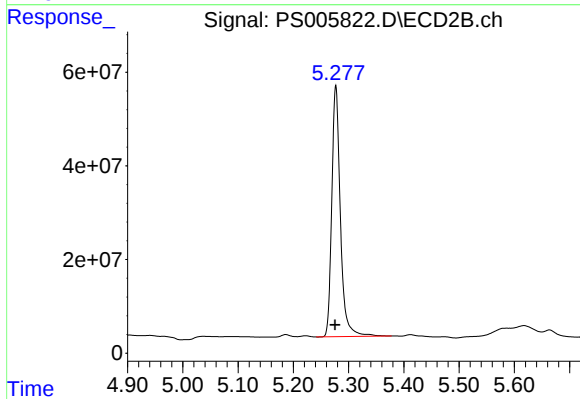

#4 2,4-DCAA


R.T.: 5.277 min
Delta R.T.: 0.001 min
Response: 580038364
Conc: 583.14 ng/ml

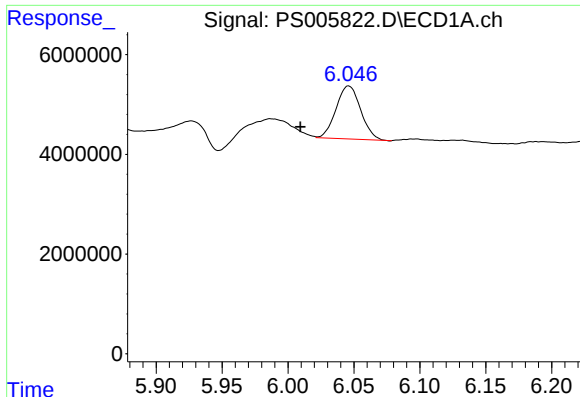

#7 MCPA


R.T.: 6.046 min
Delta R.T.: 0.037 min
Response: 13842608
Conc: 2.12 ug/ml

Instrument :
ECD_S
ClientSampleId :

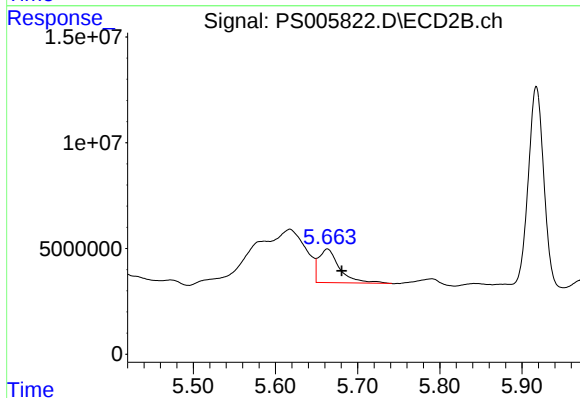


#7 MCPA

R.T.: 5.663 min
Delta R.T.: -0.018 min
Response: 28086302
Conc: 6.67 ug/ml

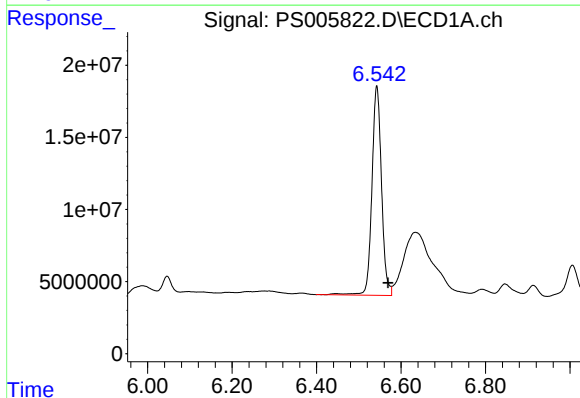


#9 2,4-D

R.T.: 6.543 min
Delta R.T.: -0.026 min
Response: 229649705
Conc: 153.24 ng/ml

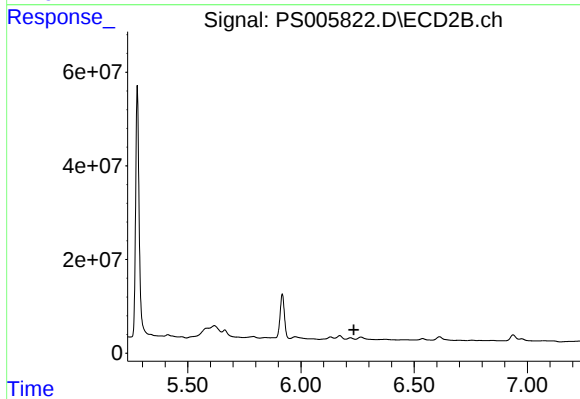

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.234 min
Response: 0
Conc: N.D.

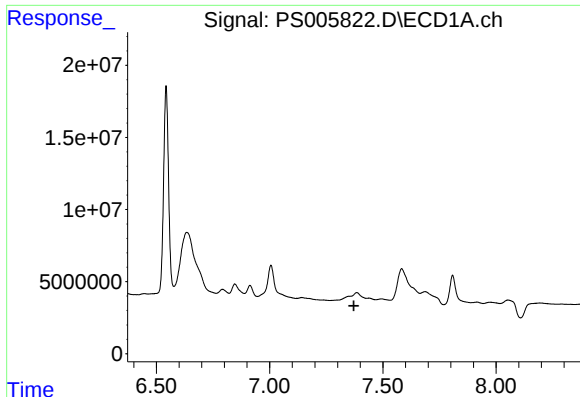

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

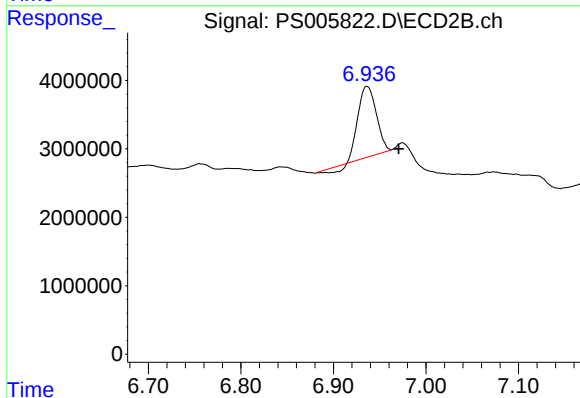


#11 2,4,5-TP (SILVEX)

R.T.: 6.936 min
Delta R.T.: -0.034 min
Response: 13422685
Conc: 2.59 ng/ml

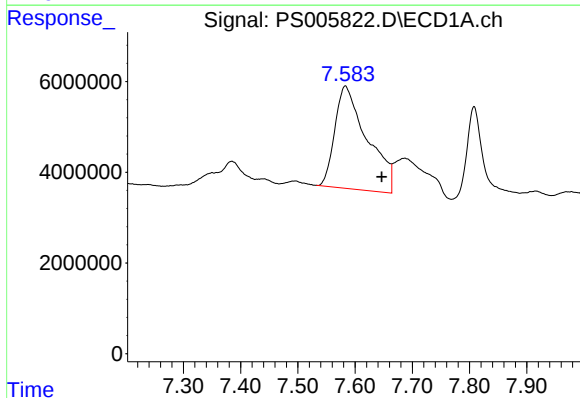


#12 2,4,5-T

R.T.: 7.583 min
Delta R.T.: -0.064 min
Response: 88724143
Conc: 10.63 ng/ml

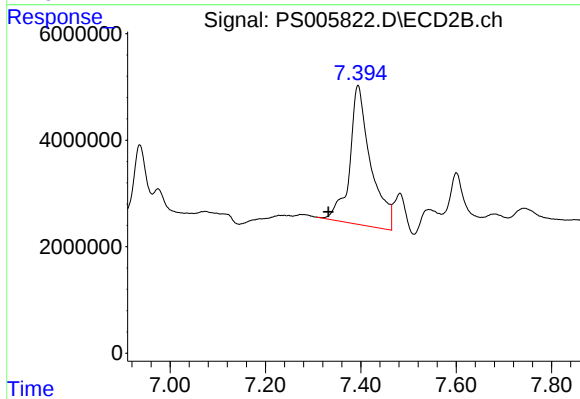

#12 2,4,5-T


R.T.: 7.394 min
Delta R.T.: 0.062 min
Response: 79746659
Conc: 16.78 ng/ml

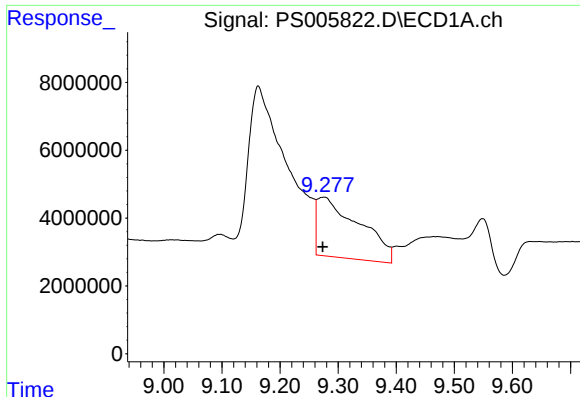

#14 DINOSEB


R.T.: 9.275 min
Delta R.T.: 0.002 min
Response: 88762859
Conc: 13.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

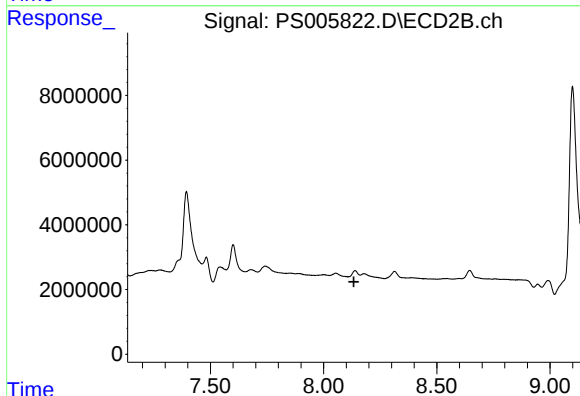


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 8.134 min
Response: 0
Conc: N.D.

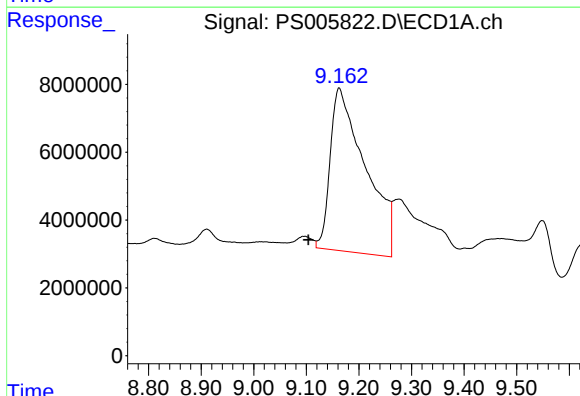


#15 Picloram

R.T.: 9.163 min
Delta R.T.: 0.059 min
Response: 223330130
Conc: 19.08 ng/ml

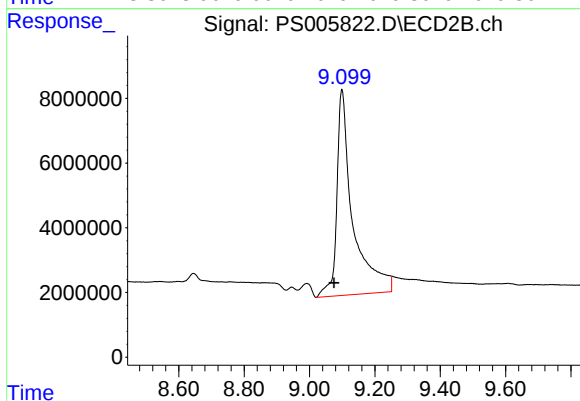

#15 Picloram


R.T.: 9.099 min
Delta R.T.: 0.024 min
Response: 215998791
Conc: 28.75 ng/ml

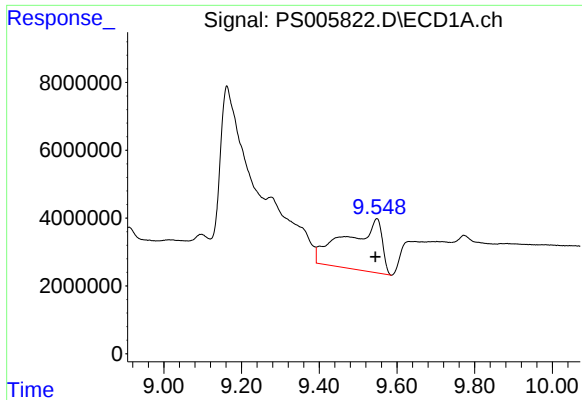

#16 DCPA

R.T.: 9.548 min
Delta R.T.: 0.003 min
Response: 98592207
Conc: 9.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

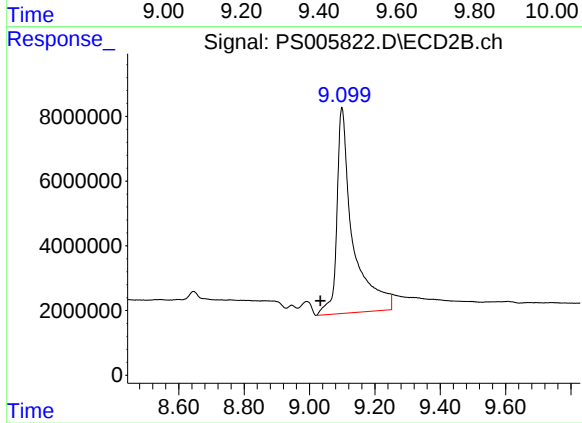

#16 DCPA

R.T.: 9.099 min
Delta R.T.: 0.066 min
Response: 215998791
Conc: 32.76 ng/ml