

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
 Data File : PS005825.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2019 14:55
 Operator : SM\AJ
 Sample : K4044-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:10:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.576	5.296	592.0E6	398.8E6	408.023	400.924
Target Compounds							
2) T	3,5-DICHL...	0.000	4.617	0 77393028		N.D.	59.656
7) T	MCPA	0.000	5.629	0 106.6E6		N.D.	25.319
8) T	DICHLORPROP	0.000	5.937	0 30346680		N.D.	32.860
9) T	2,4-D	6.560	0.000	68473620	0	45.690	N.D. #
11) T	2,4,5-TP ...	7.323	0.000	23568102	0	2.853	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
Data File : PS005825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2019 14:55
Operator : SM\AJ
Sample : K4044-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:10:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

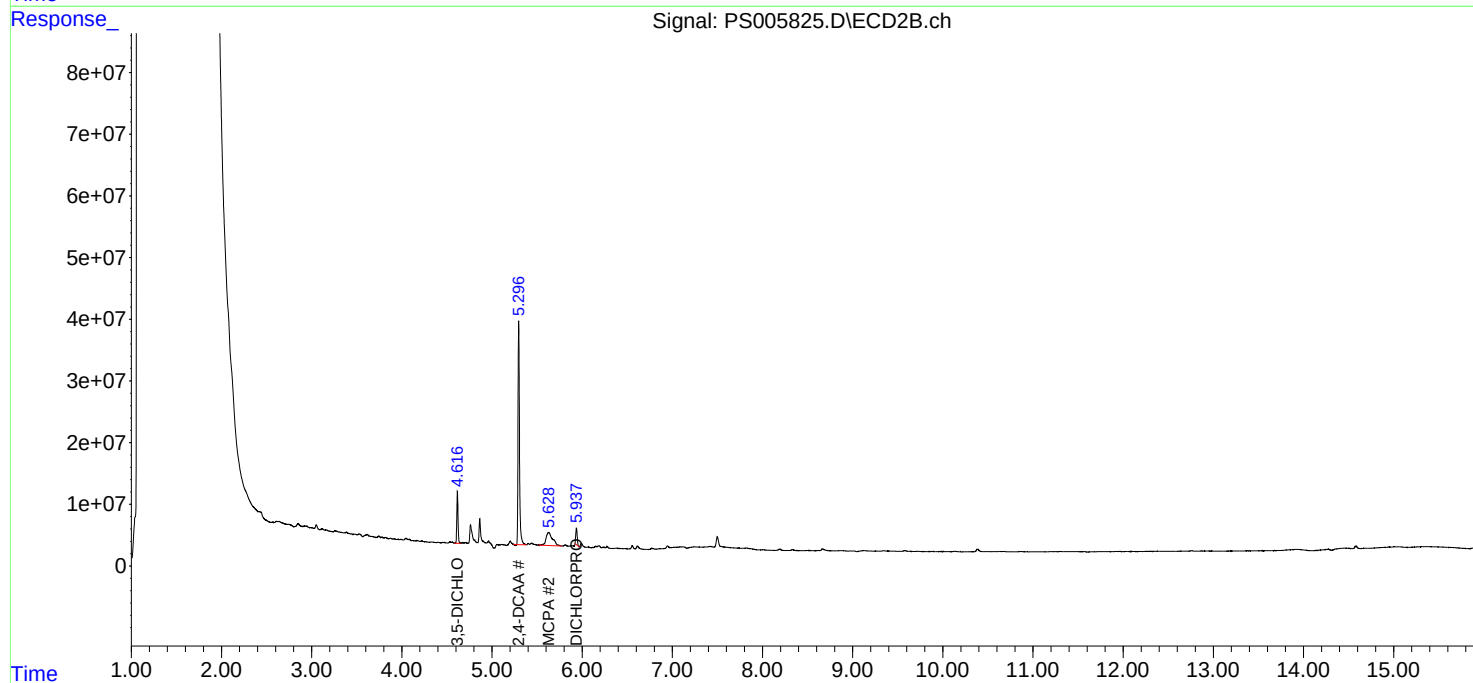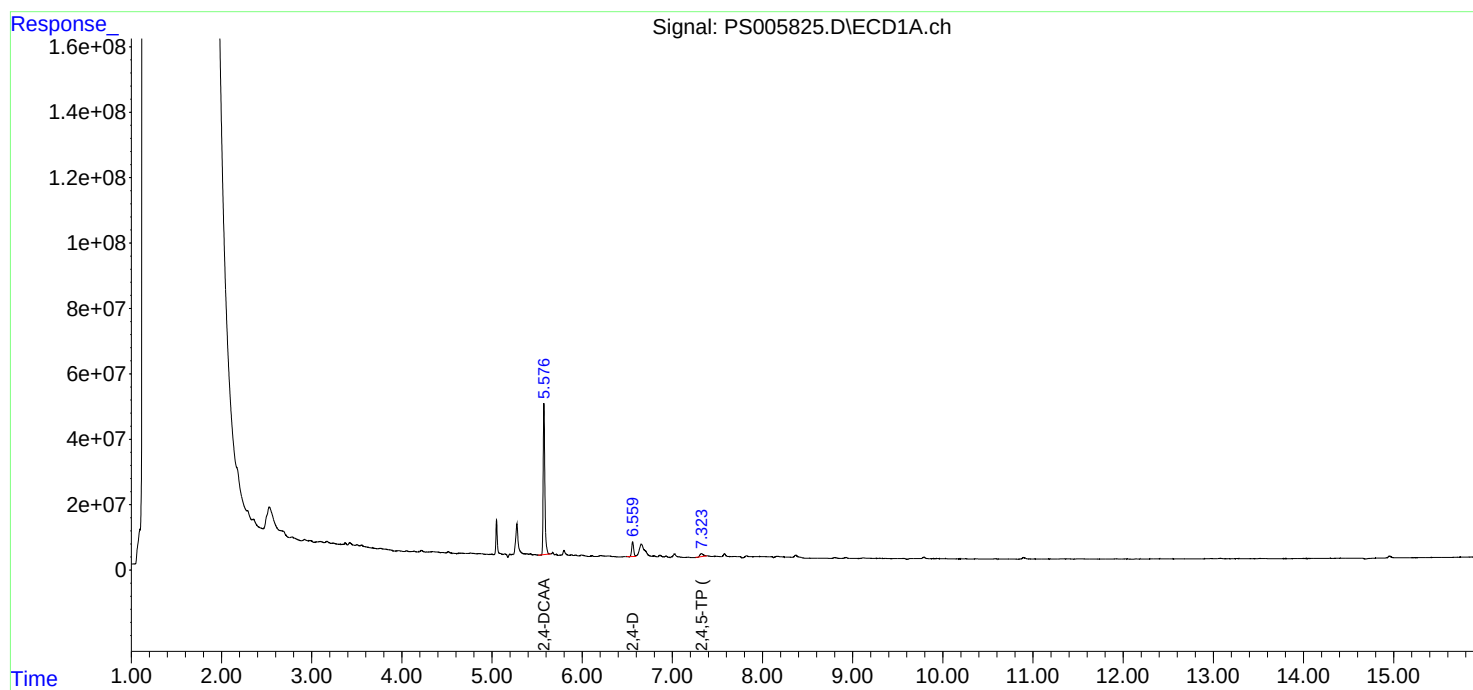


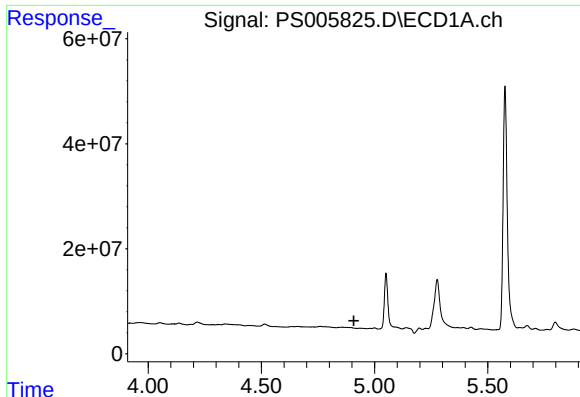

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

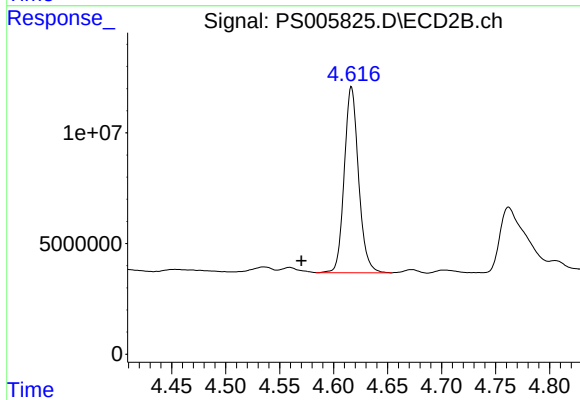


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.617 min
Delta R.T.: 0.046 min
Response: 77393028
Conc: 59.66 ng/ml

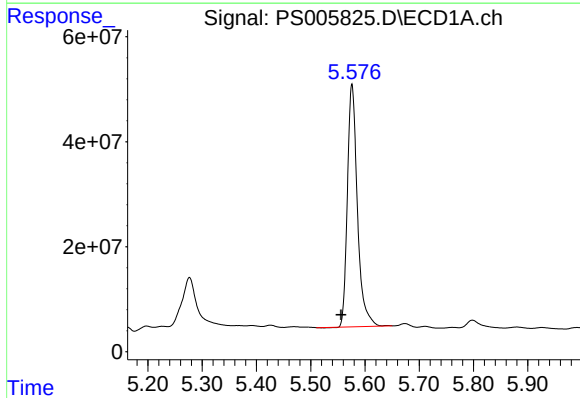


#4 2,4-DCAA

R.T.: 5.576 min
Delta R.T.: 0.020 min
Response: 591967085
Conc: 408.02 ng/ml

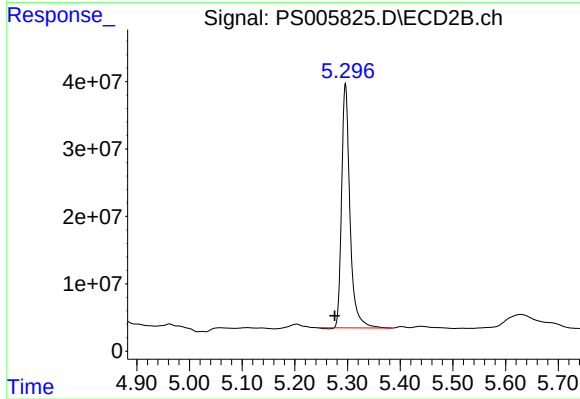

#4 2,4-DCAA


R.T.: 5.296 min
Delta R.T.: 0.020 min
Response: 398789917
Conc: 400.92 ng/ml

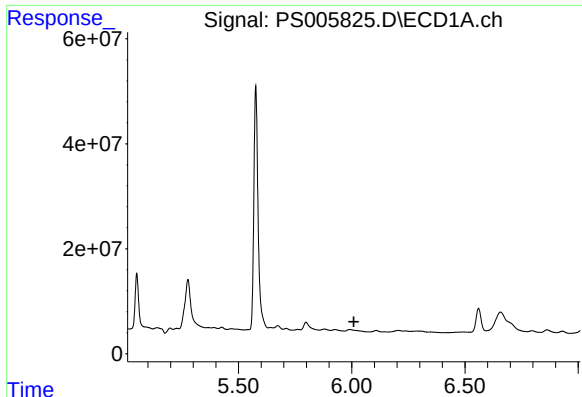

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

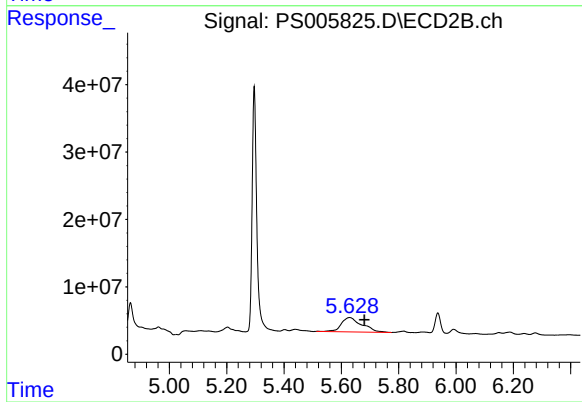


#7 MCPA

R.T.: 5.629 min
Delta R.T.: -0.052 min
Response: 106568272
Conc: 25.32 ug/ml

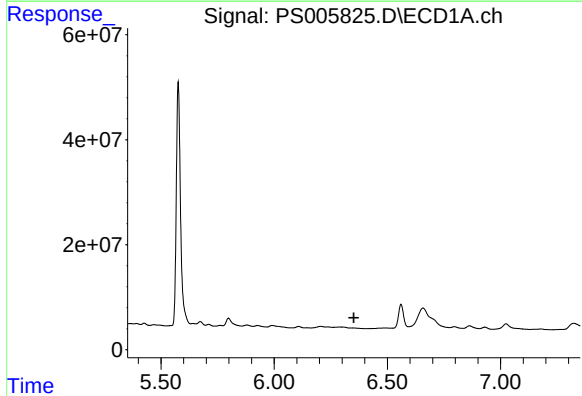


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

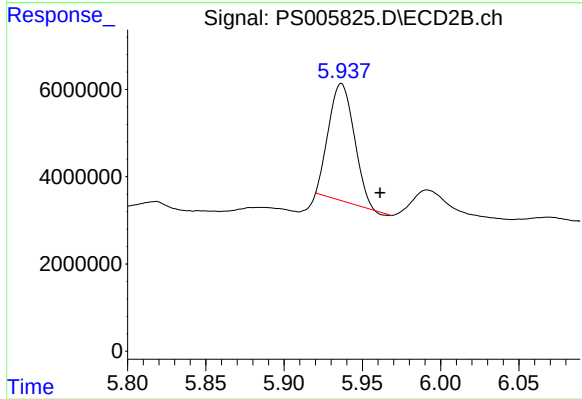

#8 DICHLORPROP


R.T.: 5.937 min
Delta R.T.: -0.025 min
Response: 30346680
Conc: 32.86 ng/ml

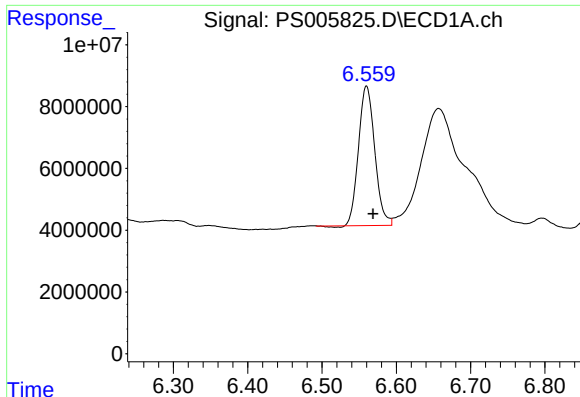

#9 2,4-D


R.T.: 6.560 min
Delta R.T.: -0.009 min
Response: 68473620
Conc: 45.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

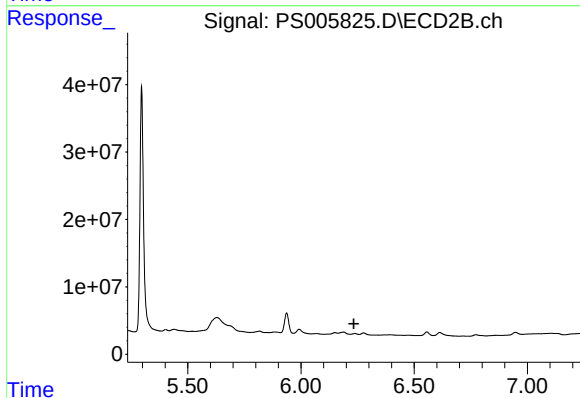


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

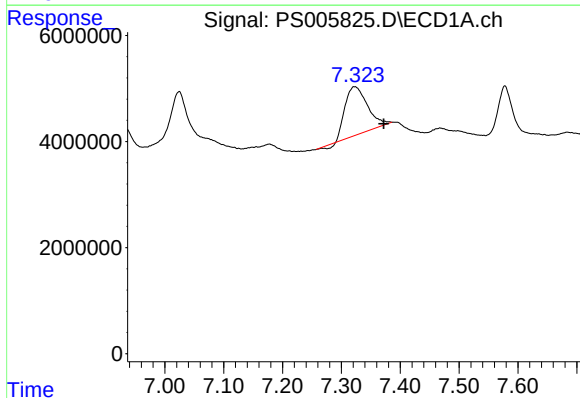

#11 2,4,5-TP (SILVEX)

R.T.: 7.323 min
Delta R.T.: -0.049 min
Response: 23568102
Conc: 2.85 ng/ml

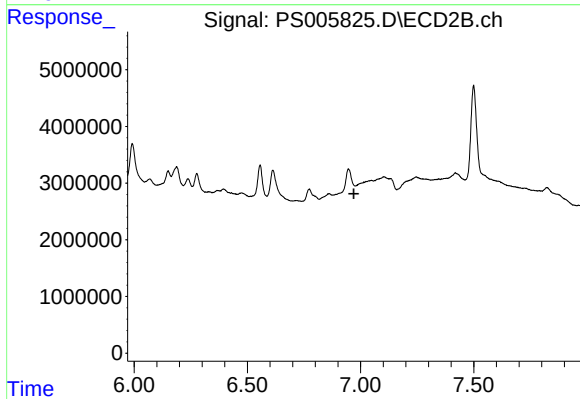

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 6.971 min
Response: 0
Conc: N.D.