

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
 Data File : PS005826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2019 15:17
 Operator : SM\AJ
 Sample : K4044-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:11:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.553	5.274	554.3E6	378.4E6	382.088	380.426
Target Compounds							
2) T	3,5-DICHL...	0.000	4.594	0	34946194	N.D.	26.937
5) T	DICAMBA	5.776	0.000	16830576	0	2.818	N.D. #
9) T	2,4-D	6.538	0.000	69699332	0	46.508	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS005826.D
Data File : PS005826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2019 15:17
Operator : SM\AJ
Sample : K4044-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:11:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

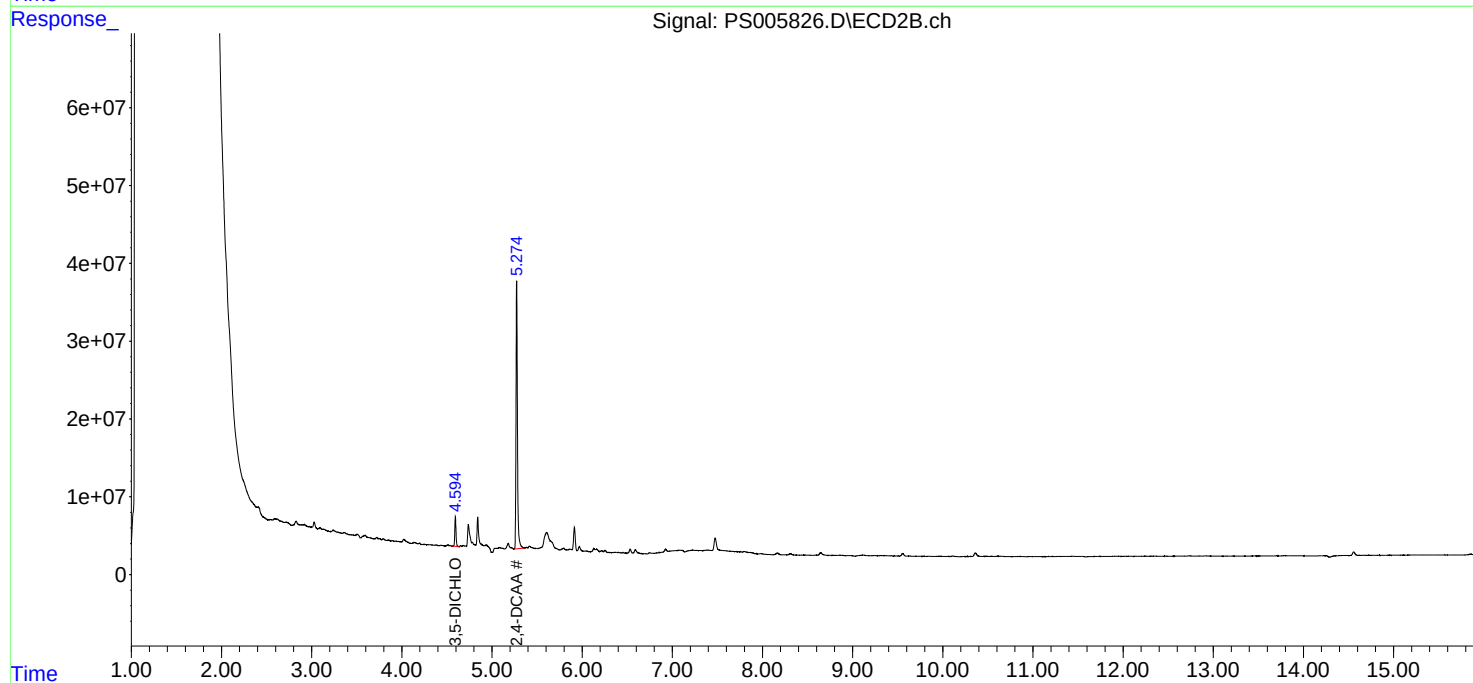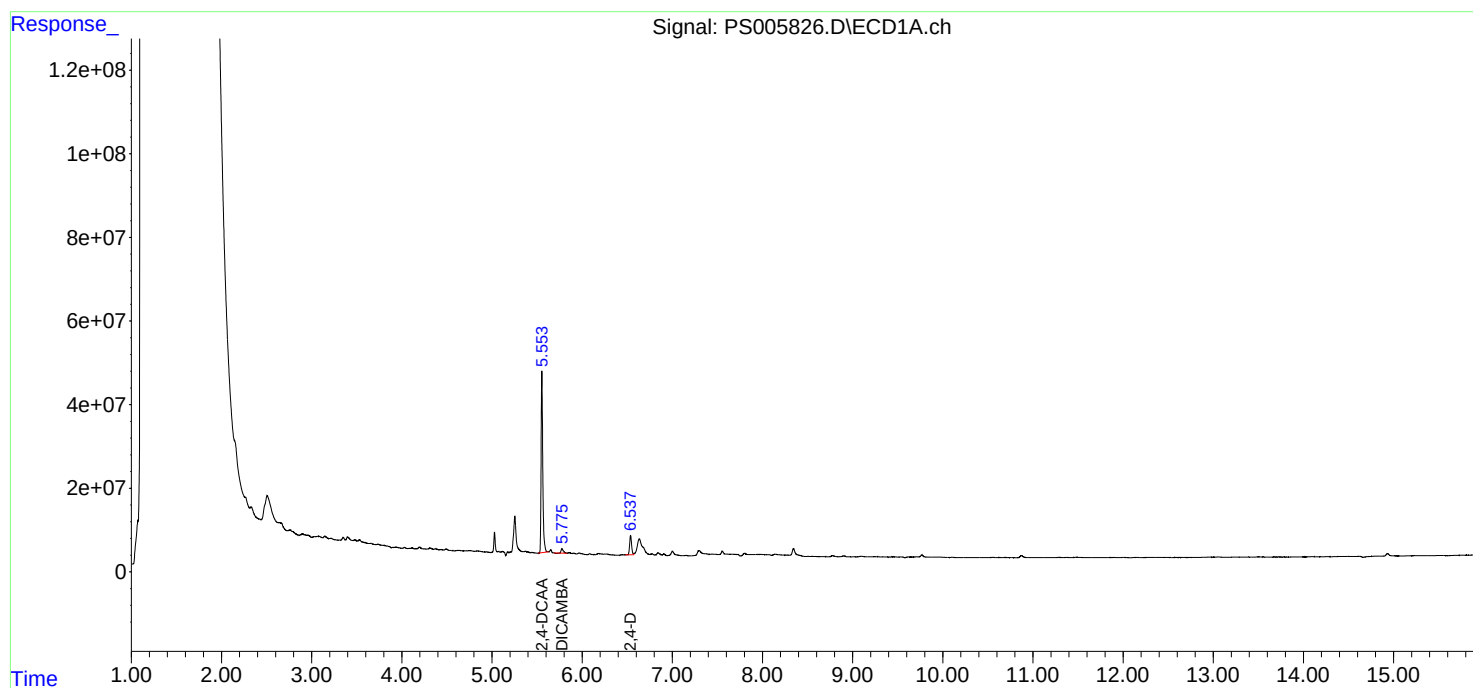


Response_

Signal: PS005826.D\ECD1A.ch

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

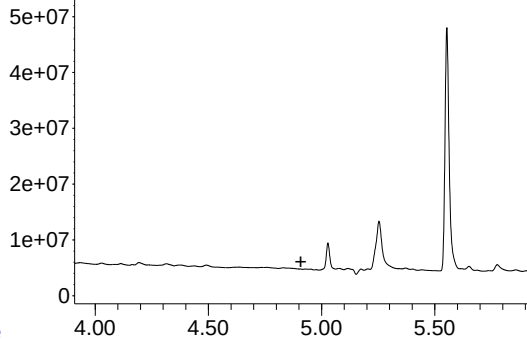


Time

Response_

Signal: PS005826.D\ECD2B.ch

#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.594 min
Delta R.T.: 0.024 min
Response: 34946194
Conc: 26.94 ng/ml

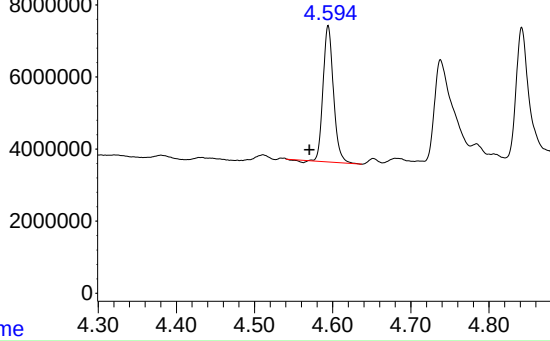


Time

Response_

Signal: PS005826.D\ECD1A.ch

#4 2,4-DCAA

R.T.: 5.553 min
Delta R.T.: -0.003 min
Response: 554340371
Conc: 382.09 ng/ml

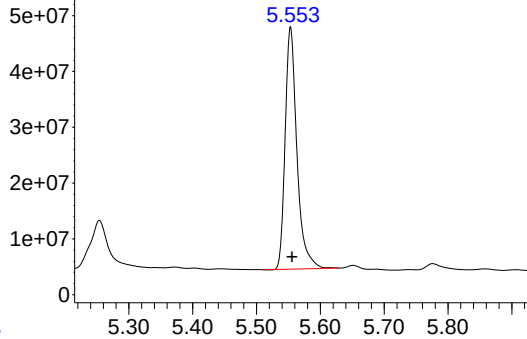


Time

Response_


Signal: PS005826.D\ECD2B.ch

#4 2,4-DCAA

R.T.: 5.274 min
Delta R.T.: -0.002 min
Response: 378401898
Conc: 380.43 ng/ml

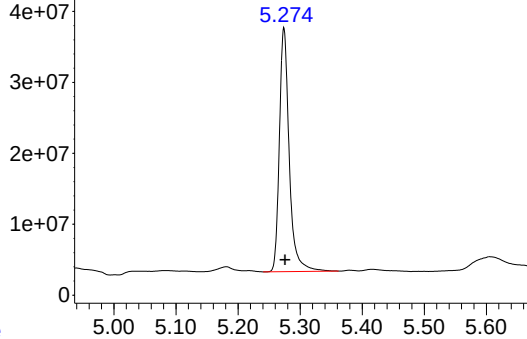


Time

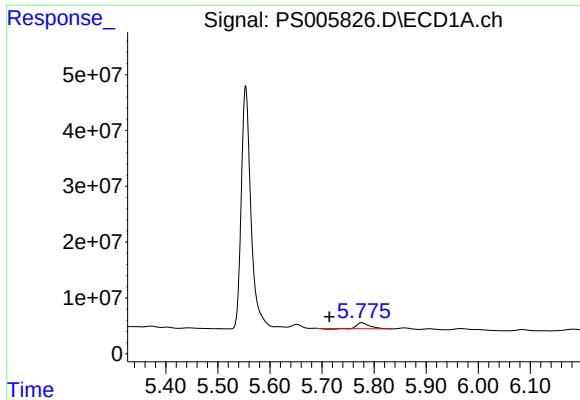

#5 DICAMBA


R.T.: 5.776 min
Delta R.T.: 0.062 min
Response: 16830576
Conc: 2.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

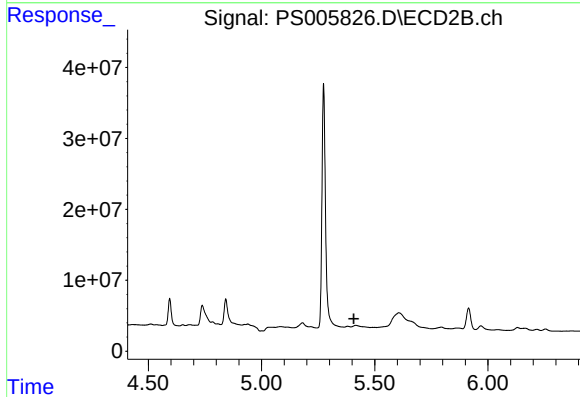


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

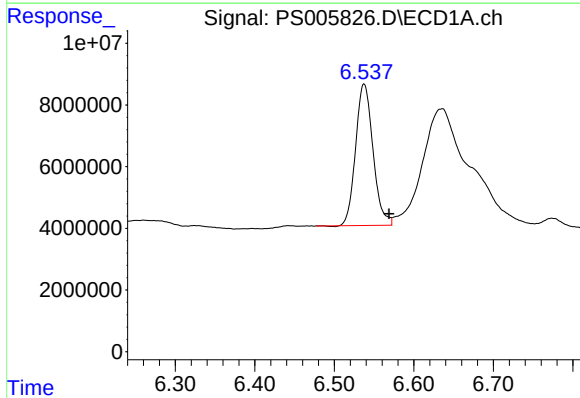

#9 2,4-D

R.T.: 6.538 min
Delta R.T.: -0.031 min
Response: 69699332
Conc: 46.51 ng/ml

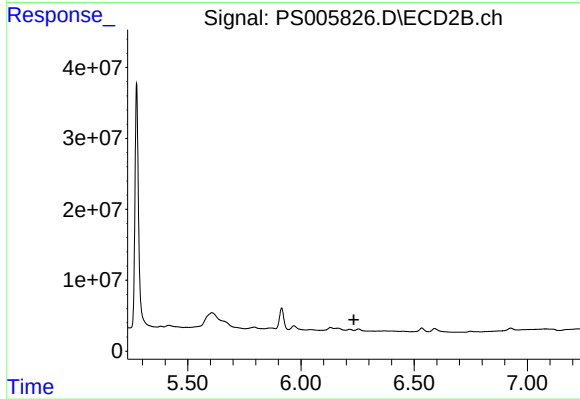

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.