

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
 Data File : PS005827.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2019 15:39
 Operator : SM\AJ
 Sample : K4044-16
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:11:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.560	5.280	620.2E6	417.5E6	427.510	419.707
Target Compounds							
2) T	3,5-DICHL...	0.000	4.600	0	44765658	N.D.	34.506
5) T	DICAMBA	5.782	0.000	21910395	0	3.669	N.D. #
7) T	MCPA	0.000	5.613	0	111.2E6	N.D.	26.414
9) T	2,4-D	6.544	0.000	116.1E6	0	77.455	N.D. #
11) T	2,4,5-TP ...	7.306	0.000	22551737	0	2.730	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
Data File : PS005827.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2019 15:39
Operator : SM\AJ
Sample : K4044-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:11:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

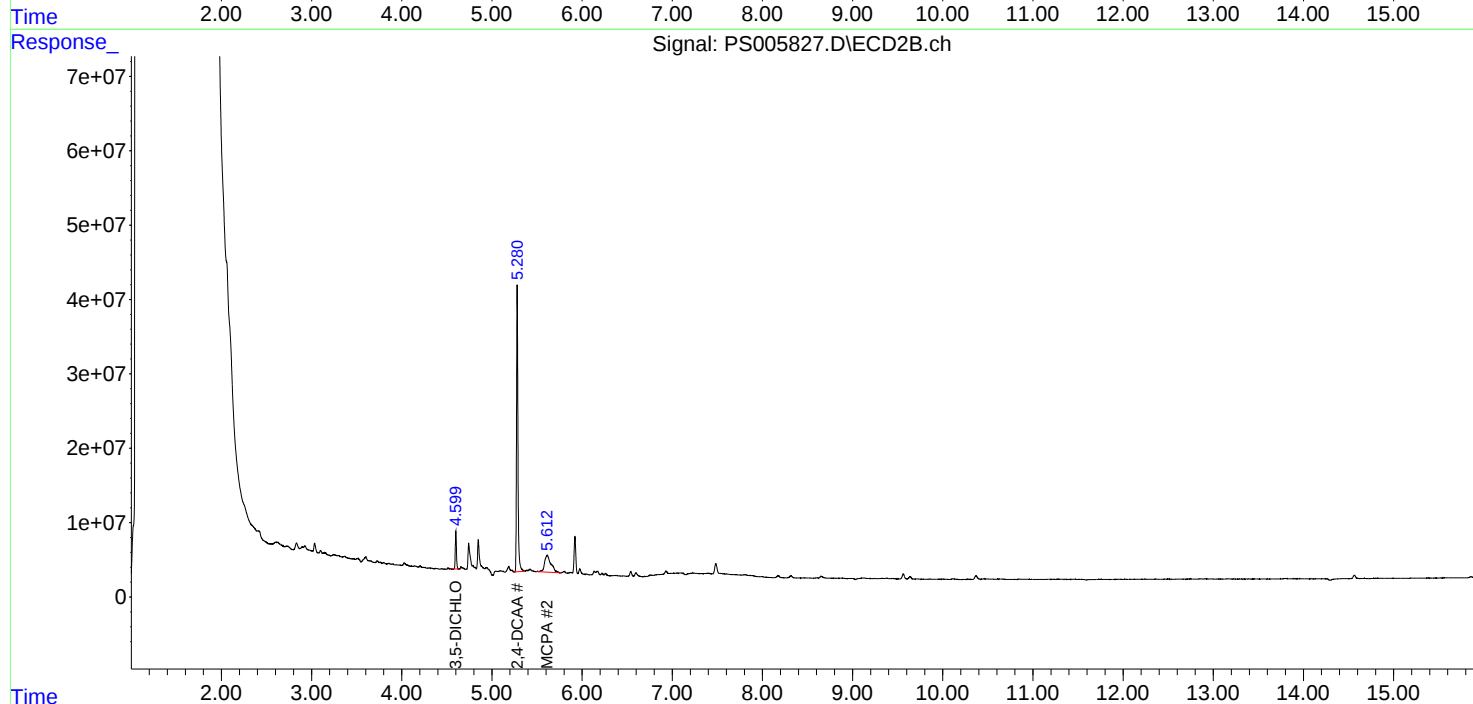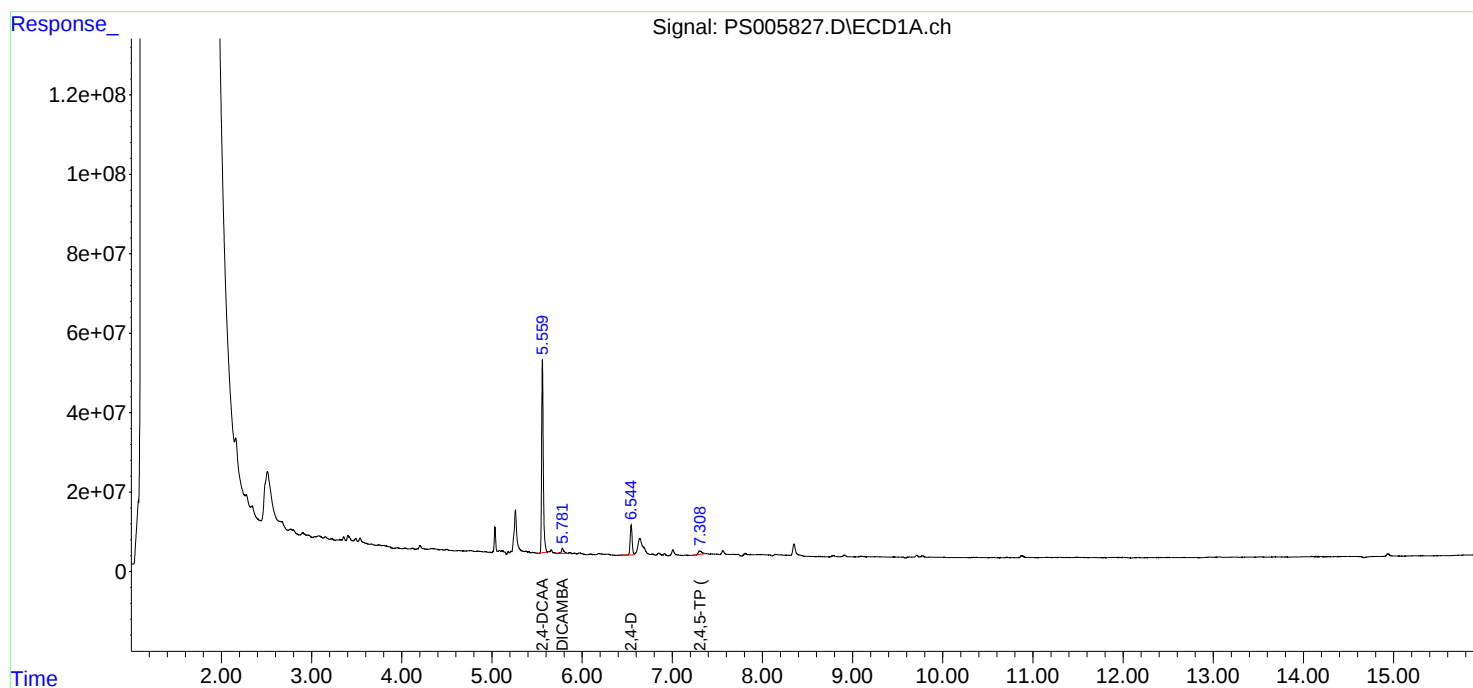


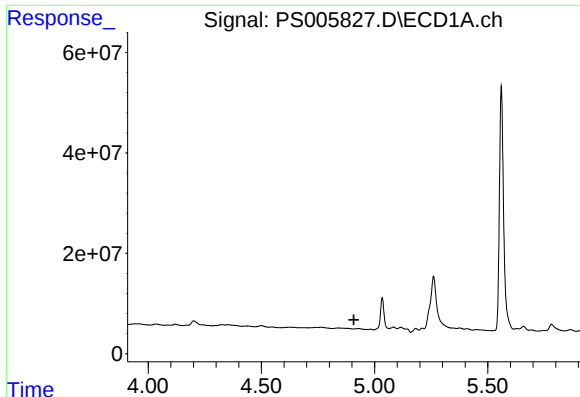

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-4

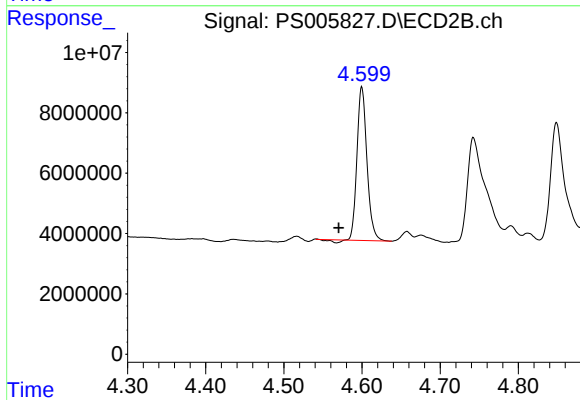


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.600 min
Delta R.T.: 0.030 min
Response: 44765658
Conc: 34.51 ng/ml

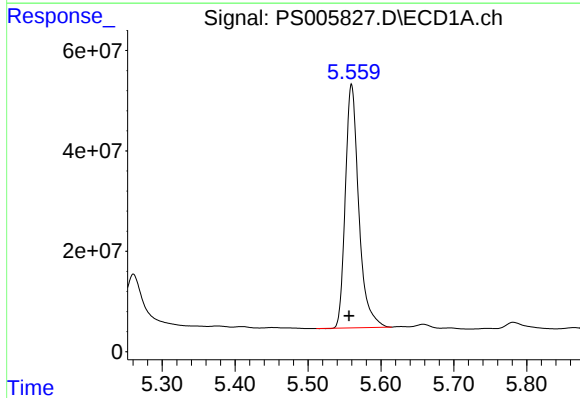


#4 2,4-DCAA

R.T.: 5.560 min
Delta R.T.: 0.004 min
Response: 620239574
Conc: 427.51 ng/ml

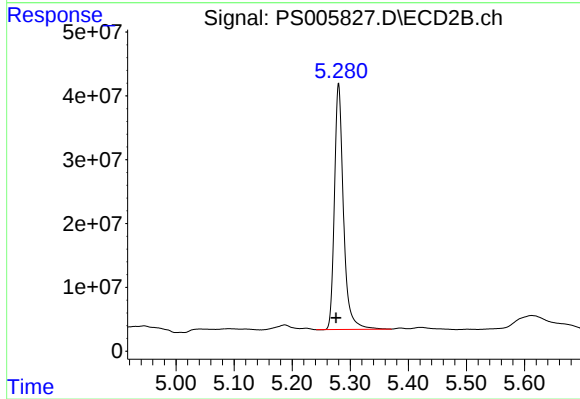

#4 2,4-DCAA


R.T.: 5.280 min
Delta R.T.: 0.004 min
Response: 417473742
Conc: 419.71 ng/ml

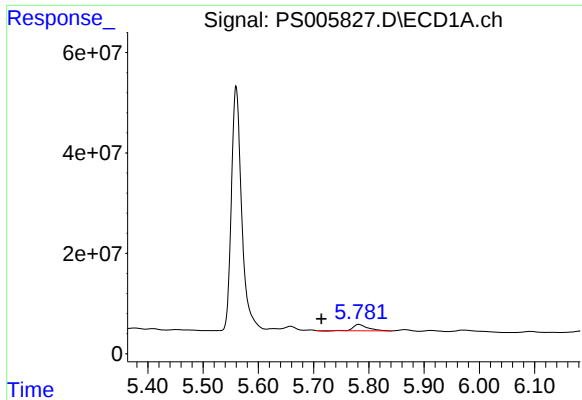

#5 DICAMBA


R.T.: 5.582 min
Delta R.T.: 0.068 min
Response: 21910395
Conc: 3.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-4

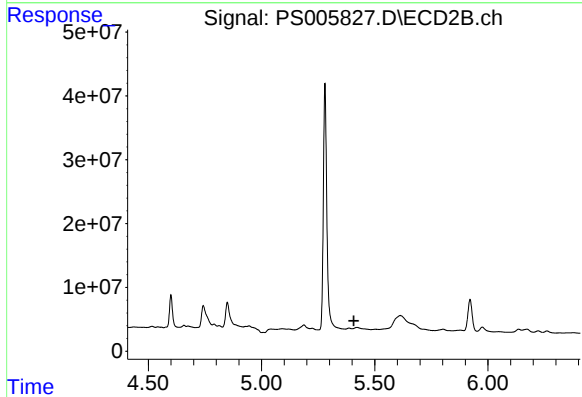


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

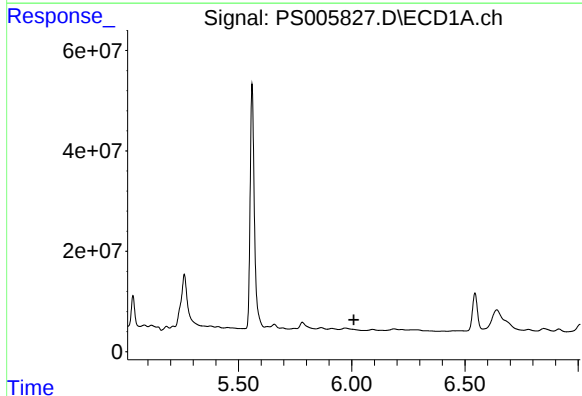


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.009 min
Response: 0
Conc: N.D.

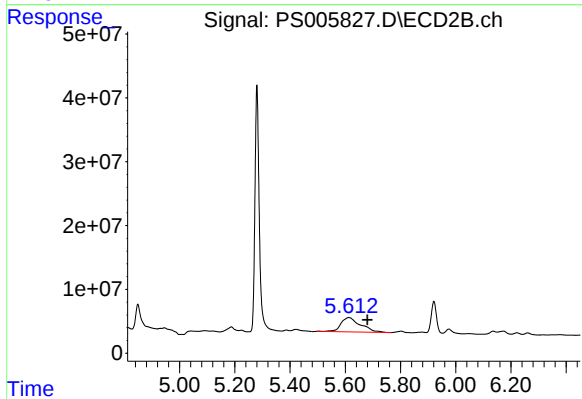

#7 MCPA


R.T.: 5.613 min
Delta R.T.: -0.068 min
Response: 111176865
Conc: 26.41 ug/ml

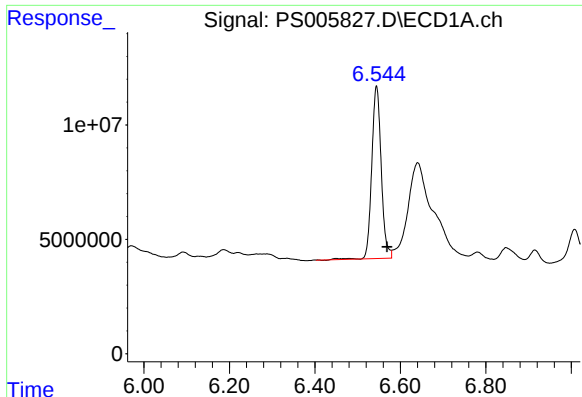

#9 2,4-D


R.T.: 6.544 min
Delta R.T.: -0.025 min
Response: 116079626
Conc: 77.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-4

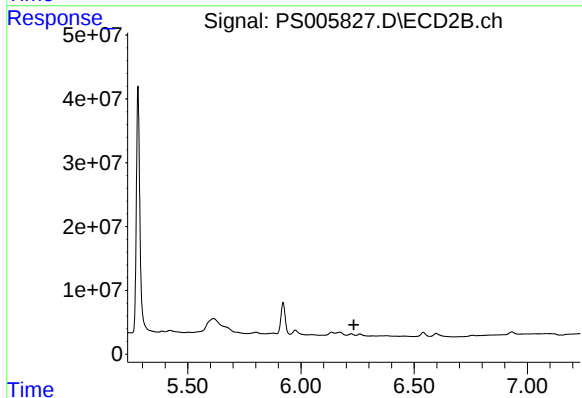


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

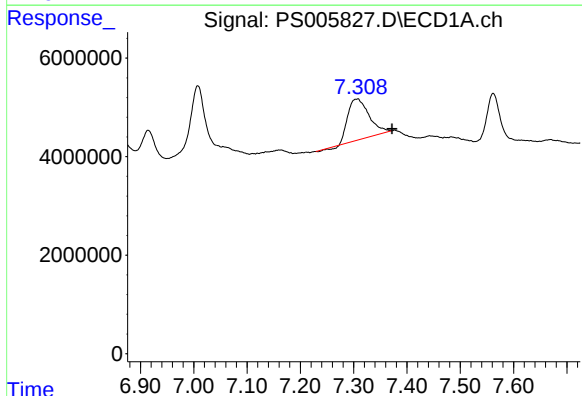

#11 2,4,5-TP (SILVEX)

R.T.: 7.306 min
Delta R.T.: -0.066 min
Response: 22551737
Conc: 2.73 ng/ml

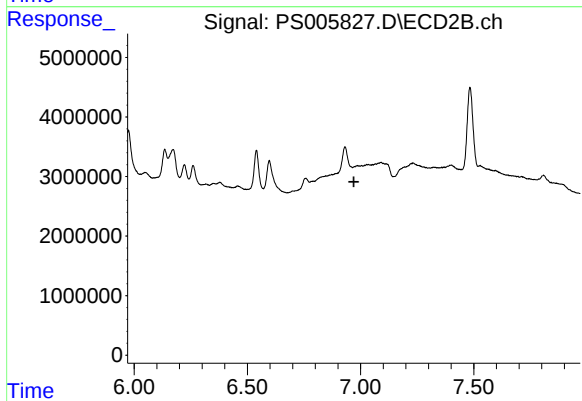

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 6.971 min
Response: 0
Conc: N.D.