

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
 Data File : PS005829.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2019 16:23
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:12:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.556	5.275	612.5E6	418.7E6	422.171	420.961
Target Compounds							
7) T	MCPA	0.000	5.611	0	112.9E6	N.D.	26.835
9) T	2,4-D	6.633	0.000	196.3E6	0	130.982	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS005829\
Data File : PS005829.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2019 16:23
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:12:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

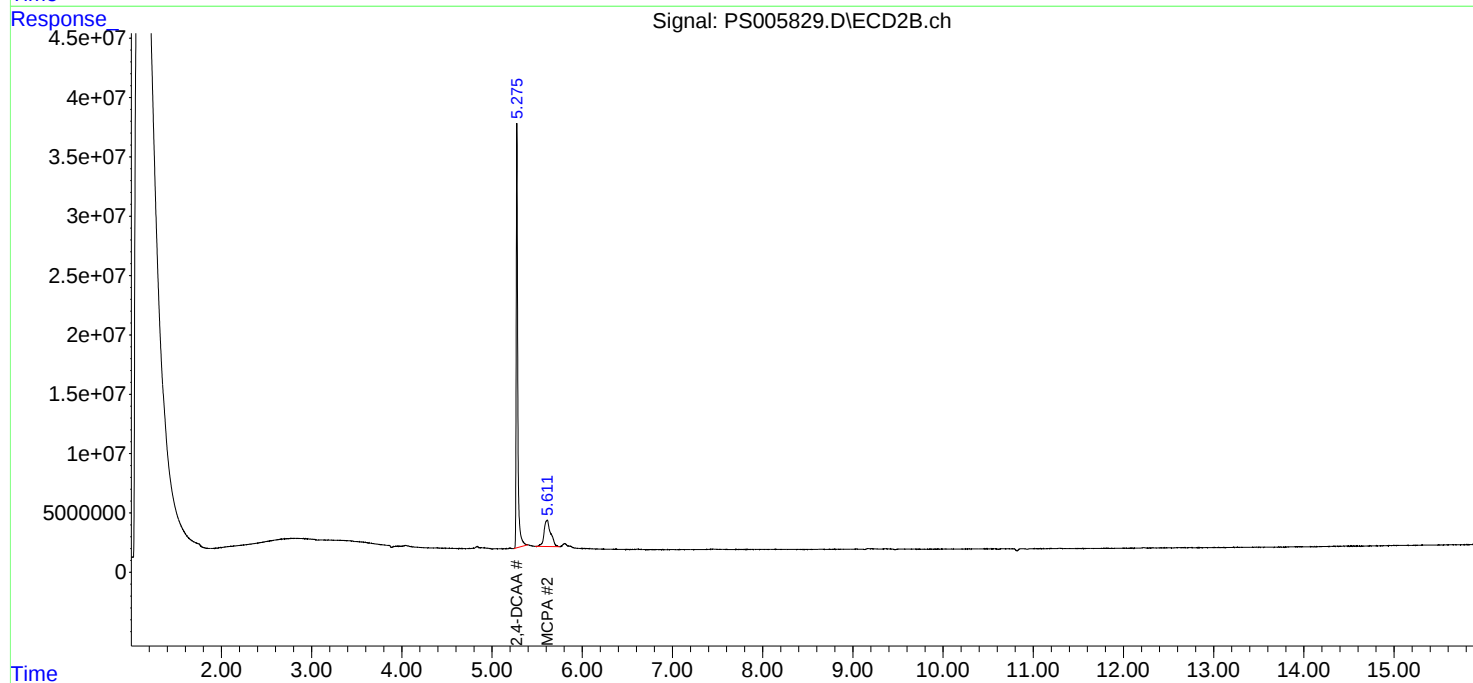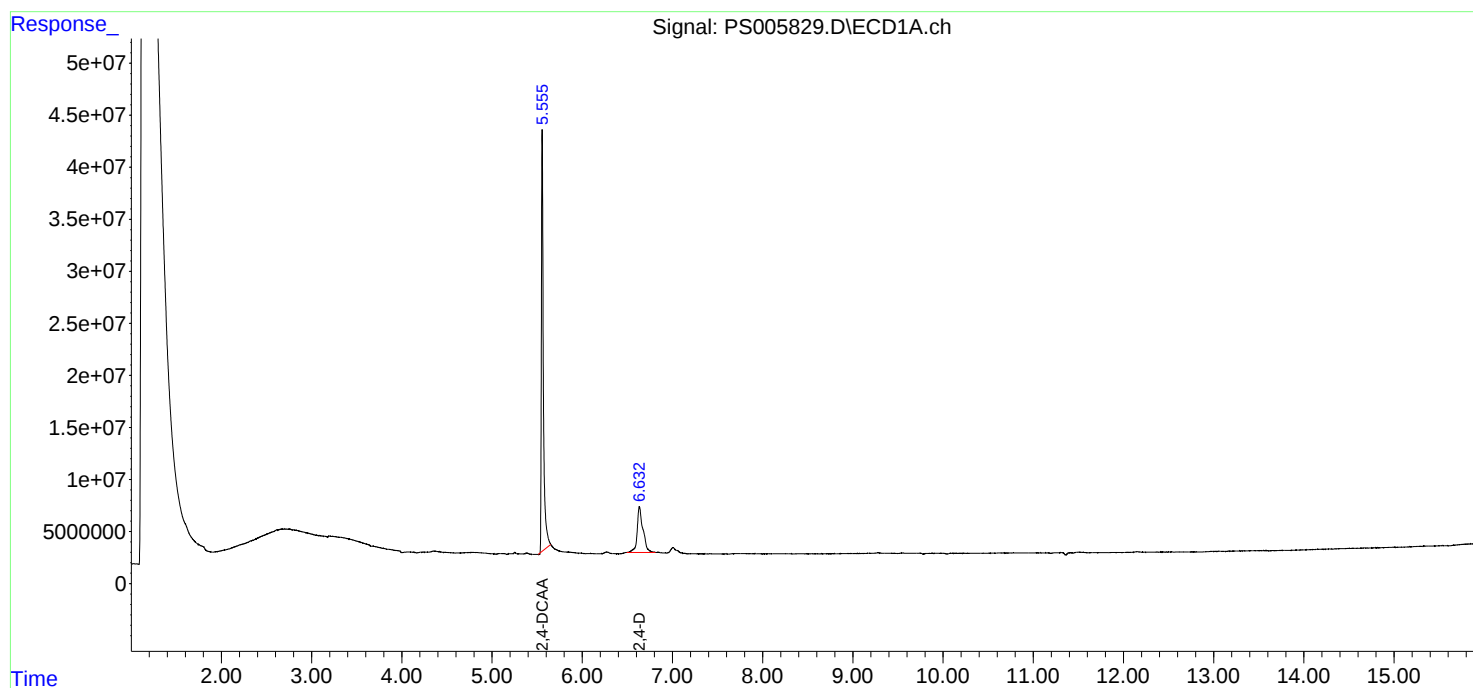


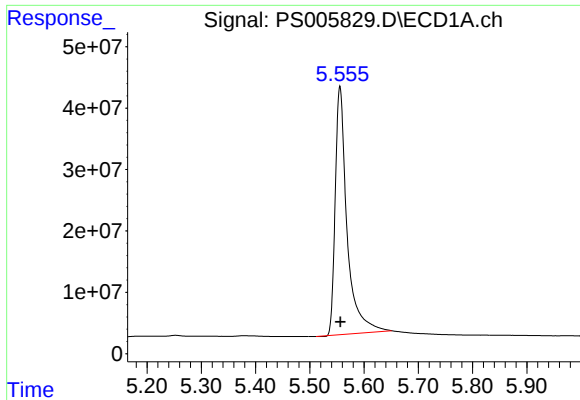

#4 2,4-DCAA


R.T.: 5.556 min
Delta R.T.: 0.000 min
Response: 612492693
Conc: 422.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

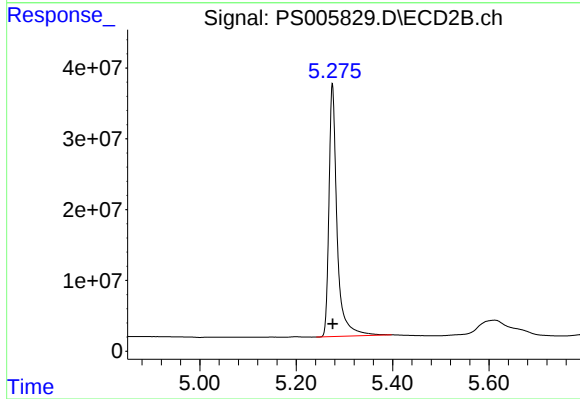


#4 2,4-DCAA

R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 418720859
Conc: 420.96 ng/ml

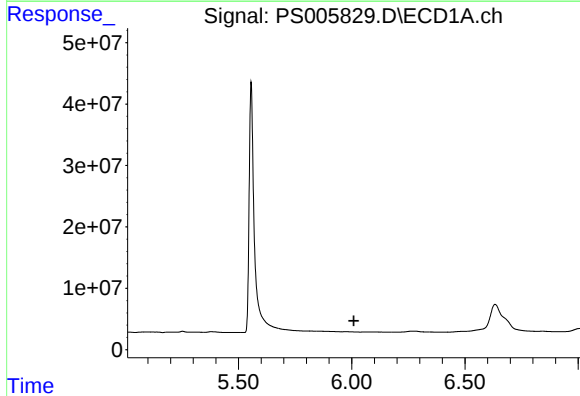


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.009 min
Response: 0
Conc: N.D.

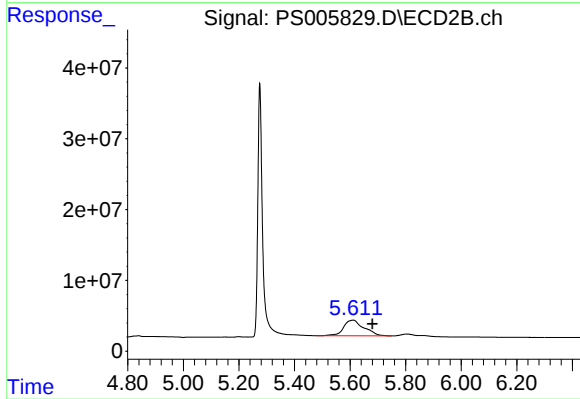

#7 MCPA


R.T.: 5.611 min
Delta R.T.: -0.070 min
Response: 112948524
Conc: 26.83 ug/ml

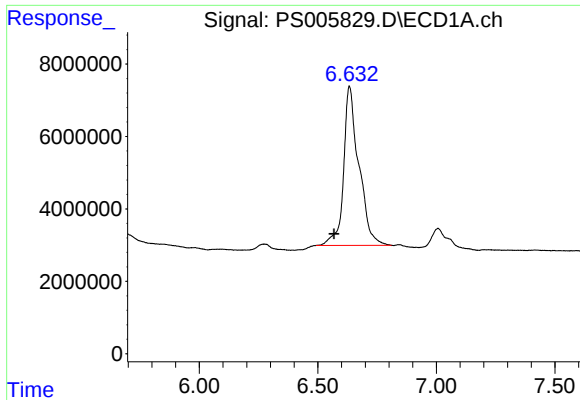

#9 2,4-D

R.T.: 6.633 min
Delta R.T.: 0.064 min
Response: 196298743
Conc: 130.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

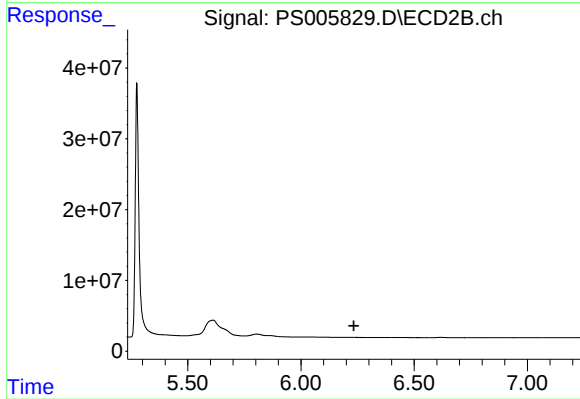

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.