

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
 Data File : PS005833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2019 17:52
 Operator : SM\AJ
 Sample : PB121890TB
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB121890TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:14:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.556	5.277	547.6E6	388.5E6	377.469	390.606
Target Compounds							
1) T	Dalapon	2.058	0.000	41967603	0	22.645	N.D. #
2) T	3,5-DICHL...	0.000	4.596	0	215.6E6	N.D.	166.151
3) T	4-Nitroph...	5.346	0.000	10483817	0	17.429	N.D. #
5) T	DICAMBA	5.777	5.383	47485974	9074148	7.951	2.431 #
6) T	MCP	5.861	0.000	17103188	0	3.691	N.D. #
7) T	MCPA	5.963	5.666	34656331	26238343	5.311	6.234
8) T	DICHLORPROP	0.000	5.971	0	16015054	N.D.	17.341
9) T	2,4-D	6.636	6.219	195.0E6	14447539	130.091	13.448 #
11) T	2,4,5-TP ...	0.000	6.925	0	31845110	N.D.	6.139



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
Data File : PS005833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2019 17:52
Operator : SM\AJ
Sample : PB121890TB
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB121890TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:14:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

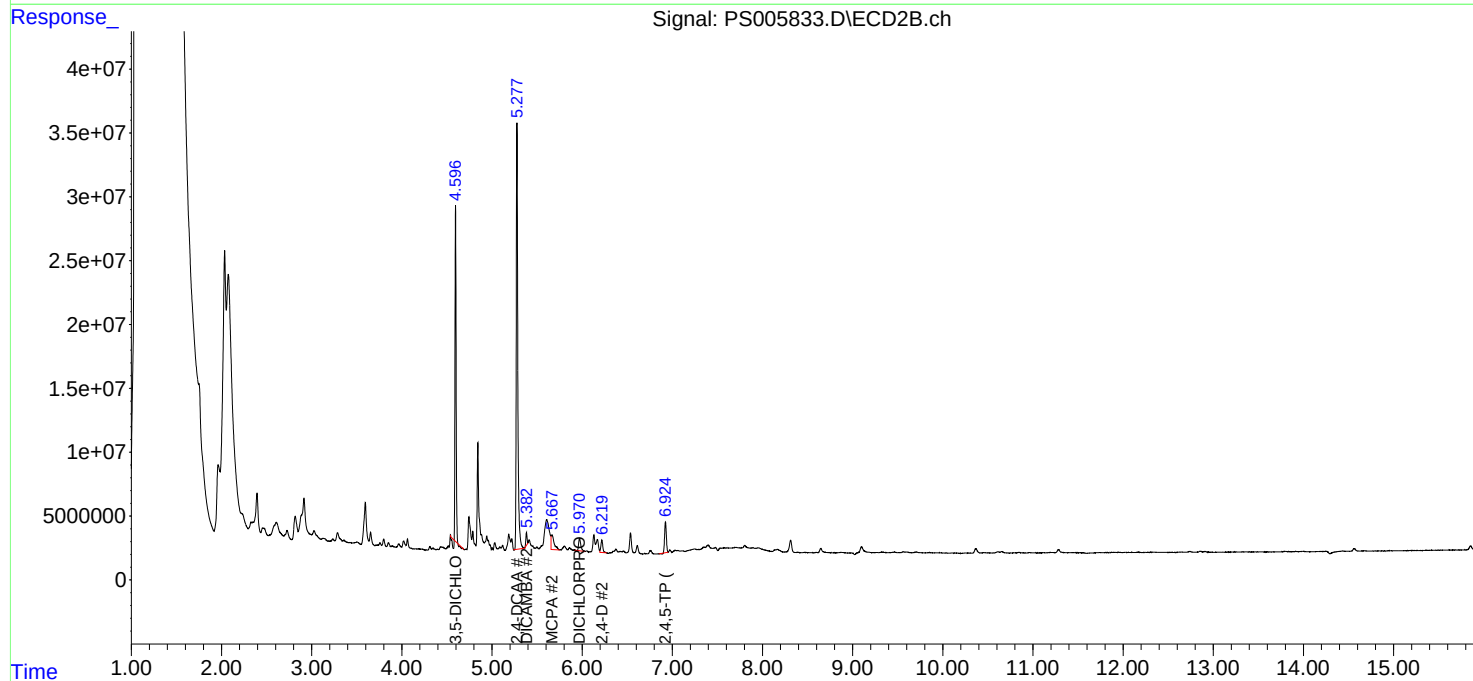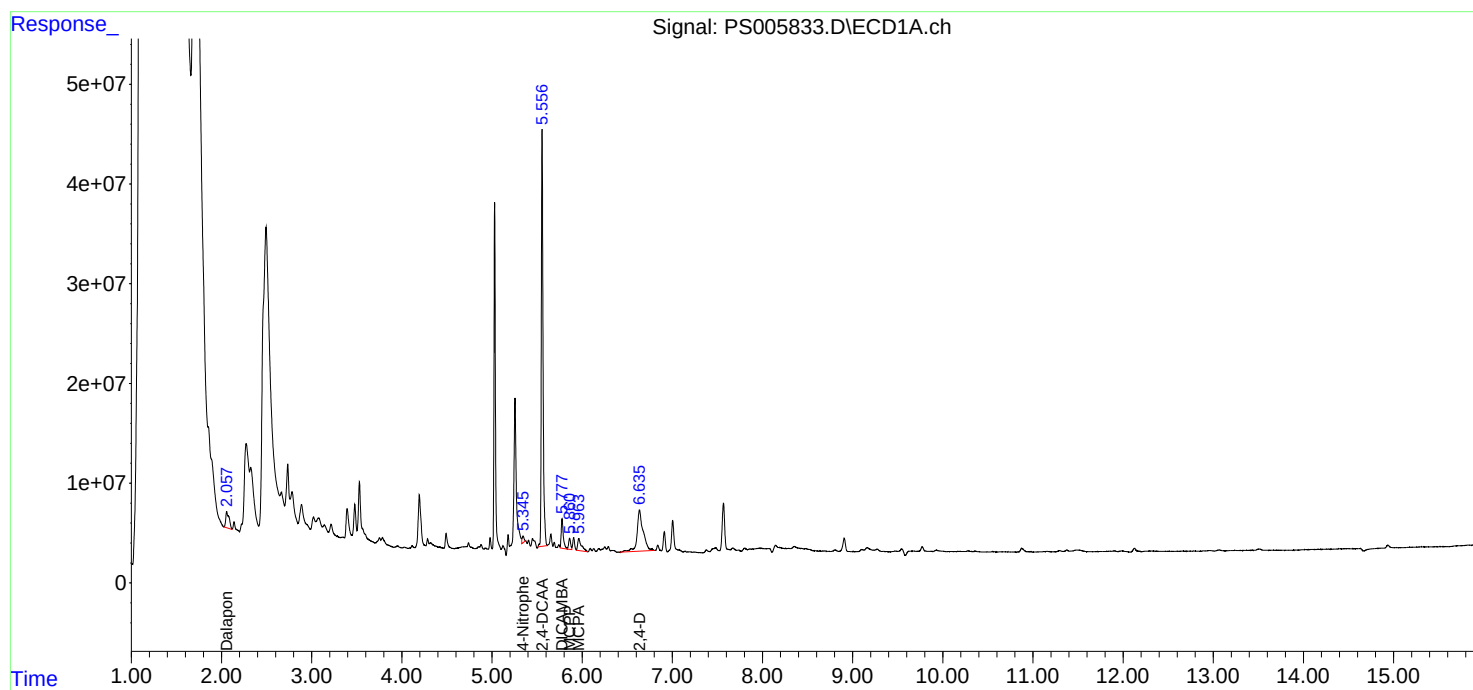


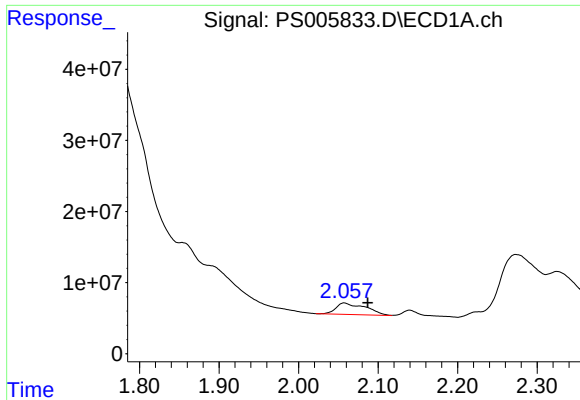

#1 Dalapon


R.T.: 2.058 min
Delta R.T.: -0.029 min
Response: 41967603
Conc: 22.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121890TB

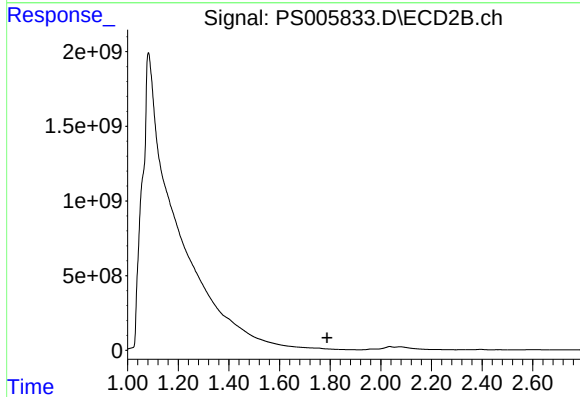


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

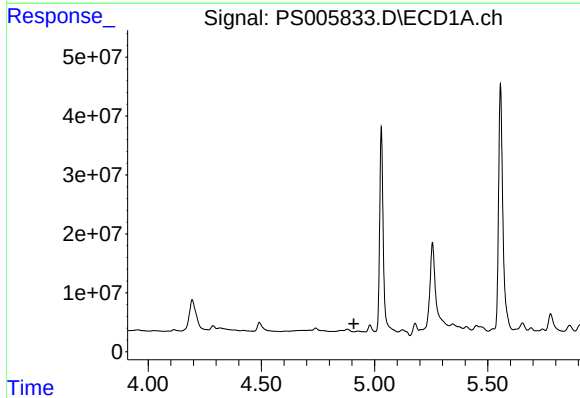


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

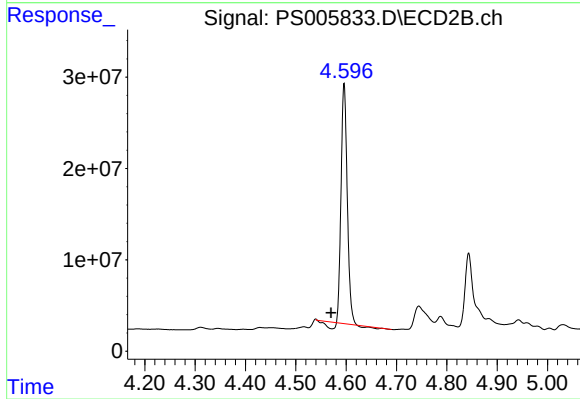

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.596 min
Delta R.T.: 0.026 min
Response: 215550492
Conc: 166.15 ng/ml

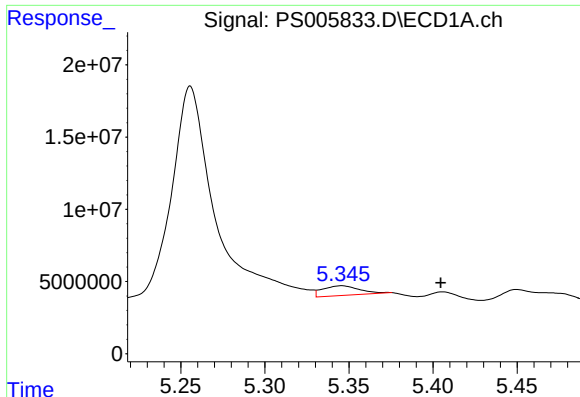

#3 4-Nitrophenol


R.T.: 5.346 min
Delta R.T.: -0.059 min
Response: 10483817
Conc: 17.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121890TB

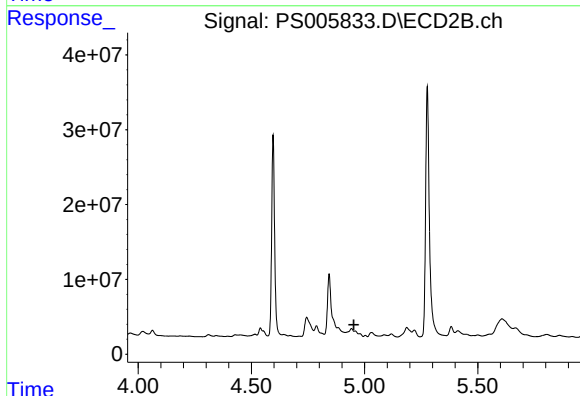


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 4.953 min
Response: 0
Conc: N.D.

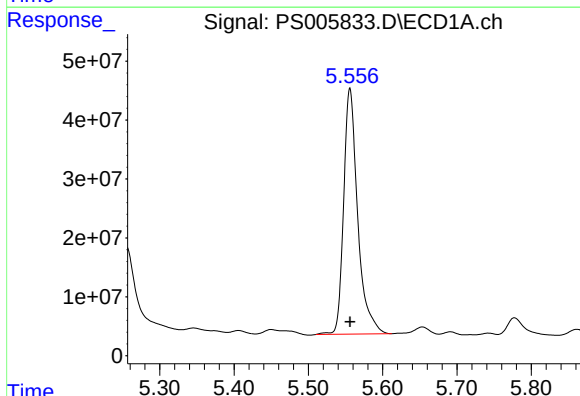


#4 2,4-DCAA

R.T.: 5.556 min
Delta R.T.: 0.000 min
Response: 547638857
Conc: 377.47 ng/ml

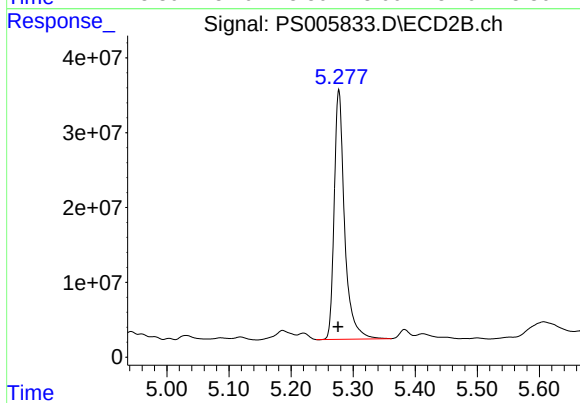

#4 2,4-DCAA


R.T.: 5.277 min
Delta R.T.: 0.001 min
Response: 388527141
Conc: 390.61 ng/ml

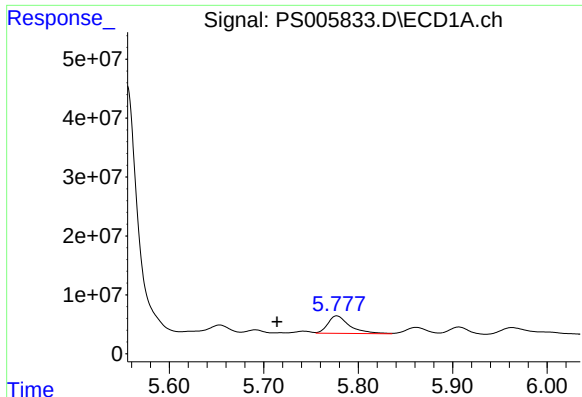

#5 DICAMBA


R.T.: 5.777 min
Delta R.T.: 0.063 min
Response: 47485974
Conc: 7.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121890TB

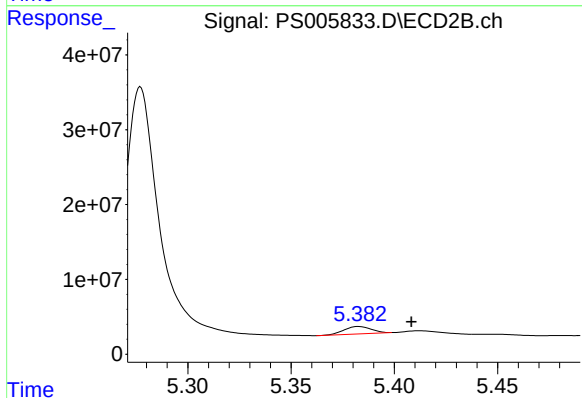


#5 DICAMBA

R.T.: 5.383 min
Delta R.T.: -0.025 min
Response: 9074148
Conc: 2.43 ng/ml

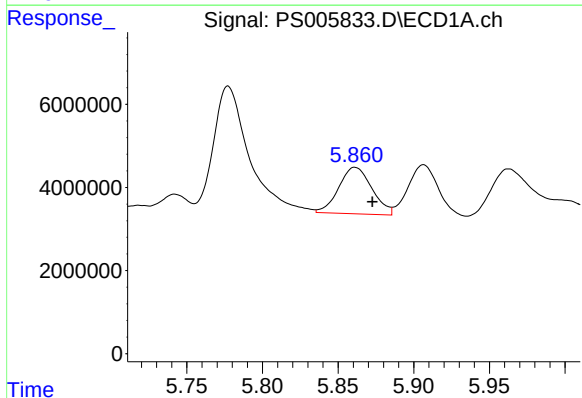


#6 MCP

R.T.: 5.861 min
Delta R.T.: -0.011 min
Response: 17103188
Conc: 3.69 ug/ml

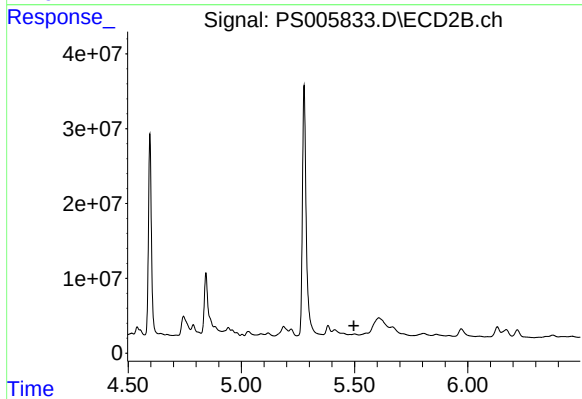

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

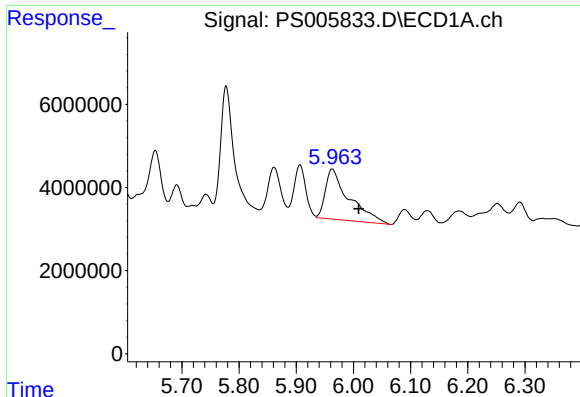

#7 MCPA


R.T.: 5.963 min
Delta R.T.: -0.046 min
Response: 34656331
Conc: 5.31 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB121890TB

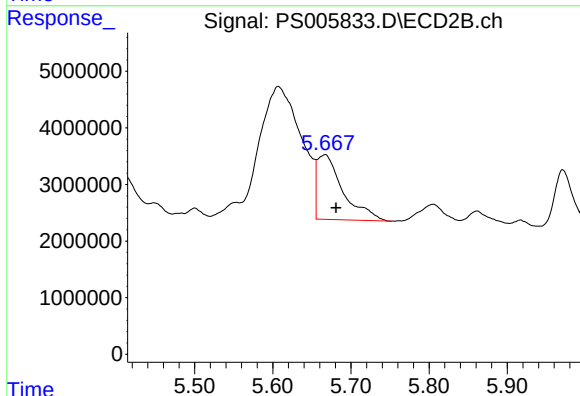


#7 MCPA

R.T.: 5.666 min
Delta R.T.: -0.014 min
Response: 26238343
Conc: 6.23 ug/ml

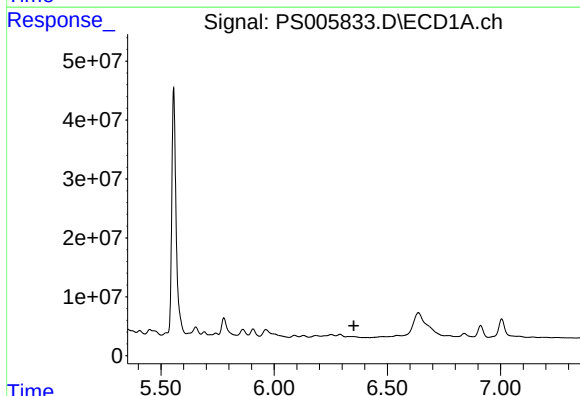


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.352 min
Response: 0
Conc: N.D.

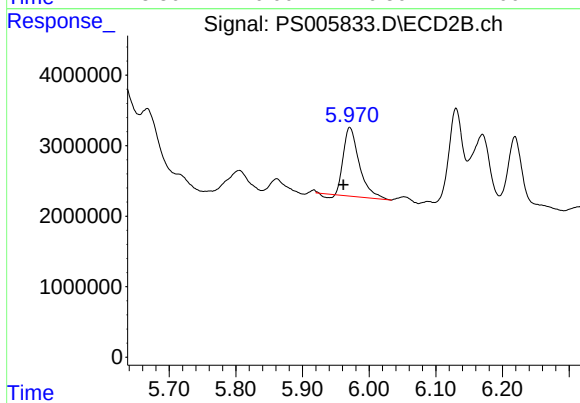

#8 DICHLORPROP


R.T.: 5.971 min
Delta R.T.: 0.010 min
Response: 16015054
Conc: 17.34 ng/ml

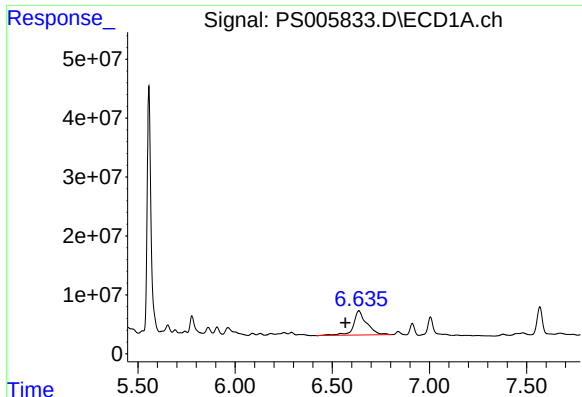

#9 2,4-D


R.T.: 6.636 min
Delta R.T.: 0.068 min
Response: 194963536
Conc: 130.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121890TB

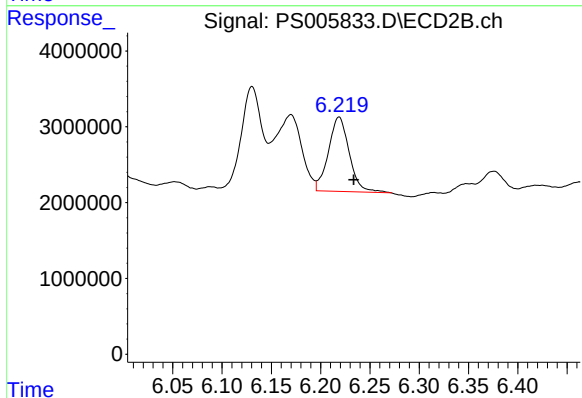


#9 2,4-D

R.T.: 6.219 min
Delta R.T.: -0.015 min
Response: 14447539
Conc: 13.45 ng/ml

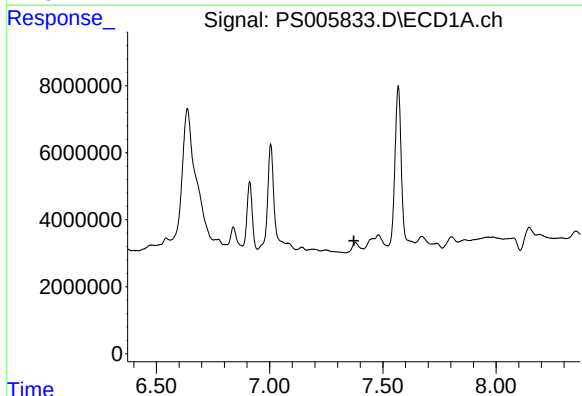

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.372 min
Response: 0
Conc: N.D.

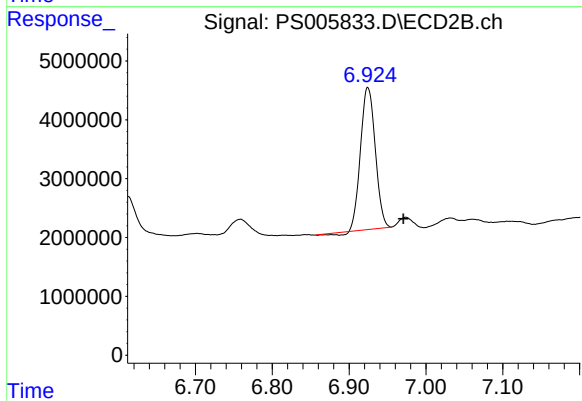

#11 2,4,5-TP (SILVEX)

R.T.: 6.925 min
Delta R.T.: -0.046 min
Response: 31845110
Conc: 6.14 ng/ml