

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
 Data File : PS005834.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2019 18:14
 Operator : SM\AJ
 Sample : K3618-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HD-01-073019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:14:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.558	5.279	587.4E6	412.0E6	404.852	414.201
Target Compounds							
1) T	Dalapon	2.060	0.000	43208698	0	23.314	N.D. #
2) T	3,5-DICHL...	0.000	4.598	0	178.3E6	N.D.	137.469
3) T	4-Nitroph...	5.348	4.982	9019810	12325155	14.995	24.880 #
5) T	DICAMBA	5.745	5.384	16976955	22920574	2.843	6.140 #
6) T	MCP	5.863	0.000	20367516	0	4.396	N.D. #
7) T	MCPA	5.966	0.000	36382623	0	5.575	N.D. #
8) T	DICHLORPROP	6.294	0.000	17228959	0	11.981	N.D. #
9) T	2,4-D	0.000	6.220	0	14347170	N.D.	13.355
11) T	2,4,5-TP ...	0.000	6.926	0	14054428	N.D.	2.709



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
Data File : PS005834.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2019 18:14
Operator : SM\AJ
Sample : K3618-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HD-01-073019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:14:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

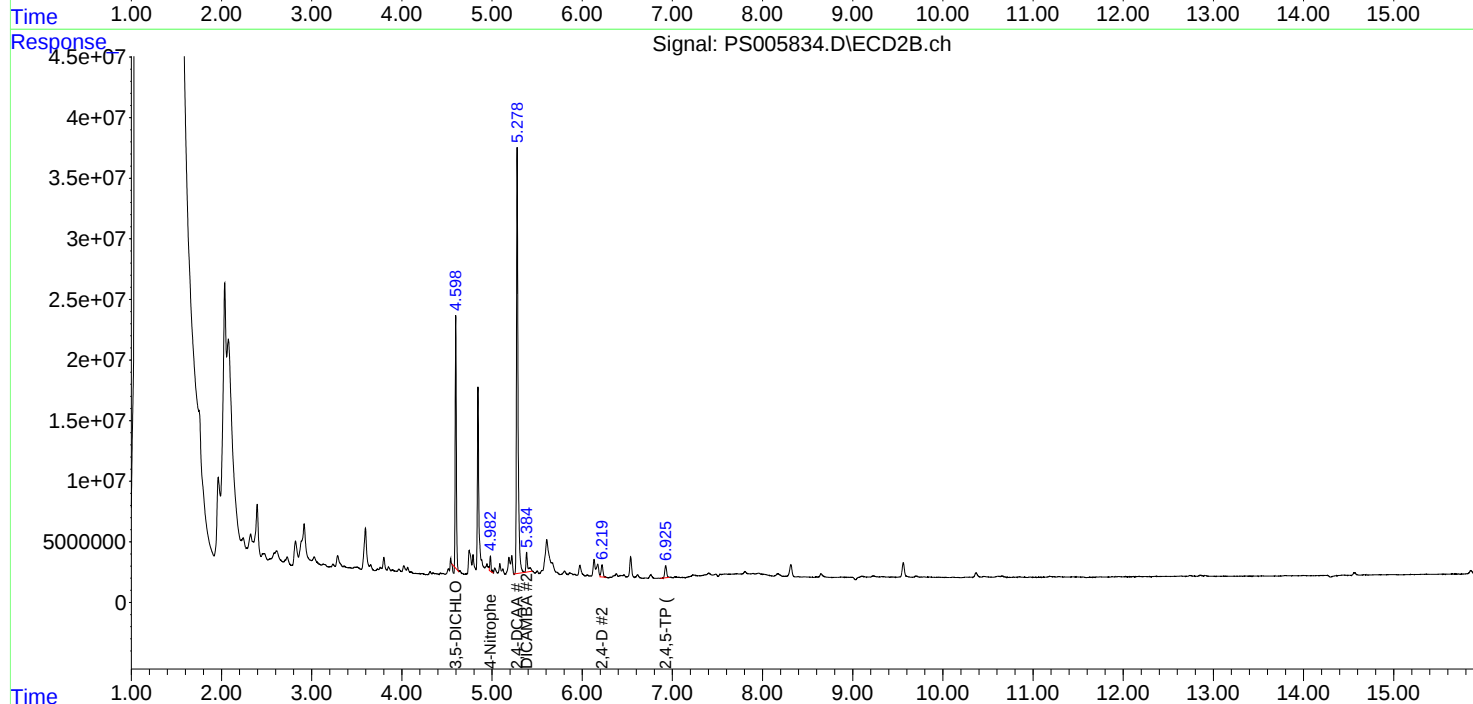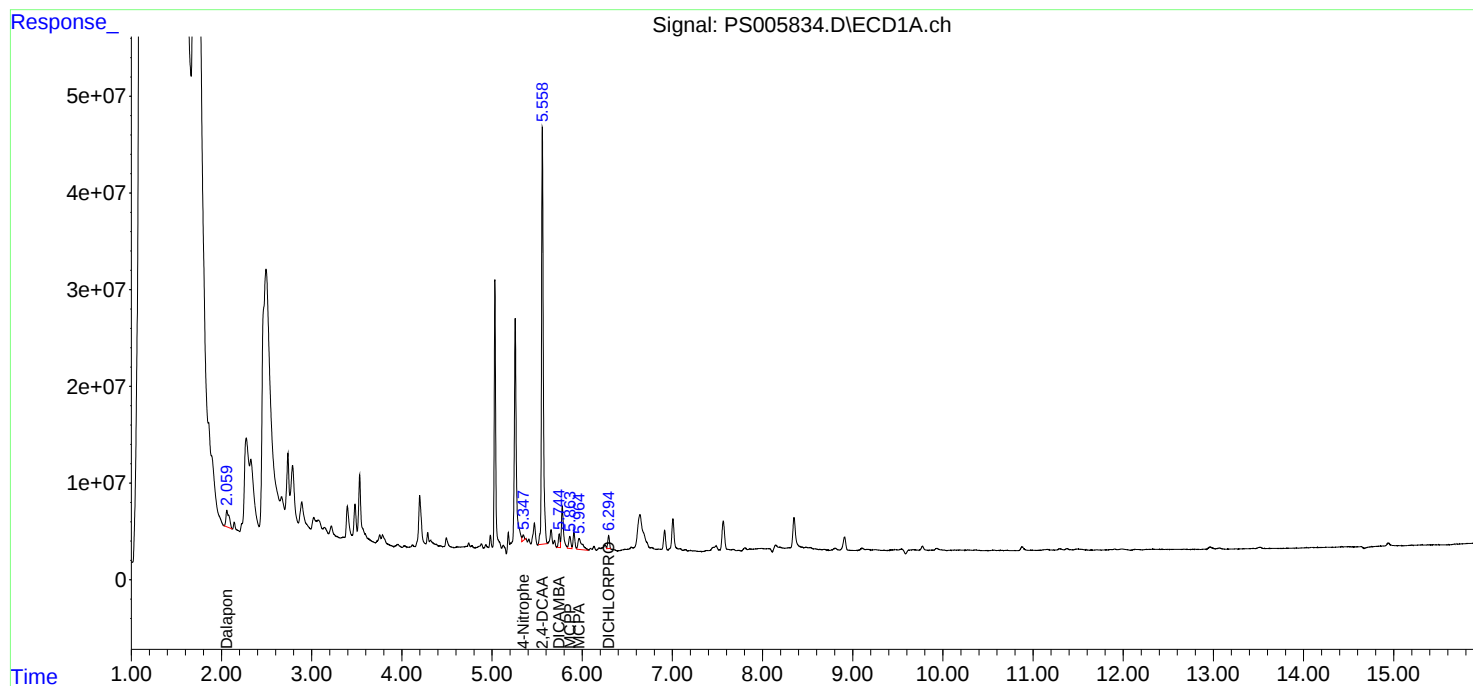


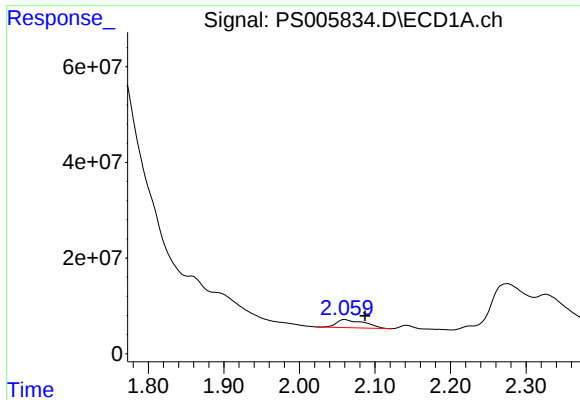

#1 Dalapon


R.T.: 2.060 min
Delta R.T.: -0.027 min
Response: 43208698
Conc: 23.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-073019

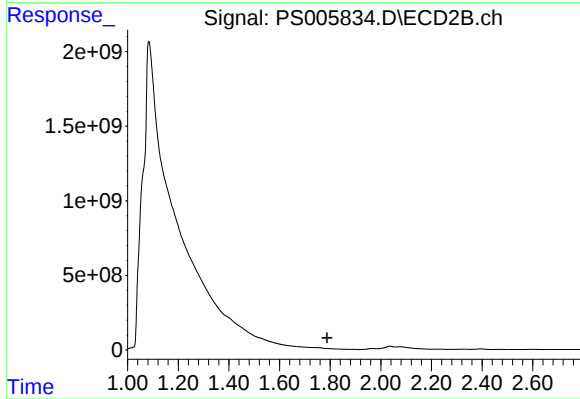


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

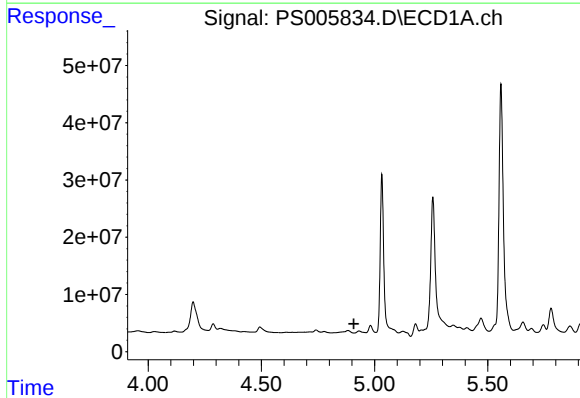


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

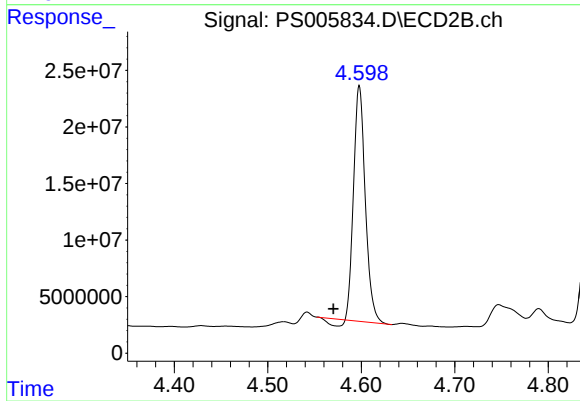

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.598 min
Delta R.T.: 0.028 min
Response: 178340079
Conc: 137.47 ng/ml

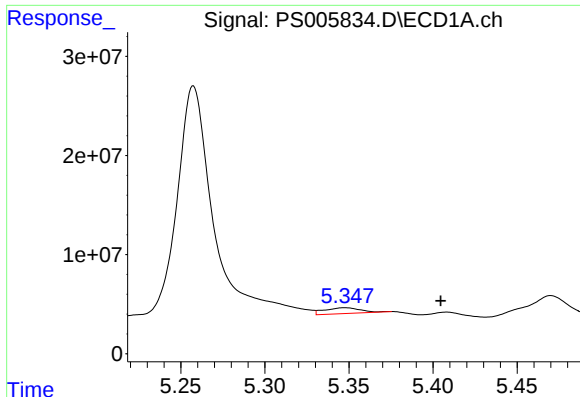

#3 4-Nitrophenol


R.T.: 5.348 min
Delta R.T.: -0.057 min
Response: 9019810
Conc: 14.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-073019

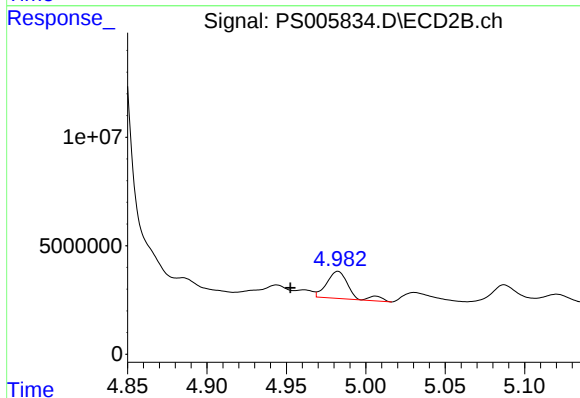


#3 4-Nitrophenol

R.T.: 4.982 min
Delta R.T.: 0.030 min
Response: 12325155
Conc: 24.88 ng/ml

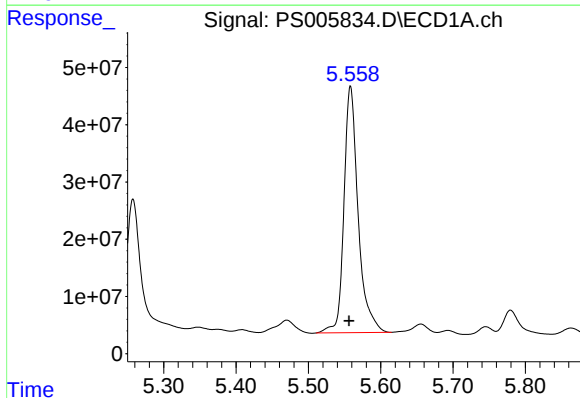


#4 2,4-DCAA

R.T.: 5.558 min
Delta R.T.: 0.002 min
Response: 587365918
Conc: 404.85 ng/ml

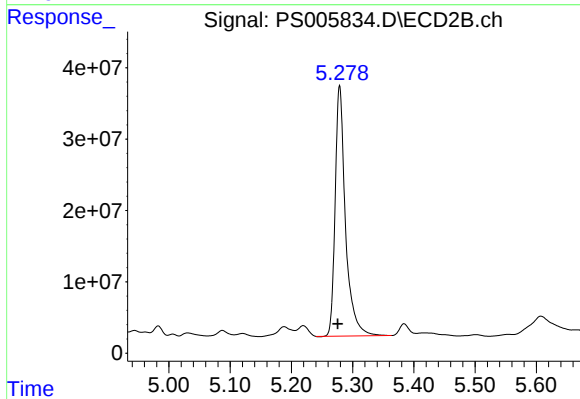

#4 2,4-DCAA


R.T.: 5.279 min
Delta R.T.: 0.003 min
Response: 411996272
Conc: 414.20 ng/ml

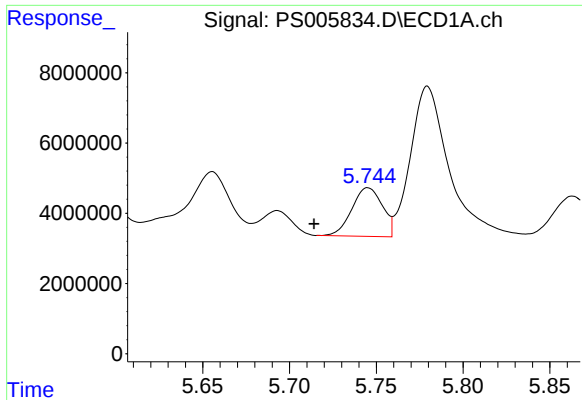

#5 DICAMBA


R.T.: 5.745 min
Delta R.T.: 0.031 min
Response: 16976955
Conc: 2.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-073019

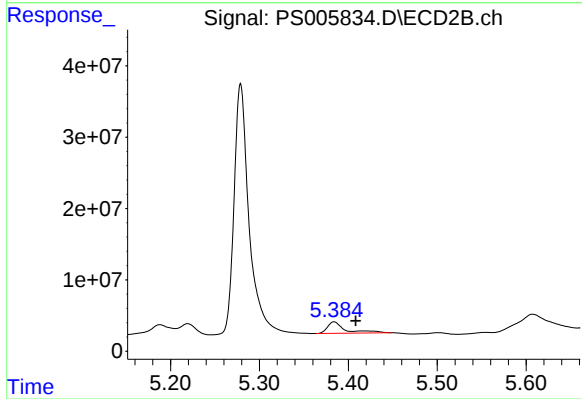


#5 DICAMBA

R.T.: 5.384 min
Delta R.T.: -0.024 min
Response: 22920574
Conc: 6.14 ng/ml

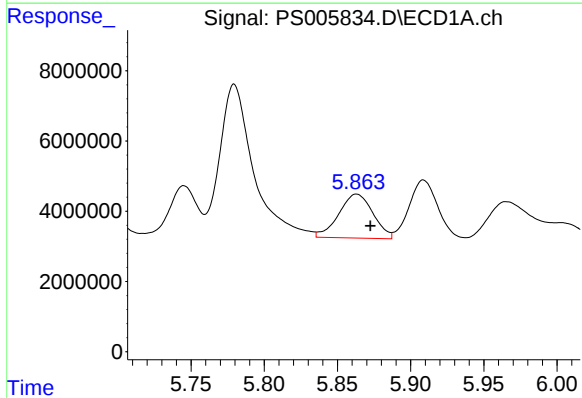


#6 MCP

R.T.: 5.863 min
Delta R.T.: -0.009 min
Response: 20367516
Conc: 4.40 ug/ml

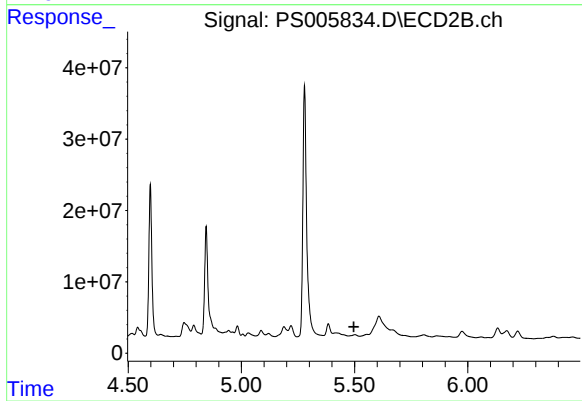

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

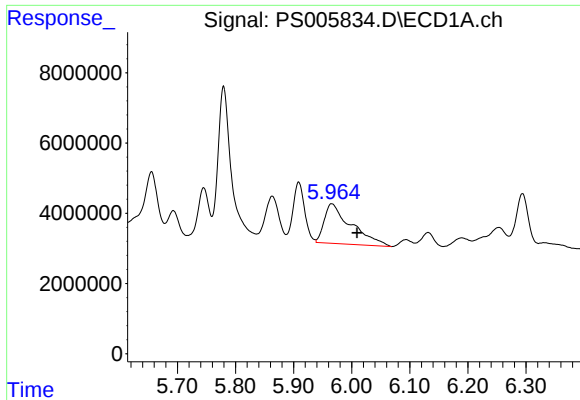

#7 MCPA


R.T.: 5.966 min
Delta R.T.: -0.043 min
Response: 36382623
Conc: 5.58 ug/ml

Instrument :
ECD_S
ClientSampleId :
HD-01-073019

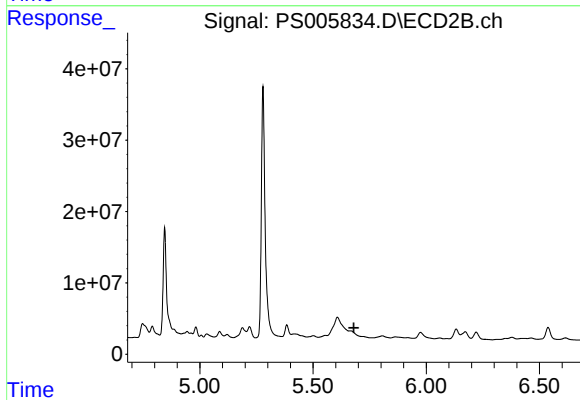


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.681 min
Response: 0
Conc: N.D.

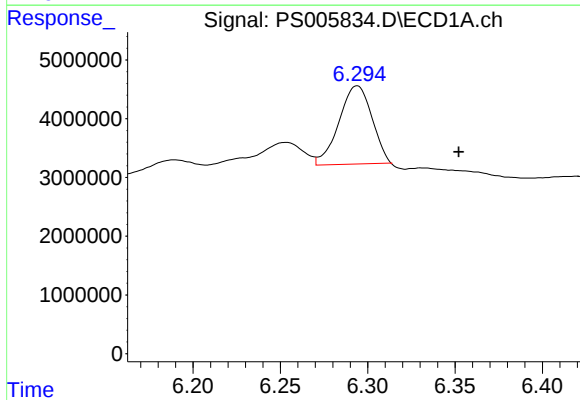


#8 DICHLORPROP

R.T.: 6.294 min
Delta R.T.: -0.058 min
Response: 17228959
Conc: 11.98 ng/ml

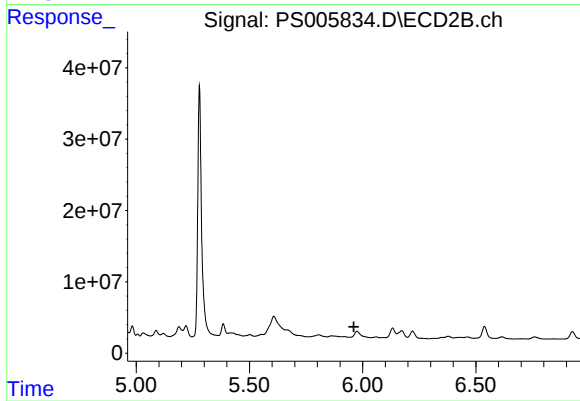

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 5.961 min
Response: 0
Conc: N.D.

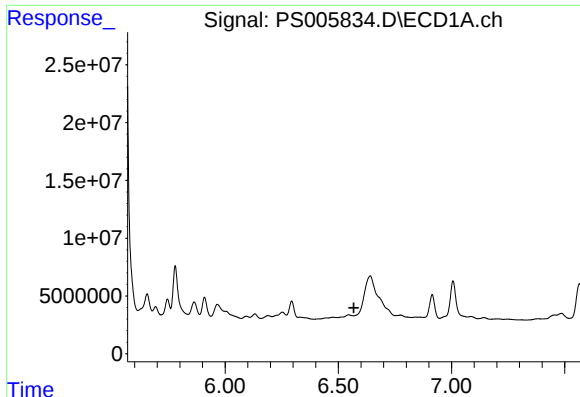

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HD-01-073019

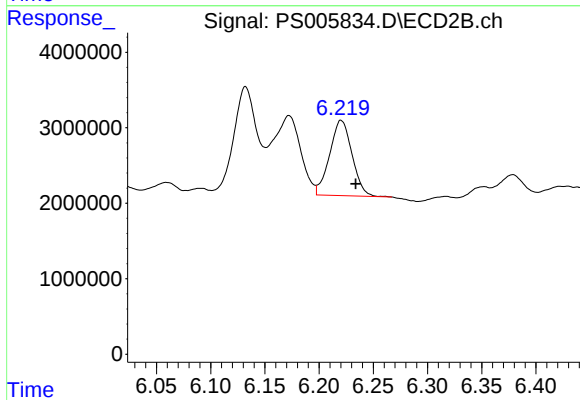


#9 2,4-D

R.T.: 6.220 min
Delta R.T.: -0.013 min
Response: 14347170
Conc: 13.35 ng/ml

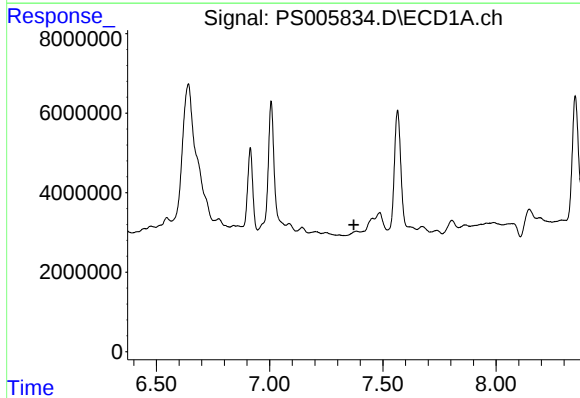

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

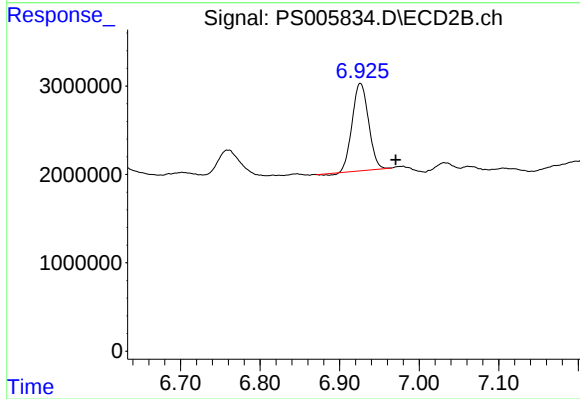

#11 2,4,5-TP (SILVEX)

R.T.: 6.926 min
Delta R.T.: -0.045 min
Response: 14054428
Conc: 2.71 ng/ml