

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
 Data File : PS005837.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2019 19:20
 Operator : SM\AJ
 Sample : K4066-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:16:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.581	5.300	447.5E6	298.1E6	308.453	299.685
Target Compounds							
1) T	Dalapon	2.082	0.000	27219258	0	14.687	N.D. #
2) T	3,5-DICHL...	0.000	4.619	0	89862481	N.D.	69.268
6) T	MCPD	5.803	0.000	28228364	0	6.092	N.D. #
7) T	MCPA	0.000	5.632	0	111.9E6	N.D.	26.576
10) T	Pentachlo...	0.000	6.559	0	26018123	N.D.	2.004
11) T	2,4,5-TP ...	0.000	6.998	0	793.9E6	N.D.	153.040
12) T	2,4,5-T	7.583	0.000	65748578	0	7.877	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
Data File : PS005837.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2019 19:20
Operator : SM\AJ
Sample : K4066-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:16:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

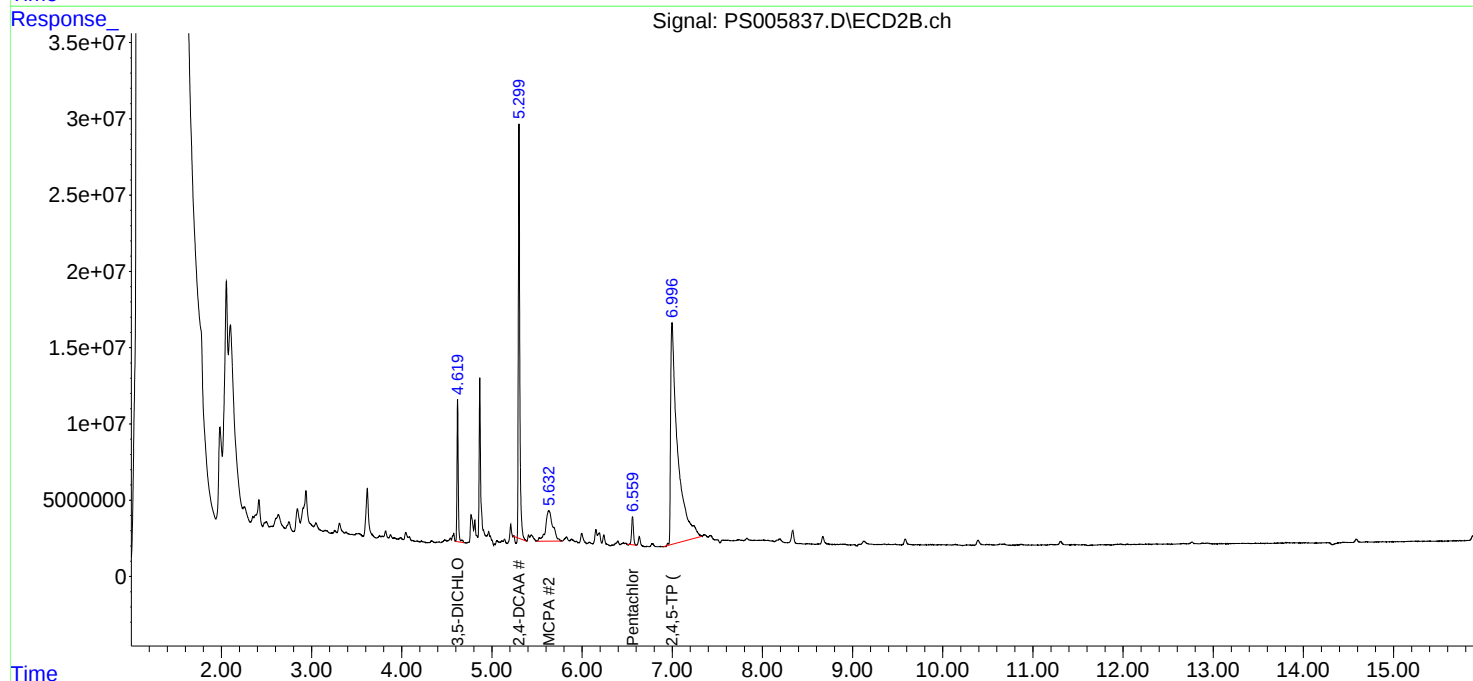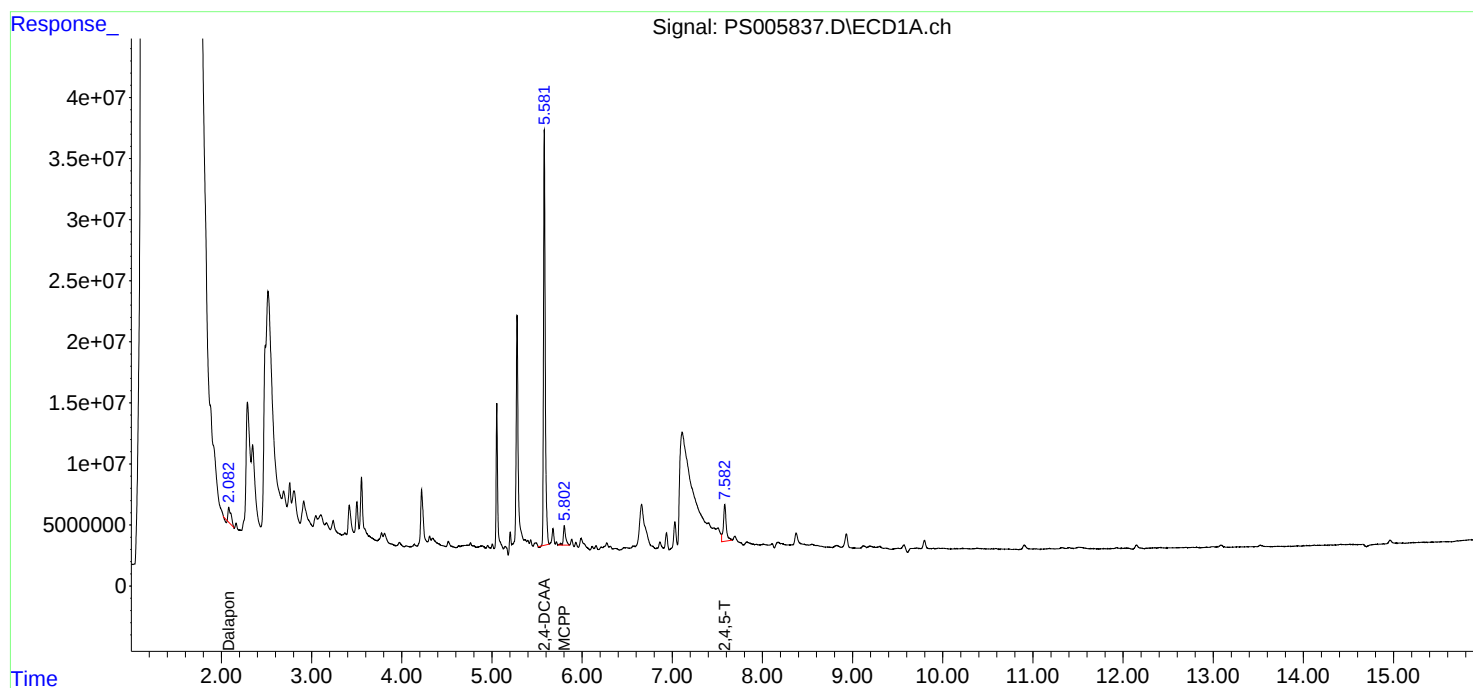


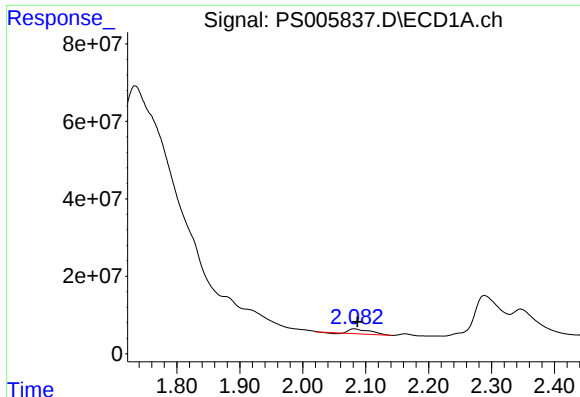

#1 Dalapon


R.T.: 2.082 min
Delta R.T.: -0.005 min
Response: 27219258
Conc: 14.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

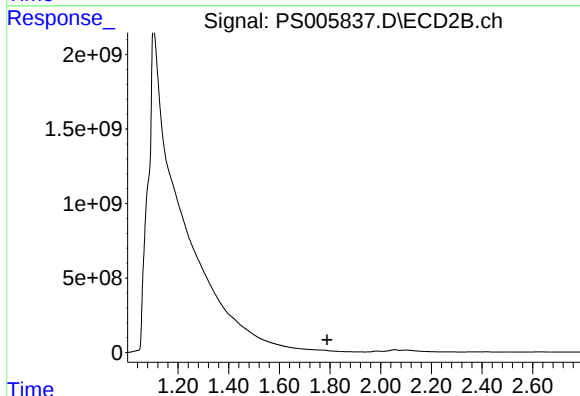


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

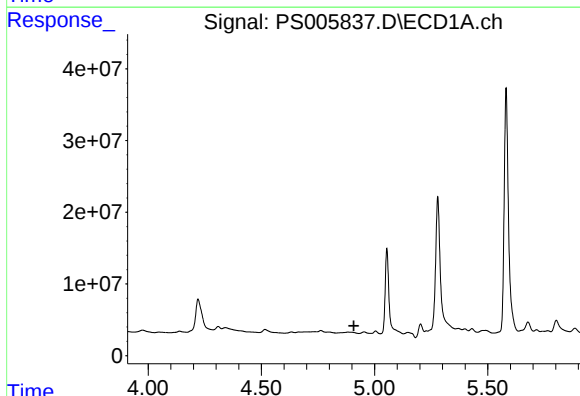


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

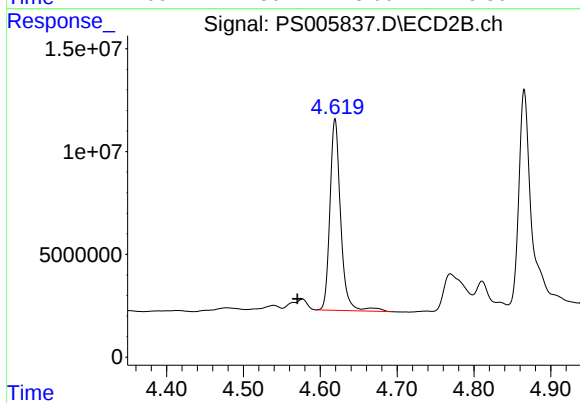

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.619 min
Delta R.T.: 0.049 min
Response: 89862481
Conc: 69.27 ng/ml

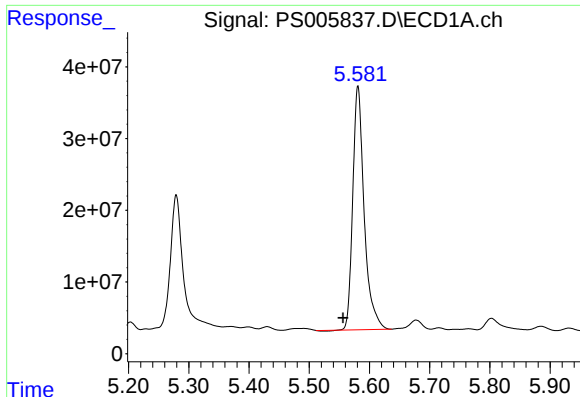

#4 2,4-DCAA


R.T.: 5.581 min
Delta R.T.: 0.025 min
Response: 447509410
Conc: 308.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

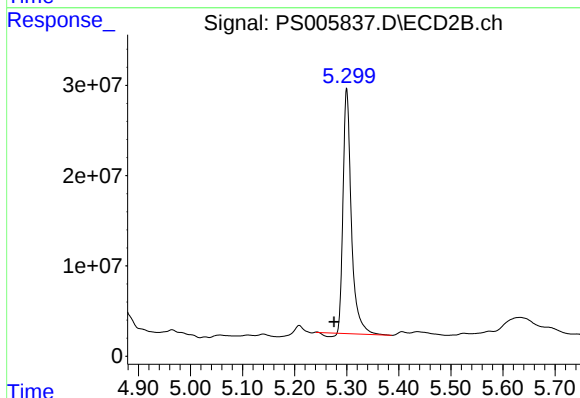


#4 2,4-DCAA

R.T.: 5.300 min
Delta R.T.: 0.024 min
Response: 298089963
Conc: 299.68 ng/ml

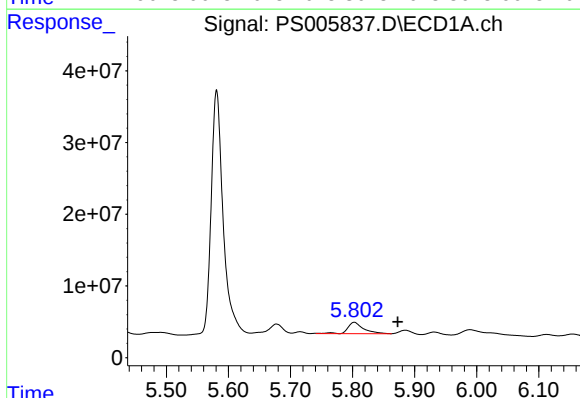


#6 MCP

R.T.: 5.803 min
Delta R.T.: -0.070 min
Response: 28228364
Conc: 6.09 ug/ml

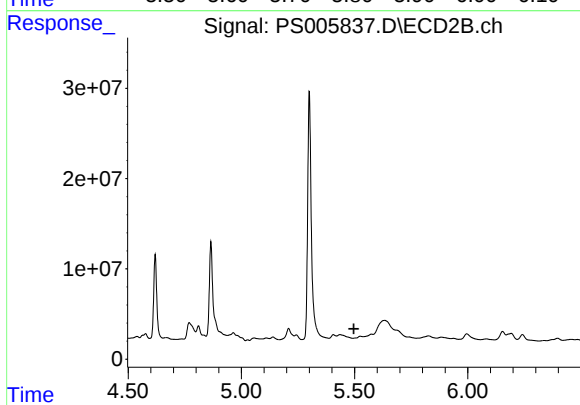

#6 MCP


R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

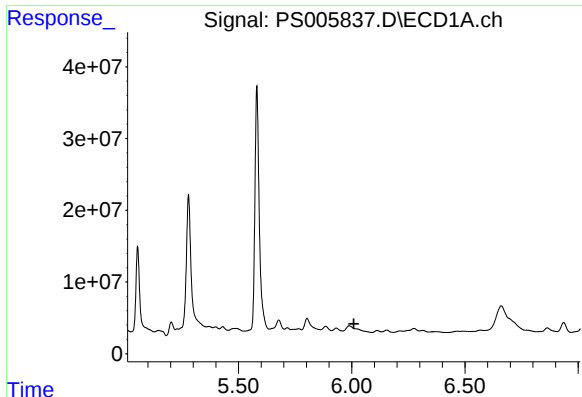

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

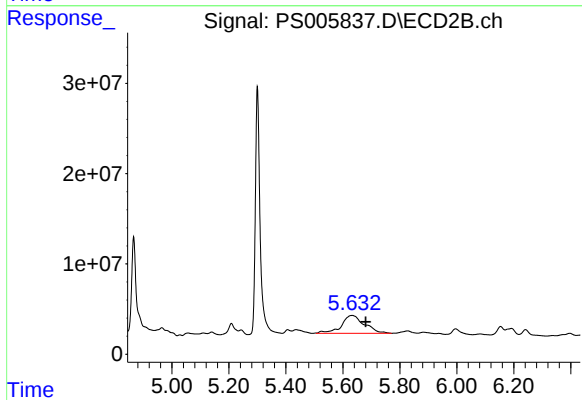


#7 MCPA

R.T.: 5.632 min
Delta R.T.: -0.049 min
Response: 111860822
Conc: 26.58 ug/ml

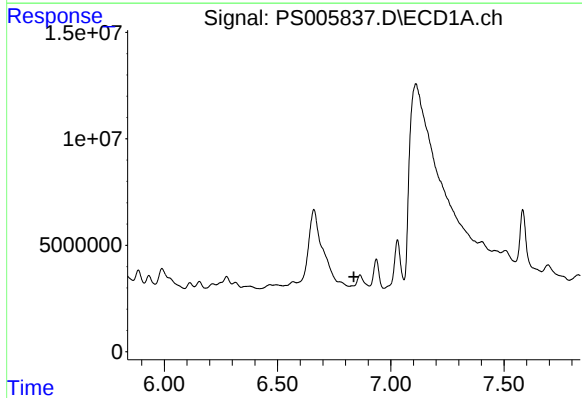


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

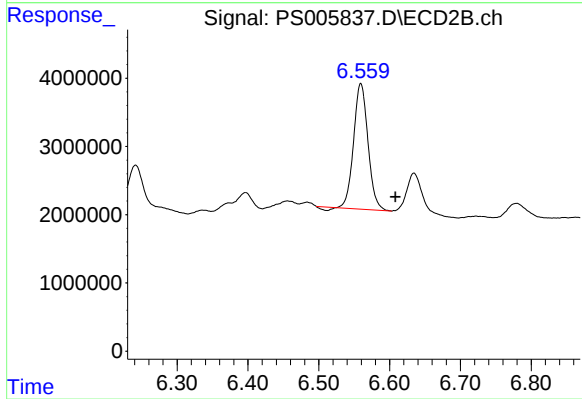

#10 Pentachlorophenol


R.T.: 6.559 min
Delta R.T.: -0.049 min
Response: 26018123
Conc: 2.00 ng/ml

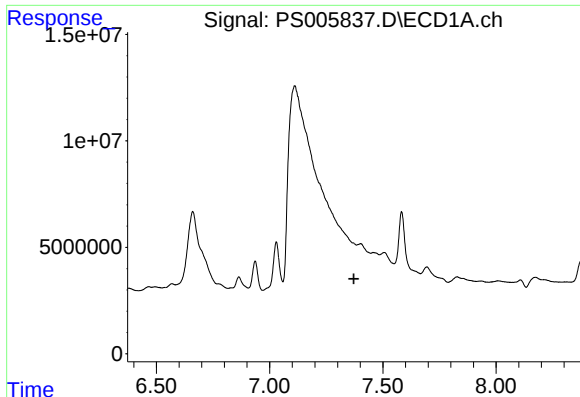

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

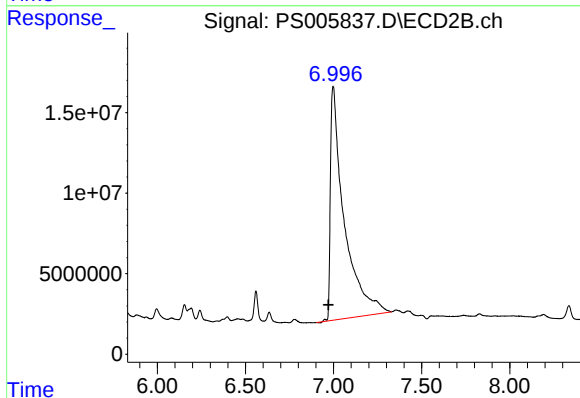


#11 2,4,5-TP (SILVEX)

R.T.: 6.998 min
Delta R.T.: 0.027 min
Response: 793866917
Conc: 153.04 ng/ml

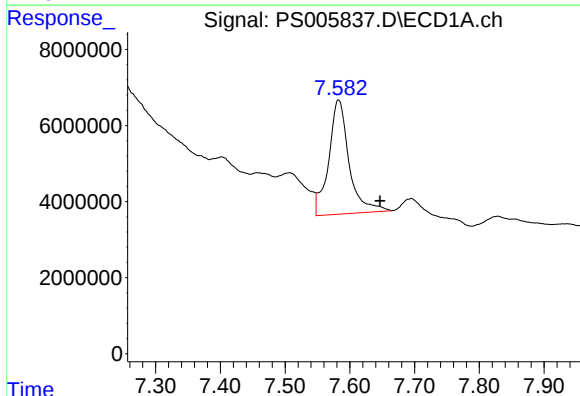

#12 2,4,5-T

R.T.: 7.583 min
Delta R.T.: -0.064 min
Response: 65748578
Conc: 7.88 ng/ml

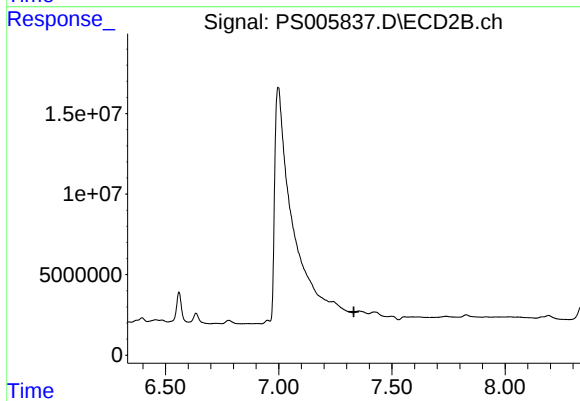

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.