

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080119\
 Data File : PS005838.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2019 19:42
 Operator : SM\AJ
 Sample : K4066-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 02:16:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.559	5.280	587.4E6	399.0E6	404.862	401.120
Target Compounds							
1) T	Dalapon	2.060	0.000	37958401	0	20.481	N.D. #
2) T	3,5-DICHL...	0.000	4.599	0	82477590	N.D.	63.576
5) T	DICAMBA	5.783	0.000	26553160	0	4.446	N.D. #
7) T	MCPA	5.968	5.611	45998151	104.7E6	7.049	24.875 #
8) T	DICHLORPROP	0.000	5.975	0	21112448	N.D.	22.861
10) T	Pentachlo...	0.000	6.539	0	26319937	N.D.	2.027
11) T	2,4,5-TP ...	0.000	7.027	0	112.1E6	N.D.	21.609



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS005838.D
Data File : PS005838.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2019 19:42
Operator : SM\AJ
Sample : K4066-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 02:16:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

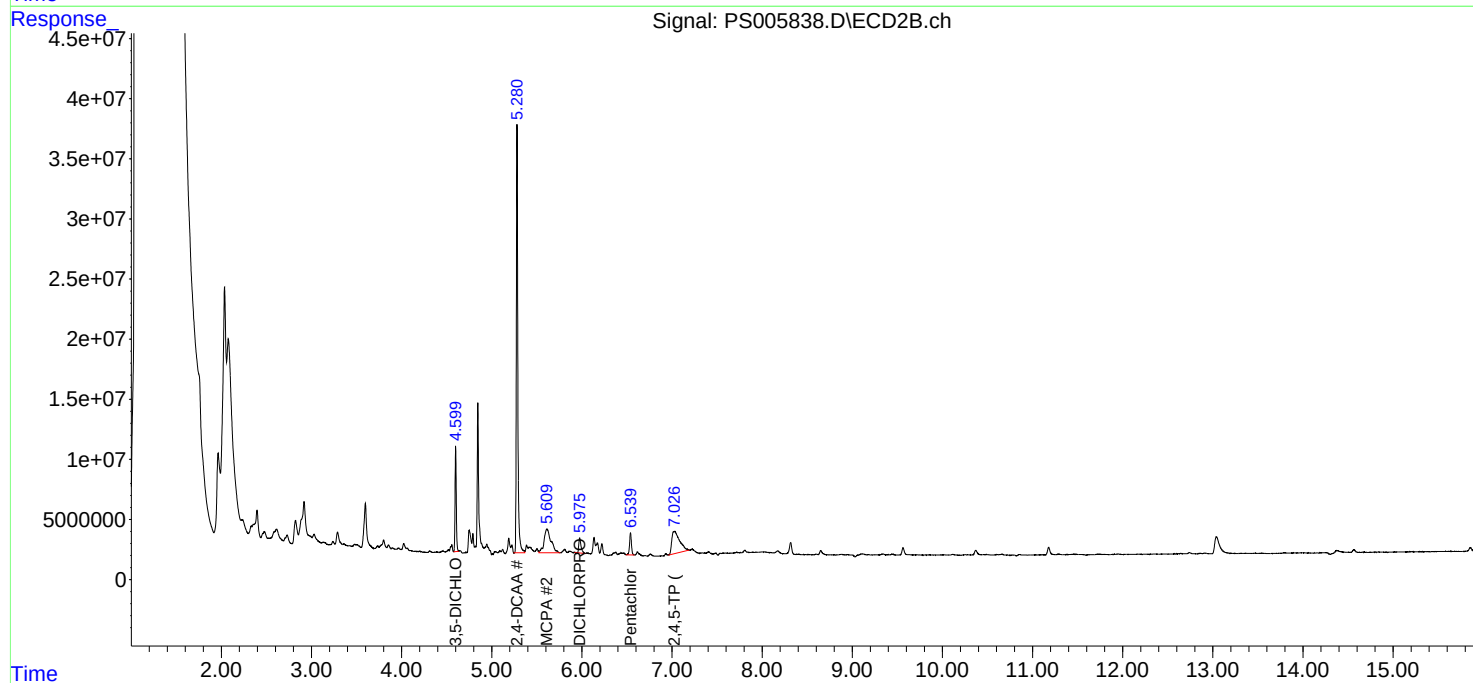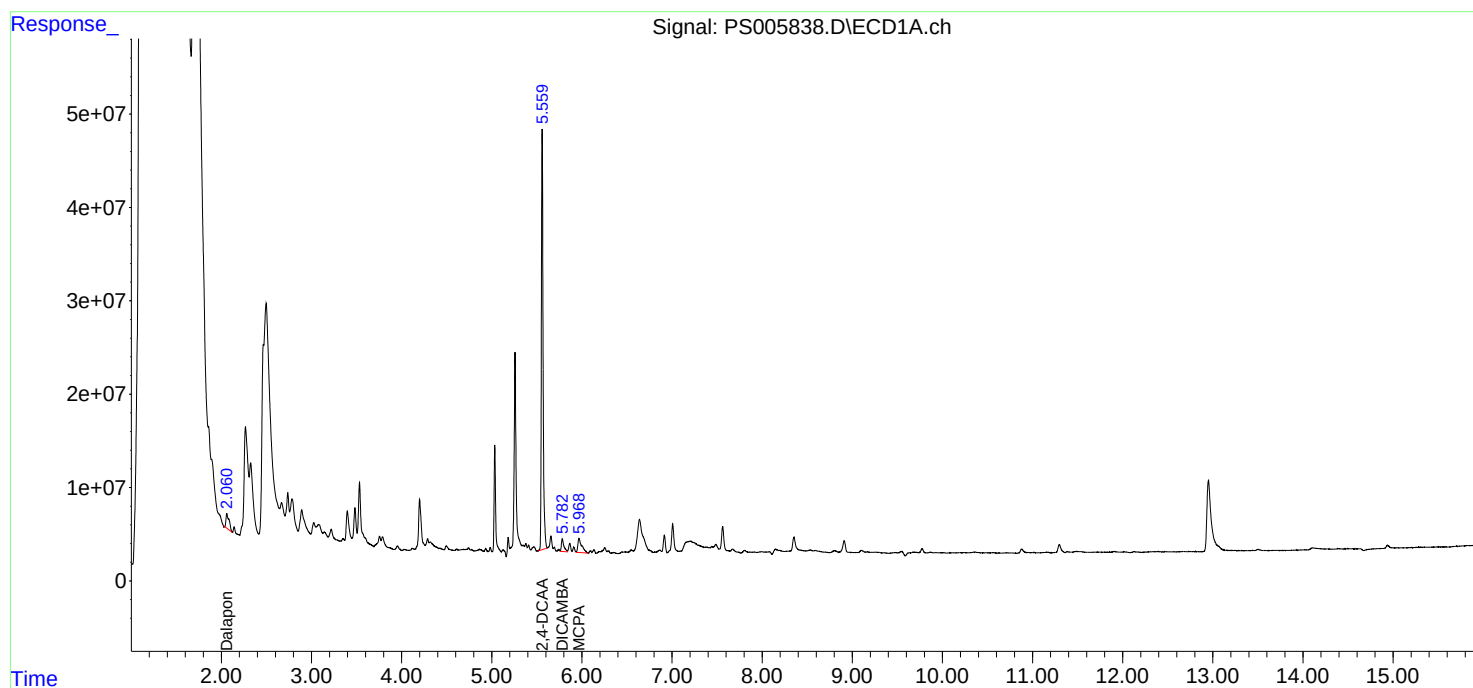


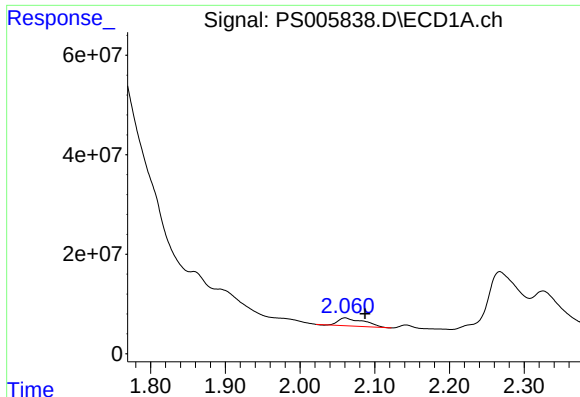

#1 Dalapon


R.T.: 2.060 min
Delta R.T.: -0.027 min
Response: 37958401
Conc: 20.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

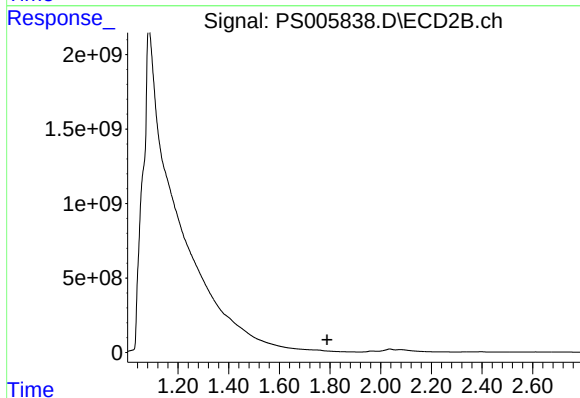


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

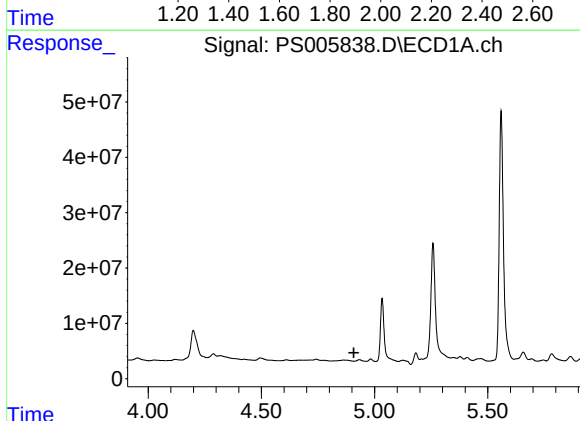


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

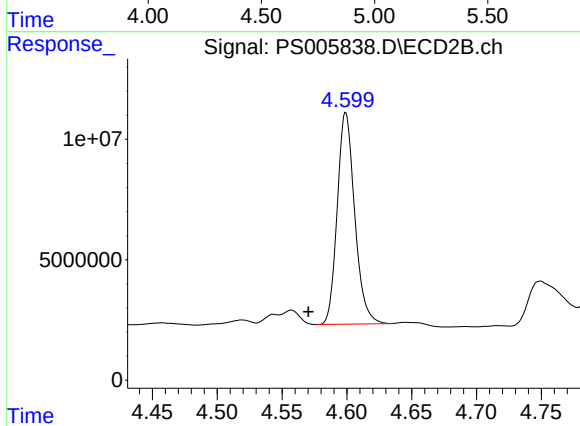

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.599 min
Delta R.T.: 0.029 min
Response: 82477590
Conc: 63.58 ng/ml

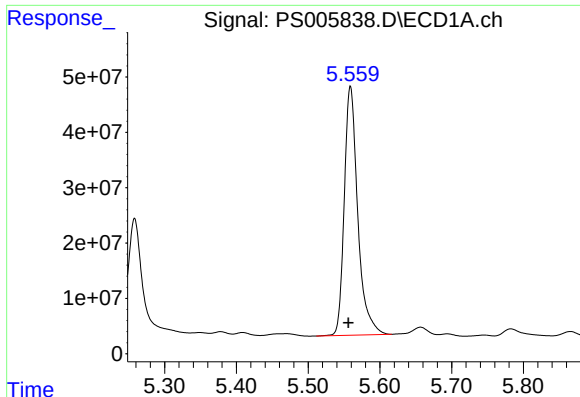

#4 2,4-DCAA


R.T.: 5.559 min
Delta R.T.: 0.003 min
Response: 587380484
Conc: 404.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

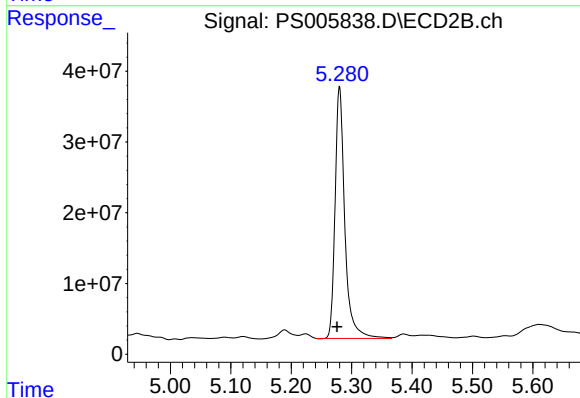


#4 2,4-DCAA

R.T.: 5.280 min
Delta R.T.: 0.004 min
Response: 398985002
Conc: 401.12 ng/ml

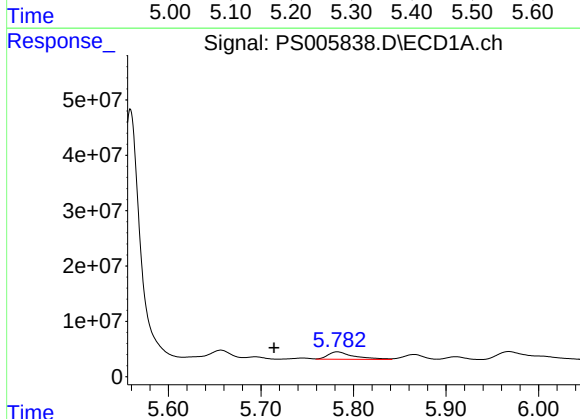


#5 DICAMBA

R.T.: 5.783 min
Delta R.T.: 0.068 min
Response: 26553160
Conc: 4.45 ng/ml

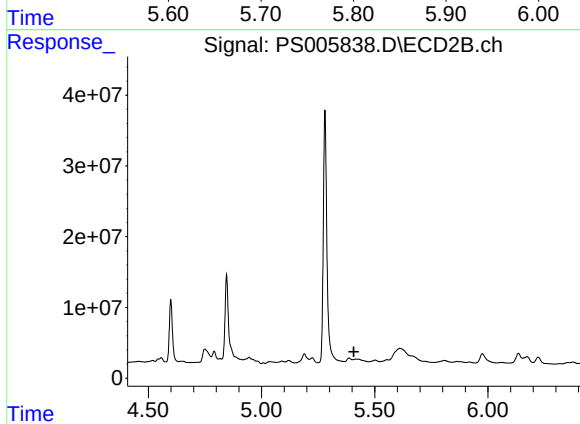

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

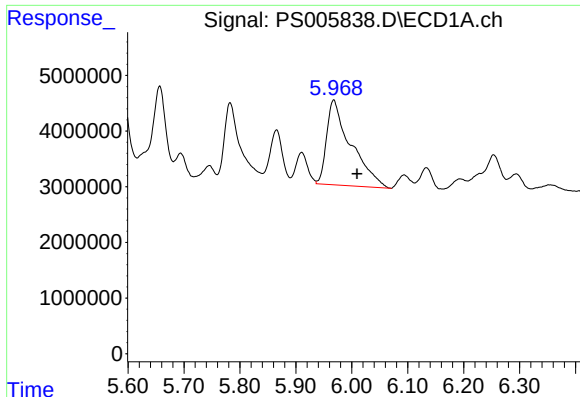

#7 MCPA


R.T.: 5.968 min
Delta R.T.: -0.042 min
Response: 45998151
Conc: 7.05 ug/ml

Instrument :
ECD_S
ClientSampleId :

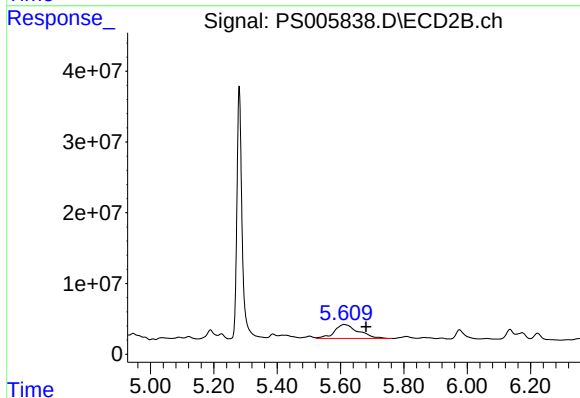


#7 MCPA

R.T.: 5.611 min
Delta R.T.: -0.070 min
Response: 104697854
Conc: 24.87 ug/ml

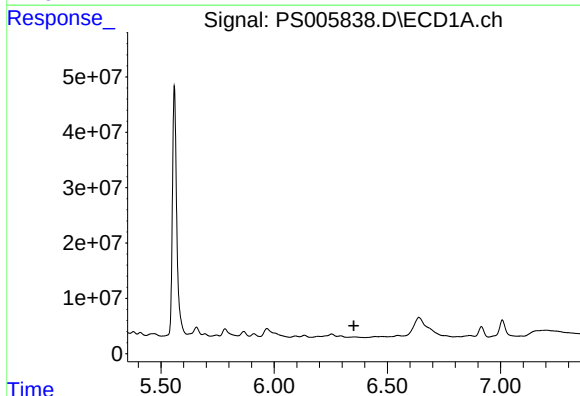


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.352 min
Response: 0
Conc: N.D.

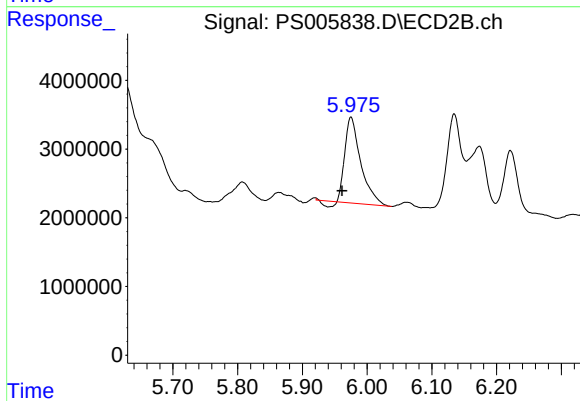

#8 DICHLORPROP


R.T.: 5.975 min
Delta R.T.: 0.014 min
Response: 21112448
Conc: 22.86 ng/ml

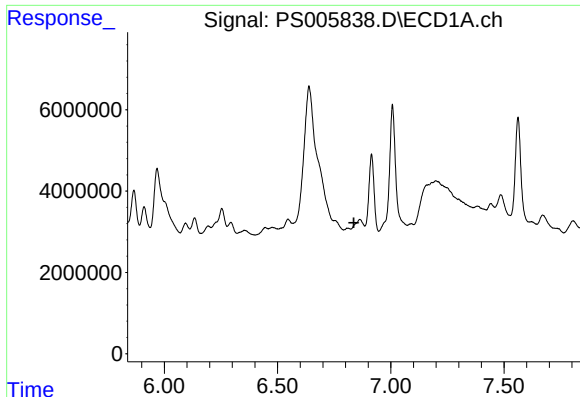

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

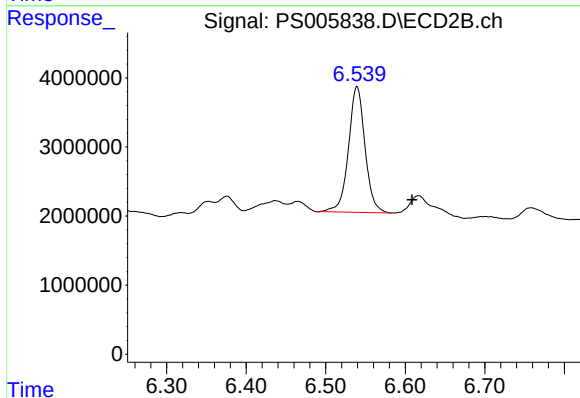


#10 Pentachlorophenol

R.T.: 6.539 min
Delta R.T.: -0.069 min
Response: 26319937
Conc: 2.03 ng/ml

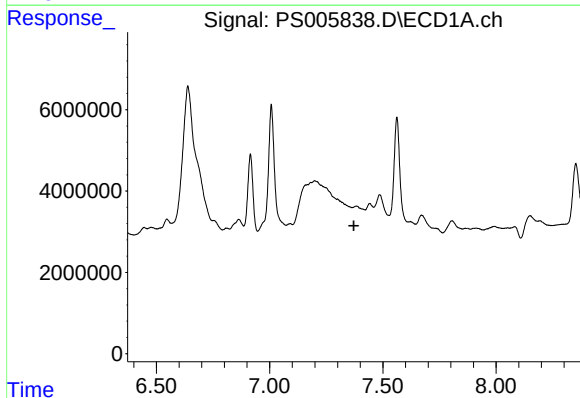

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

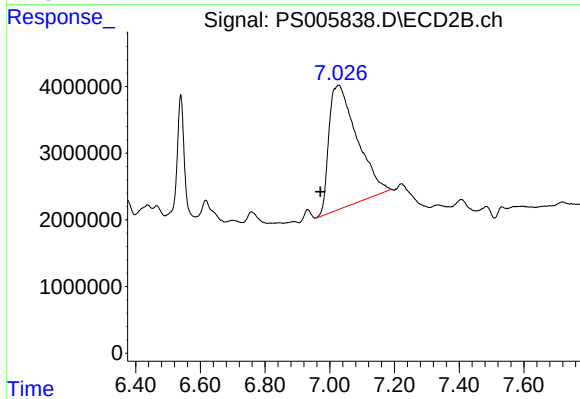

#11 2,4,5-TP (SILVEX)

R.T.: 7.027 min
Delta R.T.: 0.057 min
Response: 112094092
Conc: 21.61 ng/ml