

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080122\
 Data File : PS020116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2022 09:58
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:31:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072022.M
 Quant Title : 8080.M
 QLast Update : Wed Jul 20 17:52:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.192	6.776	1220.6E6	372.6E6	368.102	413.566
Target Compounds							
1) T	Dalapon	3.043	0.000	1755536	0	<MDL	N.D. #
7) T	MCPA	7.649f	0.000	1426765	0	<MDL	N.D. #
9) T	2,4-D	0.000	7.836	0	373451	N.D.	<MDL
11) T	2,4,5-TP ...	9.170	0.000	1021483	0	<MDL	N.D. #
12) T	2,4,5-T	9.434	0.000	6405460	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.572f	0	701448	N.D.	<MDL
14) T	DINOSEB	0.000	9.848	0	638243	N.D.	<MDL
15) T	Picloram	0.000	10.883f	0	8283846	N.D.	1.078
16) T	DCPA	11.412	0.000	446049	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080122\
Data File : PS020116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2022 09:58
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 01:31:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072022.M
Quant Title : 8080.M
QLast Update : Wed Jul 20 17:52:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

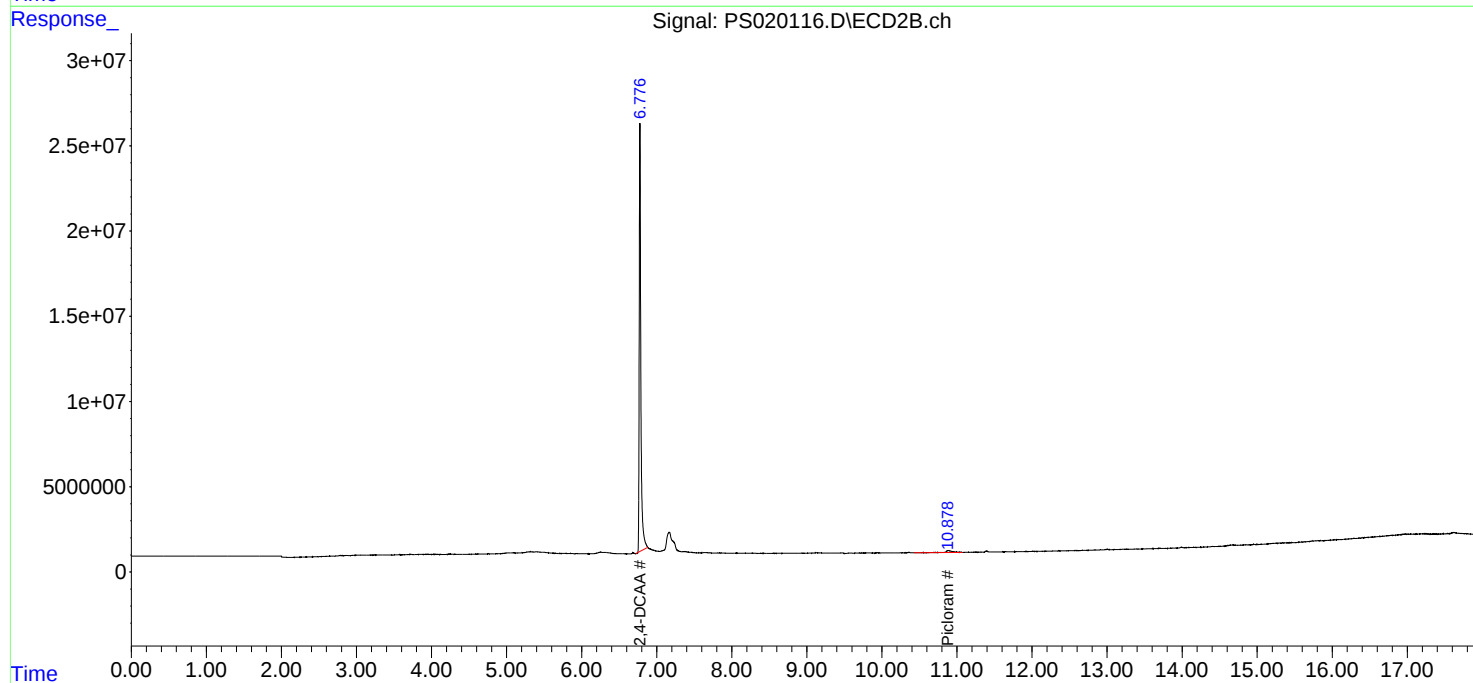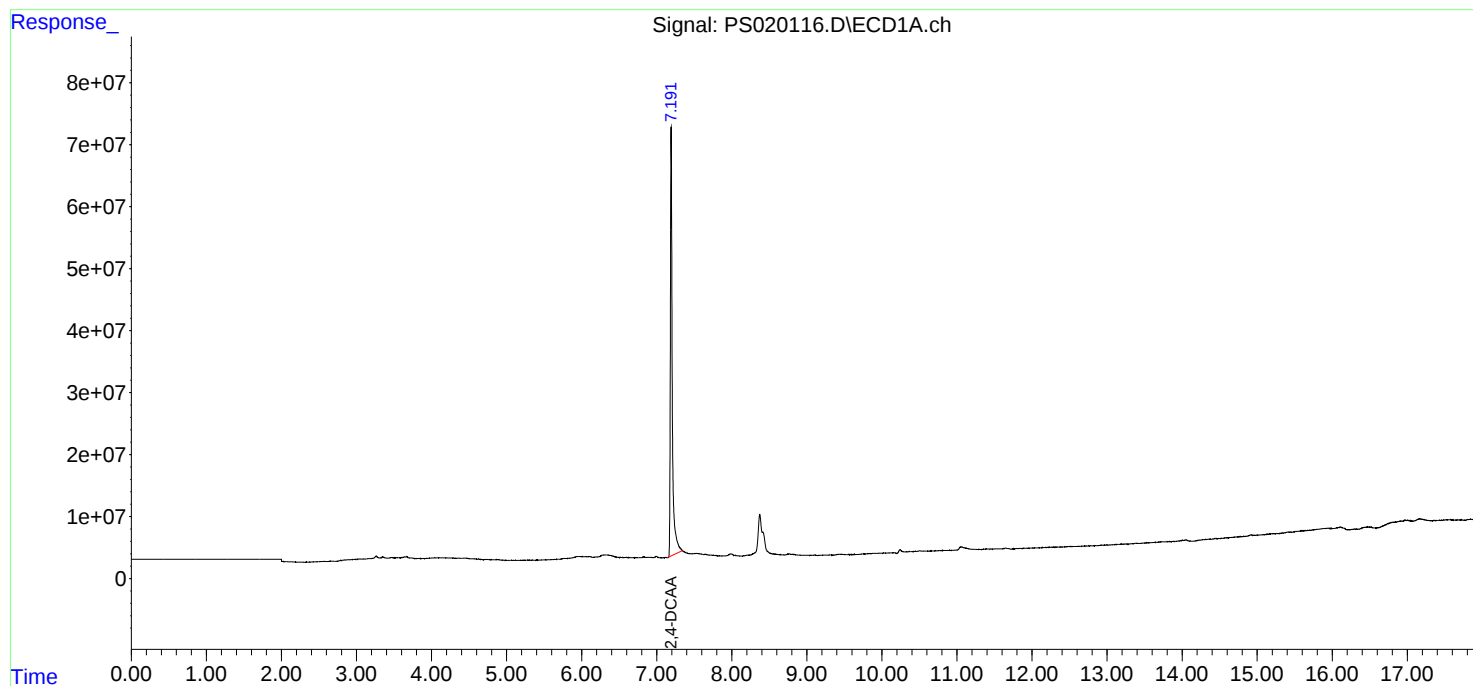


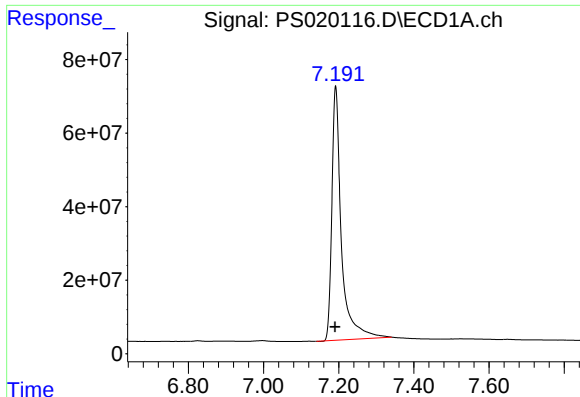

#4 2,4-DCAA


R.T.: 7.192 min
Delta R.T.: 0.001 min
Response: 1220569519
Conc: 368.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

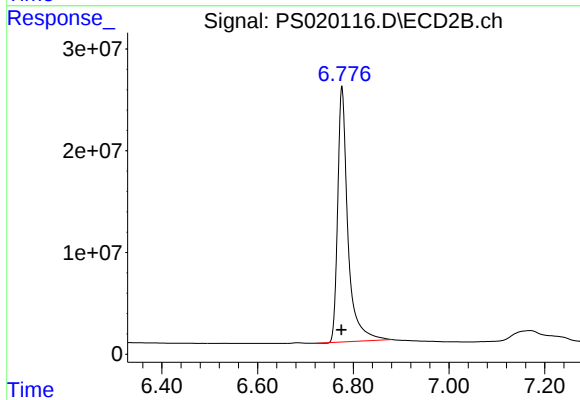


#4 2,4-DCAA

R.T.: 6.776 min
Delta R.T.: 0.000 min
Response: 372583250
Conc: 413.57 ng/ml

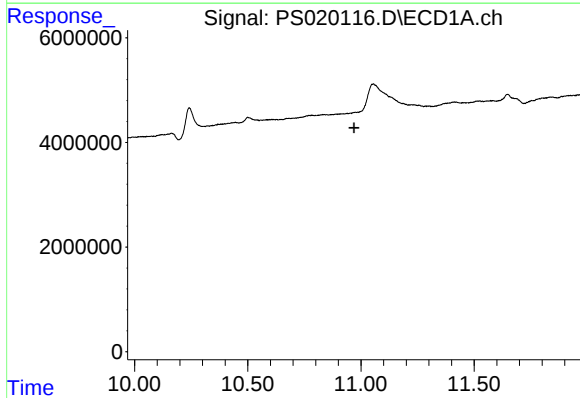

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.969 min
Response: 0
Conc: N.D.

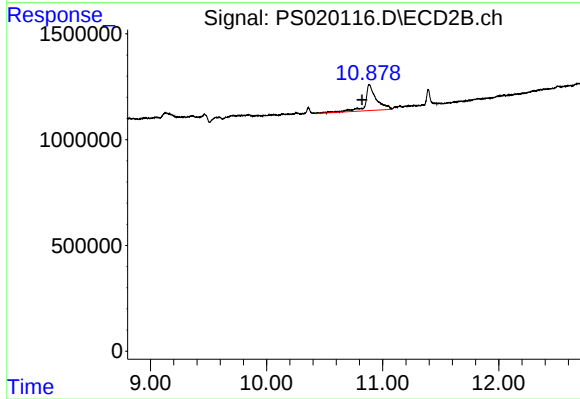

#15 Picloram

R.T.: 10.883 min
Delta R.T.: 0.058 min
Response: 8283846
Conc: 1.08 ng/ml