

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080122\
 Data File : PS020129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2022 15:13
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:35:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072022.M
 Quant Title : 8080.M
 QLast Update : Wed Jul 20 17:52:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.192	6.778	1192.0E6	378.1E6	359.478	419.679
Target Compounds							
1) T	Dalapon	2.982	0.000	220584	0	<MDL	N.D. #
7) T	MCPA	7.721	0.000	543180	0	<MDL	N.D. #
9) T	2,4-D	0.000	7.838	0	381976	N.D.	<MDL
10) T	Pentachlo...	0.000	8.277	0	972741	N.D.	<MDL
11) T	2,4,5-TP ...	9.096f	8.620	1883893	299864	<MDL	<MDL #
12) T	2,4,5-T	9.446	9.053	2769808	182078	<MDL	<MDL #
13) T	2,4-DB	0.000	9.466f	0	2232976	N.D.	3.128
14) T	DINOSEB	11.149	9.850	6109536	256048	<MDL	<MDL #
15) T	Picloram	10.975	10.777f	5294421	470734	<MDL	<MDL #
16) T	DCPA	11.418	10.777	-120894	470734	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080122\
Data File : PS020129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2022 15:13
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 01:35:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072022.M
Quant Title : 8080.M
QLast Update : Wed Jul 20 17:52:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

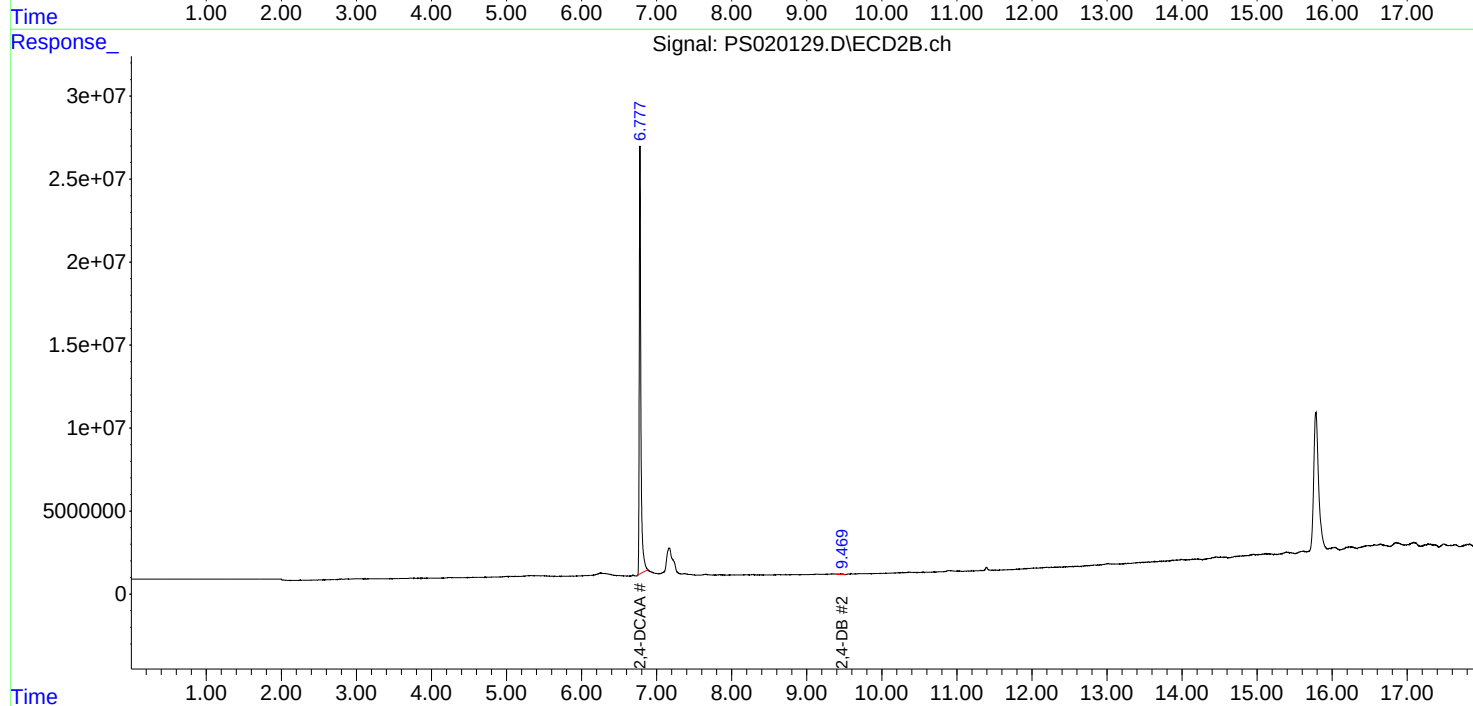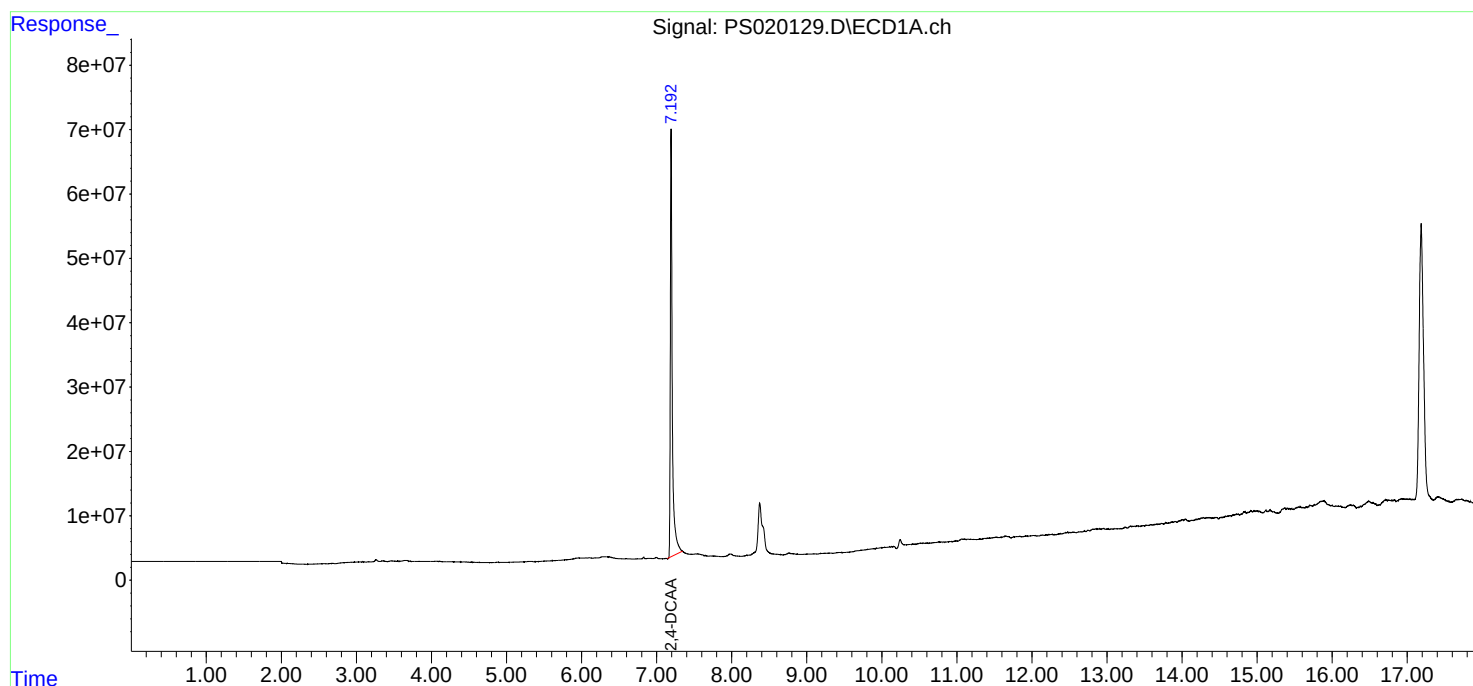


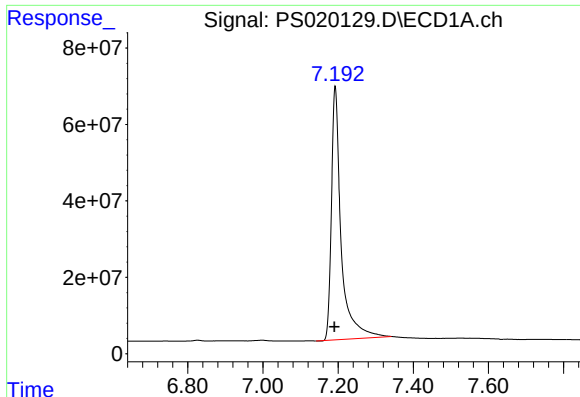

#4 2,4-DCAA


R.T.: 7.192 min
Delta R.T.: 0.002 min
Response: 1191972909
Conc: 359.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

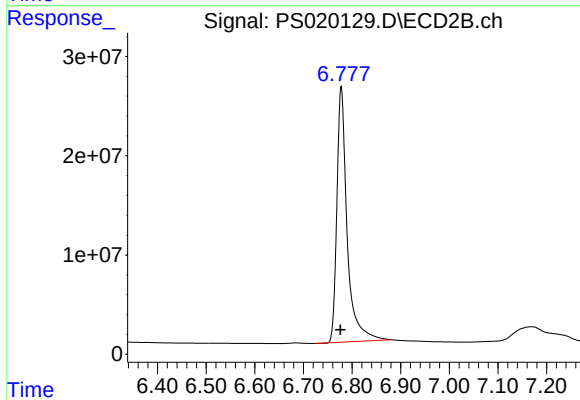


#4 2,4-DCAA

R.T.: 6.778 min
Delta R.T.: 0.002 min
Response: 378090181
Conc: 419.68 ng/ml

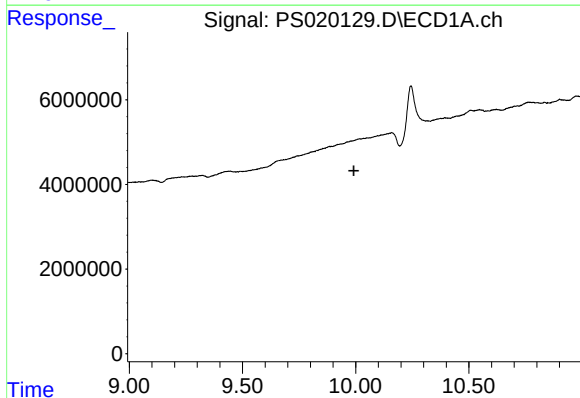

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.992 min
Response: 0
Conc: N.D.

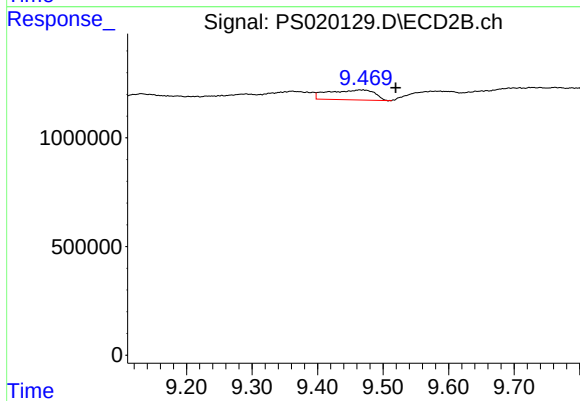

#13 2,4-DB

R.T.: 9.466 min
Delta R.T.: -0.054 min
Response: 2232976
Conc: 3.13 ng/ml