

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080124\
 Data File : PS027259.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2024 08:59
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 03:28:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.193	7.750	1269.6E6	1152.7E6	502.078	497.112
Target Compounds							
1) T	Dalapon	0.000	2.739f	0	112026	N.D.	<MDL
2) T	3,5-DICHL...	6.349f	0.000	1489072	0	<MDL	N.D. #
3) T	4-Nitroph...	6.986	7.249f	9599003	1114841	5.988	<MDL #
5) T	DICAMBA	0.000	7.942	0	6355851	N.D.	<MDL
6) T	MCPD	7.610f	8.056	8414394	506432	1.096	<MDL #
7) T	MCPA	0.000	8.277	0	3491501	N.D.	<MDL
8) T	DICHLORPROP	8.093	8.654	371739	773484	<MDL	<MDL #
9) T	2,4-D	0.000	9.032f	0	171414	N.D.	<MDL
10) T	Pentachlo...	8.623	0.000	1586026	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.887	0	769645	N.D.	<MDL
12) T	2,4,5-T	0.000	10.314	0	2708238	N.D.	<MDL
13) T	2,4-DB	10.026	0.000	5142283	0	2.380	N.D. #
15) T	Picloram	11.045	12.355	95209357	18619629	4.888	<MDL #
16) T	DCPA	0.000	12.257f	0	6457811	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080124\
Data File : PS027259.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2024 08:59
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 03:28:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
Quant Title : 8080.M
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

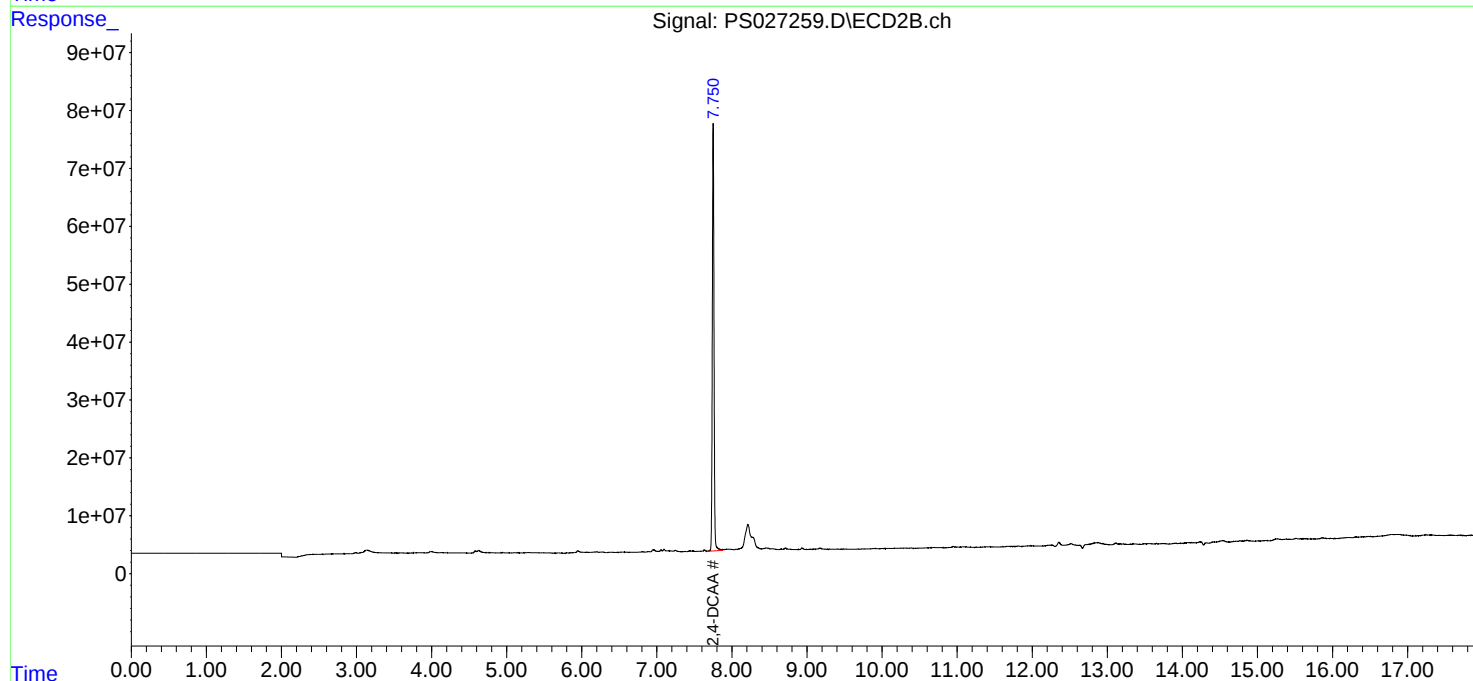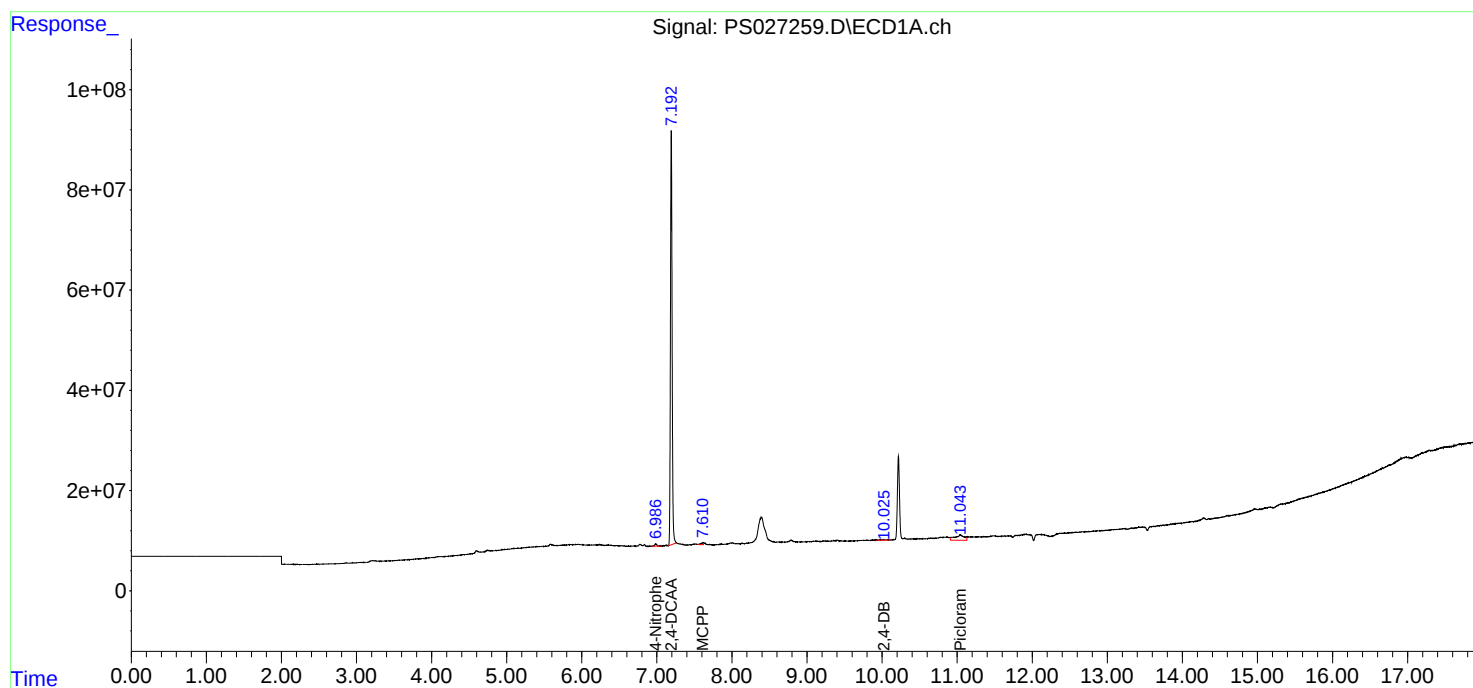


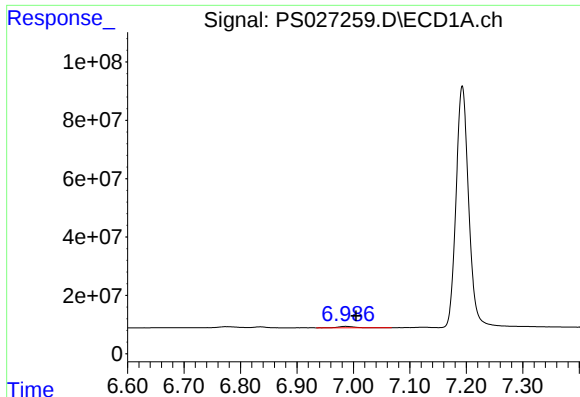

#3 4-Nitrophenol


R.T.: 6.986 min
Delta R.T.: -0.019 min
Response: 9599003
Conc: 5.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

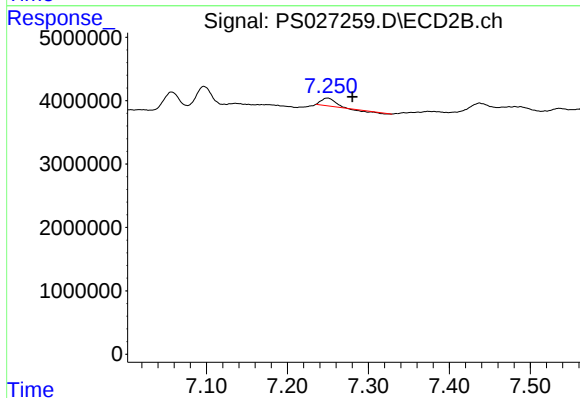


#3 4-Nitrophenol

R.T.: 7.249 min
Delta R.T.: -0.031 min
Response: 1114841
Conc: N.D.

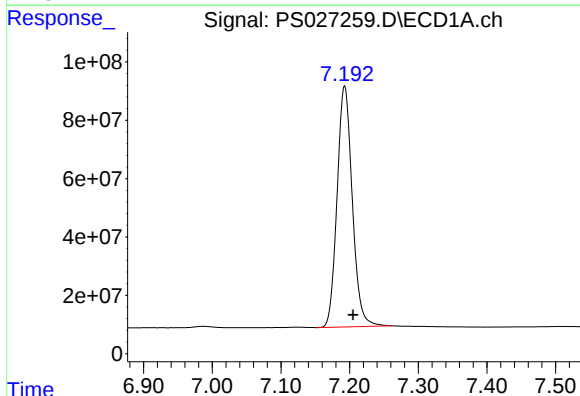


#4 2,4-DCAA

R.T.: 7.193 min
Delta R.T.: -0.012 min
Response: 1269635862
Conc: 502.08 ng/ml

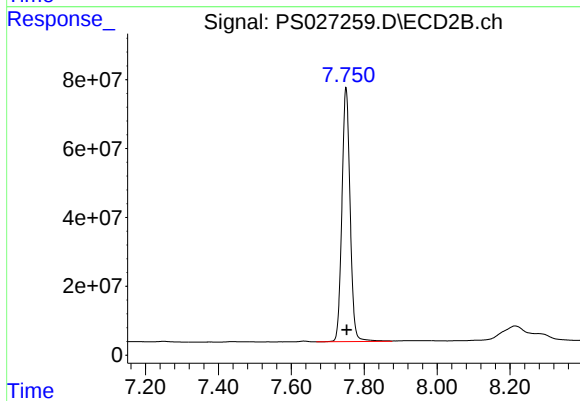

#4 2,4-DCAA


R.T.: 7.750 min
Delta R.T.: -0.002 min
Response: 1152665981
Conc: 497.11 ng/ml

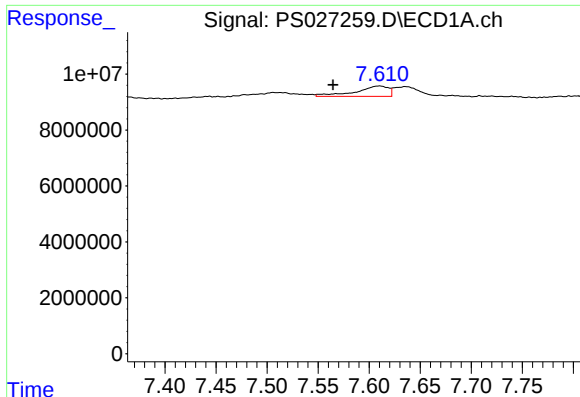

#6 MCPP


R.T.: 7.610 min
Delta R.T.: 0.045 min
Response: 8414394
Conc: 1.10 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

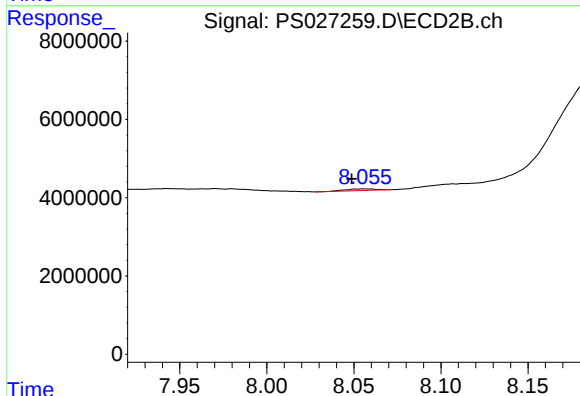


#6 MCPP

R.T.: 8.056 min
Delta R.T.: 0.007 min
Response: 506432
Conc: N.D.

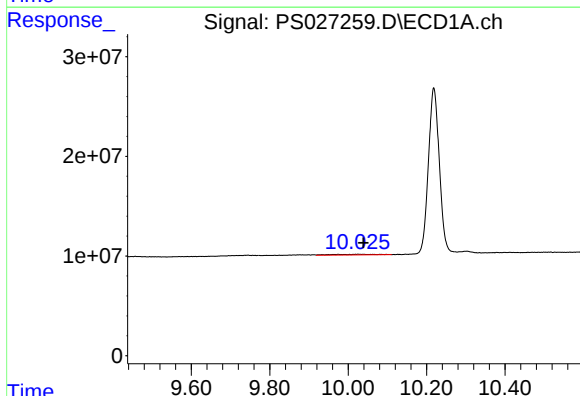


#13 2,4-DB

R.T.: 10.026 min
Delta R.T.: -0.013 min
Response: 5142283
Conc: 2.38 ng/ml

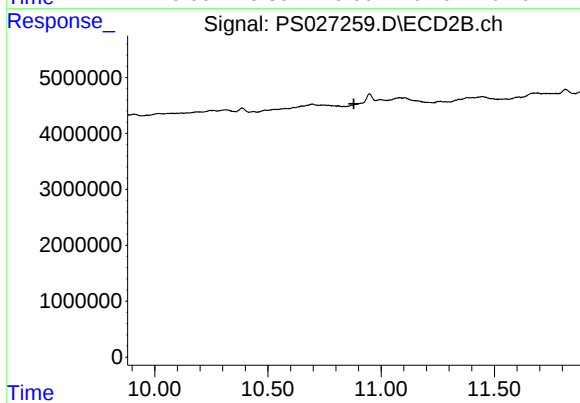

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.880 min
Response: 0
Conc: N.D.

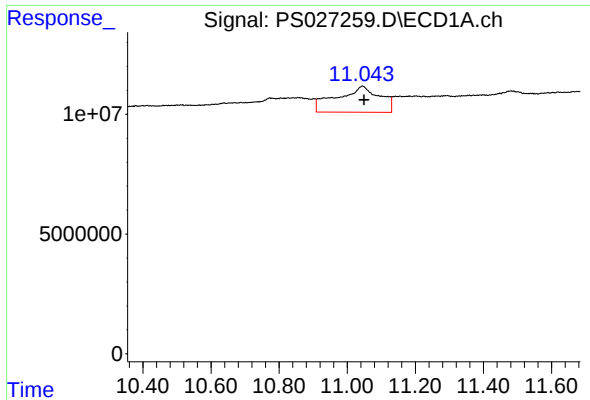

#15 Picloram

R.T.: 11.045 min
Delta R.T.: -0.005 min
Response: 95209357
Conc: 4.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

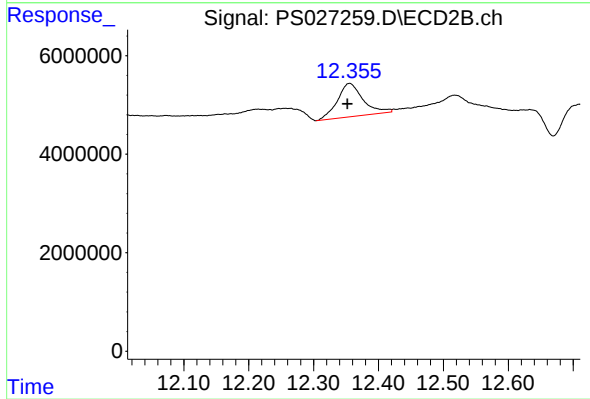

#15 Picloram

R.T.: 12.355 min
Delta R.T.: 0.003 min
Response: 18619629
Conc: N.D.