

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080124\
 Data File : PS027276.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2024 18:57
 Operator : AR\AJ
 Sample : P3402-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 355

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 03:34:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	7.763	1046944	1162418	<MDL	<MDL #
Target Compounds							
1) T	Dalapon	0.000	2.678	0	58437	N.D.	<MDL
5) T	DICAMBA	0.000	7.948	0	4291176	N.D.	<MDL
6) T	MCPD	7.613f	8.038	25279690	46442	3.293	<MDL #
7) T	MCPA	7.725	8.278	241437	20668444	<MDL	1.974 #
8) T	DICHLORPROP	0.000	8.669	0	184192	N.D.	<MDL
10) T	Pentachlo...	0.000	9.553f	0	301660	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	9.911	0	2740495	N.D.	<MDL
12) T	2,4,5-T	9.448	0.000	739073	0	<MDL	N.D. #
13) T	2,4-DB	10.021	10.857	8960039	781769	4.146	<MDL #
14) T	DINOSEB	11.222	11.254	4206723	3600933	<MDL	<MDL #
15) T	Picloram	11.014f	12.357	5521028	335229	<MDL	<MDL #
16) T	DCPA	11.545	12.301	5307601	11828294	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080124\
Data File : PS027276.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2024 18:57
Operator : AR\AJ
Sample : P3402-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
355

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 03:34:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
Quant Title : 8080.M
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

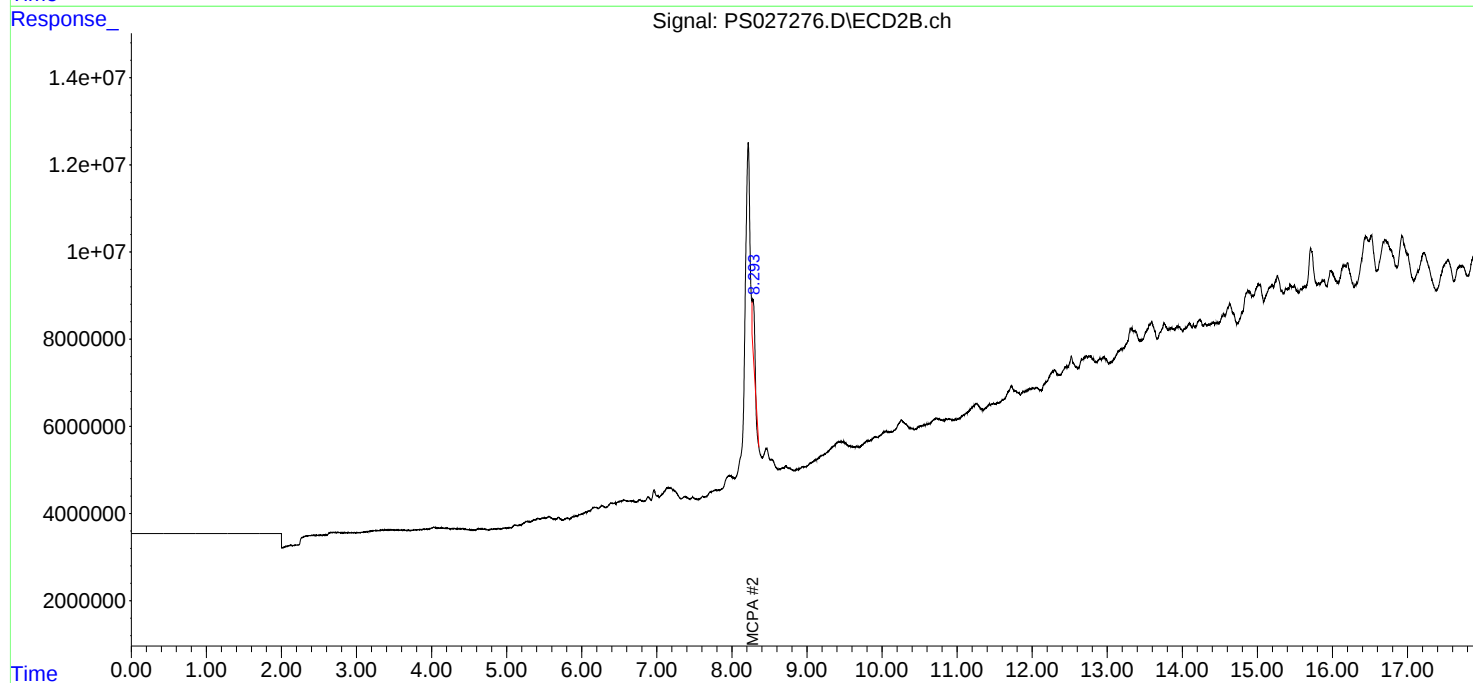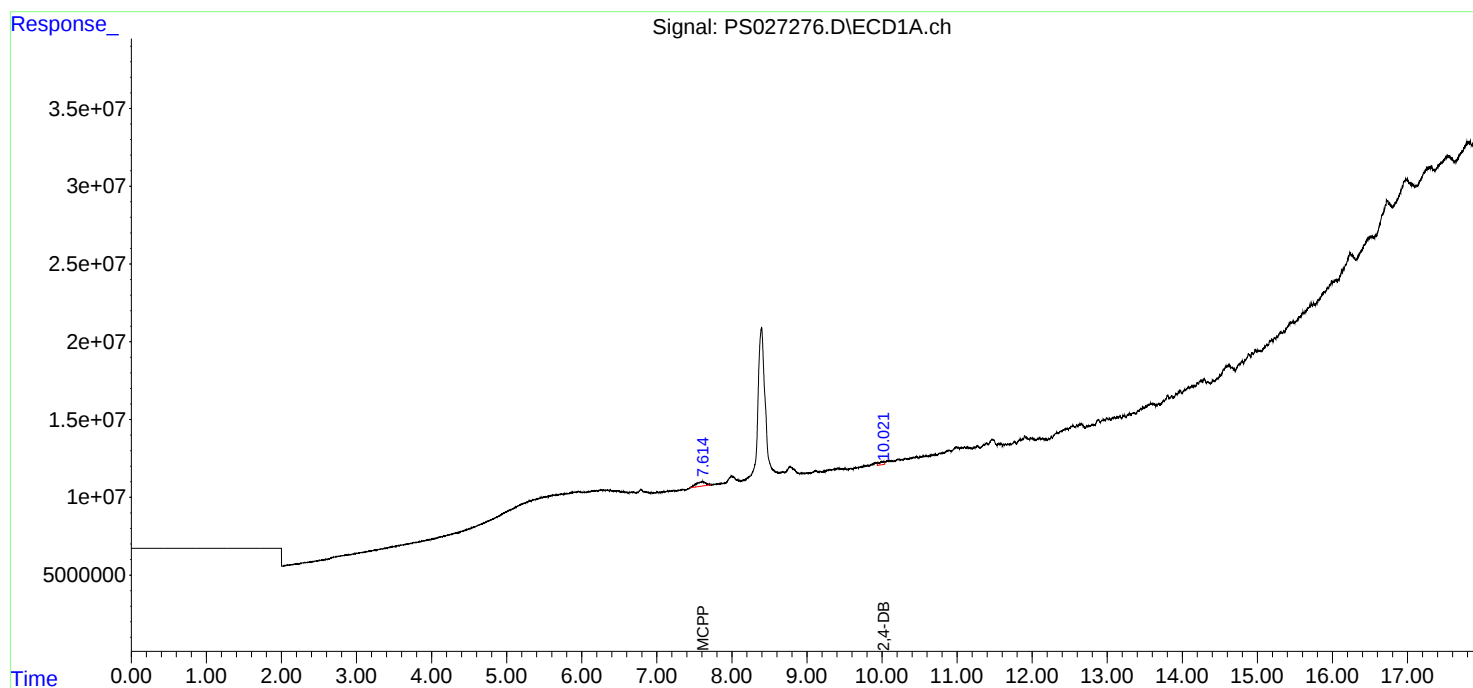


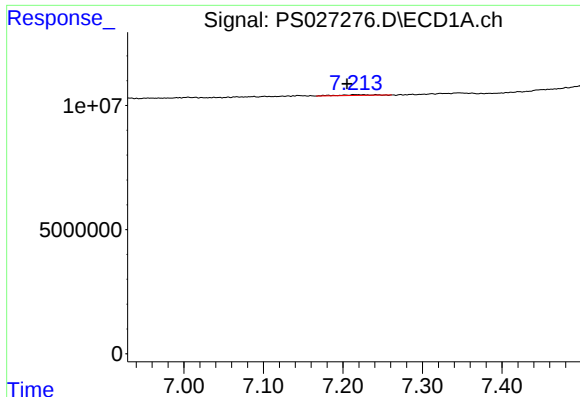

#4 2,4-DCAA


R.T.: 7.216 min
Delta R.T.: 0.011 min
Response: 1046944
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
355

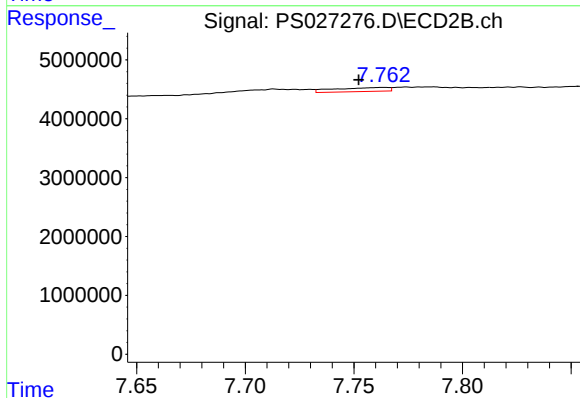


#4 2,4-DCAA

R.T.: 7.763 min
Delta R.T.: 0.011 min
Response: 1162418
Conc: N.D.

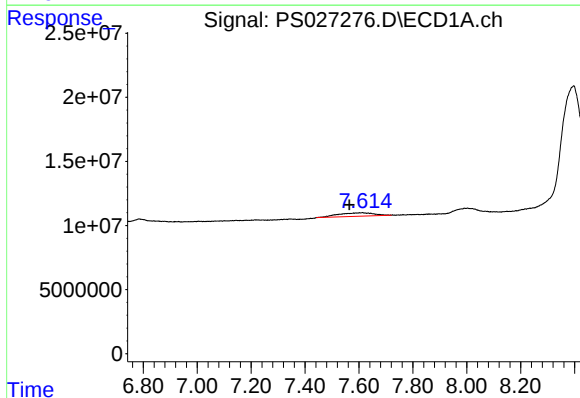


#6 MCPP

R.T.: 7.613 min
Delta R.T.: 0.048 min
Response: 25279690
Conc: 3.29 ug/ml

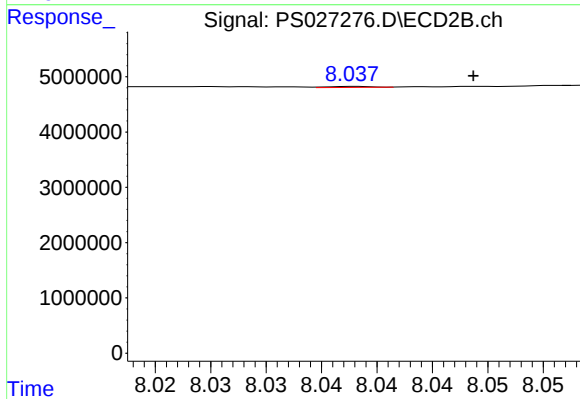

#6 MCPP


R.T.: 8.038 min
Delta R.T.: -0.010 min
Response: 46442
Conc: N.D.

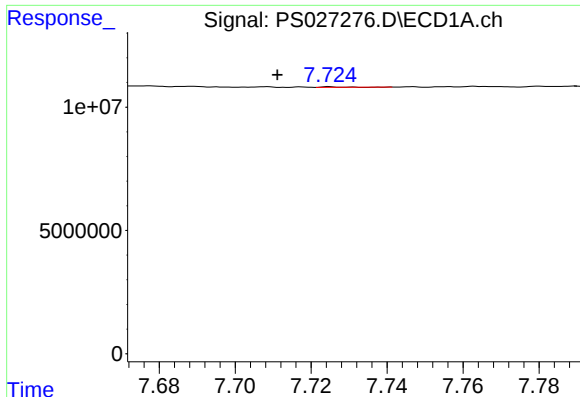

#7 MCPA


R.T.: 7.725 min
Delta R.T.: 0.014 min
Response: 241437
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
355

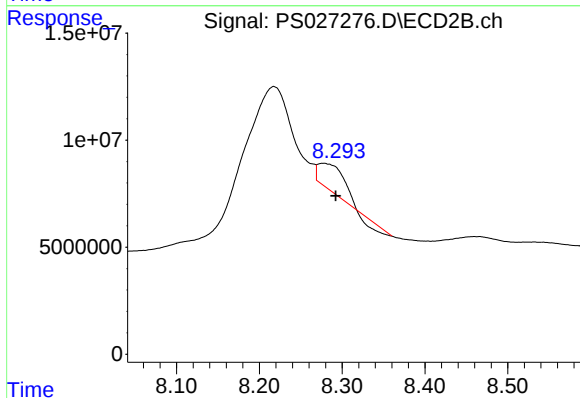


#7 MCPA

R.T.: 8.278 min
Delta R.T.: -0.014 min
Response: 20668444
Conc: 1.97 ug/ml

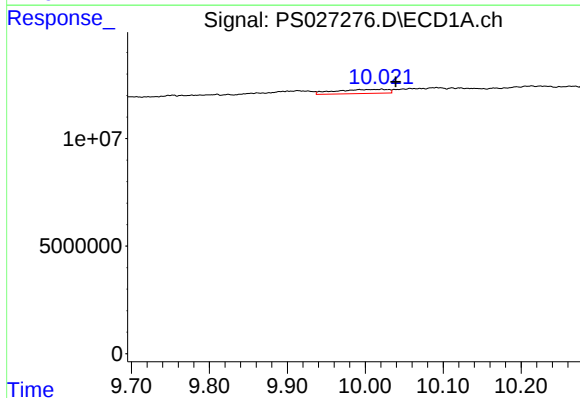

#13 2,4-DB

R.T.: 10.021 min
Delta R.T.: -0.018 min
Response: 8960039
Conc: 4.15 ng/ml

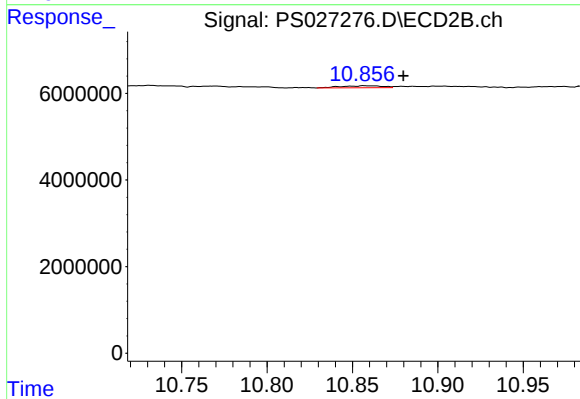

#13 2,4-DB

R.T.: 10.857 min
Delta R.T.: -0.023 min
Response: 781769
Conc: N.D.