

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080221\
 Data File : PS016257.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2021 11:36
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 14:59:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.187	6.767	599.8E6	245.7E6	407.692	471.076
Target Compounds							
5) T	DICAMBA	0.000	6.937	0	4598717	N.D.	2.110
10) T	Pentachlo...	0.000	8.267	0	2375242	N.D.	<MDL
15) T	Picloram	11.008f	10.835	12333090	7080078	1.236	1.758 #
16) T	DCPA	0.000	10.835f	0	7080078	N.D.	1.575



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080221\
Data File : PS016257.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2021 11:36
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 14:59:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

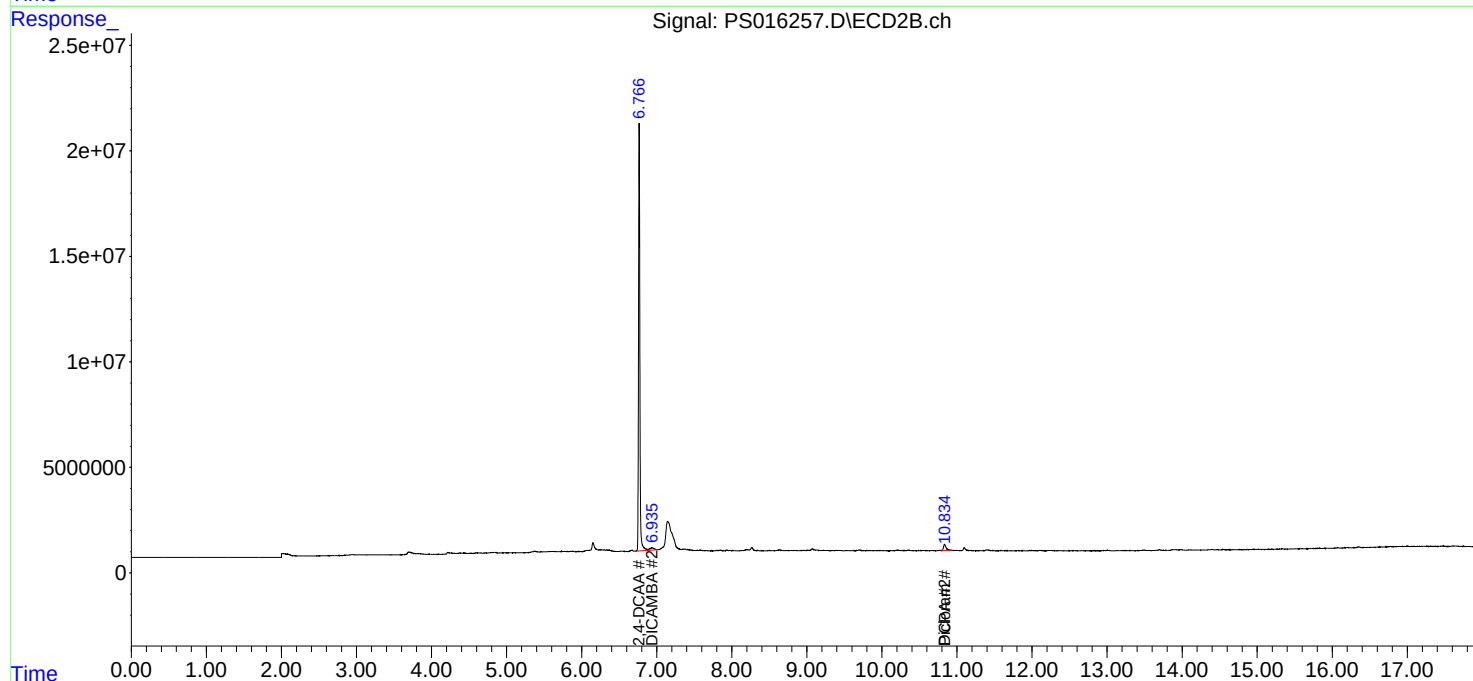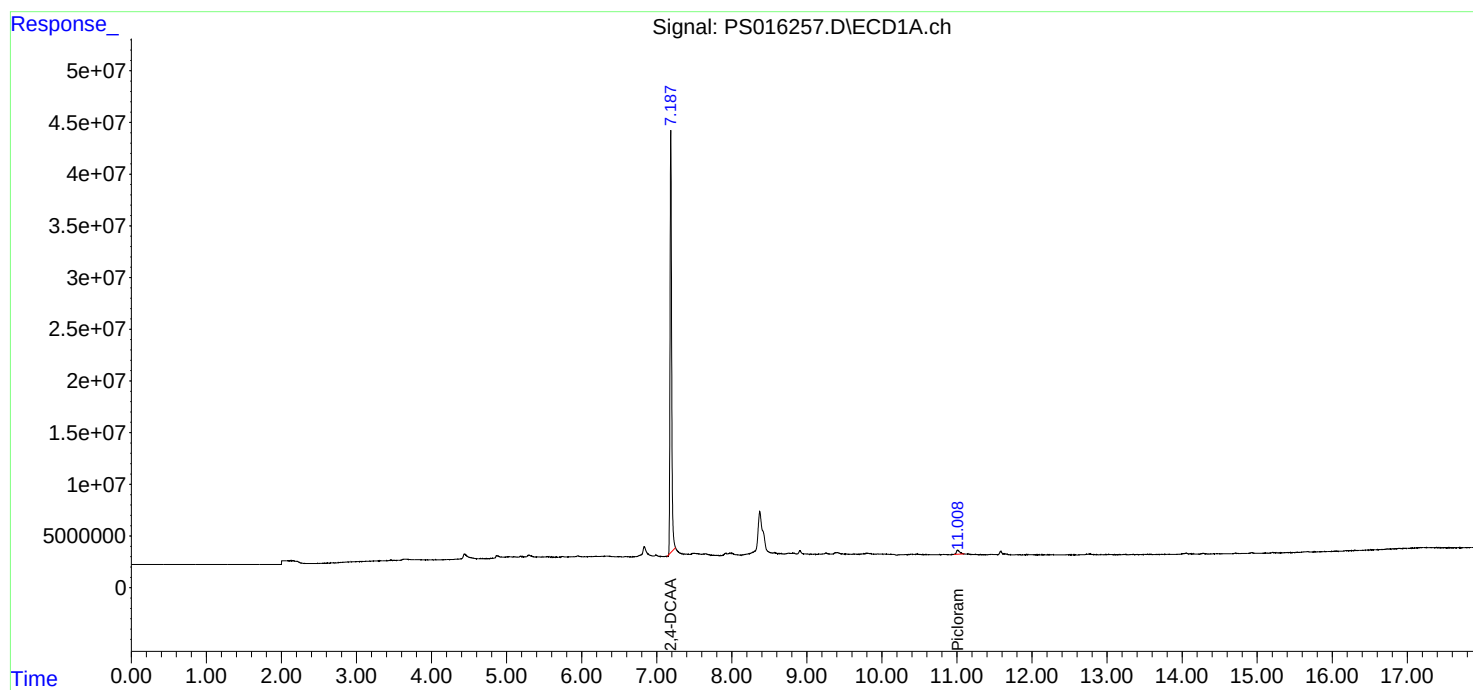


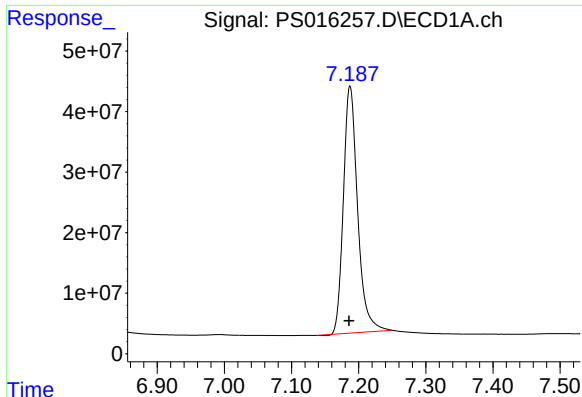

#4 2,4-DCAA


R.T.: 7.187 min
Delta R.T.: 0.001 min
Response: 599759059
Conc: 407.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

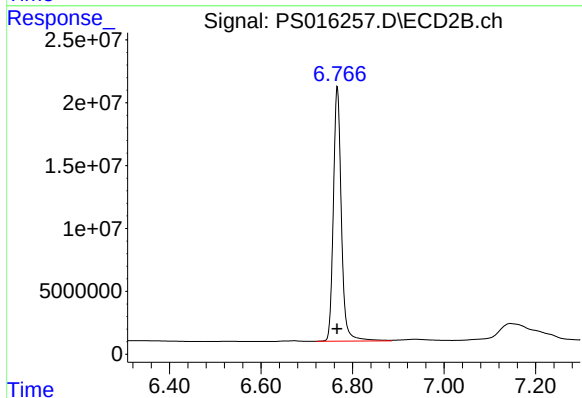


#4 2,4-DCAA

R.T.: 6.767 min
Delta R.T.: 0.000 min
Response: 245724815
Conc: 471.08 ng/ml

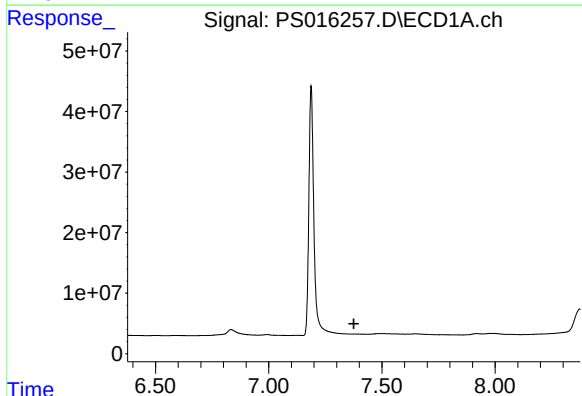


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.377 min
Response: 0
Conc: N.D.

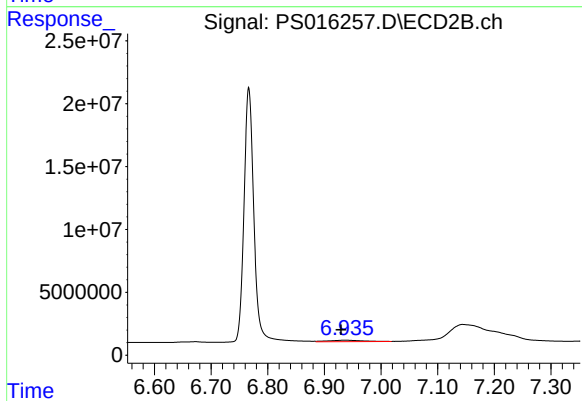

#5 DICAMBA


R.T.: 6.937 min
Delta R.T.: 0.007 min
Response: 4598717
Conc: 2.11 ng/ml

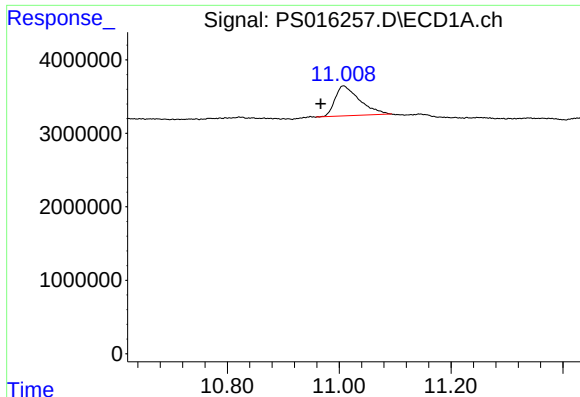

#15 Picloram


R.T.: 11.008 min
Delta R.T.: 0.041 min
Response: 12333090
Conc: 1.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

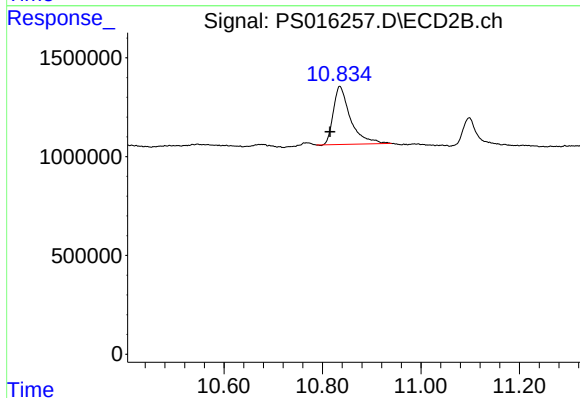


#15 Picloram

R.T.: 10.835 min
Delta R.T.: 0.020 min
Response: 7080078
Conc: 1.76 ng/ml

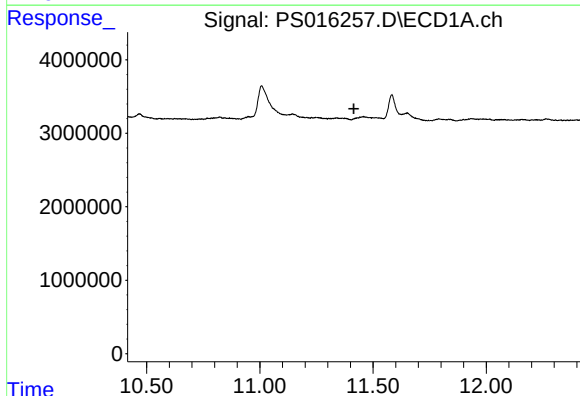

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.415 min
Response: 0
Conc: N.D.

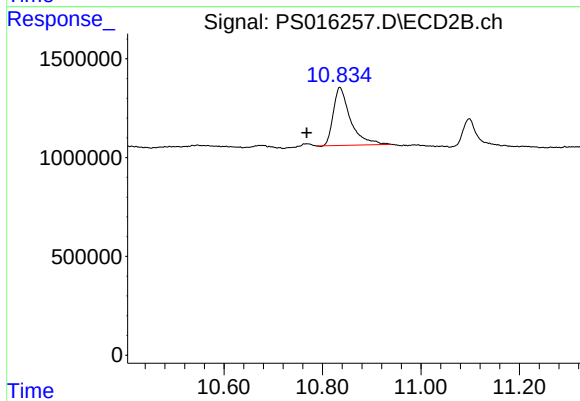

#16 DCPA

R.T.: 10.835 min
Delta R.T.: 0.067 min
Response: 7080078
Conc: 1.58 ng/ml