

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080223\
 Data File : PS023902.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2023 12:36
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 22:07:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072023.M
 Quant Title : 8080.M
 QLast Update : Thu Jul 20 19:21:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.364	6.800	2010867	571287	1.014	<MDL	#
Target Compounds								
1) T	Dalapon	2.520	2.572	4039848	1105085	1.886	<MDL	#
2) T	3,5-DICHL...	5.773	5.930f	1143332	396859	<MDL	<MDL	#
3) T	4-Nitroph...	6.209	6.392	2839317	146678	2.284	<MDL	#
5) T	DICAMBA	6.520	6.973	1130765	251521	<MDL	<MDL	#
8) T	DICHLORPROP	7.095	7.596	277210	1792357	<MDL	2.373	#
9) T	2,4-D	7.309	7.810f	25028621	643156	9.702	<MDL	#
10) T	Pentachlo...	7.532	8.295	1954225	649257	<MDL	<MDL	#
11) T	2,4,5-TP ...	8.061	8.654	1440476	645490	<MDL	<MDL	#
12) T	2,4,5-T	8.315	9.026	2254239	531667	<MDL	<MDL	#
13) T	2,4-DB	8.816	9.535	240039	564107	<MDL	1.138	#
14) T	DINOSEB	9.878	0.000	658279	0	<MDL	N.D.	#
15) T	Picloram	9.701	10.817	53835646	25574315	3.513	4.217	
16) T	DCPA	10.126	10.817	1568330	25574315	<MDL	5.379	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080223\
Data File : PS023902.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2023 12:36
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 22:07:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072023.M
Quant Title : 8080.M
QLast Update : Thu Jul 20 19:21:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

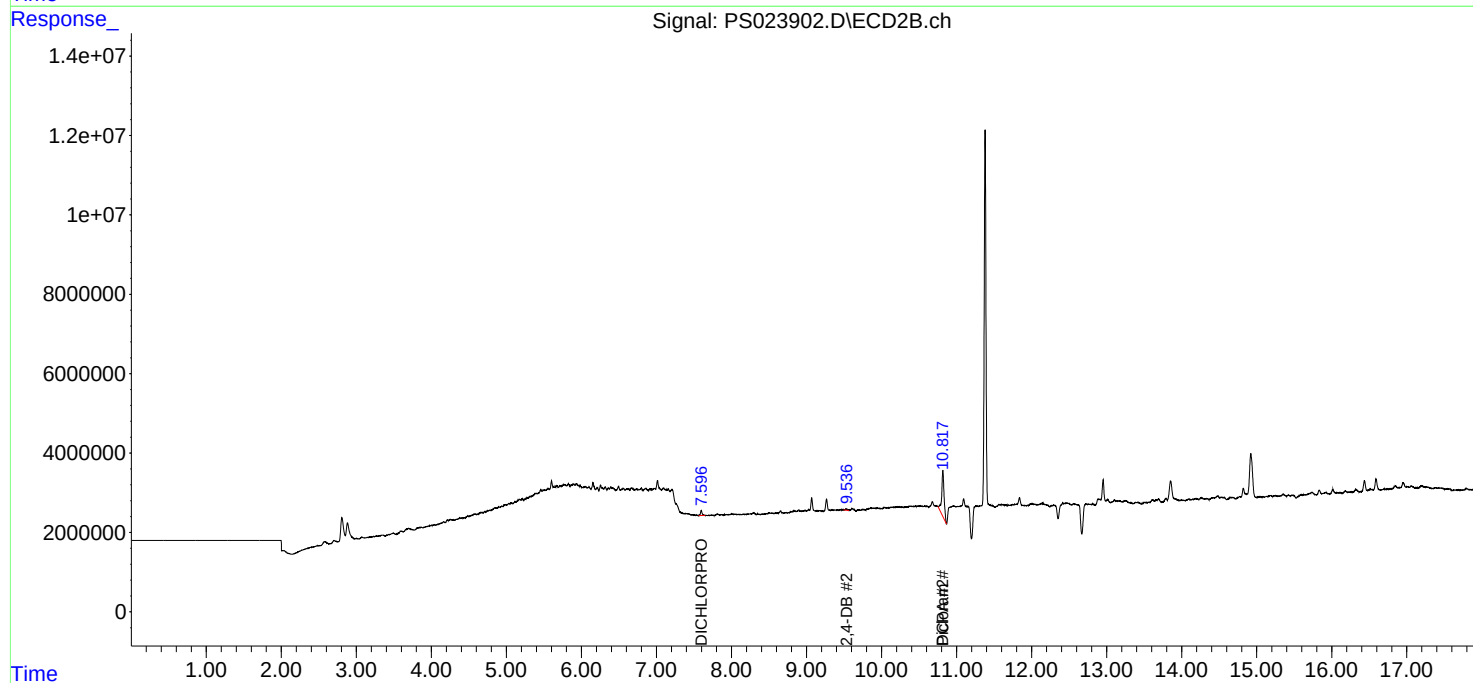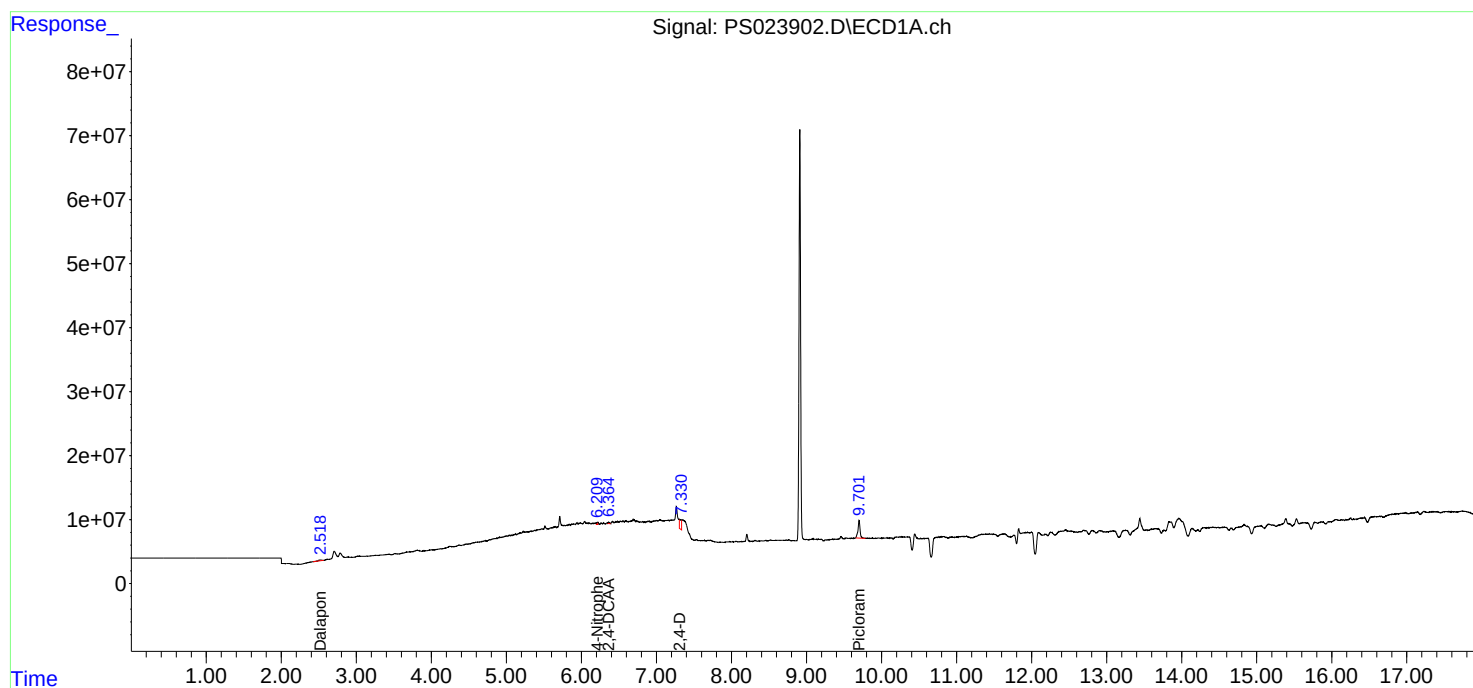


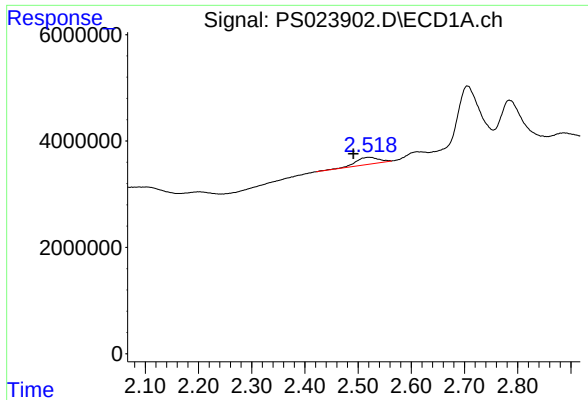

#1 Dalapon


R.T.: 2.520 min
Delta R.T.: 0.029 min
Response: 4039848
Conc: 1.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

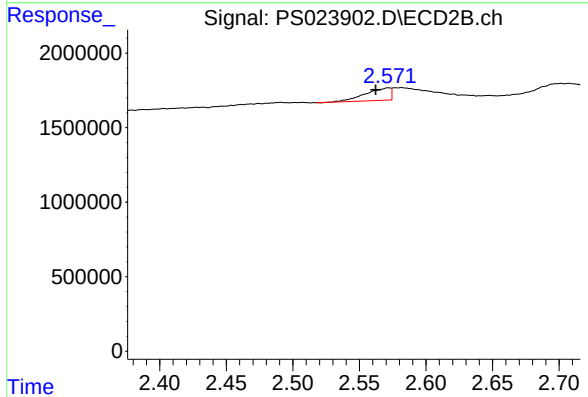


#1 Dalapon

R.T.: 2.572 min
Delta R.T.: 0.010 min
Response: 1105085
Conc: N.D.

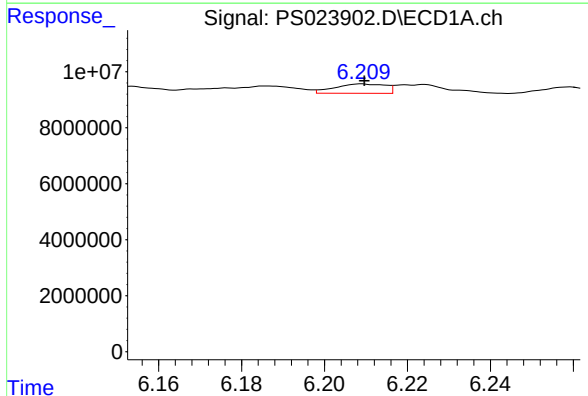


#3 4-Nitrophenol

R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 2839317
Conc: 2.28 ng/ml

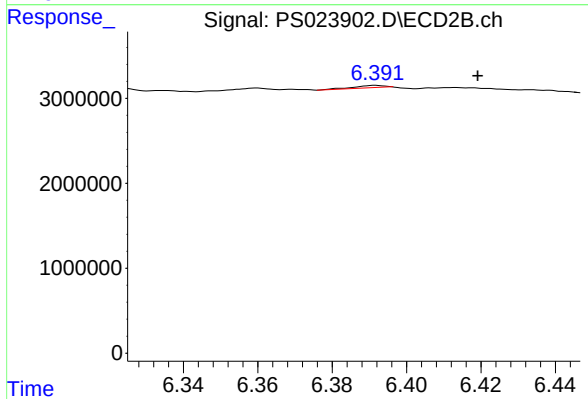

#3 4-Nitrophenol


R.T.: 6.392 min
Delta R.T.: -0.027 min
Response: 146678
Conc: N.D.

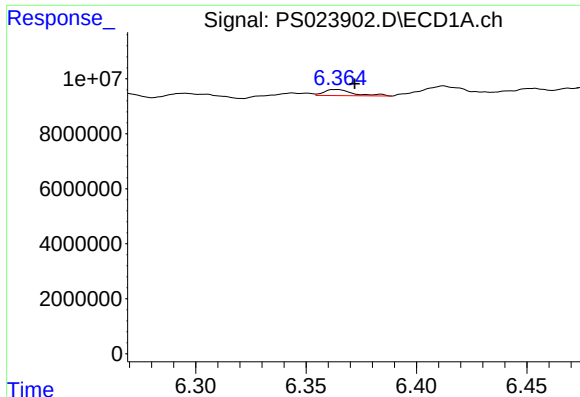

#4 2,4-DCAA


R.T.: 6.364 min
Delta R.T.: -0.008 min
Response: 2010867
Conc: 1.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

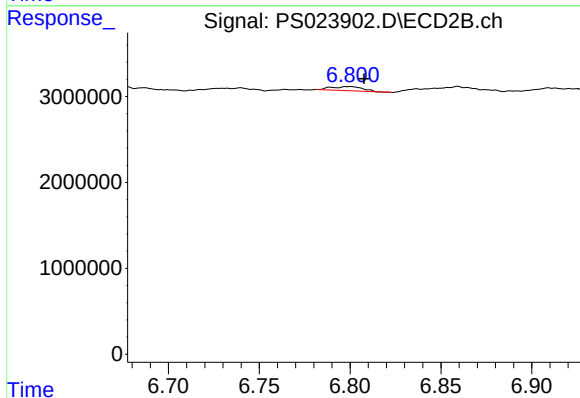


#4 2,4-DCAA

R.T.: 6.800 min
Delta R.T.: -0.008 min
Response: 571287
Conc: N.D.

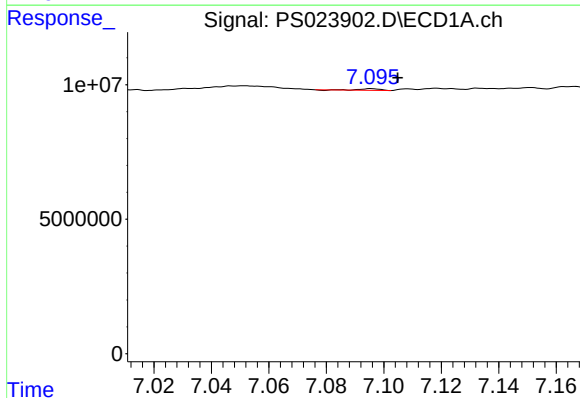


#8 DICHLORPROP

R.T.: 7.095 min
Delta R.T.: -0.010 min
Response: 277210
Conc: N.D.

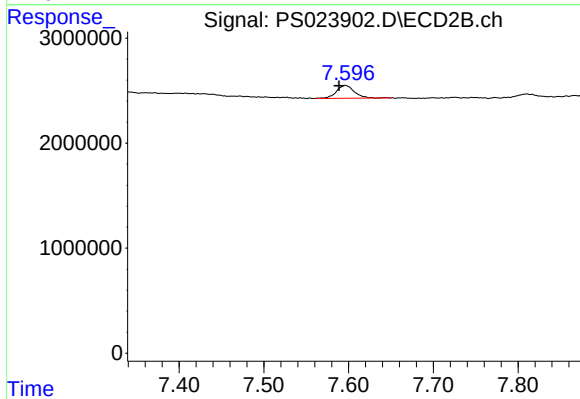

#8 DICHLORPROP


R.T.: 7.596 min
Delta R.T.: 0.007 min
Response: 1792357
Conc: 2.37 ng/ml

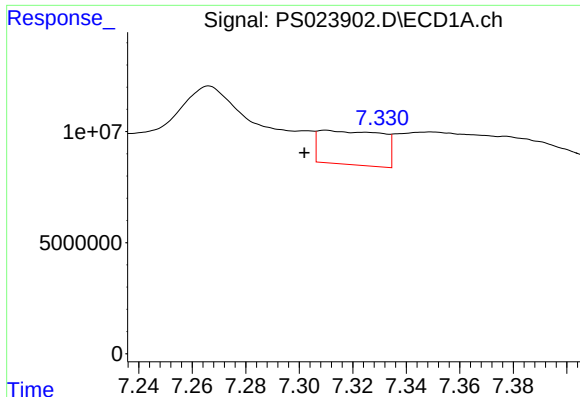

#9 2,4-D


R.T.: 7.309 min
Delta R.T.: 0.007 min
Response: 25028621
Conc: 9.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

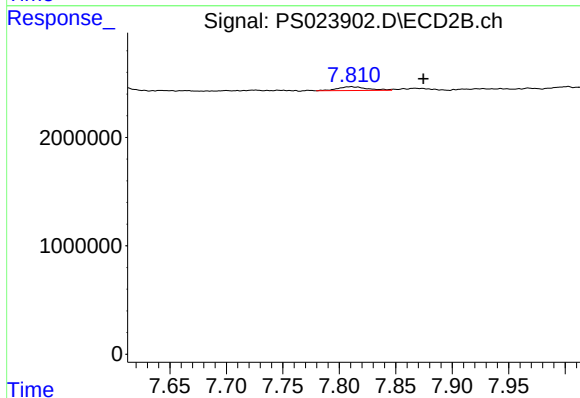


#9 2,4-D

R.T.: 7.810 min
Delta R.T.: -0.064 min
Response: 643156
Conc: N.D.

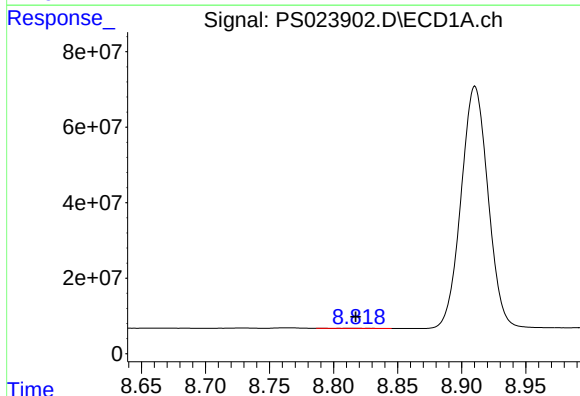


#13 2,4-DB

R.T.: 8.816 min
Delta R.T.: -0.002 min
Response: 240039
Conc: N.D.

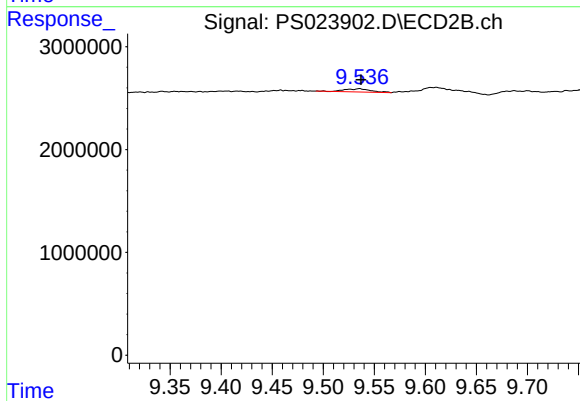

#13 2,4-DB


R.T.: 9.535 min
Delta R.T.: -0.002 min
Response: 564107
Conc: 1.14 ng/ml

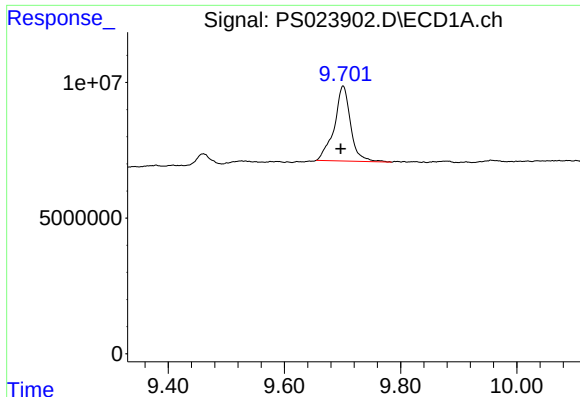

#15 Picloram


R.T.: 9.701 min
Delta R.T.: 0.004 min
Response: 53835646
Conc: 3.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

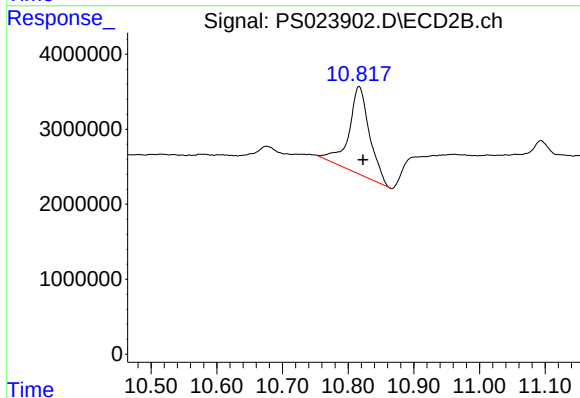


#15 Picloram

R.T.: 10.817 min
Delta R.T.: -0.006 min
Response: 25574315
Conc: 4.22 ng/ml

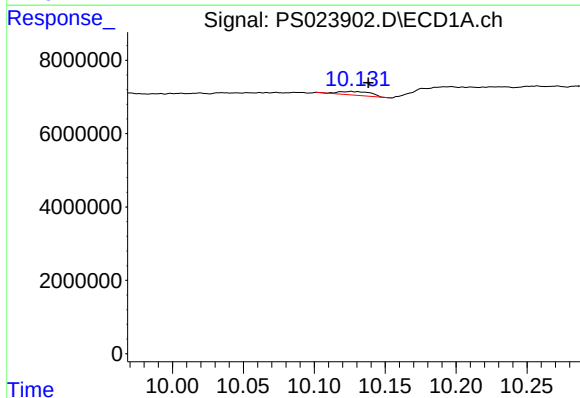

#16 DCPA

R.T.: 10.126 min
Delta R.T.: -0.012 min
Response: 1568330
Conc: N.D.

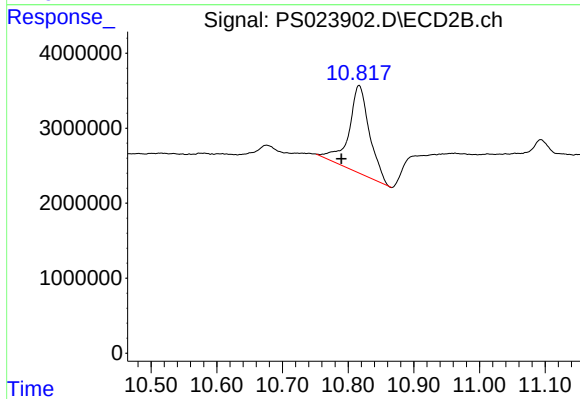

#16 DCPA

R.T.: 10.817 min
Delta R.T.: 0.027 min
Response: 25574315
Conc: 5.38 ng/ml