

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080223\
 Data File : PS023903.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2023 13:00
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 22:07:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072023.M
 Quant Title : 8080.M
 QLast Update : Thu Jul 20 19:21:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.371	6.804	1029.9E6	340.7E6	519.464	500.930
Target Compounds							
1) T	Dalapon	0.000	2.599	0	68977	N.D.	<MDL
2) T	3,5-DICHL...	5.710	0.000	1545634	0	<MDL	N.D. #
3) T	4-Nitroph...	6.211	6.351f	7039975	71771	5.663	<MDL #
8) T	DICHLORPROP	7.153f	7.600	672882	1628308	<MDL	2.155 #
9) T	2,4-D	0.000	7.813f	0	397588	N.D.	<MDL
11) T	2,4,5-TP ...	8.053	0.000	1544684	0	<MDL	N.D. #
12) T	2,4,5-T	8.311	9.071	877174	4158155	<MDL	1.056 #
13) T	2,4-DB	8.758f	0.000	1509903	0	<MDL	N.D. #
14) T	DINOSEB	9.874	0.000	219942	0	<MDL	N.D. #
15) T	Picloram	9.697	10.818	44389566	16484436	2.896	2.718
16) T	DCPA	10.124	10.818	585646	16484436	<MDL	3.467 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080223\
Data File : PS023903.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2023 13:00
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 22:07:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072023.M
Quant Title : 8080.M
QLast Update : Thu Jul 20 19:21:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

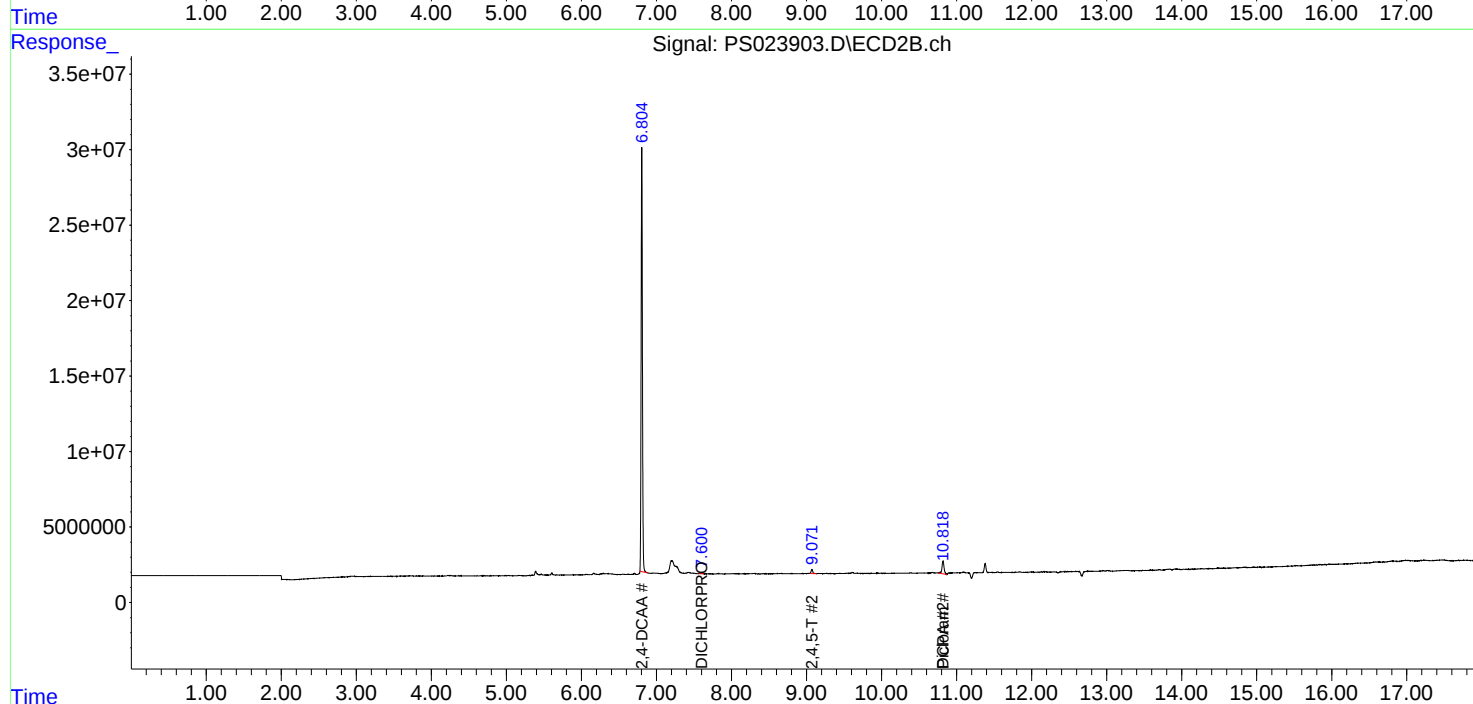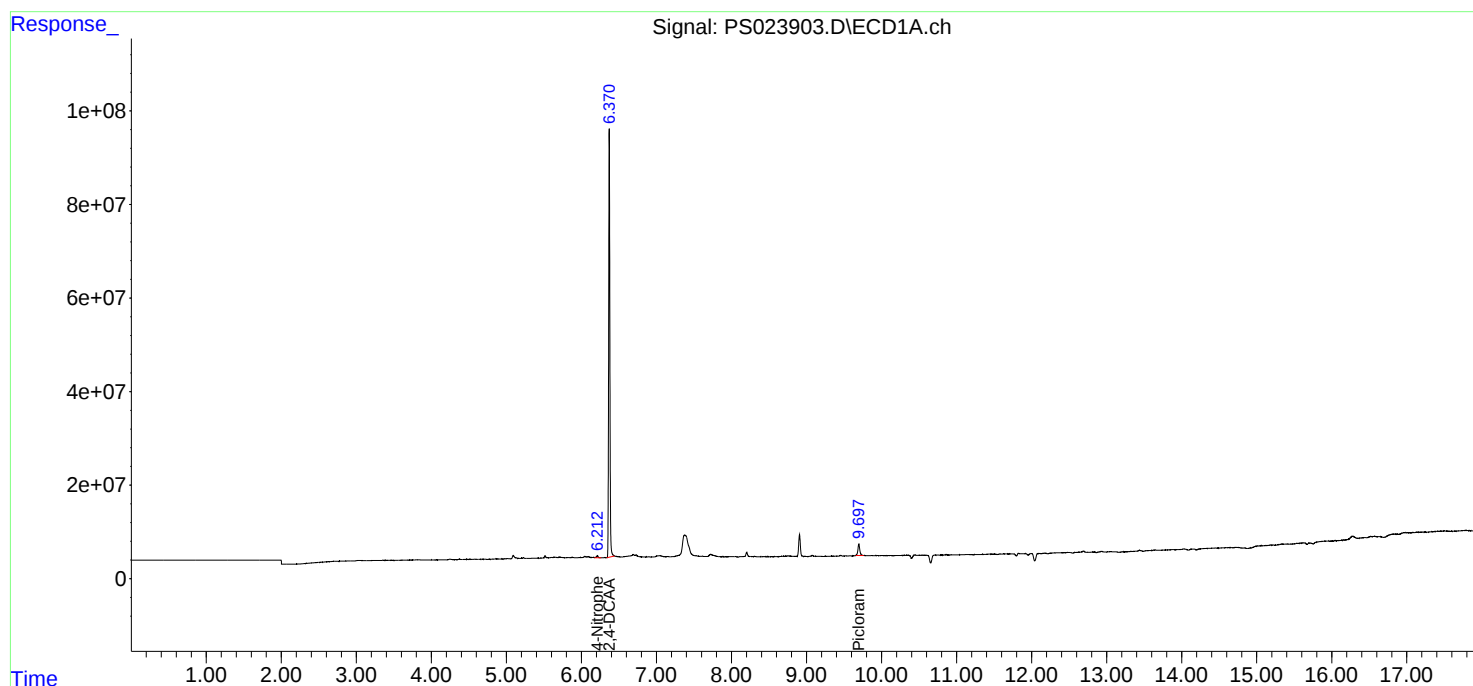


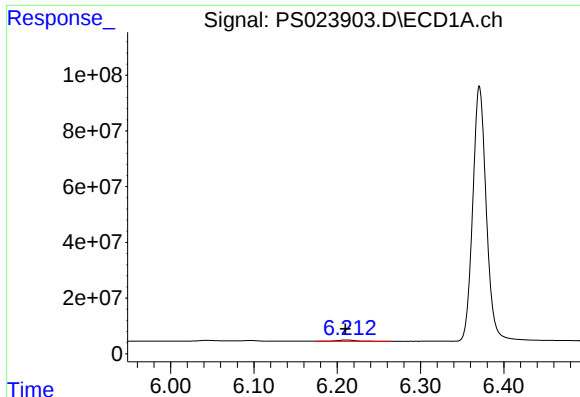

#3 4-Nitrophenol


R.T.: 6.211 min
Delta R.T.: 0.002 min
Response: 7039975
Conc: 5.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

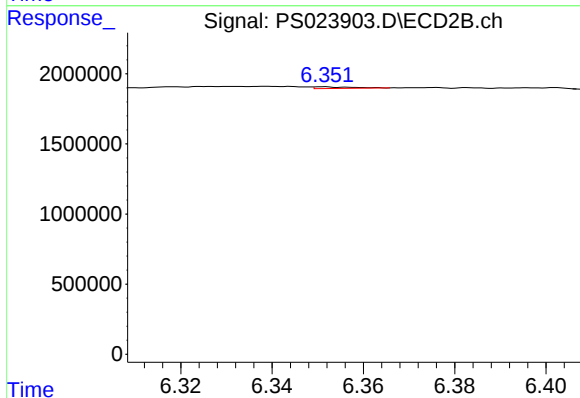


#3 4-Nitrophenol

R.T.: 6.351 min
Delta R.T.: -0.068 min
Response: 71771
Conc: N.D.

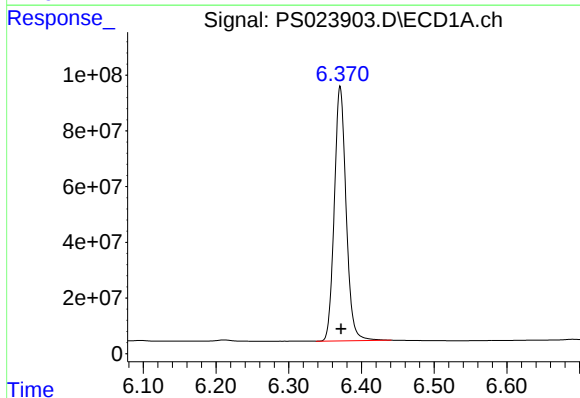


#4 2,4-DCAA

R.T.: 6.371 min
Delta R.T.: -0.001 min
Response: 1029909272
Conc: 519.46 ng/ml

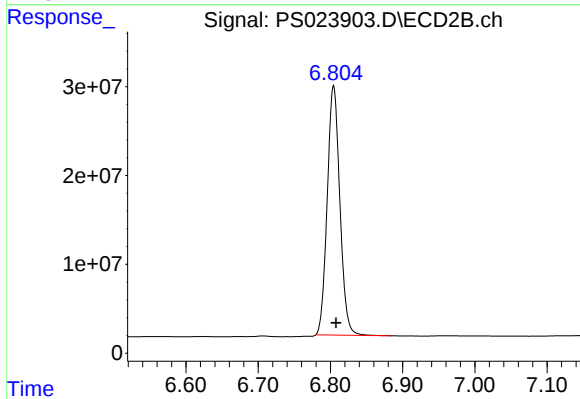

#4 2,4-DCAA


R.T.: 6.804 min
Delta R.T.: -0.003 min
Response: 340681822
Conc: 500.93 ng/ml

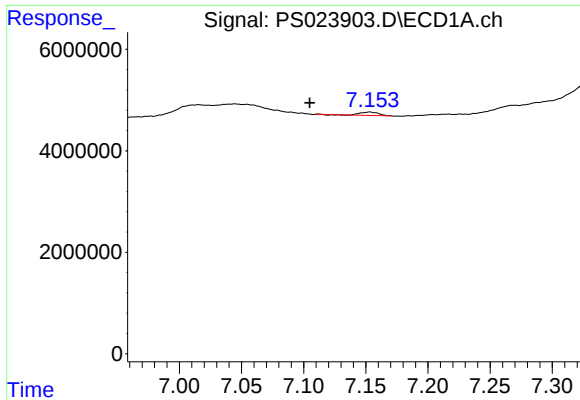

#8 DICHLORPROP


R.T.: 7.153 min
Delta R.T.: 0.048 min
Response: 672882
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

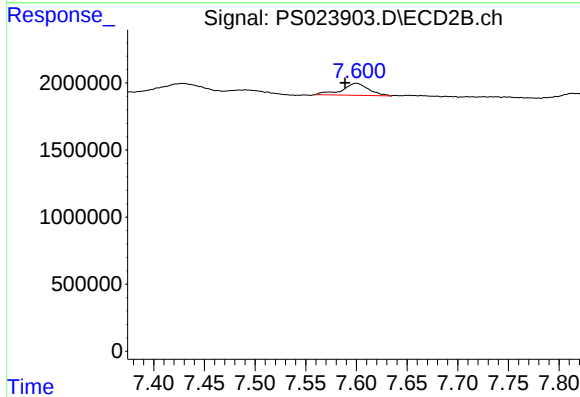


#8 DICHLORPROP

R.T.: 7.600 min
Delta R.T.: 0.011 min
Response: 1628308
Conc: 2.16 ng/ml

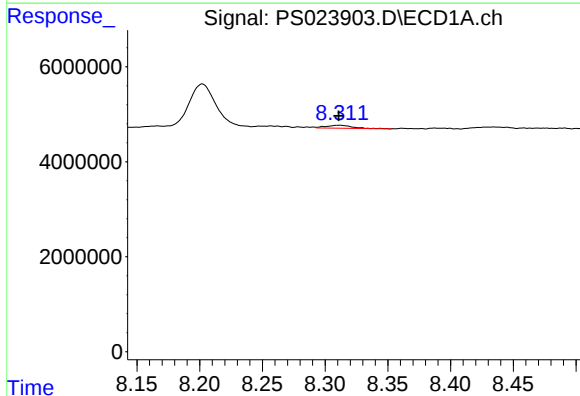


#12 2,4,5-T

R.T.: 8.311 min
Delta R.T.: 0.000 min
Response: 877174
Conc: N.D.

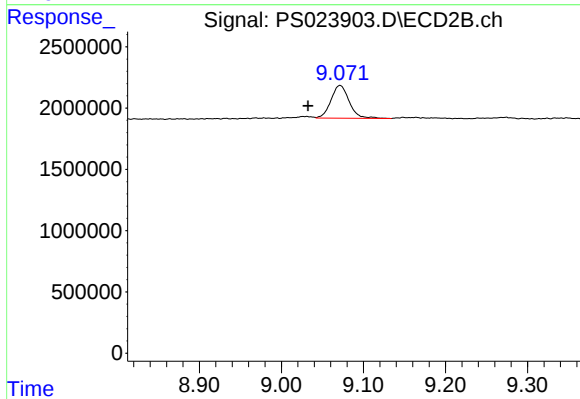

#12 2,4,5-T


R.T.: 9.071 min
Delta R.T.: 0.039 min
Response: 4158155
Conc: 1.06 ng/ml

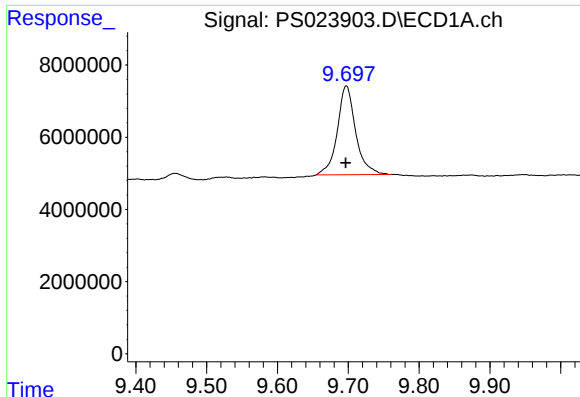

#15 Picloram


R.T.: 9.697 min
Delta R.T.: 0.000 min
Response: 44389566
Conc: 2.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

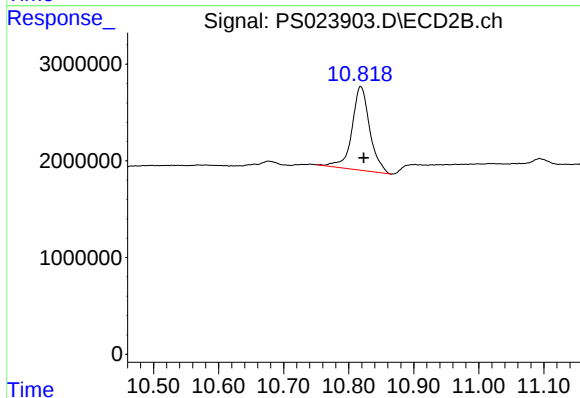


#15 Picloram

R.T.: 10.818 min
Delta R.T.: -0.005 min
Response: 16484436
Conc: 2.72 ng/ml

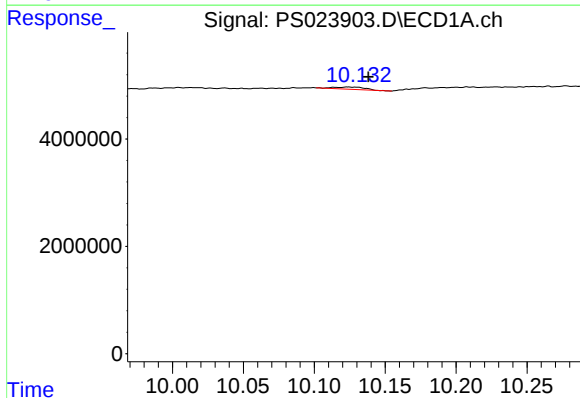

#16 DCPA

R.T.: 10.124 min
Delta R.T.: -0.014 min
Response: 585646
Conc: N.D.

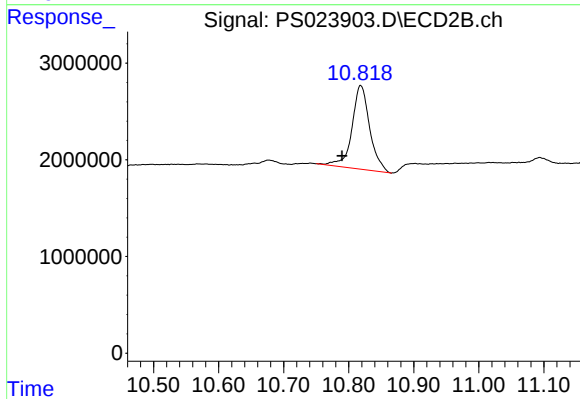

#16 DCPA

R.T.: 10.818 min
Delta R.T.: 0.029 min
Response: 16484436
Conc: 3.47 ng/ml