

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080224\
 Data File : PS027280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2024 08:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 12:26:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.192	7.750	1292.5E6	1163.3E6	511.137	501.698
Target Compounds							
3) T	4-Nitroph...	6.991	7.251f	6593718	1150552	4.113	<MDL #
5) T	DICAMBA	7.397	7.947	299483	9257780	<MDL	<MDL #
6) T	MCP	0.000	8.049	0	80517	N.D.	<MDL
8) T	DICHLORPROP	8.105	8.655	299704	781666	<MDL	<MDL #
10) T	Pentachlo...	8.623	0.000	1337843	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.905	0	513017	N.D.	<MDL
12) T	2,4,5-T	0.000	10.315	0	1302719	N.D.	<MDL
13) T	2,4-DB	10.032	0.000	2203517	0	1.020	N.D. #
14) T	DINOSEB	11.257	11.255	1525799	583736	<MDL	<MDL #
15) T	Picloram	11.049	12.358	35112682	17195198	1.803	<MDL #
16) T	DCPA	0.000	12.264f	0	1088222	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080224\
Data File : PS027280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2024 08:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 12:26:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS071224.M
Quant Title : 8080.M
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

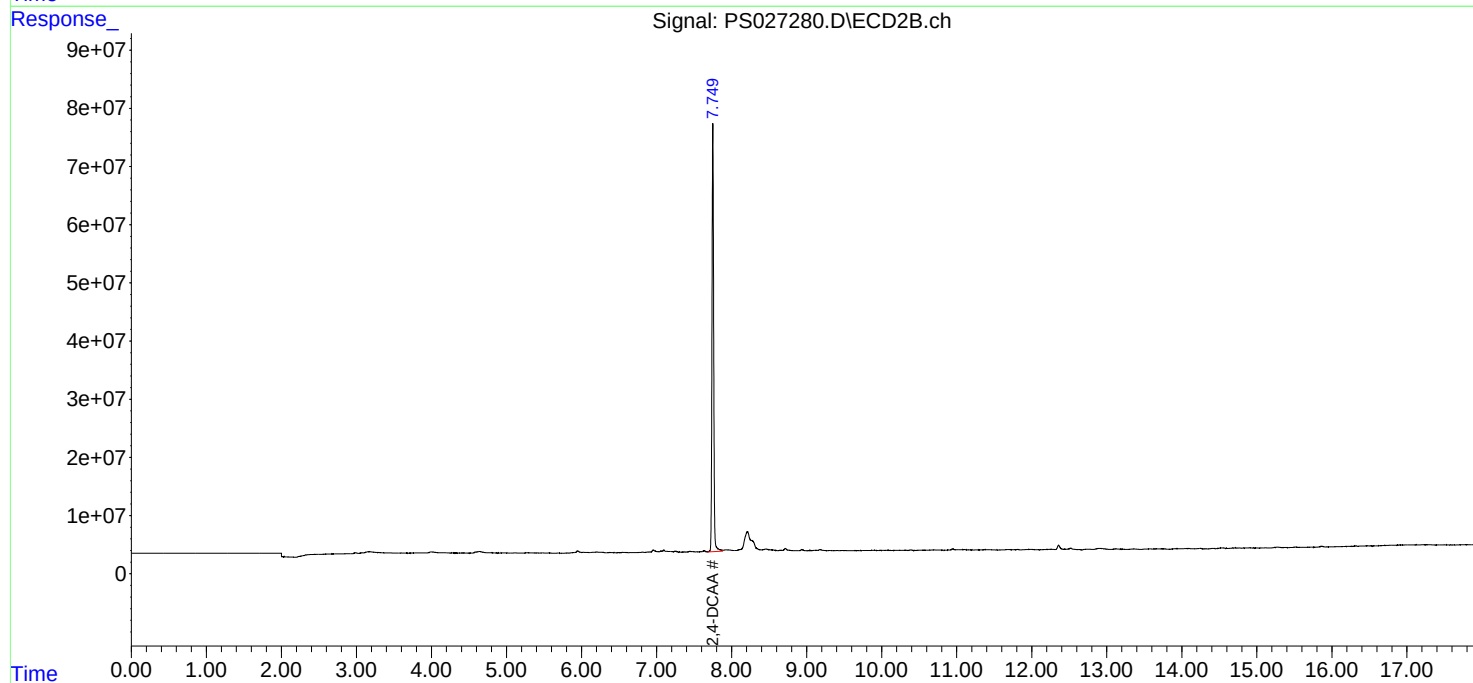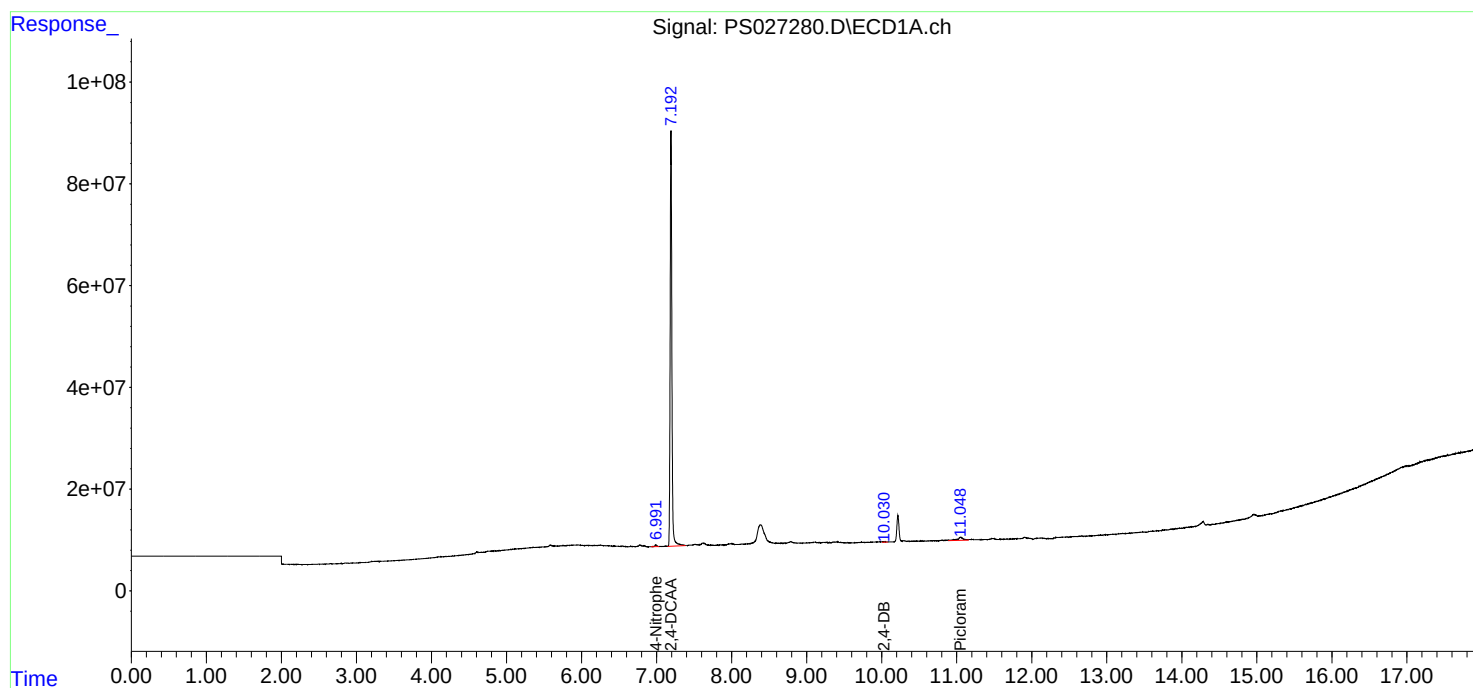


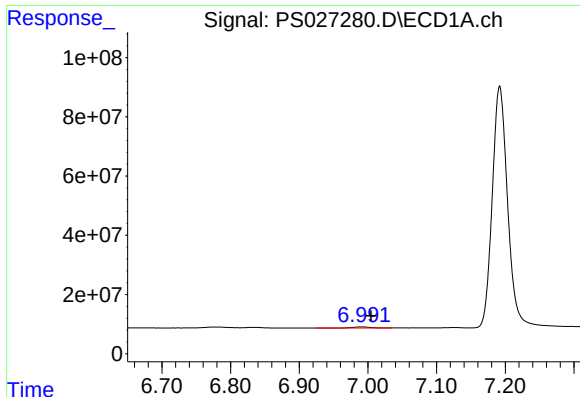

#3 4-Nitrophenol


R.T.: 6.991 min
Delta R.T.: -0.014 min
Response: 6593718
Conc: 4.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

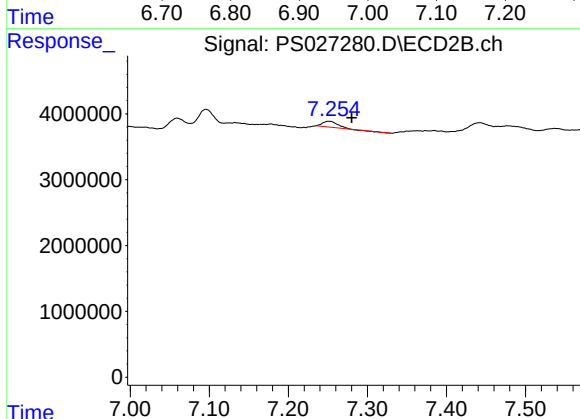


#3 4-Nitrophenol

R.T.: 7.251 min
Delta R.T.: -0.029 min
Response: 1150552
Conc: N.D.

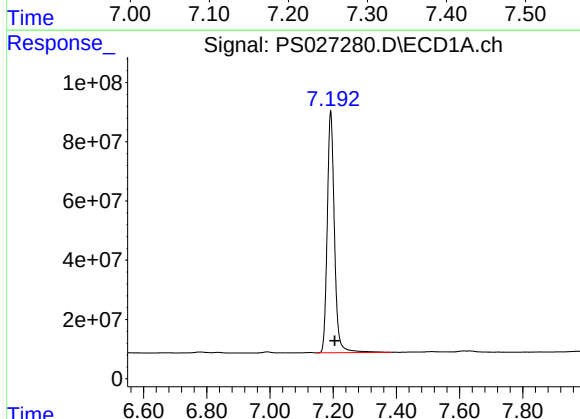


#4 2,4-DCAA

R.T.: 7.192 min
Delta R.T.: -0.013 min
Response: 1292544144
Conc: 511.14 ng/ml

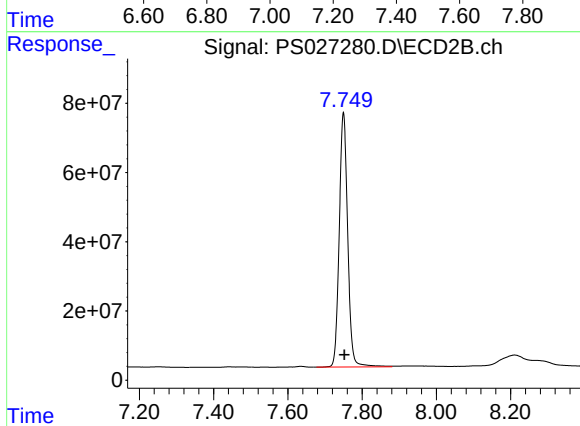

#4 2,4-DCAA


R.T.: 7.750 min
Delta R.T.: -0.003 min
Response: 1163299323
Conc: 501.70 ng/ml

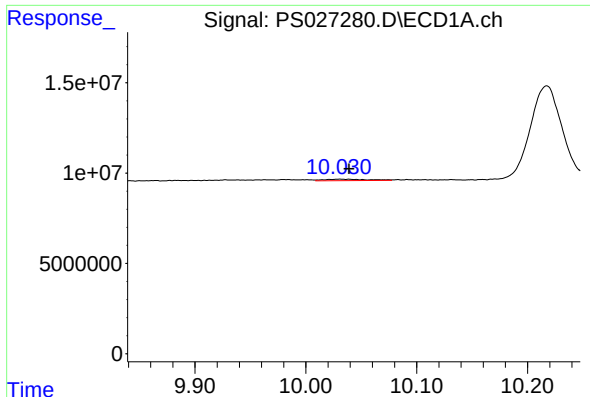

#13 2,4-DB


R.T.: 10.032 min
Delta R.T.: -0.007 min
Response: 2203517
Conc: 1.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

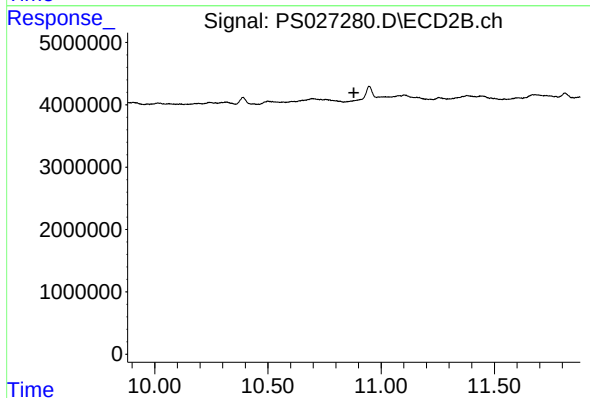


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.880 min
Response: 0
Conc: N.D.

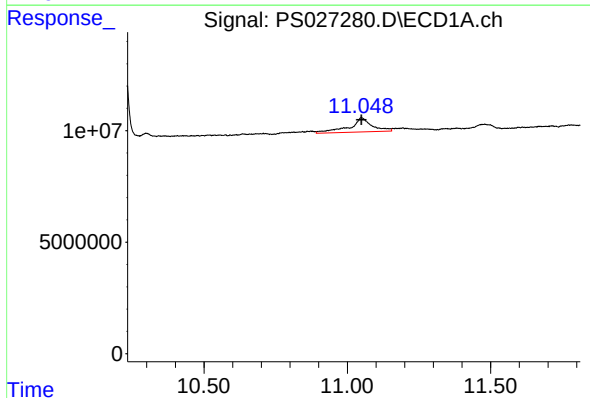

#15 Picloram

R.T.: 11.049 min
Delta R.T.: 0.000 min
Response: 35112682
Conc: 1.80 ng/ml

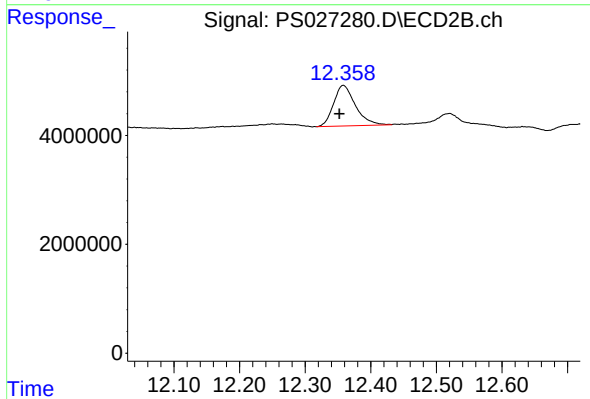

#15 Picloram

R.T.: 12.358 min
Delta R.T.: 0.006 min
Response: 17195198
Conc: N.D.