

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080318\
 Data File : PS001381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2018 21:22
 Operator : UA
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 22:53:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.616	11.035	137.4E6	133.5E6	740.519	734.008
Target Compounds							
1) T	Dalapon	3.010	2.427	153.1E6	152.0E6	645.619m	667.027
2) T	3,5-DICHL...	10.031	9.182	184.9E6	170.9E6	685.101m	670.695m
3) T	4-Nitroph...	11.208	10.182	75030469	66913348	651.937m	656.406m
5) T	DICAMBA	11.930	11.323	503.8E6	469.8E6	700.689m	685.444
6) T	MCPD	12.269	11.547	37489764	31891928	74.591m	73.498m
7) T	MCPA	12.521	11.923	54865852	47097129	69.571	72.430m
8) T	DICHLORPROP	13.122	12.448	127.5E6	118.0E6	698.457m	665.977
9) T	2,4-D	13.482	12.919	171.5E6	160.0E6	698.711	674.310m
10) T	Pentachlo...	13.871	13.474	2007.9E6	1926.1E6	713.173	699.838m
11) T	2,4,5-TP ...	14.739	14.087	795.9E6	758.2E6	709.135m	693.386m
12) T	2,4,5-T	15.137	14.659	786.3E6	579.9E6	706.652	627.761
13) T	2,4-DB	15.888	15.304	96334989	90396124	669.161	678.841
14) T	DINOSEB	17.387	15.735	544.8E6	496.8E6	709.313	698.873
15) T	Picloram	17.145	16.917	967.5E6	932.5E6	612.087m	676.438
16) T	DCPA	17.727	16.973	977.1E6	876.1E6	723.758	606.572



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS001381.D
Data File : PS001381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2018 21:22
Operator : UA
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 22:53:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

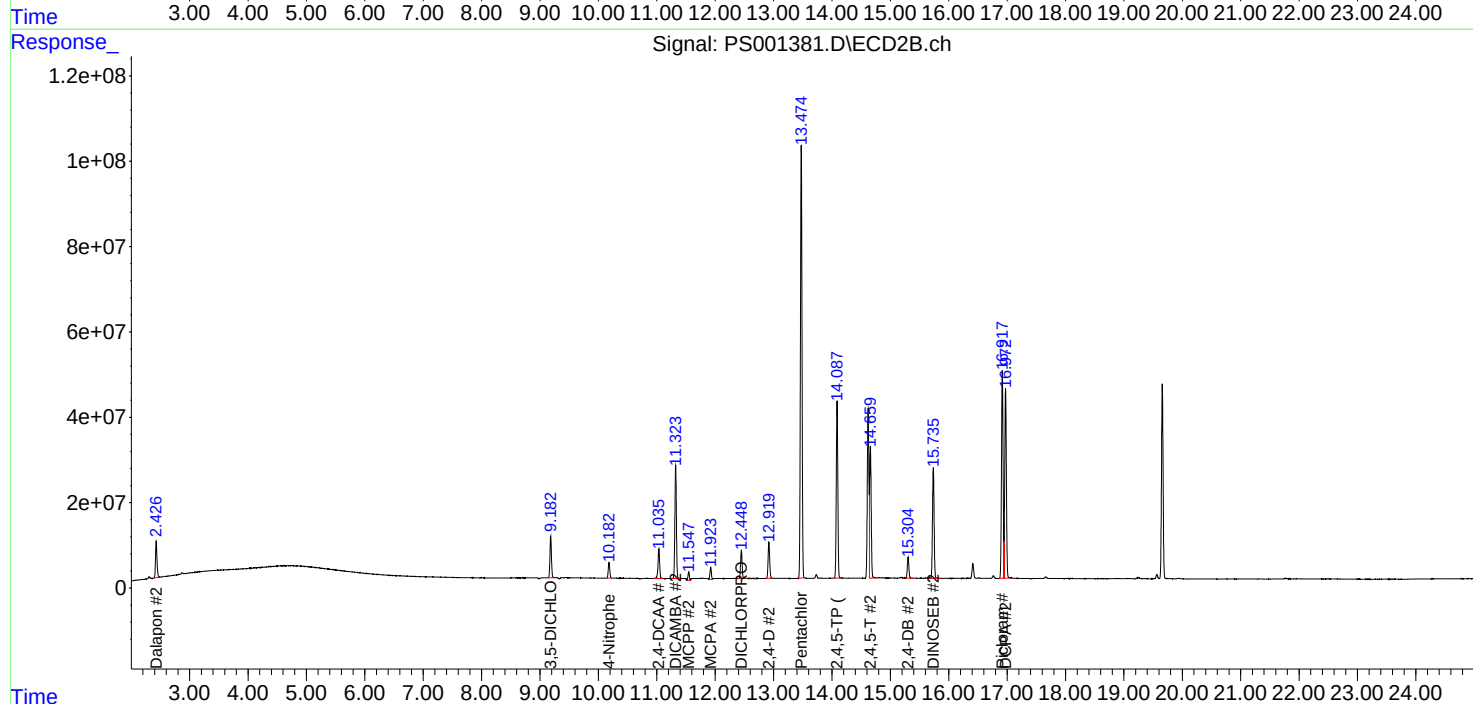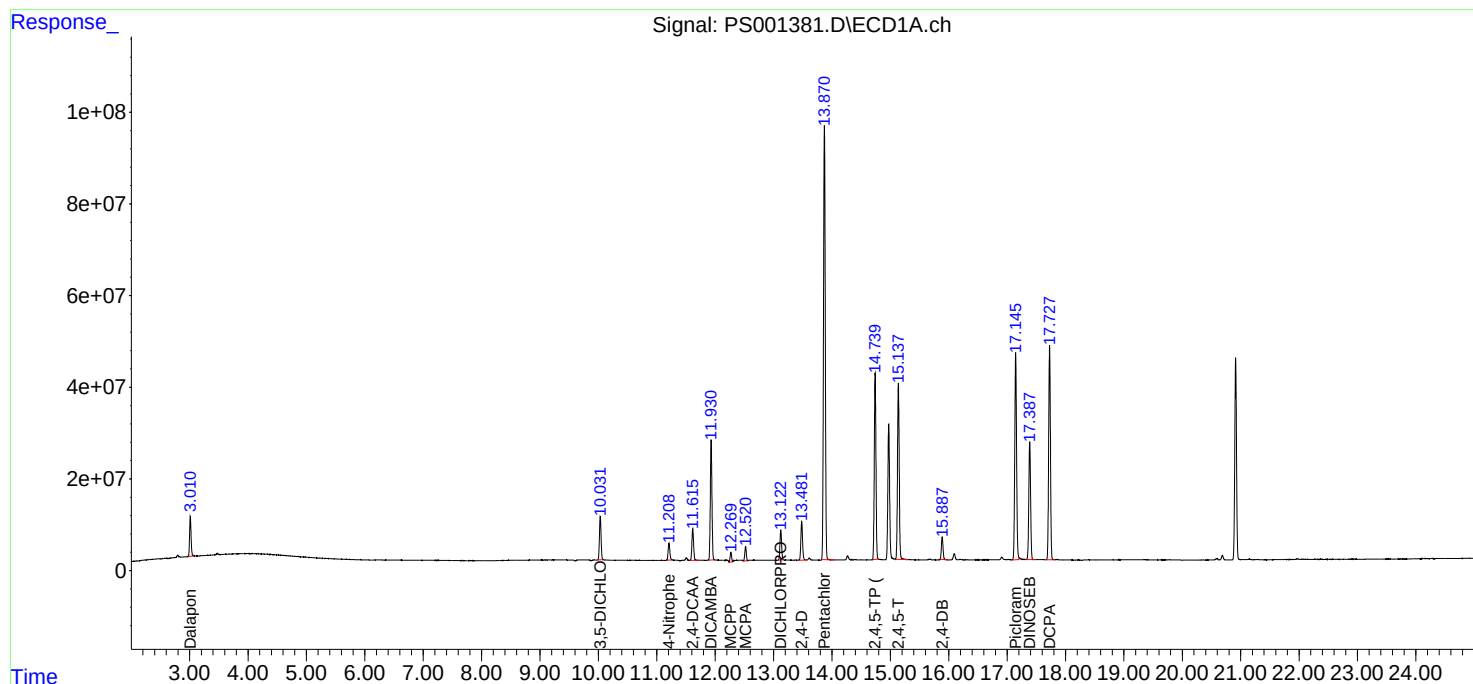


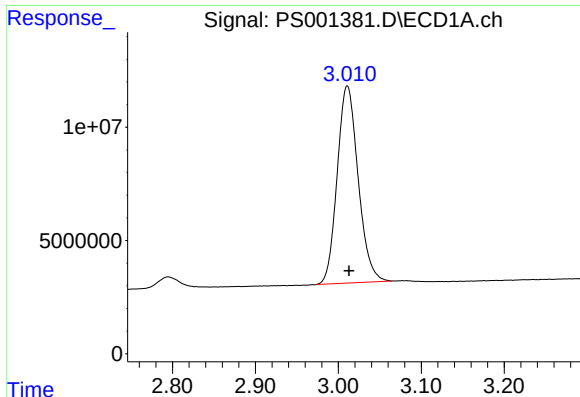

#1 Dalapon


R.T.: 3.010 min
Delta R.T.: -0.003 min
Response: 153092645
Conc: 645.62 ng/ml m

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

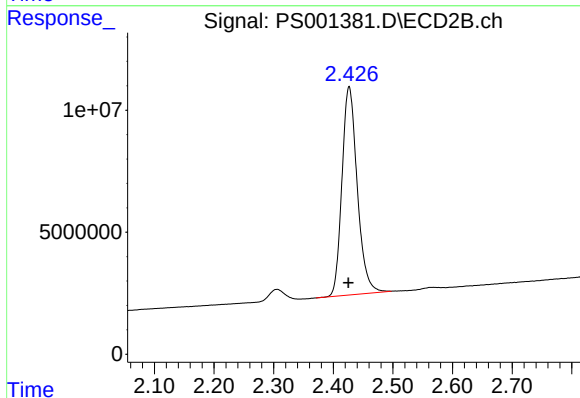


#1 Dalapon

R.T.: 2.427 min
Delta R.T.: 0.001 min
Response: 151996947
Conc: 667.03 ng/ml

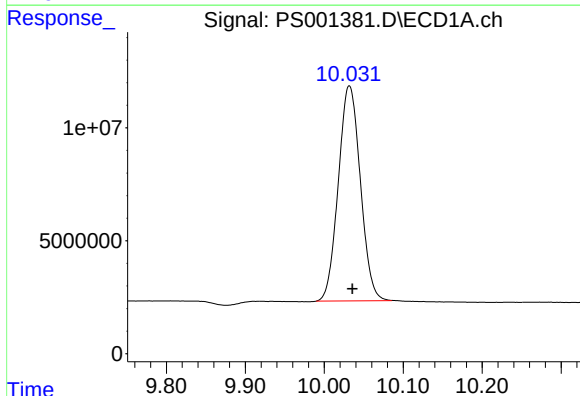


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.031 min
Delta R.T.: -0.004 min
Response: 184906074
Conc: 685.10 ng/ml m

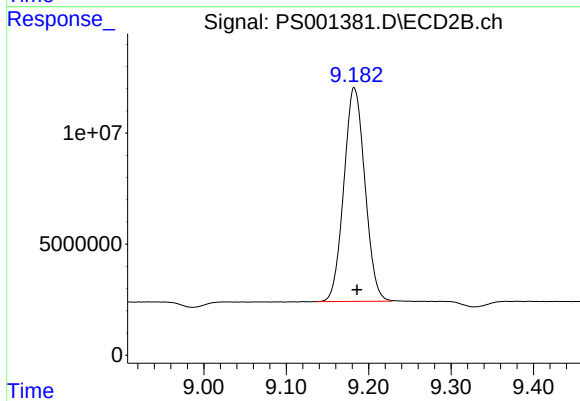

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.182 min
Delta R.T.: -0.004 min
Response: 170858732
Conc: 670.69 ng/ml m

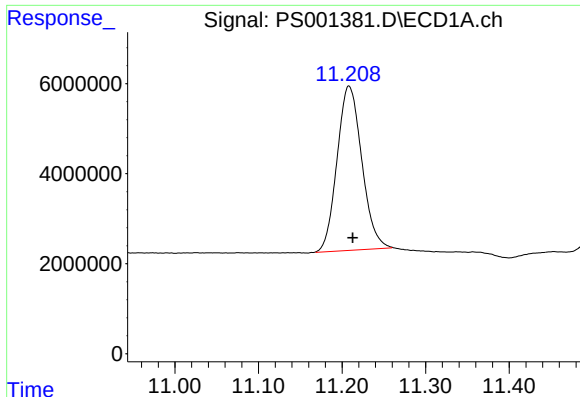

#3 4-Nitrophenol


R.T.: 11.208 min
Delta R.T.: -0.005 min
Response: 75030469
Conc: 651.94 ng/ml m

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

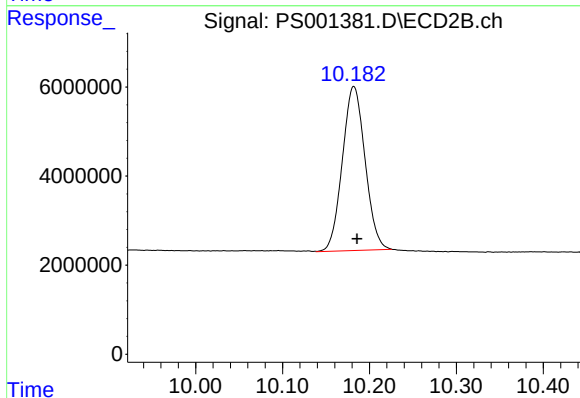


#3 4-Nitrophenol

R.T.: 10.182 min
Delta R.T.: -0.004 min
Response: 66913348
Conc: 656.41 ng/ml m

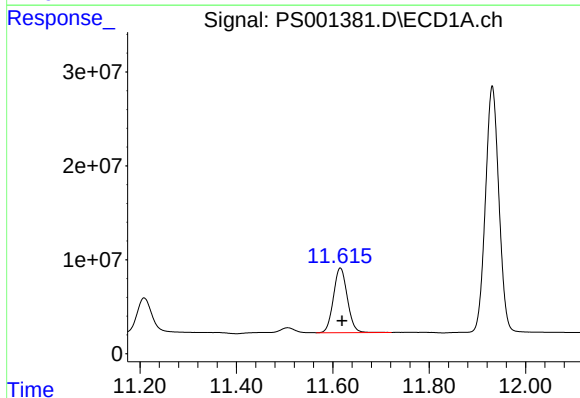


#4 2,4-DCAA

R.T.: 11.616 min
Delta R.T.: -0.004 min
Response: 137403141
Conc: 740.52 ng/ml

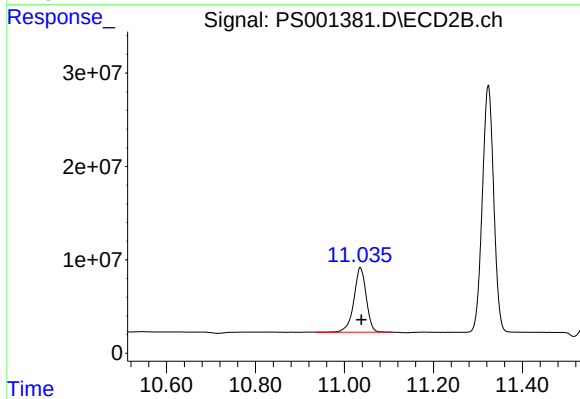

#4 2,4-DCAA


R.T.: 11.035 min
Delta R.T.: -0.003 min
Response: 133497664
Conc: 734.01 ng/ml

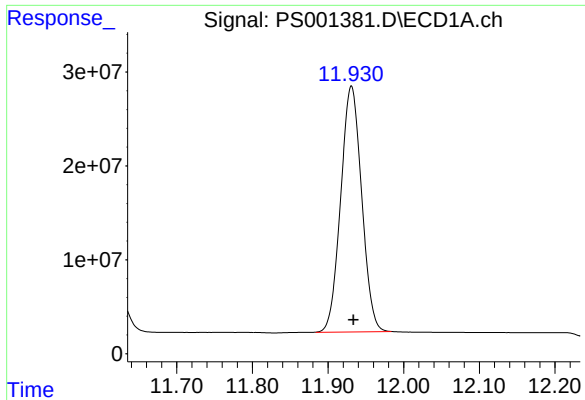

#5 DICAMBA


R.T.: 11.930 min
Delta R.T.: -0.003 min
Response: 503776975
Conc: 700.69 ng/ml m

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

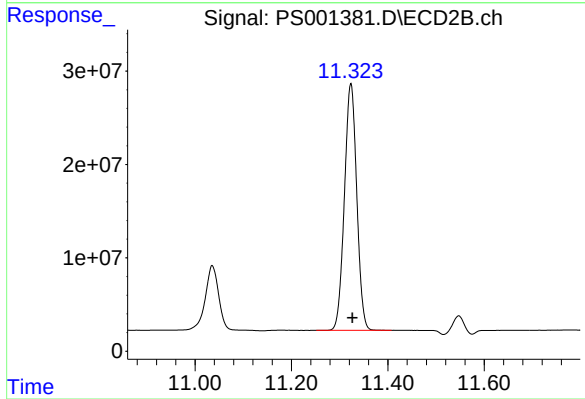


#5 DICAMBA

R.T.: 11.323 min
Delta R.T.: -0.003 min
Response: 469791259
Conc: 685.44 ng/ml

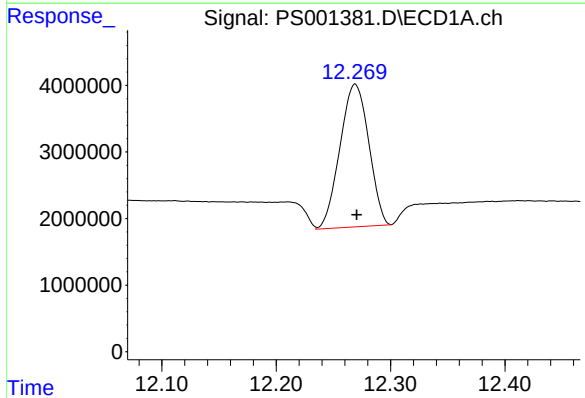


#6 MCP

R.T.: 12.269 min
Delta R.T.: -0.002 min
Response: 37489764
Conc: 74.59 ug/ml m

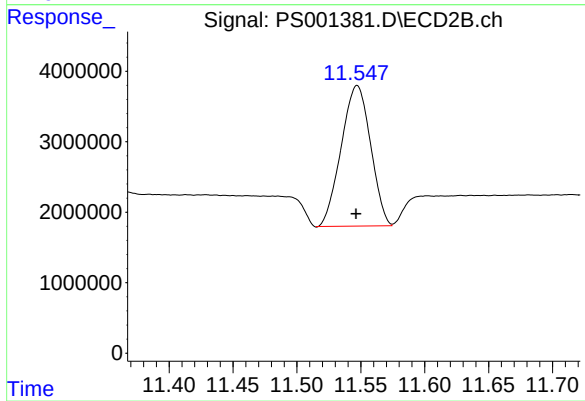

#6 MCP


R.T.: 11.547 min
Delta R.T.: 0.000 min
Response: 31891928
Conc: 73.50 ug/ml m

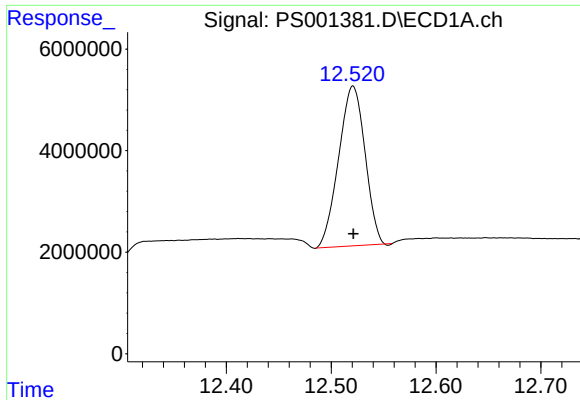

#7 MCPA


R.T.: 12.521 min
Delta R.T.: 0.000 min
Response: 54865852
Conc: 69.57 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

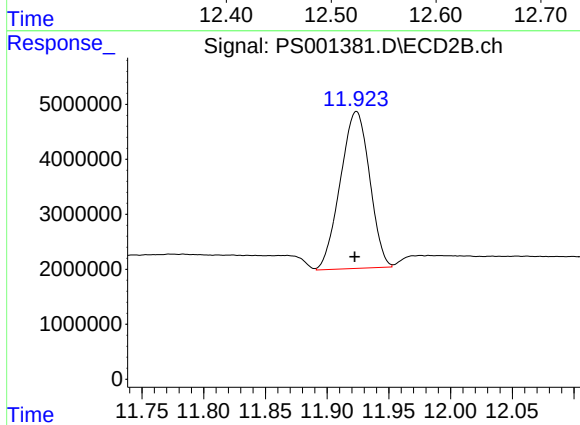


#7 MCPA

R.T.: 11.923 min
Delta R.T.: 0.000 min
Response: 47097129
Conc: 72.43 ug/ml m

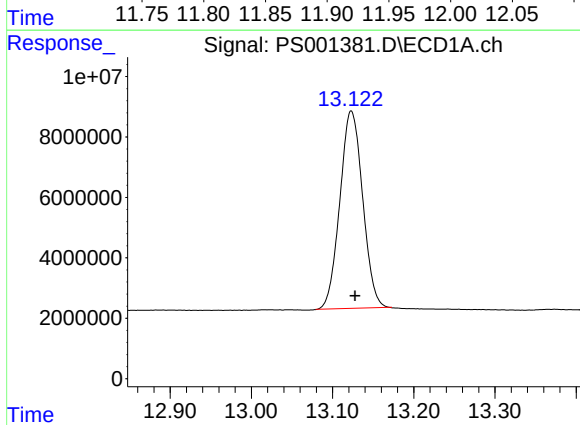


#8 DICHLORPROP

R.T.: 13.122 min
Delta R.T.: -0.005 min
Response: 127496242
Conc: 698.46 ng/ml m

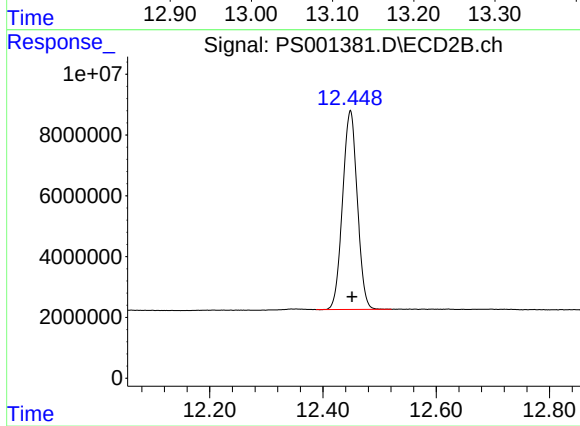

#8 DICHLORPROP


R.T.: 12.448 min
Delta R.T.: -0.003 min
Response: 117975764
Conc: 665.98 ng/ml

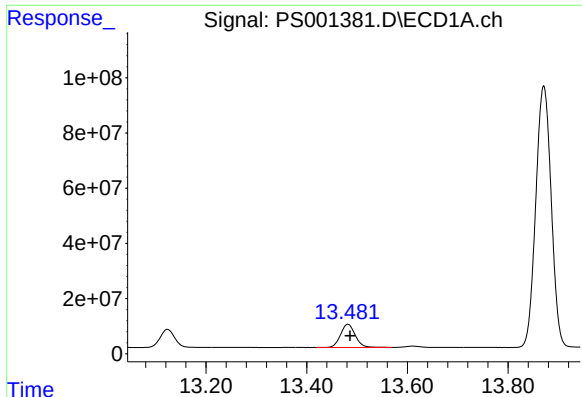

#9 2,4-D


R.T.: 13.482 min
Delta R.T.: -0.004 min
Response: 171510456
Conc: 698.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

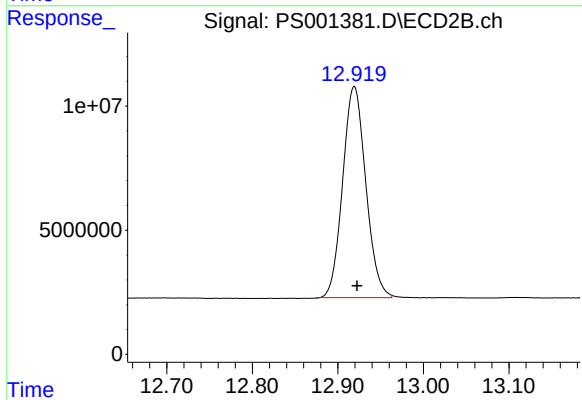


#9 2,4-D

R.T.: 12.919 min
Delta R.T.: -0.004 min
Response: 160009007
Conc: 674.31 ng/ml m

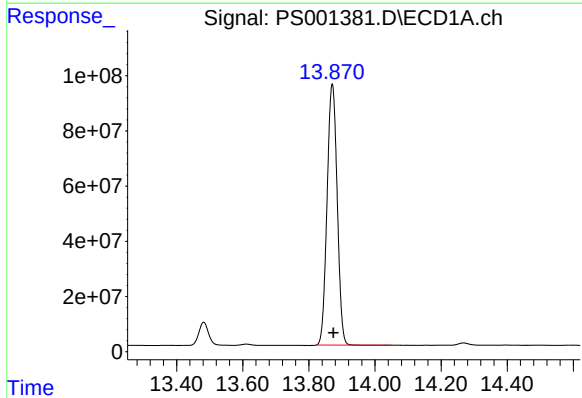


#10 Pentachlorophenol

R.T.: 13.871 min
Delta R.T.: -0.004 min
Response: 2007942839
Conc: 713.17 ng/ml

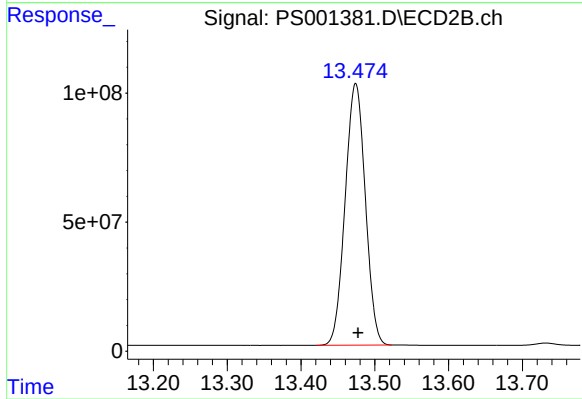

#10 Pentachlorophenol


R.T.: 13.474 min
Delta R.T.: -0.004 min
Response: 1926079940
Conc: 699.84 ng/ml m

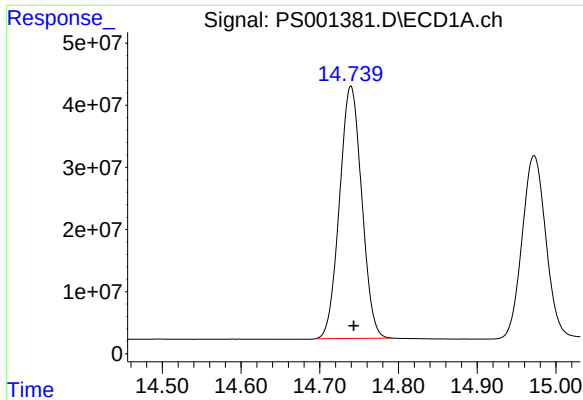

#11 2,4,5-TP (SILVEX)


R.T.: 14.739 min
Delta R.T.: -0.004 min
Response: 795877240
Conc: 709.14 ng/ml m

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

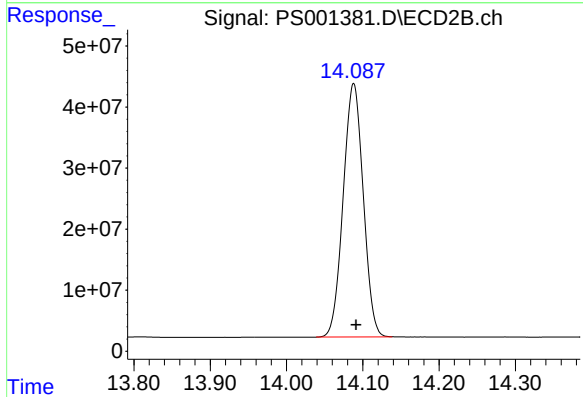


#11 2,4,5-TP (SILVEX)

R.T.: 14.087 min
Delta R.T.: -0.004 min
Response: 758184554
Conc: 693.39 ng/ml m

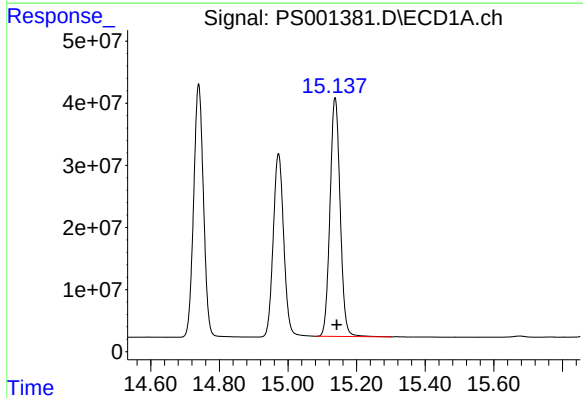


#12 2,4,5-T

R.T.: 15.137 min
Delta R.T.: -0.004 min
Response: 786316585
Conc: 706.65 ng/ml

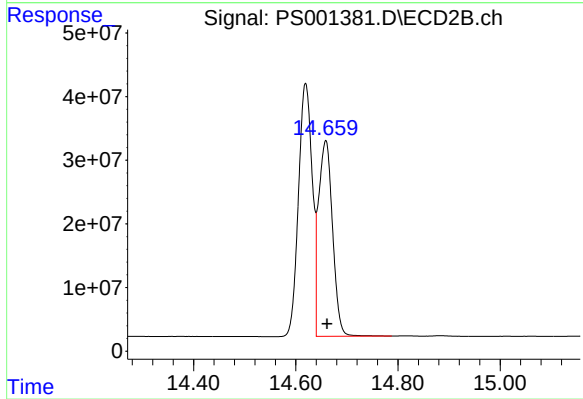

#12 2,4,5-T


R.T.: 14.659 min
Delta R.T.: -0.003 min
Response: 579880374
Conc: 627.76 ng/ml

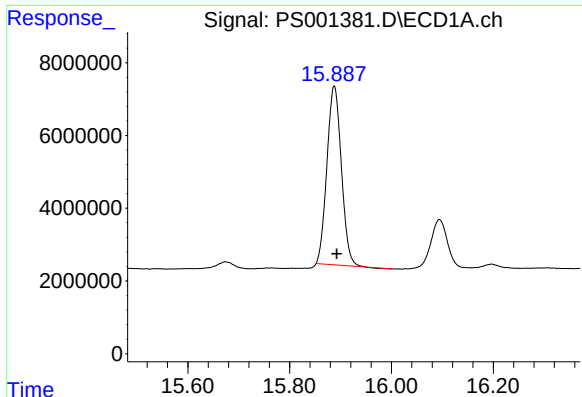

#13 2,4-DB


R.T.: 15.888 min
Delta R.T.: -0.005 min
Response: 96334989
Conc: 669.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

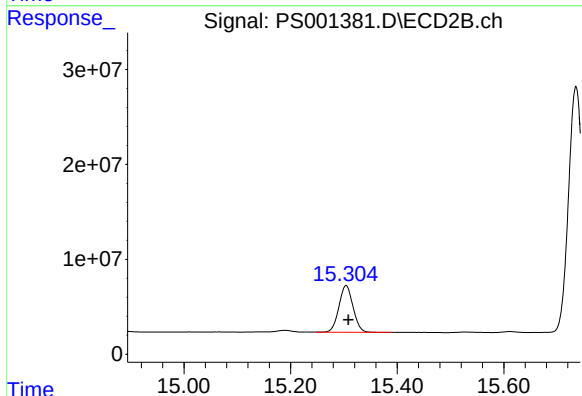


#13 2,4-DB

R.T.: 15.304 min
Delta R.T.: -0.004 min
Response: 90396124
Conc: 678.84 ng/ml

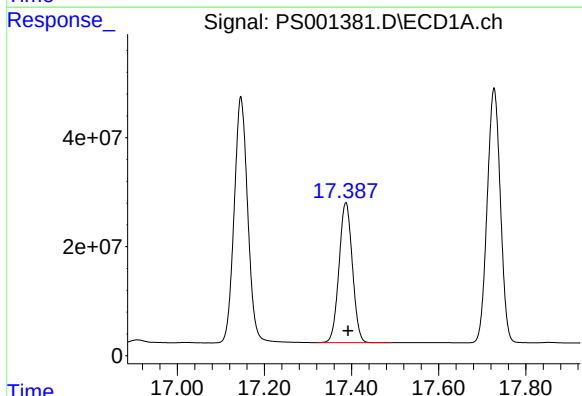


#14 DINOSEB

R.T.: 17.387 min
Delta R.T.: -0.005 min
Response: 544798332
Conc: 709.31 ng/ml

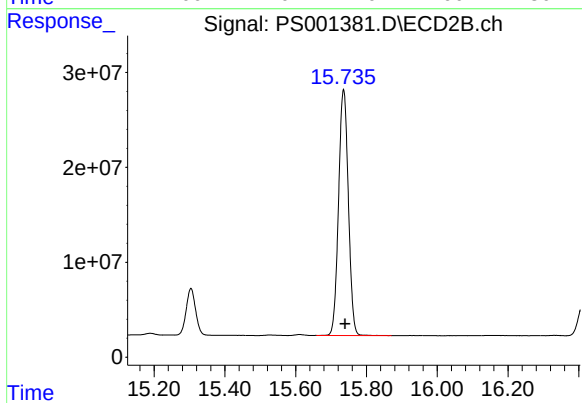

#14 DINOSEB


R.T.: 15.735 min
Delta R.T.: -0.004 min
Response: 496764186
Conc: 698.87 ng/ml

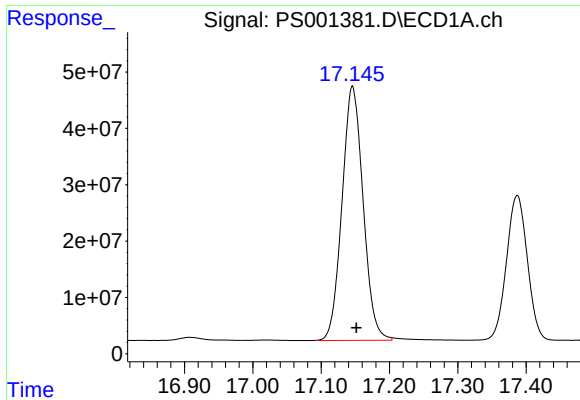

#15 Picloram


R.T.: 17.145 min
Delta R.T.: -0.006 min
Response: 967492423
Conc: 612.09 ng/ml m

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

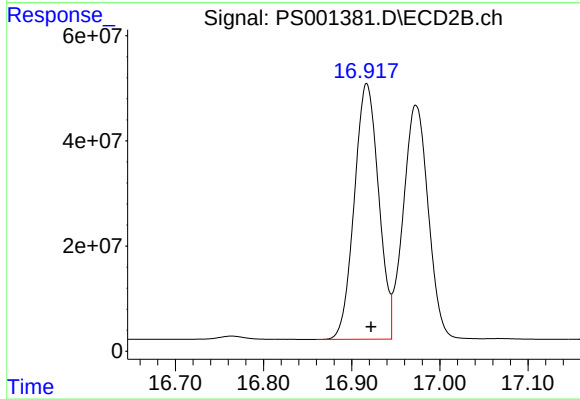


#15 Picloram

R.T.: 16.917 min
Delta R.T.: -0.005 min
Response: 932476815
Conc: 676.44 ng/ml

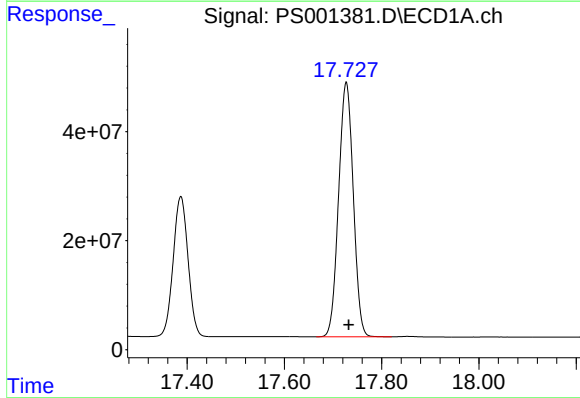

#16 DCPA

R.T.: 17.727 min
Delta R.T.: -0.005 min
Response: 977133337
Conc: 723.76 ng/ml

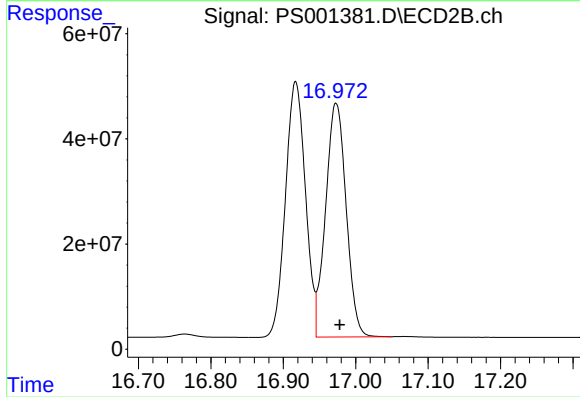

#16 DCPA

R.T.: 16.973 min
Delta R.T.: -0.005 min
Response: 876066966
Conc: 606.57 ng/ml