

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080322\
 Data File : PS020168.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2022 02:46
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 04:40:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.185	6.761	1397.0E6	424.4E6	473.775	520.813
Target Compounds							
1) T	Dalapon	3.005	0.000	535269	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.389	0.000	746220	0	<MDL	N.D. #
5) T	DICAMBA	0.000	6.987f	0	1187693	N.D.	<MDL
6) T	MCP	7.474f	6.987	1041973	1187693	<MDL	<MDL #
7) T	MCPA	7.708	0.000	7696902	0	<MDL	N.D. #
10) T	Pentachlo...	8.601	8.260	3685352	1511141	<MDL	<MDL #
11) T	2,4,5-TP ...	9.161	0.000	2586404	0	<MDL	N.D. #
12) T	2,4,5-T	9.419	0.000	17333343	0	<MDL	N.D. #
13) T	2,4-DB	9.958	0.000	2889435	0	<MDL	N.D. #
14) T	DINOSEB	11.131	0.000	21996088	0	1.383	N.D. #
15) T	Picloram	10.952	10.857f	82544737	18687446	2.611	2.477
16) T	DCPA	11.405	10.752	5163425	2524162	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080322\
Data File : PS020168.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2022 02:46
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 04:40:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

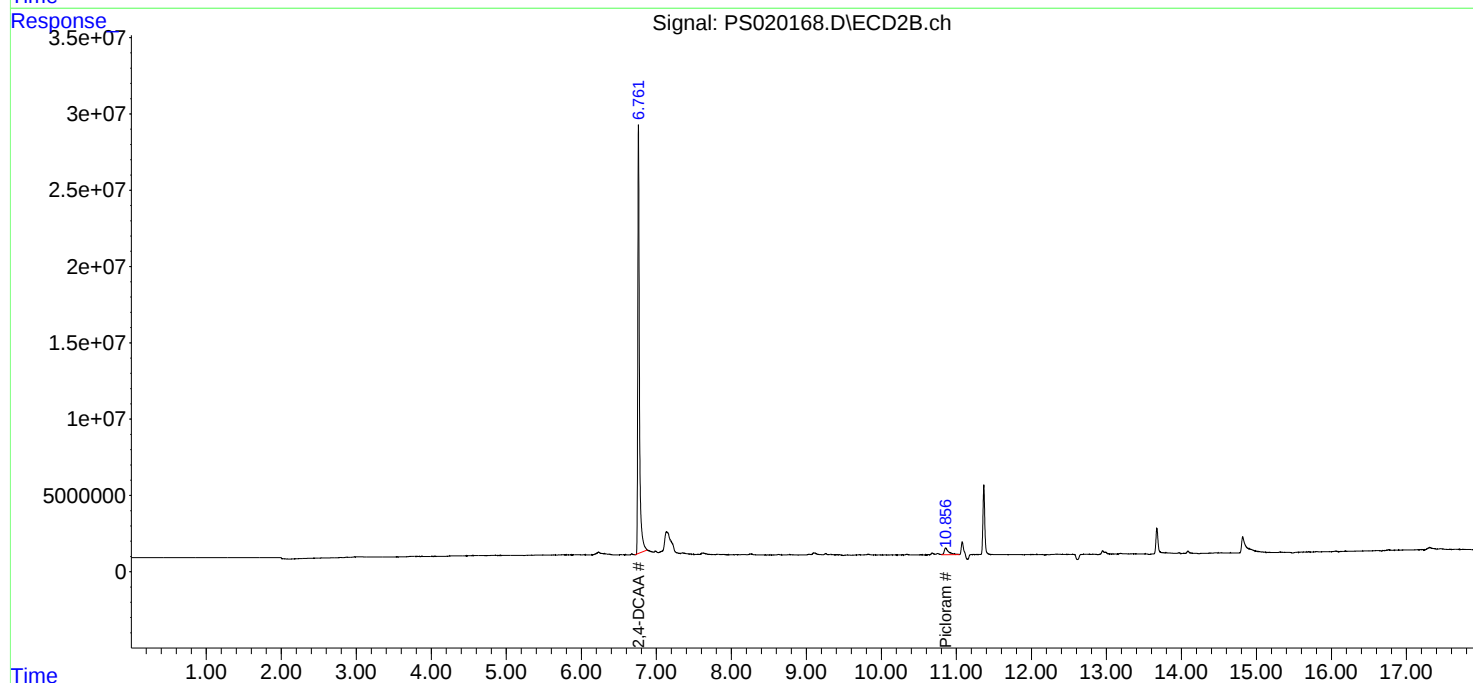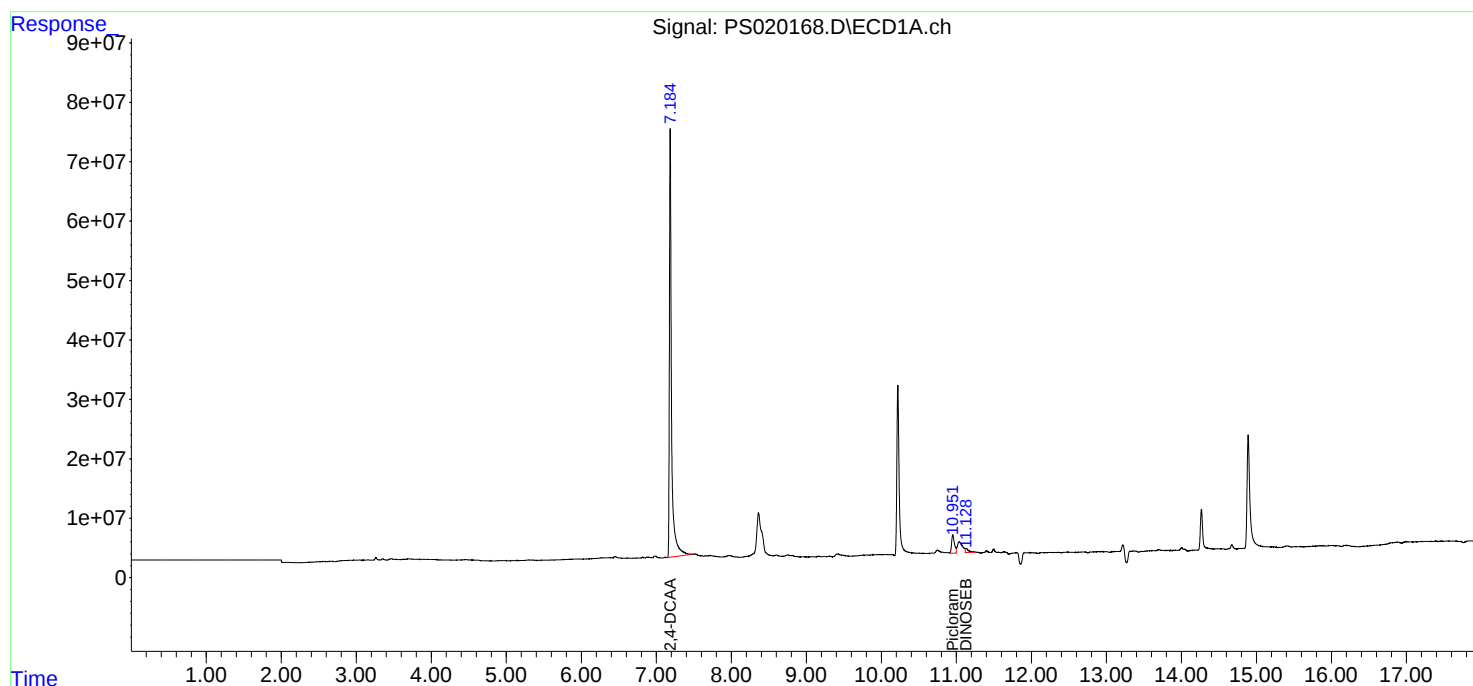


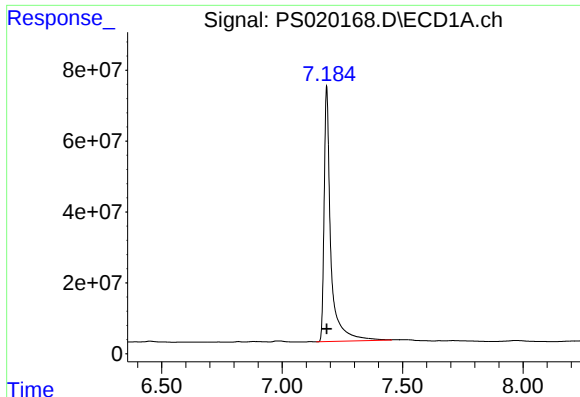

#4 2,4-DCAA


R.T.: 7.185 min
Delta R.T.: 0.000 min
Response: 1397031174
Conc: 473.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

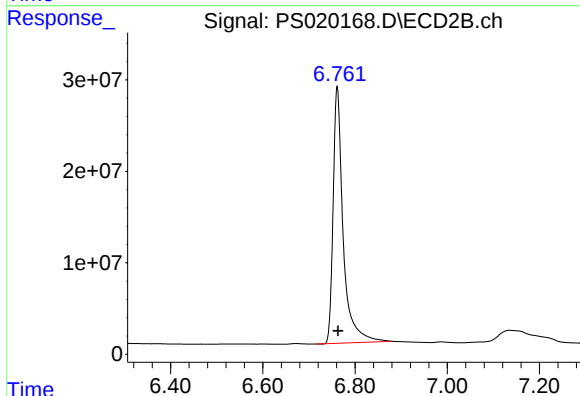


#4 2,4-DCAA

R.T.: 6.761 min
Delta R.T.: -0.002 min
Response: 424439806
Conc: 520.81 ng/ml

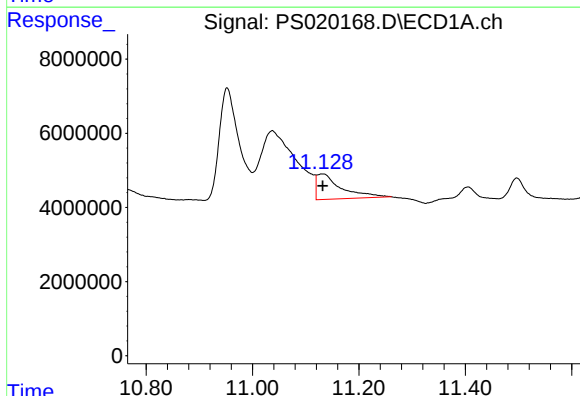


#14 DINOSEB

R.T.: 11.131 min
Delta R.T.: 0.000 min
Response: 21996088
Conc: 1.38 ng/ml

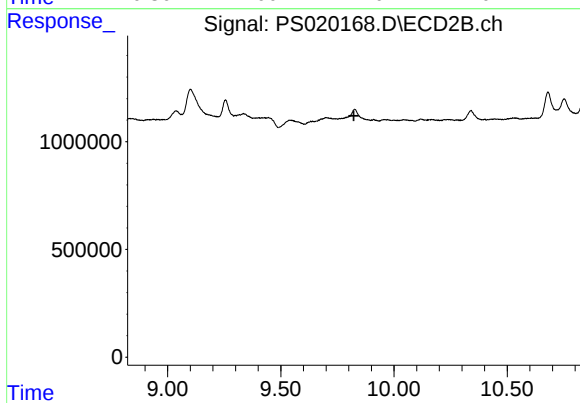

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.823 min
Response: 0
Conc: N.D.

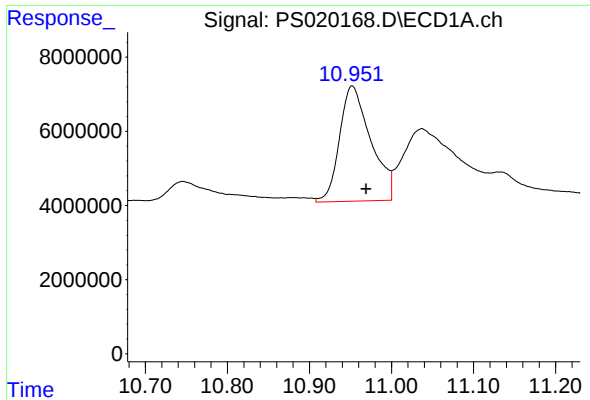

#15 Picloram

R.T.: 10.952 min
Delta R.T.: -0.017 min
Response: 82544737
Conc: 2.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

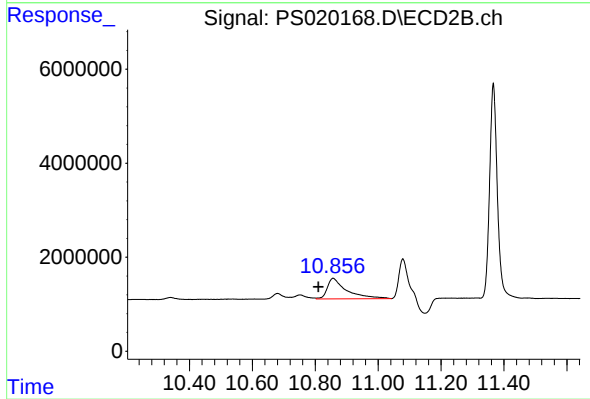

#15 Picloram

R.T.: 10.857 min
Delta R.T.: 0.047 min
Response: 18687446
Conc: 2.48 ng/ml