

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080422\
 Data File : PS020170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2022 08:46
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 02:43:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.190	0.000	722479	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	3.047f	0.000	1041889	0	<MDL	N.D. #
3) T	4-Nitroph...	7.025	0.000	640373	0	<MDL	N.D. #
5) T	DICAMBA	7.366	0.000	1109725	0	<MDL	N.D. #
6) T	MCP	7.526	0.000	3279006	0	<MDL	N.D. #
7) T	MCPA	7.686	0.000	1382149	0	<MDL	N.D. #
8) T	DICHLORPROP	8.104f	0.000	1745703	0	<MDL	N.D. #
9) T	2,4-D	8.301	0.000	1474347	0	<MDL	N.D. #
10) T	Pentachlo...	8.607	0.000	940770	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.155	0.000	676307	0	<MDL	N.D. #
12) T	2,4,5-T	9.461	0.000	2712132	0	<MDL	N.D. #
13) T	2,4-DB	10.059f	0.000	888994	0	<MDL	N.D. #
14) T	DINOSEB	11.137	0.000	3081332	0	<MDL	N.D. #
15) T	Picloram	11.003	10.833	101.7E6	32956199	3.216	4.368 #
16) T	DCPA	11.400	0.000	2303287	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080422\
Data File : PS020170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2022 08:46
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 02:43:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

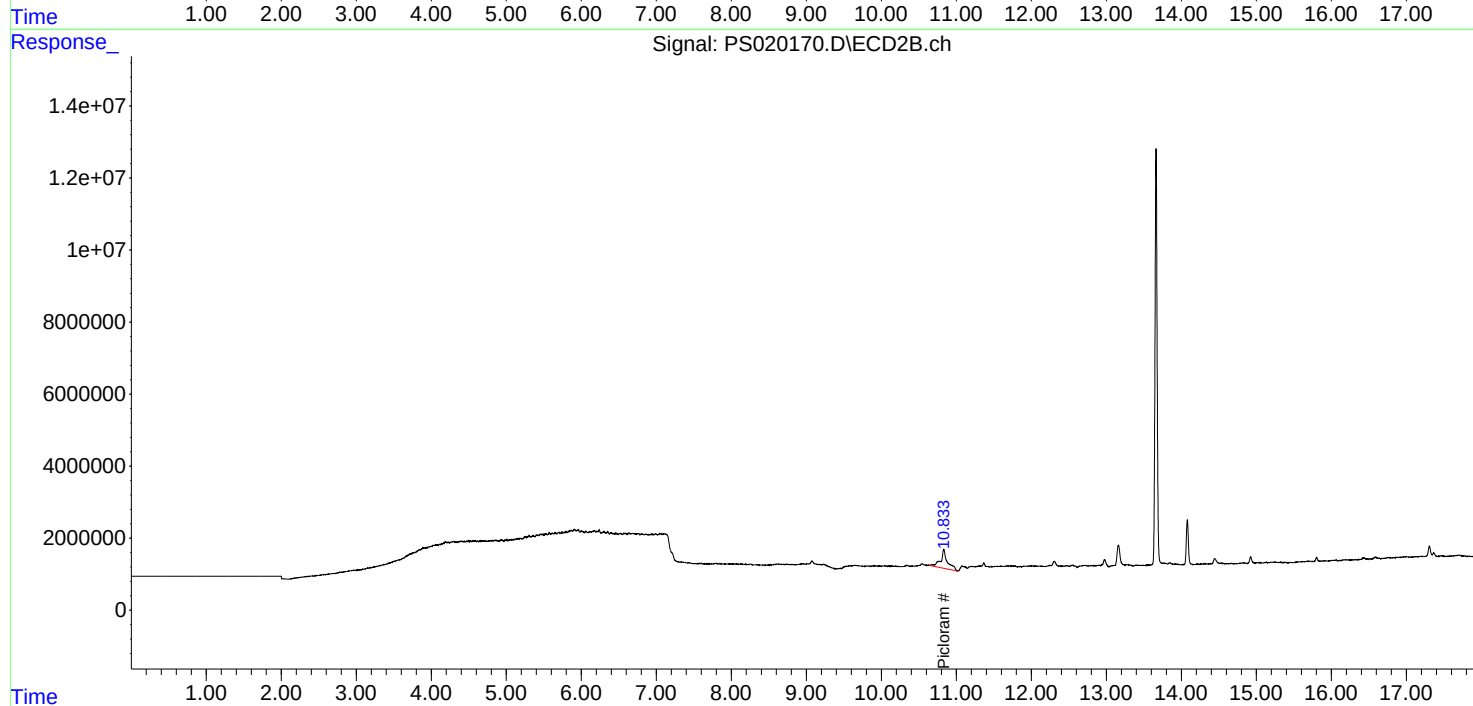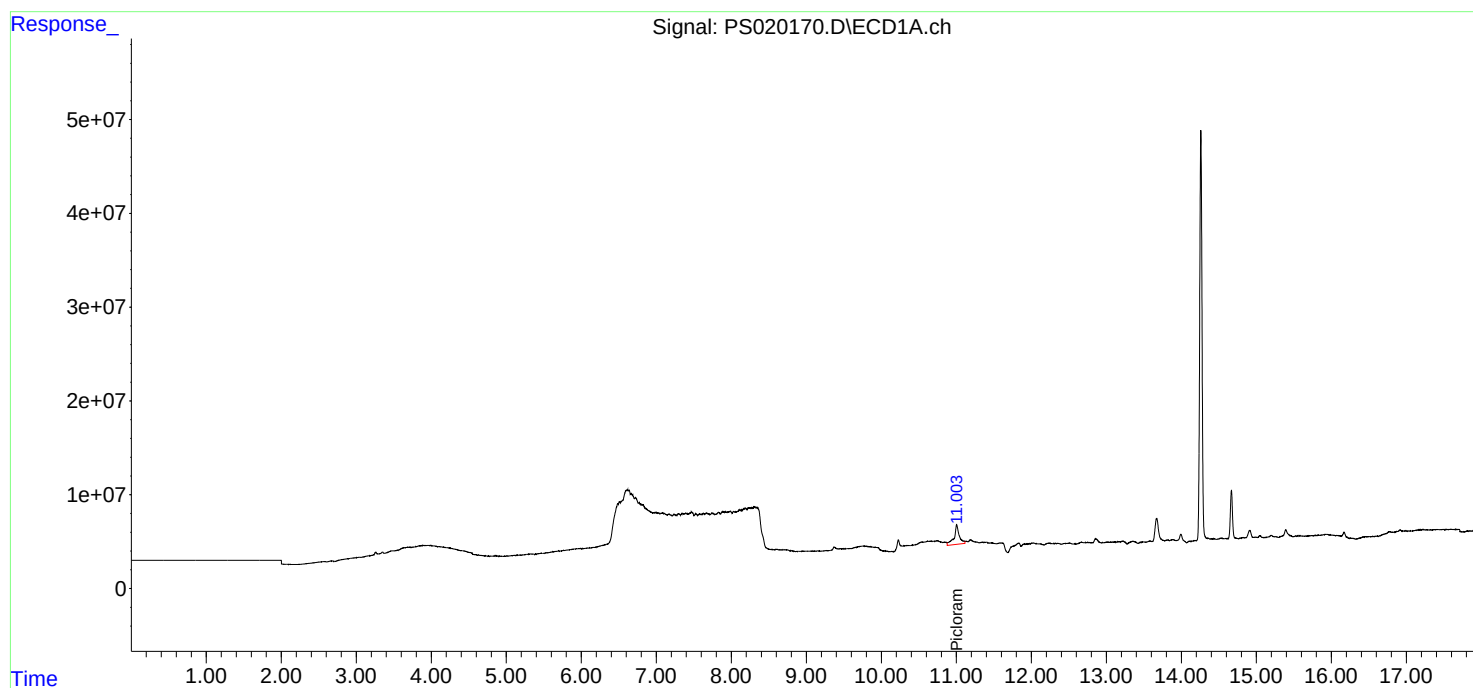


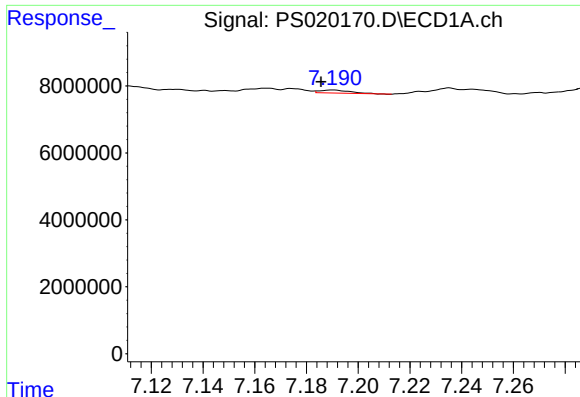

#4 2,4-DCAA


R.T.: 7.190 min
Delta R.T.: 0.005 min
Response: 722479
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

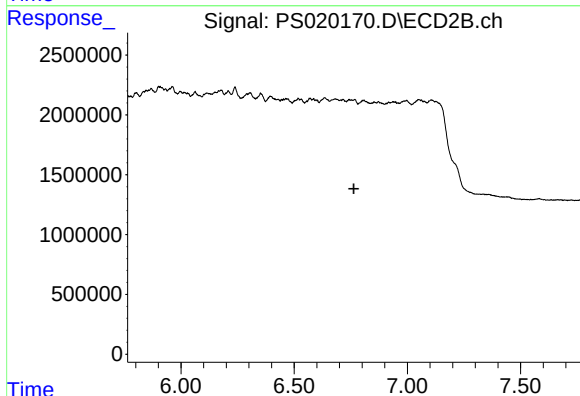


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

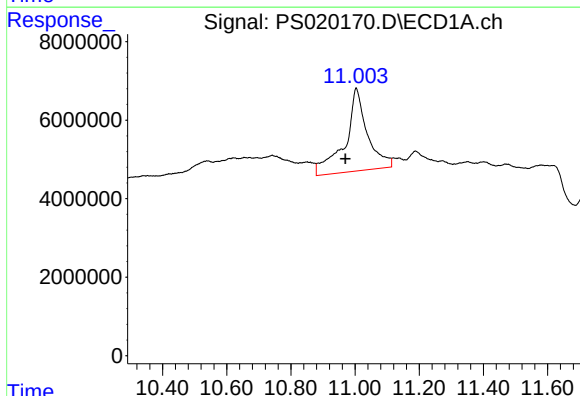

#15 Picloram

R.T.: 11.003 min
Delta R.T.: 0.034 min
Response: 101693998
Conc: 3.22 ng/ml

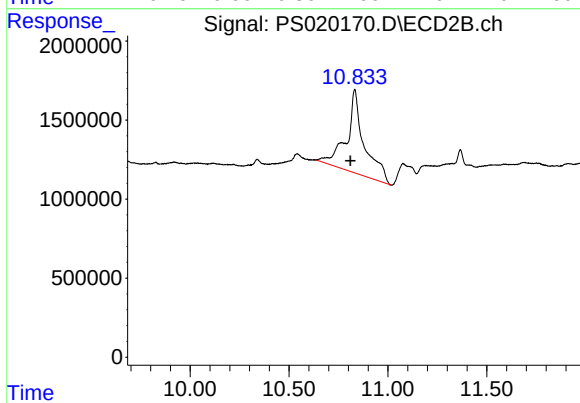

#15 Picloram

R.T.: 10.833 min
Delta R.T.: 0.023 min
Response: 32956199
Conc: 4.37 ng/ml