

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080422\
 Data File : PS020171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2022 09:11
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 02:43:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.186	6.762	1391.2E6	422.5E6	471.804	518.408
Target Compounds							
1) T	Dalapon	3.042	0.000	1482760	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.454f	0.000	7145388	0	1.837	N.D. #
5) T	DICAMBA	0.000	6.988f	0	1594108	N.D.	<MDL
6) T	MCP	7.472f	6.988	1069704	1594108	<MDL	<MDL #
11) T	2,4,5-TP ...	9.168	0.000	641663	0	<MDL	N.D. #
12) T	2,4,5-T	9.441	0.000	11641848	0	<MDL	N.D. #
13) T	2,4-DB	10.017	0.000	1114477	0	<MDL	N.D. #
15) T	Picloram	10.959	10.868f	84870213	7867290	2.684	1.043 #
16) T	DCPA	11.412	10.682f	1598773	1759567	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080422\
Data File : PS020171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2022 09:11
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 02:43:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

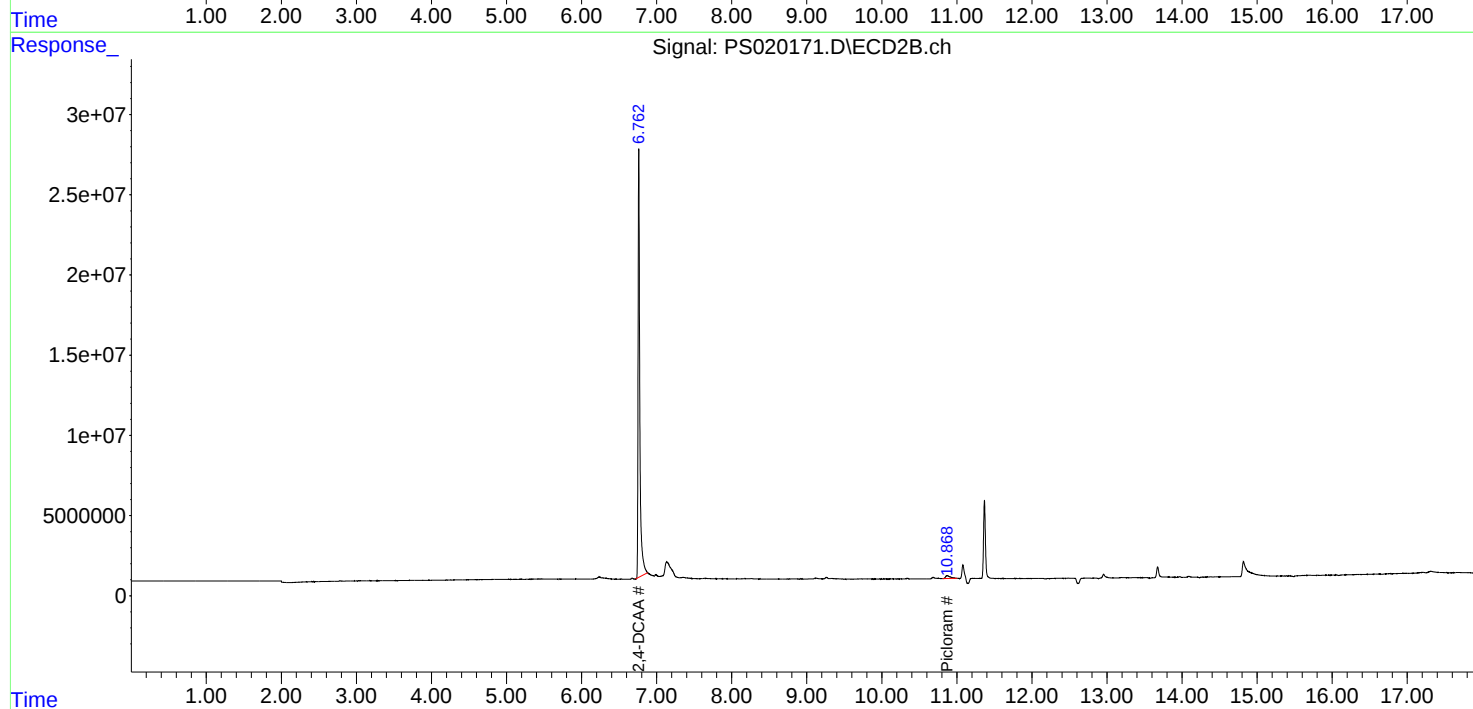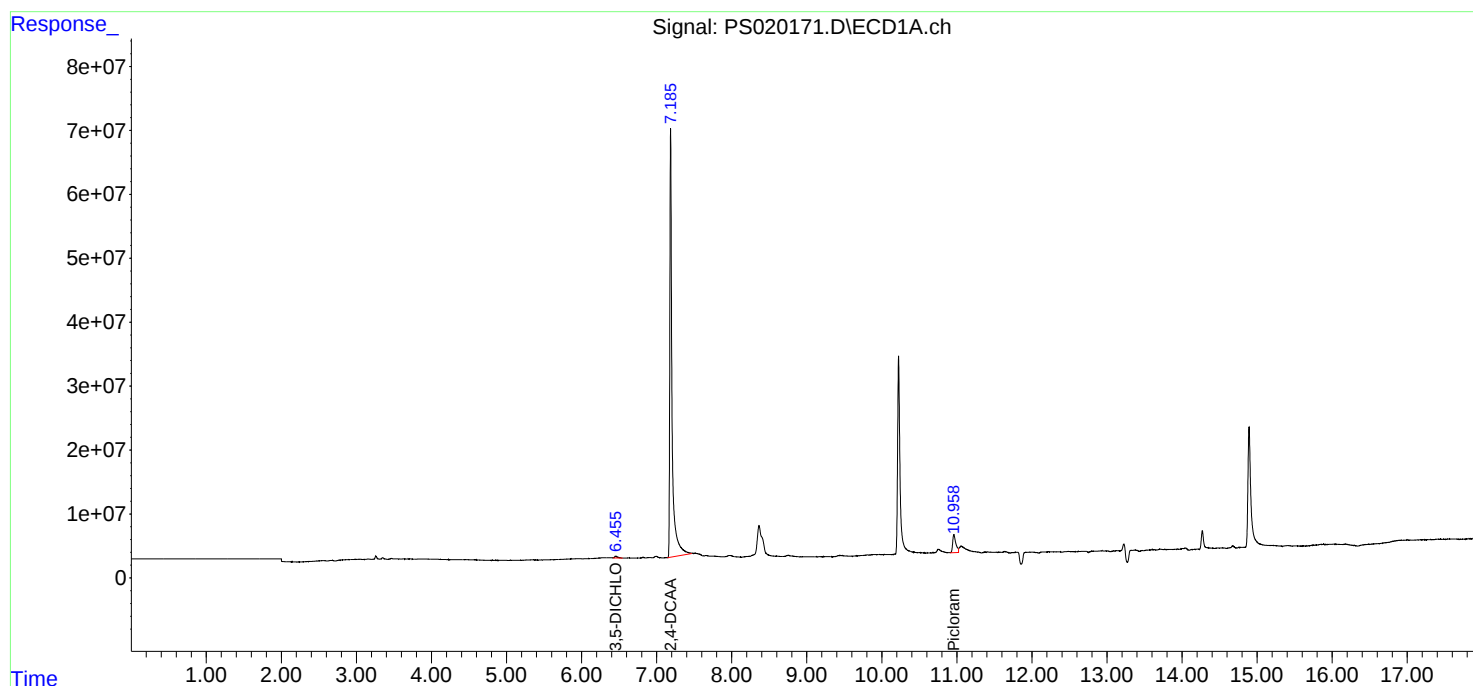


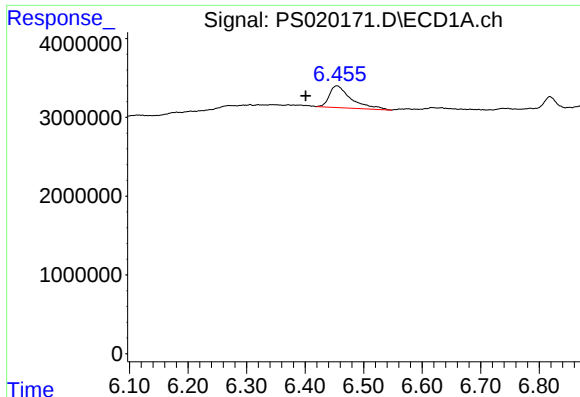

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.454 min
Delta R.T.: 0.053 min
Response: 7145388
Conc: 1.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

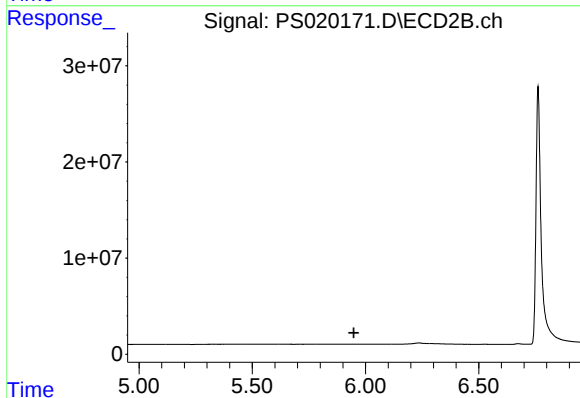


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

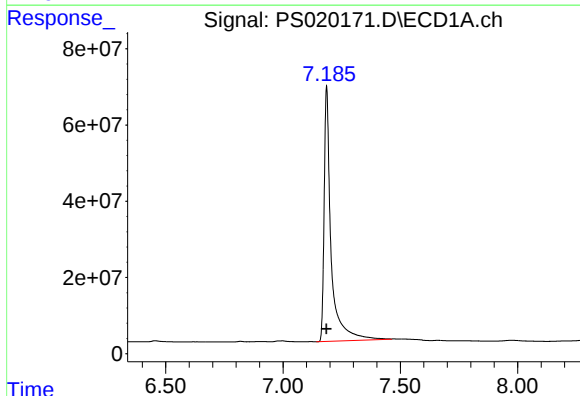


#4 2,4-DCAA

R.T.: 7.186 min
Delta R.T.: 0.000 min
Response: 1391219293
Conc: 471.80 ng/ml

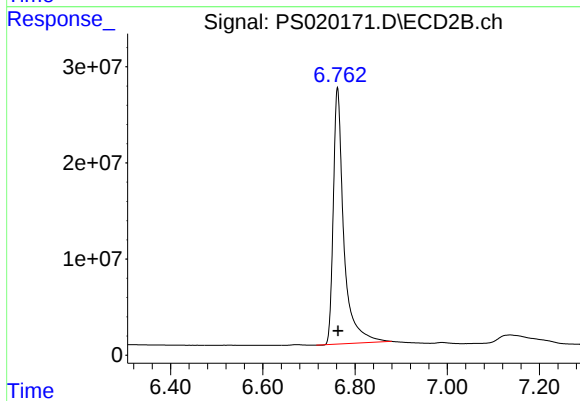

#4 2,4-DCAA


R.T.: 6.762 min
Delta R.T.: -0.001 min
Response: 422479428
Conc: 518.41 ng/ml

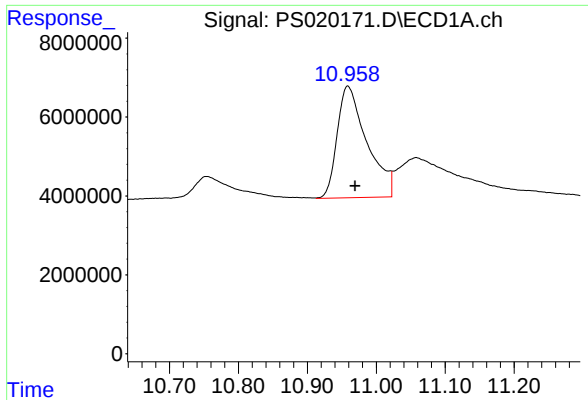

#15 Picloram

R.T.: 10.959 min
Delta R.T.: -0.010 min
Response: 84870213
Conc: 2.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

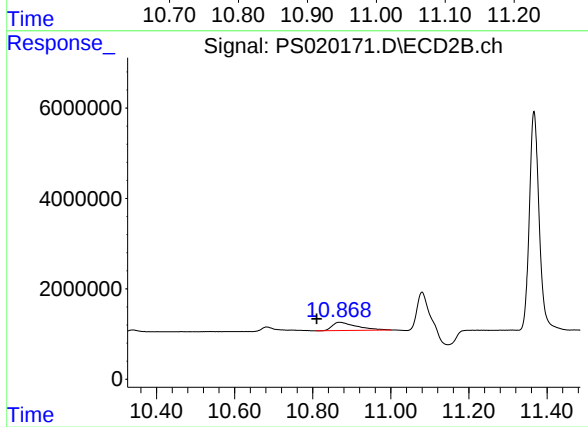

#15 Picloram

R.T.: 10.868 min
Delta R.T.: 0.057 min
Response: 7867290
Conc: 1.04 ng/ml