

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080422\
 Data File : PS020182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Aug 2022 15:53
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 02:51:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.185	6.762	1429.1E6	428.3E6	484.651	525.513
Target Compounds							
1) T	Dalapon	3.046f	0.000	1748838	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.397	0.000	518214	0	<MDL	N.D. #
5) T	DICAMBA	0.000	6.987f	0	3175098	N.D.	<MDL
6) T	MCP	7.519	6.987	5159529	3175098	<MDL	1.164 #
7) T	MCPA	7.654	0.000	2492323	0	<MDL	N.D. #
9) T	2,4-D	8.365f	0.000	39873762	0	13.240	N.D. #
11) T	2,4,5-TP ...	9.165	0.000	885400	0	<MDL	N.D. #
12) T	2,4,5-T	9.429	0.000	8667098	0	<MDL	N.D. #
13) T	2,4-DB	10.004	0.000	1258369	0	<MDL	N.D. #
15) T	Picloram	10.950	10.877f	137.1E6	2875771	4.337	<MDL #
16) T	DCPA	11.406	0.000	607903	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080422\
Data File : PS020182.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Aug 2022 15:53
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 02:51:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

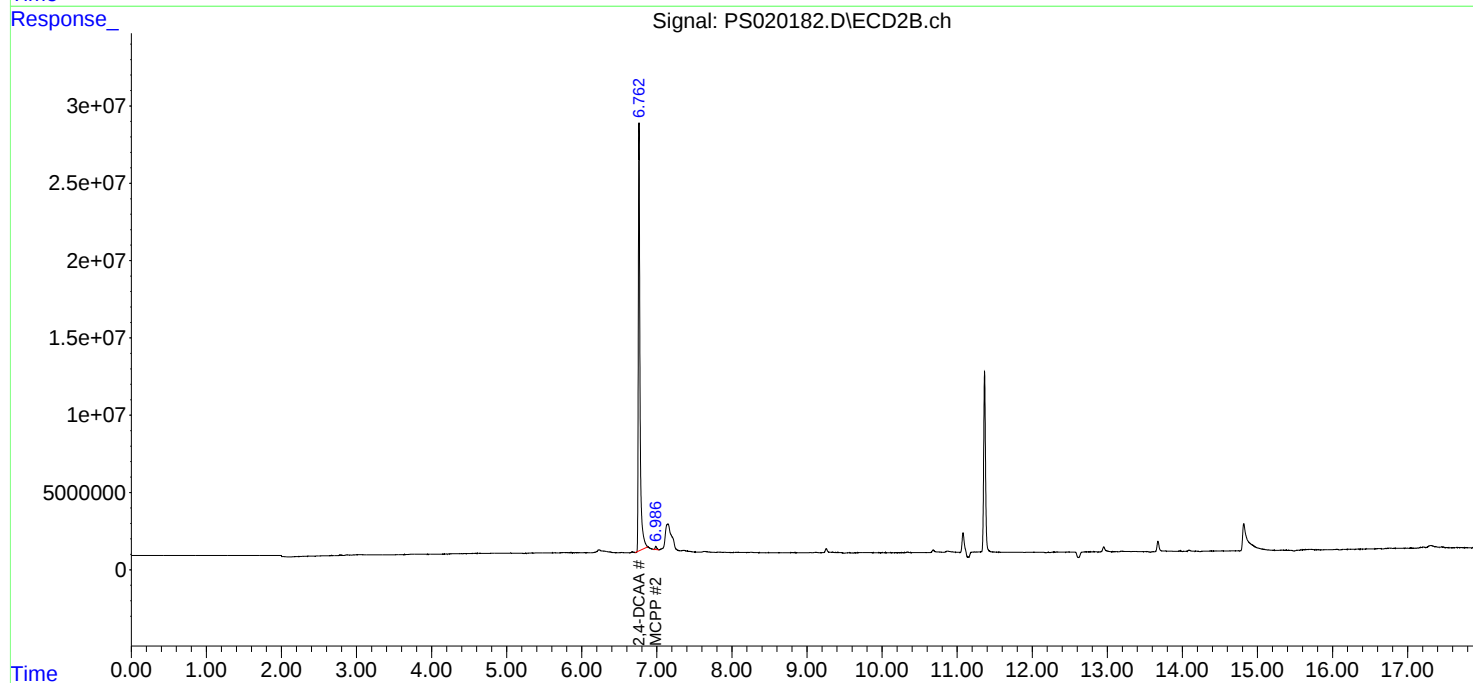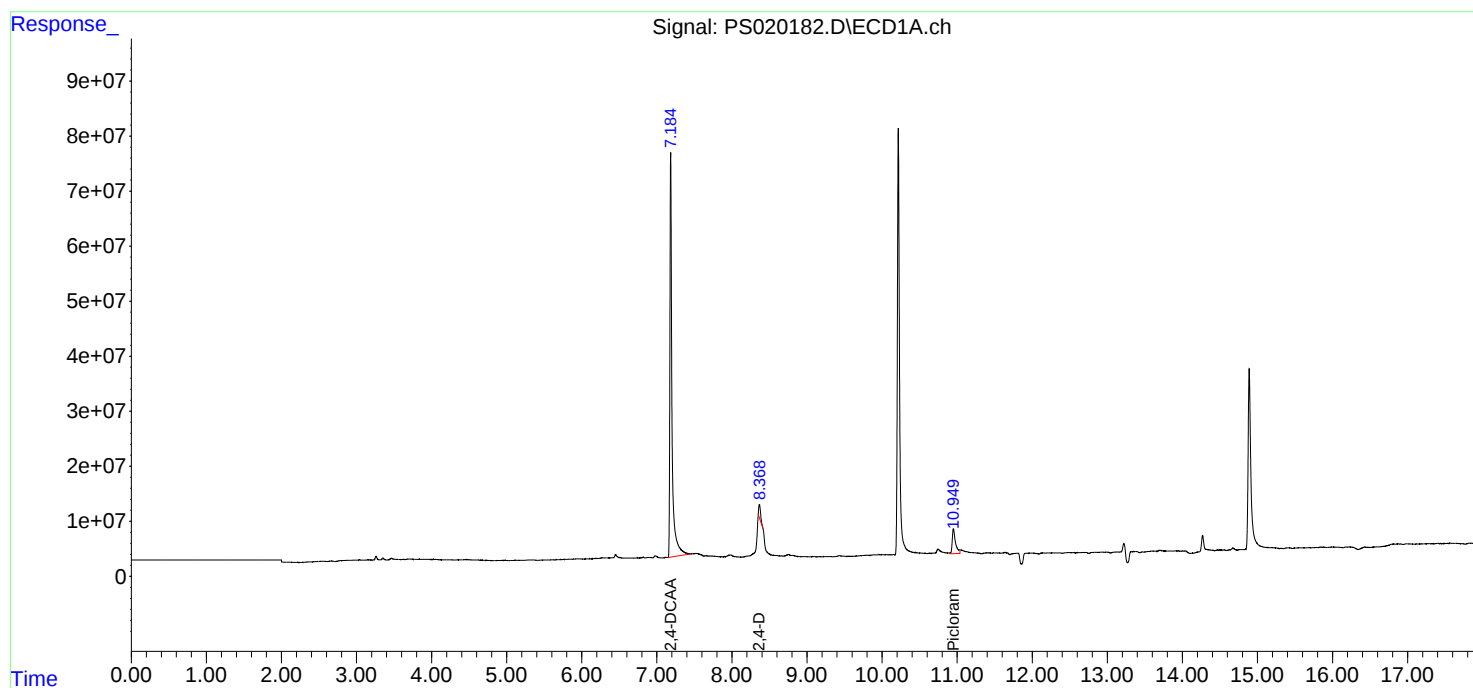


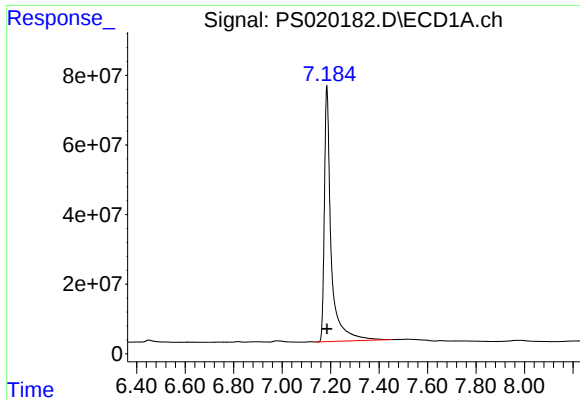

#4 2,4-DCAA


R.T.: 7.185 min
Delta R.T.: 0.000 min
Response: 1429101002
Conc: 484.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

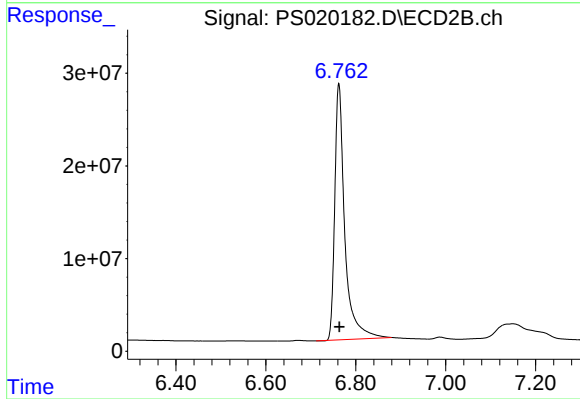


#4 2,4-DCAA

R.T.: 6.762 min
Delta R.T.: -0.001 min
Response: 428269666
Conc: 525.51 ng/ml

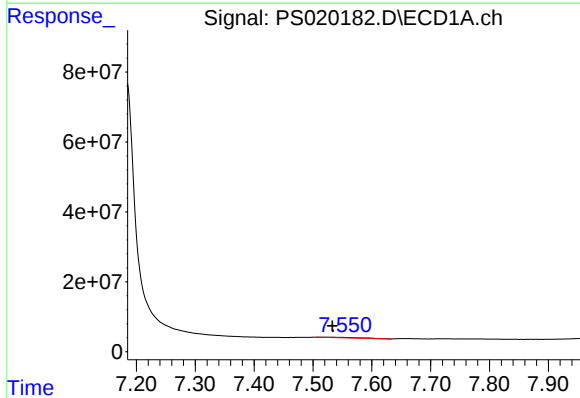


#6 MCPP

R.T.: 7.519 min
Delta R.T.: -0.014 min
Response: 5159529
Conc: N.D.

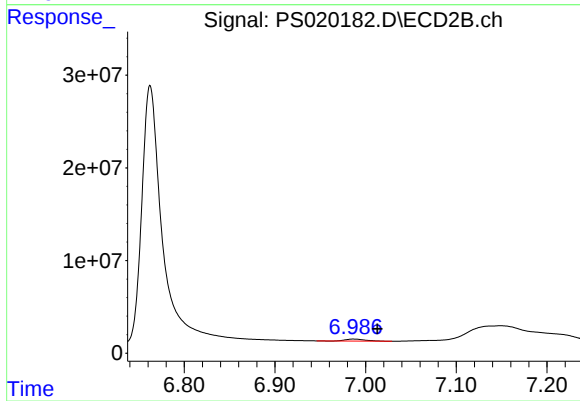

#6 MCPP


R.T.: 6.987 min
Delta R.T.: -0.026 min
Response: 3175098
Conc: 1.16 ug/ml

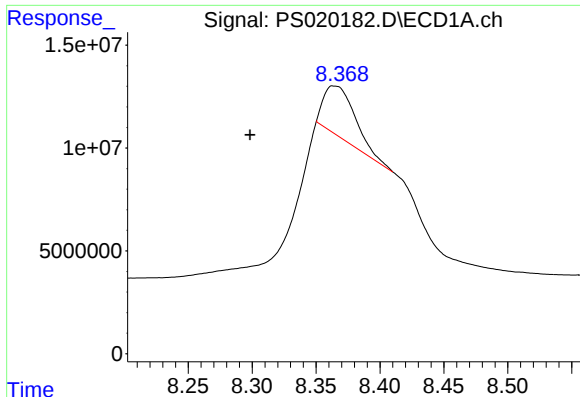

#9 2,4-D


R.T.: 8.365 min
Delta R.T.: 0.066 min
Response: 39873762
Conc: 13.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

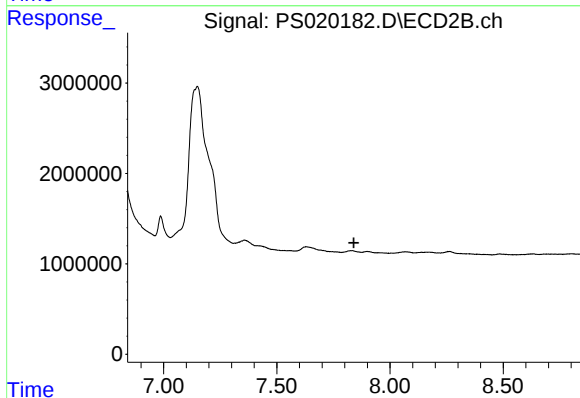


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.840 min
Response: 0
Conc: N.D.

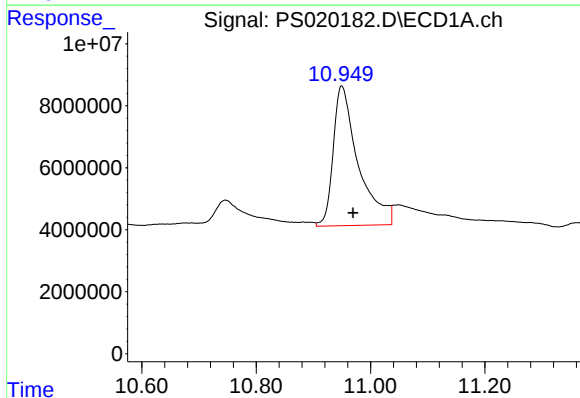

#15 Picloram

R.T.: 10.950 min
Delta R.T.: -0.019 min
Response: 137141329
Conc: 4.34 ng/ml

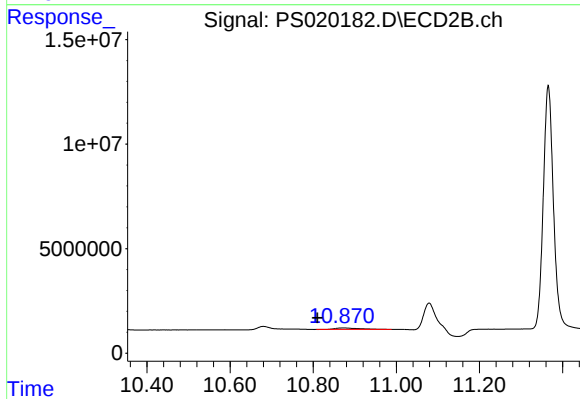

#15 Picloram

R.T.: 10.877 min
Delta R.T.: 0.067 min
Response: 2875771
Conc: N.D.