

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080519\
 Data File : PS005846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2019 10:59
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 17:17:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	4.945	0.000	1160.8E6	0	559.630	N.D.	#
3) T	4-Nitroph...	5.412	0.000	300.8E6	0	499.985	N.D.	#
6) T	MCP	5.909	0.000	327.4E6	0	70.654	N.D.	#
7) T	MCPA	6.023	0.000	143.7E6	0	22.021	N.D.	#
8) T	DICHLORPROP	6.339	0.000	176.6E6	0	122.801	N.D.	#
9) T	2,4-D	6.551	0.000	315.5E6	0	210.497	N.D.	#
10) T	Pentachlo...	6.835	0.000	97523449	0	4.665	N.D.	#
12) T	2,4,5-T	7.667	0.000	19404897	0	2.325	N.D.	#
15) T	Picloram	9.137	0.000	22873899	0	1.954	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080519\
Data File : PS005846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2019 10:59
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 17:17:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

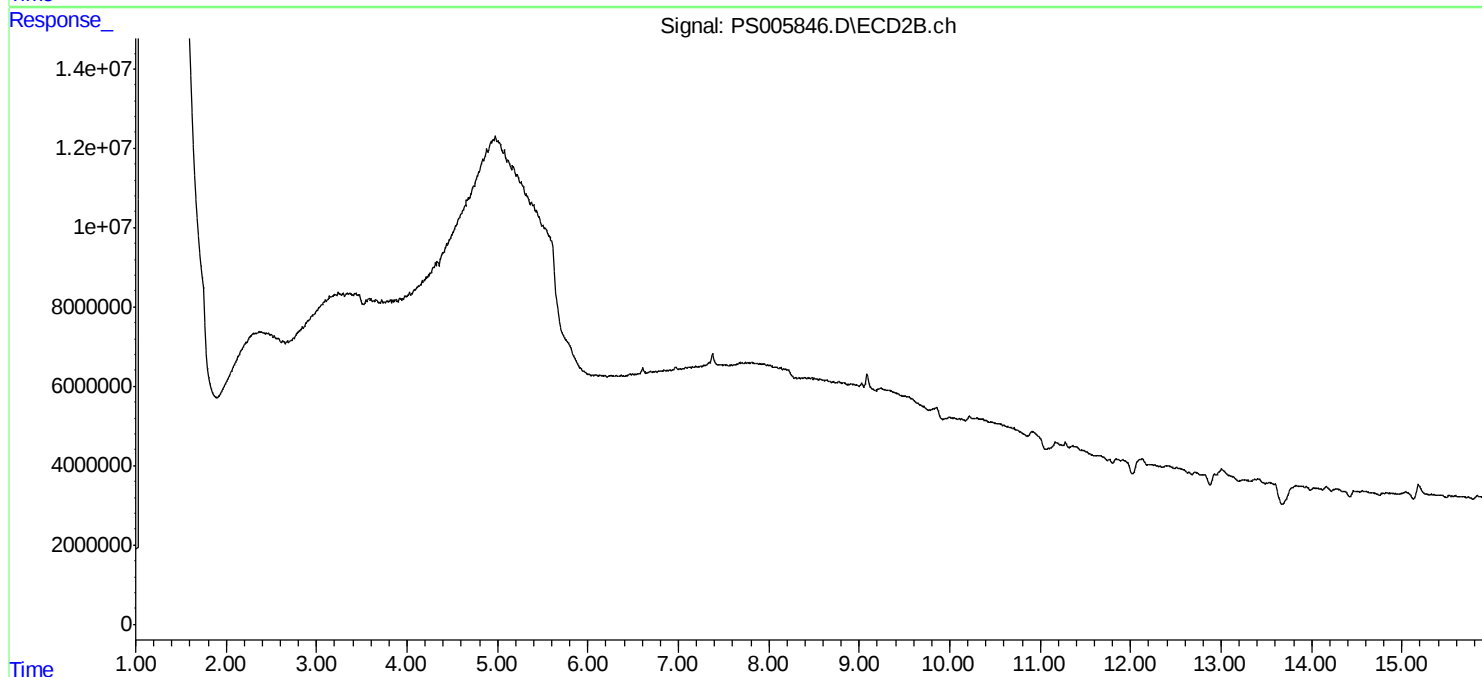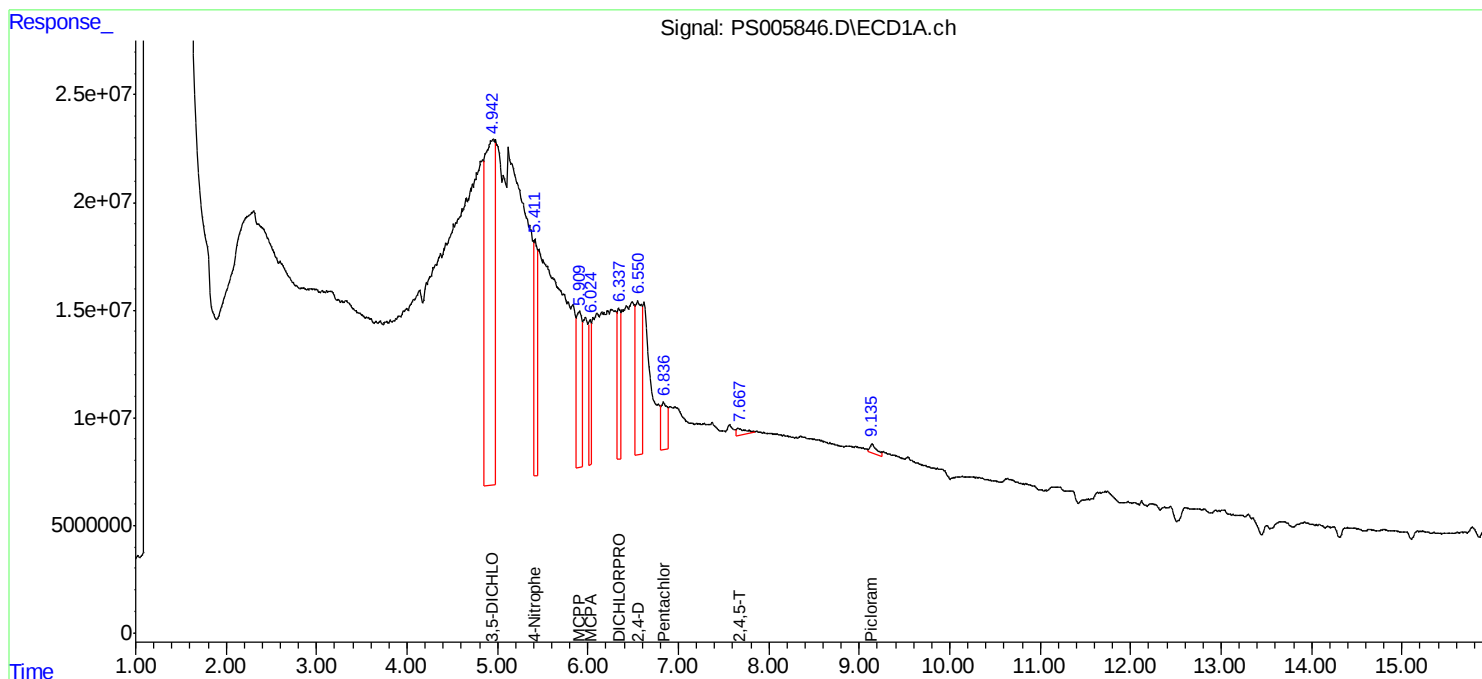


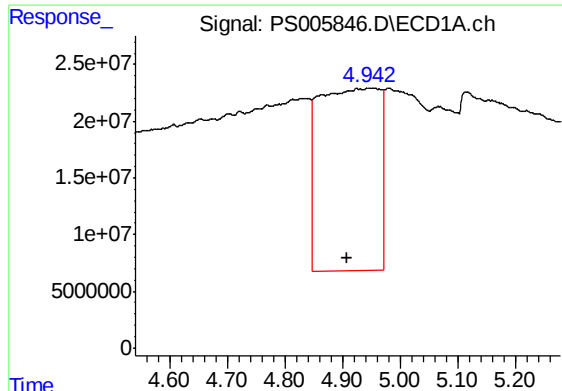

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.945 min
Delta R.T.: 0.036 min
Response: 1160764295
Conc: 559.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

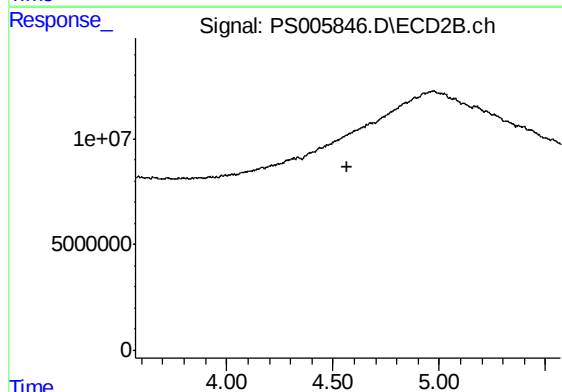


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.570 min
Response: 0
Conc: N.D.

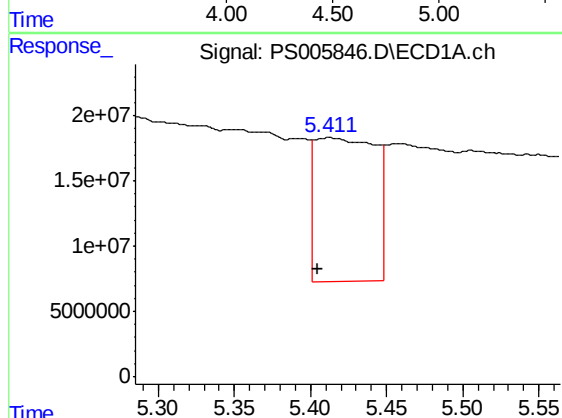


#3 4-Nitrophenol

R.T.: 5.412 min
Delta R.T.: 0.008 min
Response: 300754594
Conc: 499.98 ng/ml

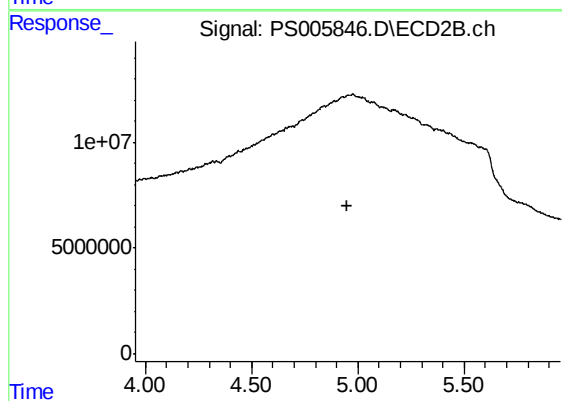

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

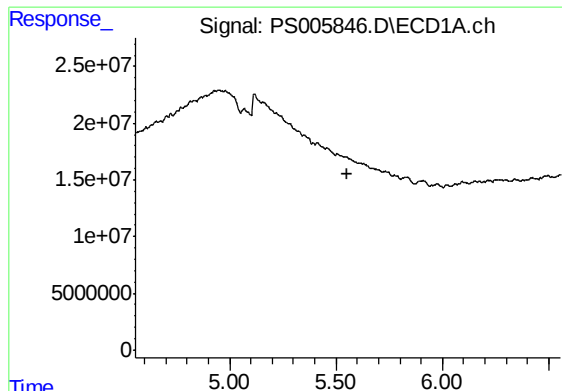

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.556 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

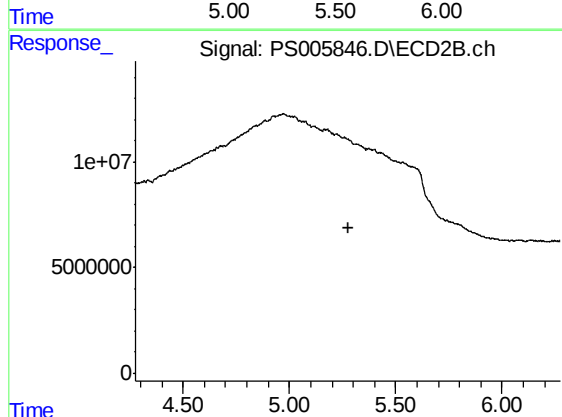


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.276 min
Response: 0
Conc: N.D.

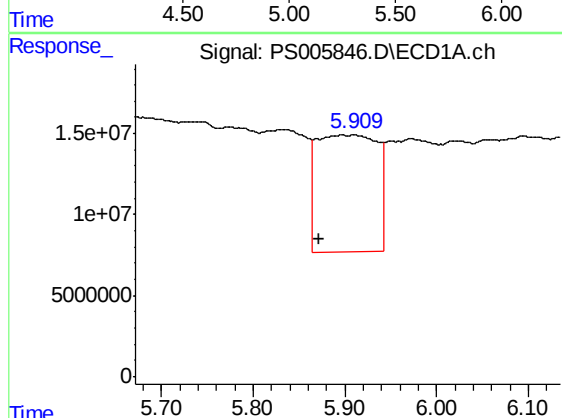


#6 MCP

R.T.: 5.909 min
Delta R.T.: 0.037 min
Response: 327367843
Conc: 70.65 ug/ml

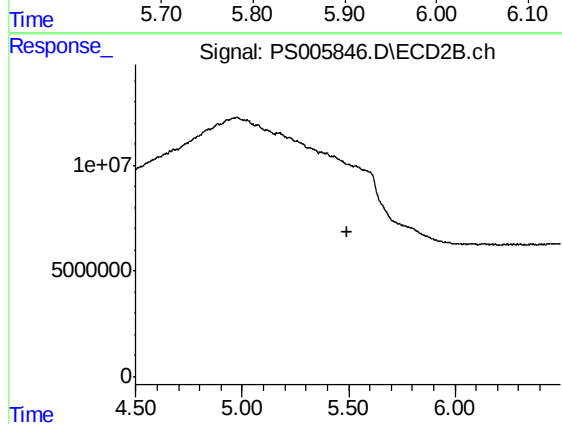

#6 MCP


R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

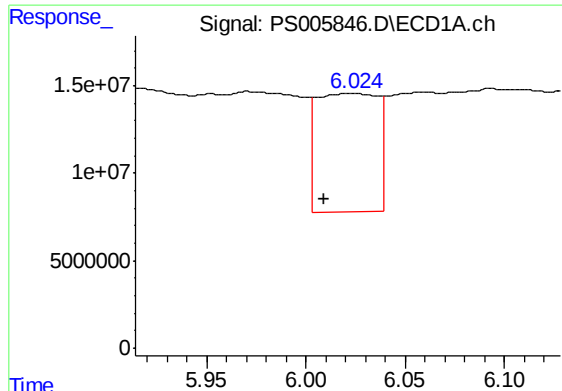

#7 MCPA


R.T.: 6.023 min
Delta R.T.: 0.014 min
Response: 143702626
Conc: 22.02 ug/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

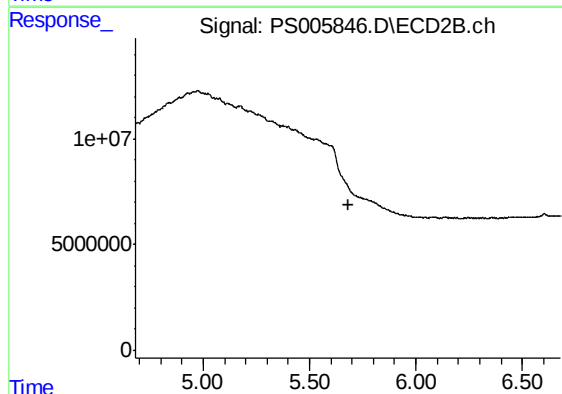


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.681 min
Response: 0
Conc: N.D.

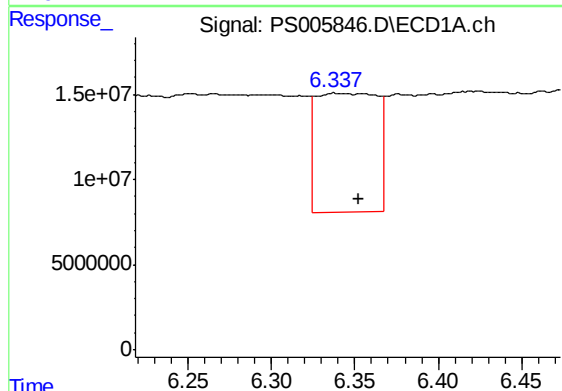


#8 DICHLORPROP

R.T.: 6.339 min
Delta R.T.: -0.013 min
Response: 176595420
Conc: 122.80 ng/ml

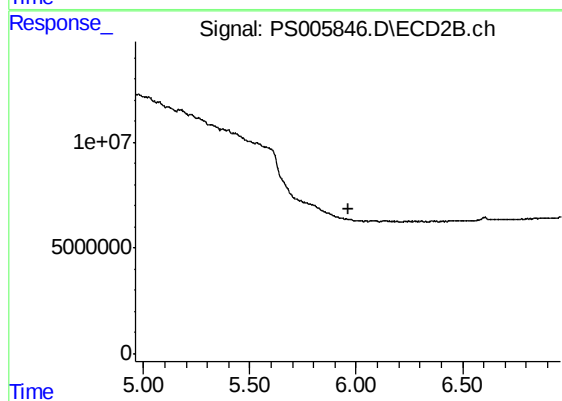

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 5.961 min
Response: 0
Conc: N.D.

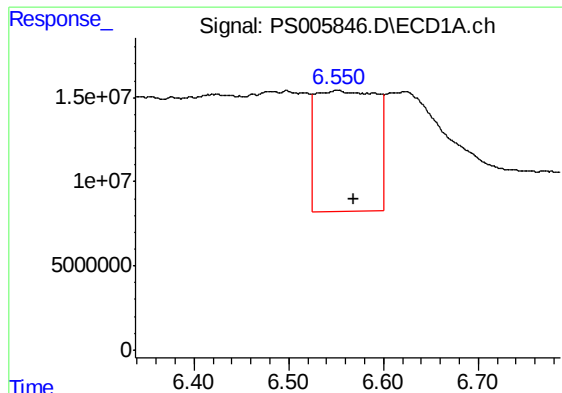

#9 2,4-D


R.T.: 6.551 min
Delta R.T.: -0.018 min
Response: 315464772
Conc: 210.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

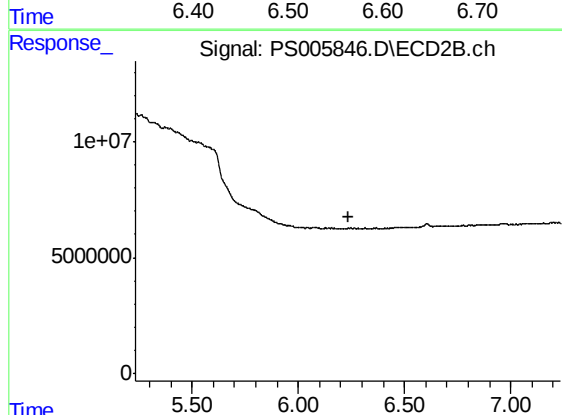


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

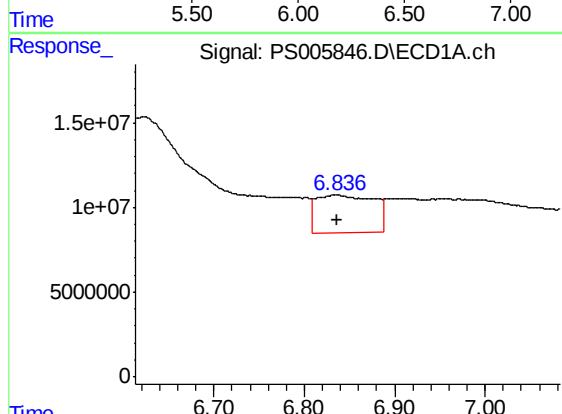


#10 Pentachlorophenol

R.T.: 6.835 min
Delta R.T.: -0.001 min
Response: 97523449
Conc: 4.66 ng/ml

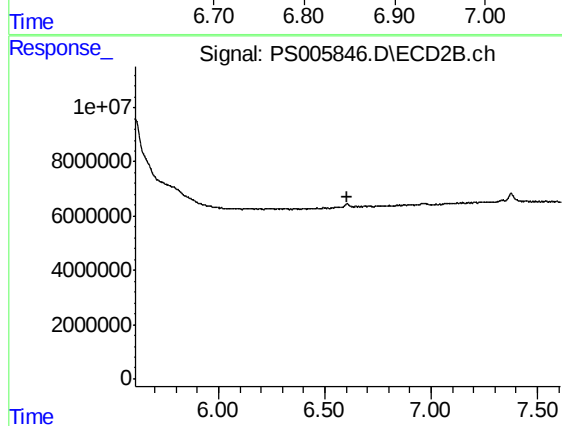

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.608 min
Response: 0
Conc: N.D.

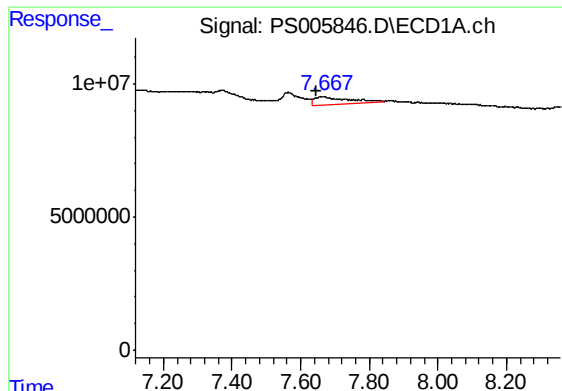

#12 2,4,5-T


R.T.: 7.667 min
Delta R.T.: 0.020 min
Response: 19404897
Conc: 2.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

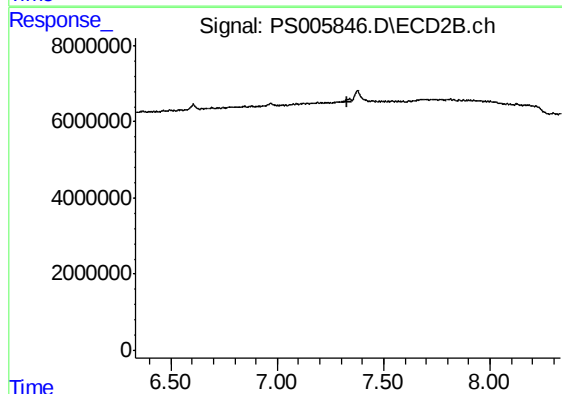


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.332 min
Response: 0
Conc: N.D.

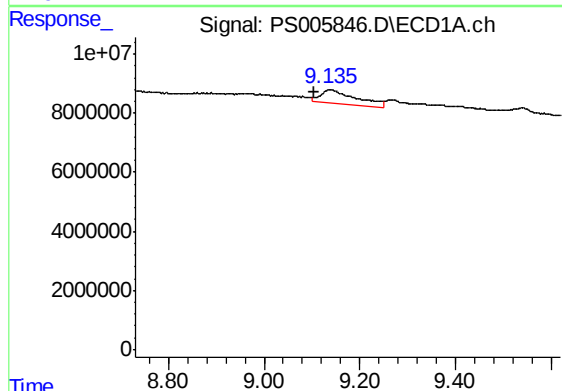

#15 Picloram

R.T.: 9.137 min
Delta R.T.: 0.033 min
Response: 22873899
Conc: 1.95 ng/ml

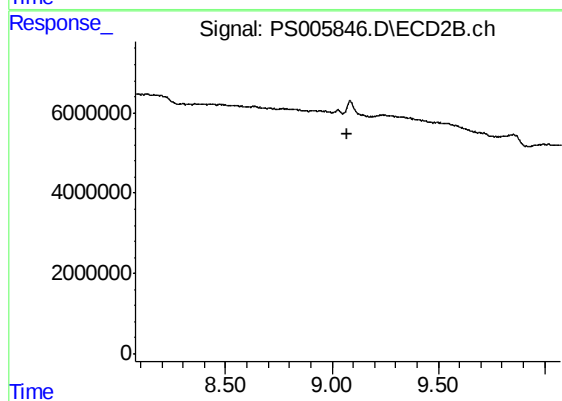

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.075 min
Response: 0
Conc: N.D.