

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080519\
 Data File : PS005866.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2019 20:30
 Operator : SM\AJ
 Sample : K4095-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 05:13:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.559	5.279	421.4E6	248.2E6	290.439	249.539
Target Compounds							
1) T	Dalapon	2.058	0.000	183.5E6	0	98.986	N.D. #
2) T	3,5-DICHL...	4.884	4.598	61510135	235.6E6	29.655	181.579 #
3) T	4-Nitroph...	5.407	0.000	30739375	0	51.102	N.D. #
5) T	DICAMBA	5.692	5.384	27037184	8269618	4.527	2.215 #
6) T	MCPD	5.861	0.000	27478073	0	5.930	N.D. #
7) T	MCPA	5.968	5.614	57815040	143.0E6	8.860	33.967 #
8) T	DICHLORPROP	6.333	0.000	23956764	0	16.659	N.D. #
9) T	2,4-D	6.638	0.000	394.5E6	0	263.254	N.D. #
11) T	2,4,5-TP ...	0.000	6.926	0	93002538	N.D.	17.929
13) T	2,4-DB	8.194	0.000	5345464	0	5.062	N.D. #
15) T	Picloram	9.105	0.000	4892029	0	<MDL	N.D. #
16) T	DCPA	9.539	0.000	10720948	0	1.054	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS005866.D
Data File : PS005866.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2019 20:30
Operator : SM\AJ
Sample : K4095-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 05:13:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

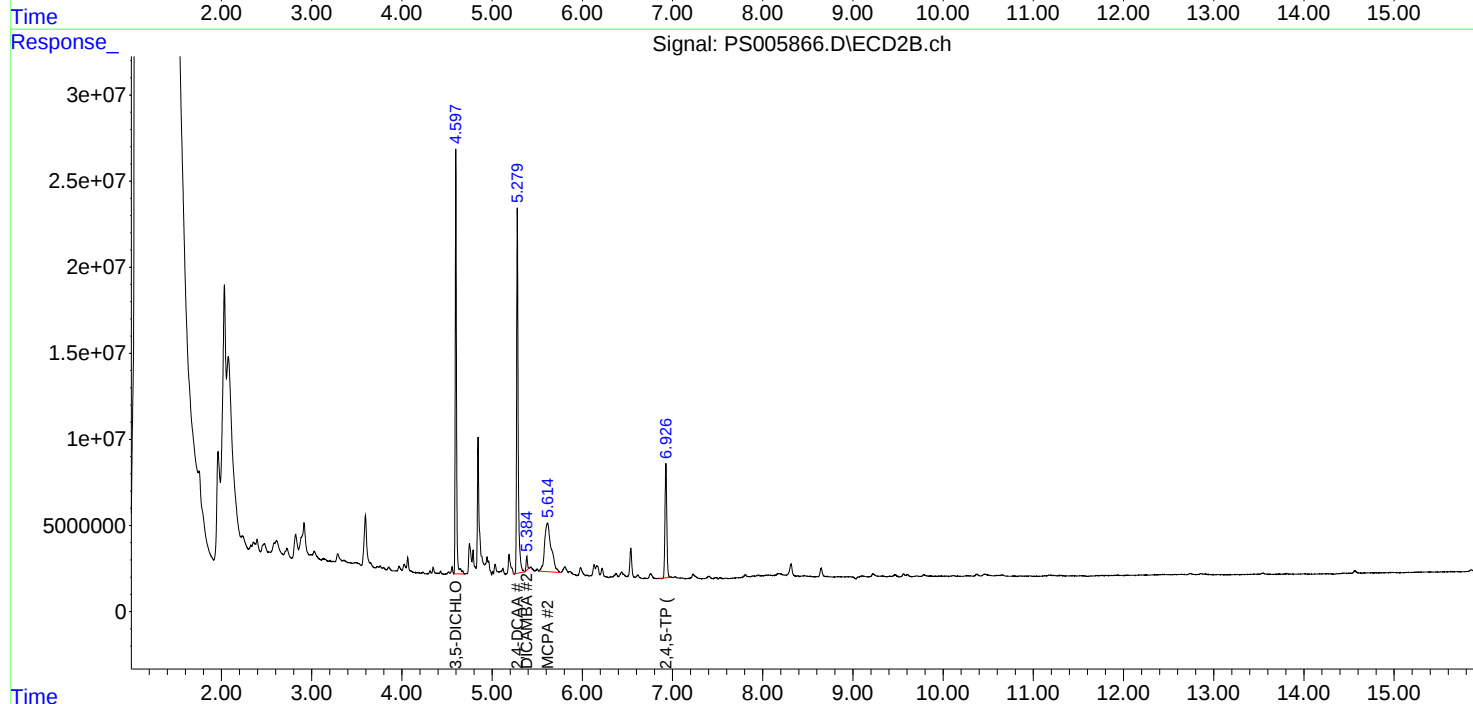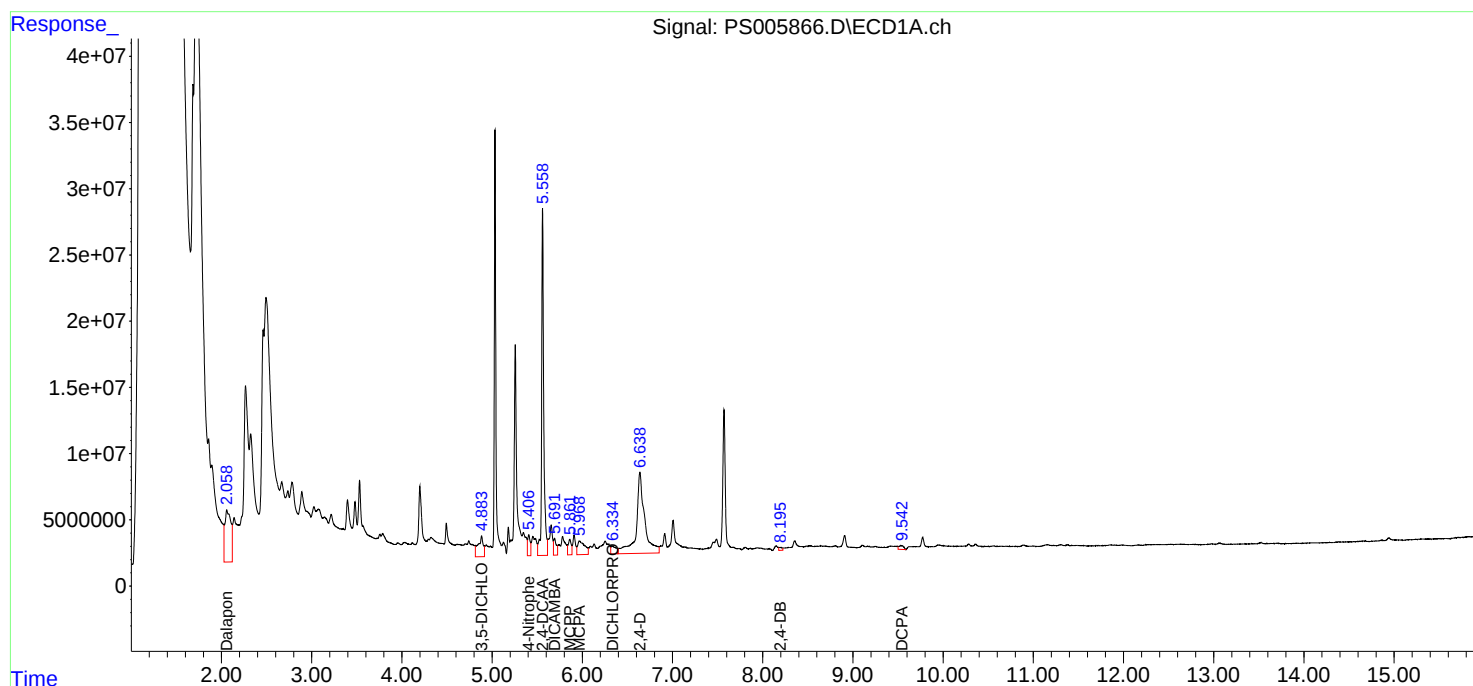


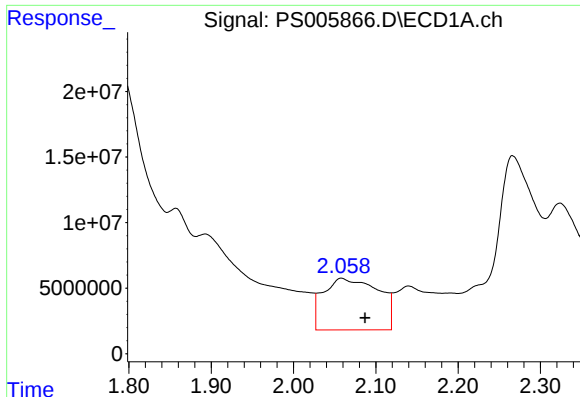

#1 Dalapon


R.T.: 2.058 min
Delta R.T.: -0.029 min
Response: 183451425
Conc: 98.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

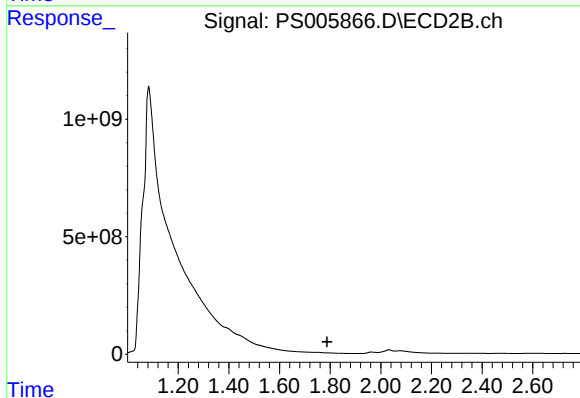


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

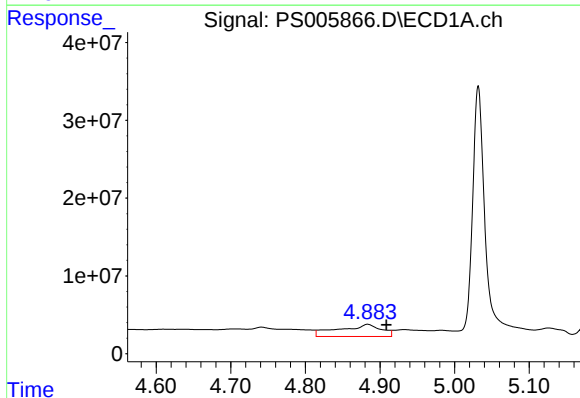


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.884 min
Delta R.T.: -0.025 min
Response: 61510135
Conc: 29.66 ng/ml

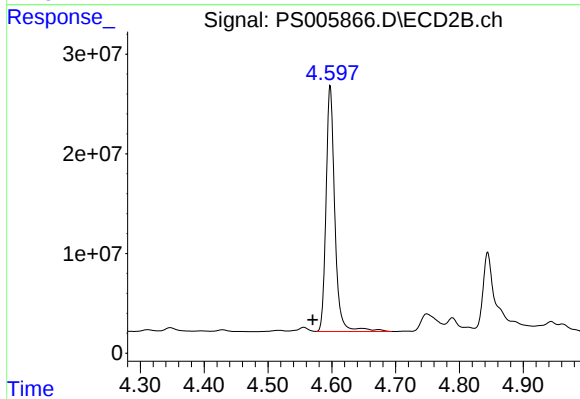

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.598 min
Delta R.T.: 0.027 min
Response: 235564470
Conc: 181.58 ng/ml

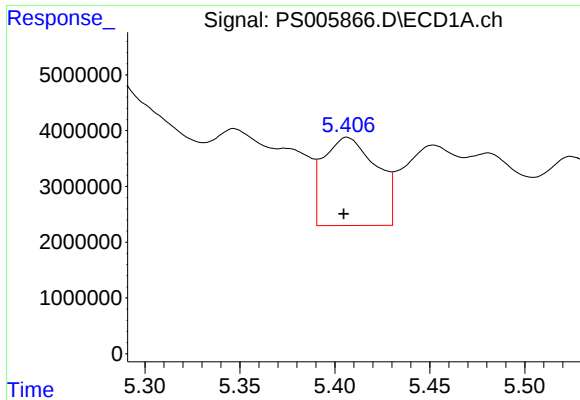

#3 4-Nitrophenol


R.T.: 5.407 min
Delta R.T.: 0.002 min
Response: 30739375
Conc: 51.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

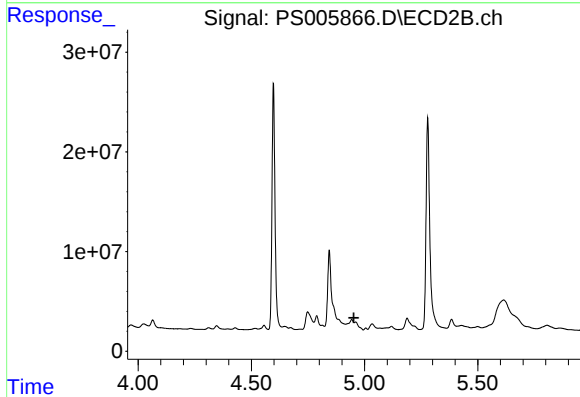


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

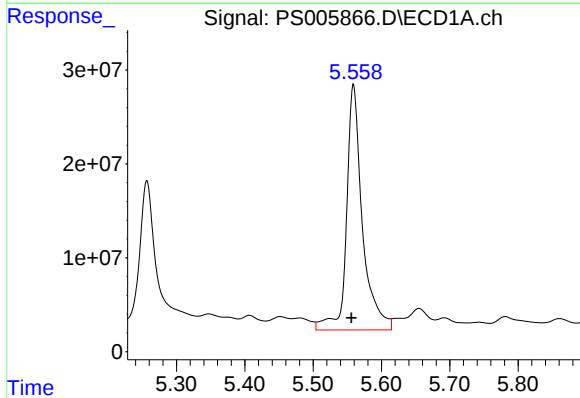


#4 2,4-DCAA

R.T.: 5.559 min
Delta R.T.: 0.003 min
Response: 421373584
Conc: 290.44 ng/ml

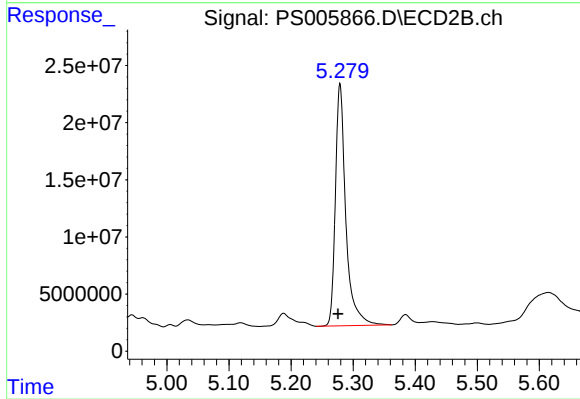

#4 2,4-DCAA


R.T.: 5.279 min
Delta R.T.: 0.003 min
Response: 248211454
Conc: 249.54 ng/ml

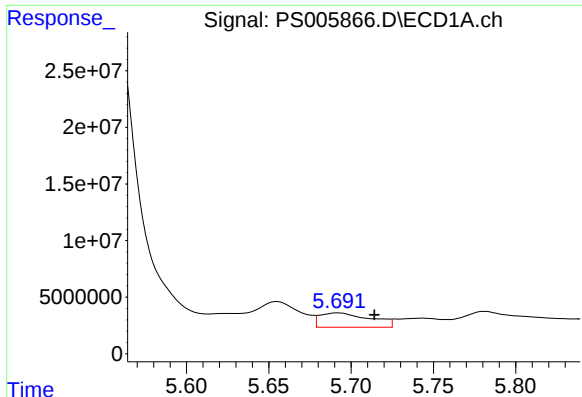

#5 DICAMBA


R.T.: 5.692 min
Delta R.T.: -0.023 min
Response: 27037184
Conc: 4.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

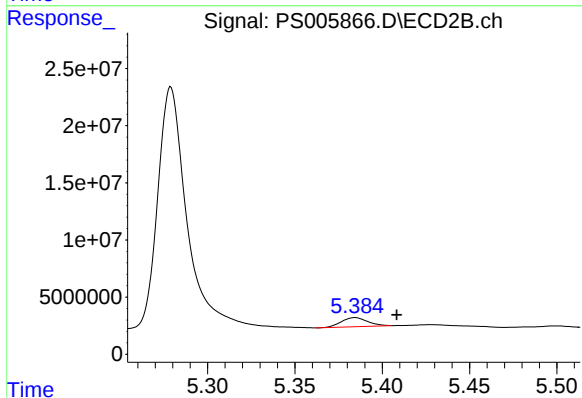


#5 DICAMBA

R.T.: 5.384 min
Delta R.T.: -0.024 min
Response: 8269618
Conc: 2.22 ng/ml

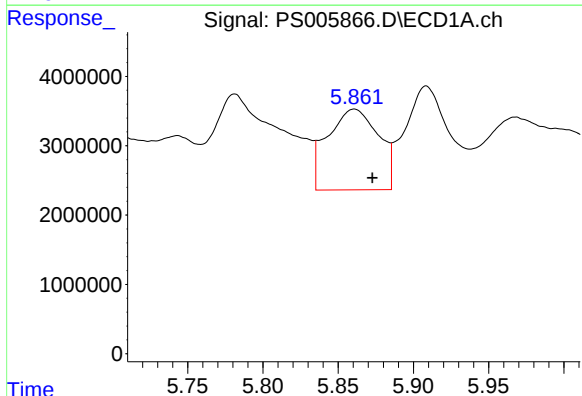


#6 MCP

R.T.: 5.861 min
Delta R.T.: -0.012 min
Response: 27478073
Conc: 5.93 ug/ml

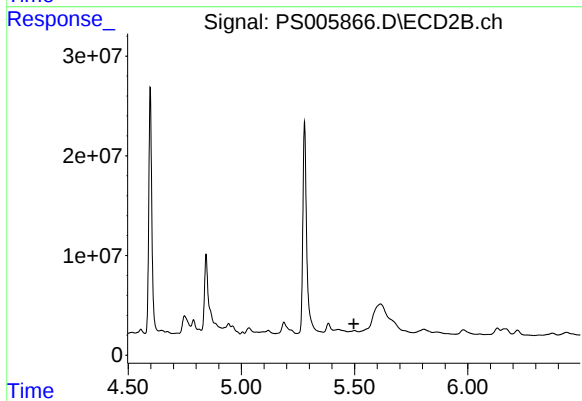

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.497 min
Response: 0
Conc: N.D.

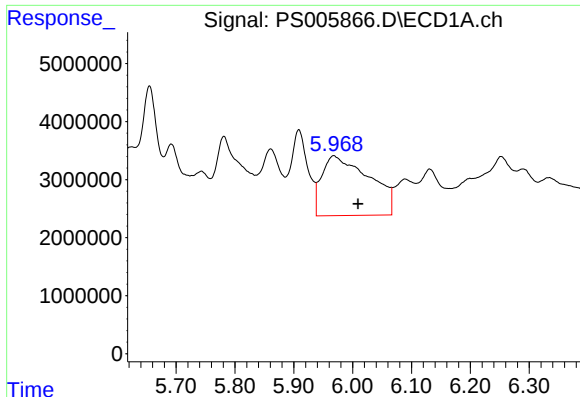

#7 MCPA


R.T.: 5.968 min
Delta R.T.: -0.041 min
Response: 57815040
Conc: 8.86 ug/ml

Instrument :
ECD_S
ClientSampleId :

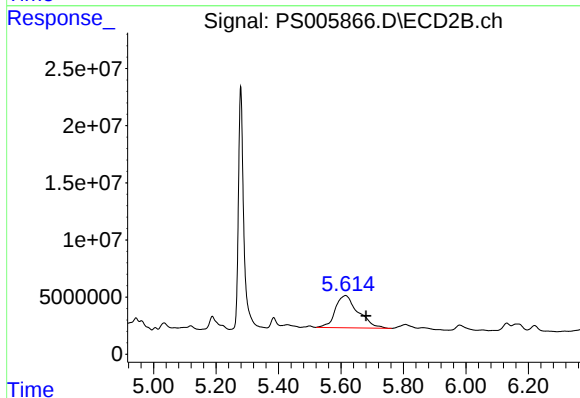


#7 MCPA

R.T.: 5.614 min
Delta R.T.: -0.066 min
Response: 142966790
Conc: 33.97 ug/ml

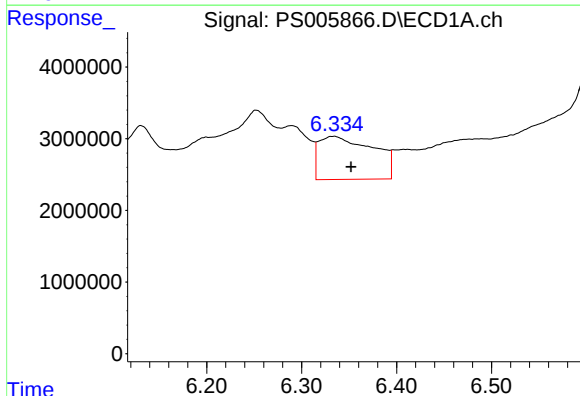


#8 DICHLORPROP

R.T.: 6.333 min
Delta R.T.: -0.019 min
Response: 23956764
Conc: 16.66 ng/ml

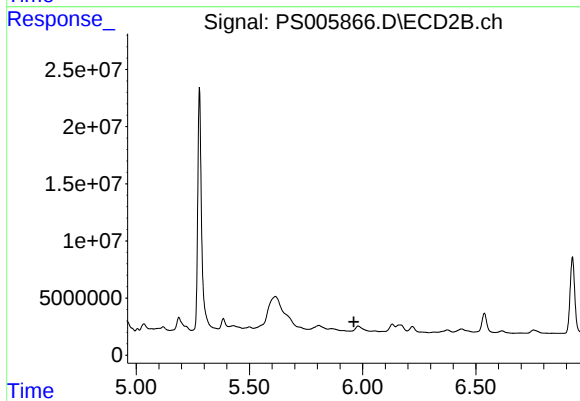

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 5.961 min
Response: 0
Conc: N.D.

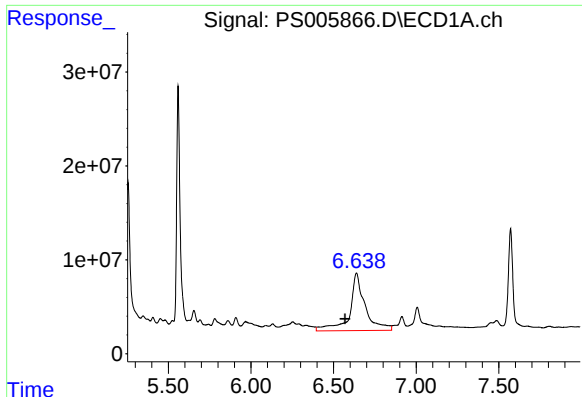

#9 2,4-D


R.T.: 6.638 min
Delta R.T.: 0.069 min
Response: 394530556
Conc: 263.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

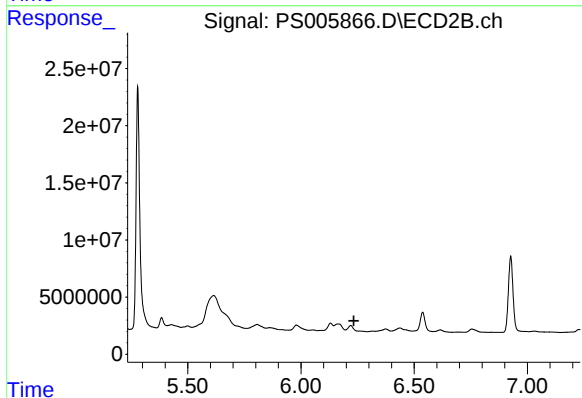


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

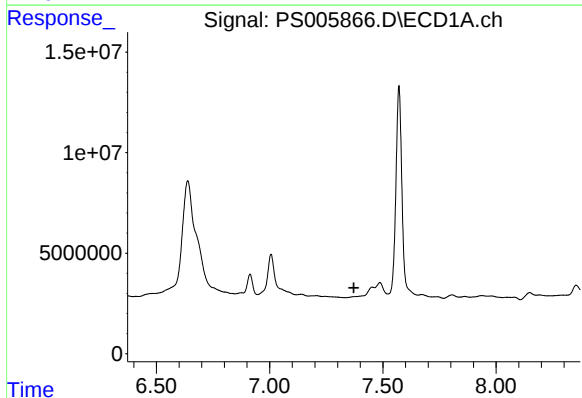


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.372 min
Response: 0
Conc: N.D.

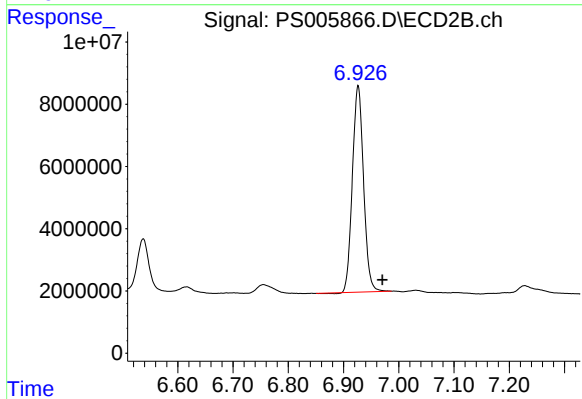

#11 2,4,5-TP (SILVEX)


R.T.: 6.926 min
Delta R.T.: -0.044 min
Response: 93002538
Conc: 17.93 ng/ml

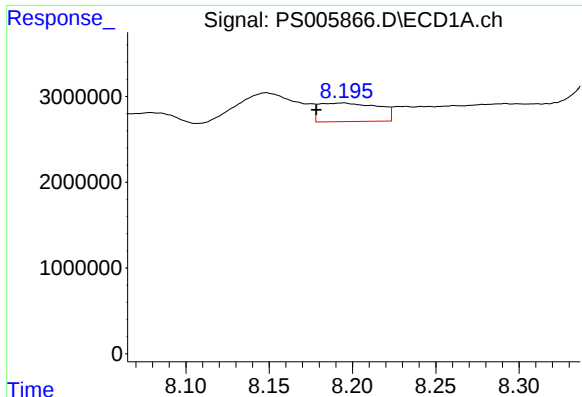

#13 2,4-DB


R.T.: 8.194 min
Delta R.T.: 0.015 min
Response: 5345464
Conc: 5.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

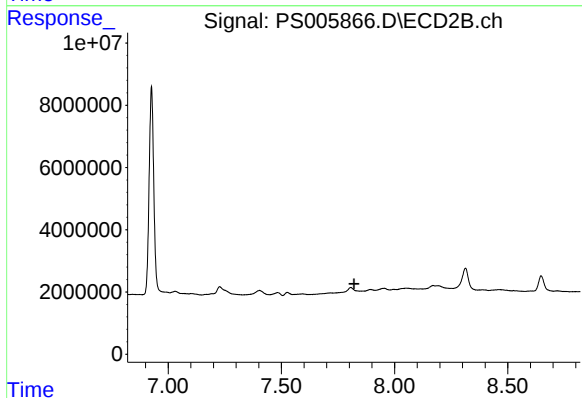


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.821 min
Response: 0
Conc: N.D.

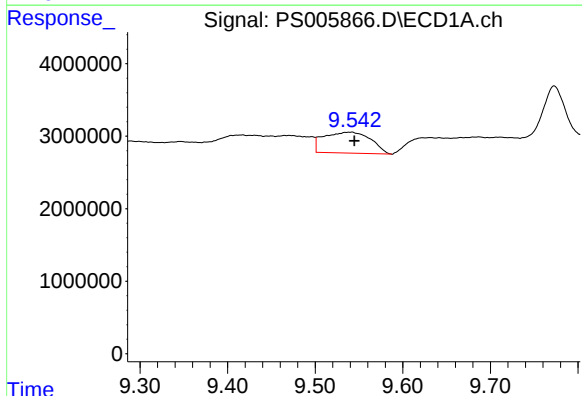

#16 DCPA

R.T.: 9.539 min
Delta R.T.: -0.006 min
Response: 10720948
Conc: 1.05 ng/ml

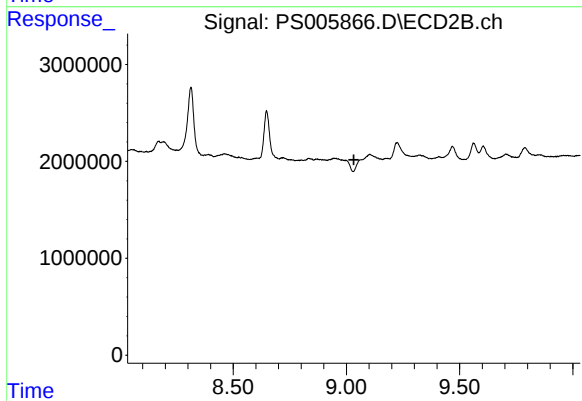

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.033 min
Response: 0
Conc: N.D.