

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080522\
 Data File : PS020184.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2022 09:57
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 07:27:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.118f	0.000	747252	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	3.042	0.000	1616483	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.439	0.000	849.3E6	0	218.343	N.D. #
5) T	DICAMBA	7.332	6.981f	197630	241.6E6	<MDL	67.797 #
6) T	MCP	7.521	6.981	3917806	241.6E6	<MDL	88.581 #
7) T	MCPA	7.727f	0.000	12357137	0	<MDL	N.D. #
12) T	2,4,5-T	9.430	0.000	4203083	0	<MDL	N.D. #
15) T	Picloram	10.937	10.774	729.2E6	1072911	23.062	<MDL #
16) T	DCPA	11.376	10.774	-932190	1072911	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080522\
Data File : PS020184.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2022 09:57
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 07:27:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

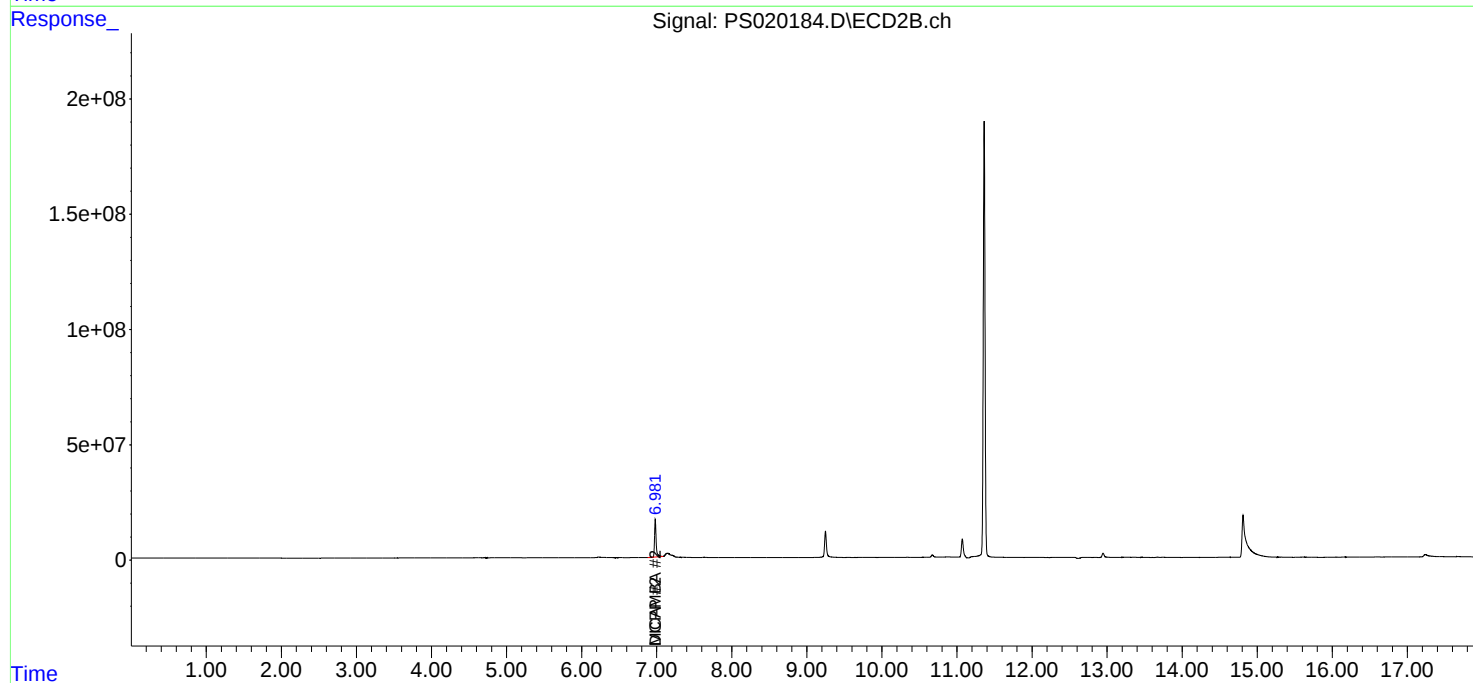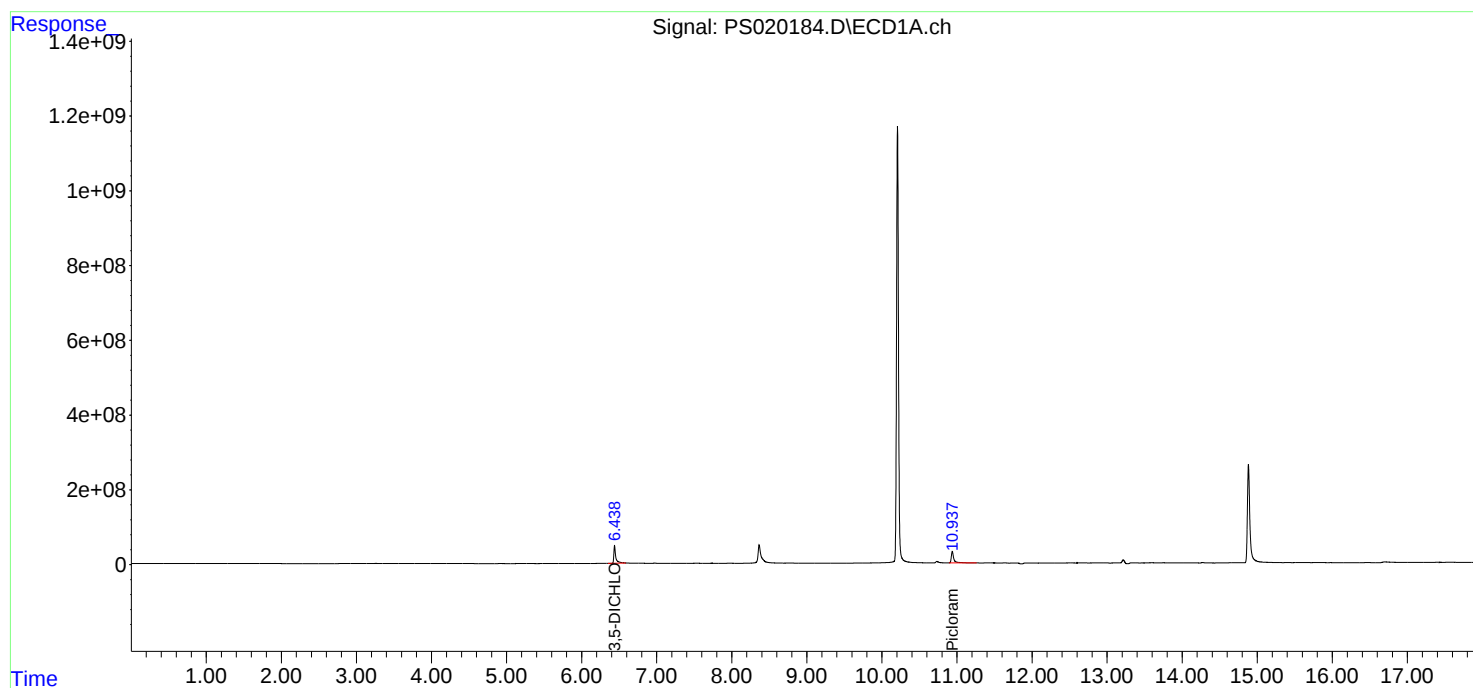


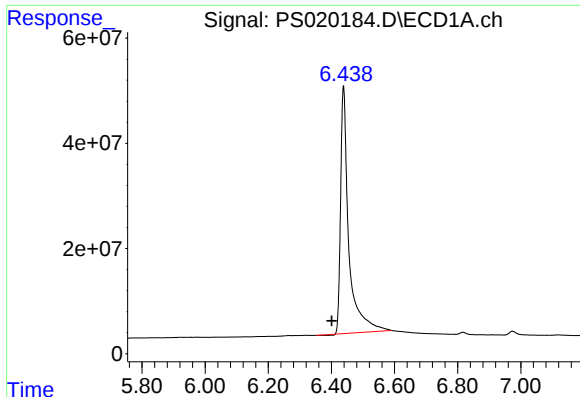

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.439 min
Delta R.T.: 0.037 min
Response: 849333194
Conc: 218.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

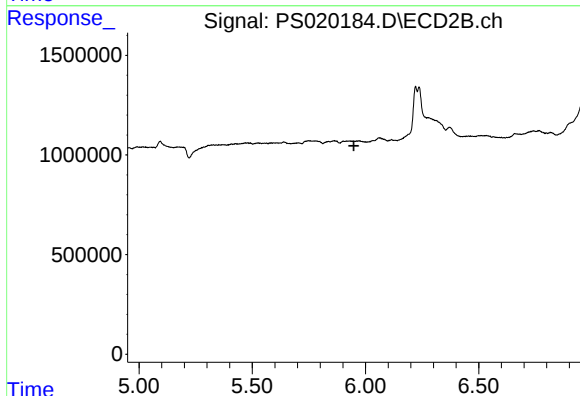


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

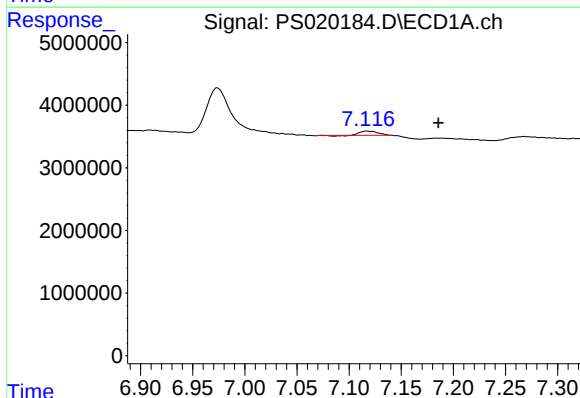


#4 2,4-DCAA

R.T.: 7.118 min
Delta R.T.: -0.067 min
Response: 747252
Conc: N.D.

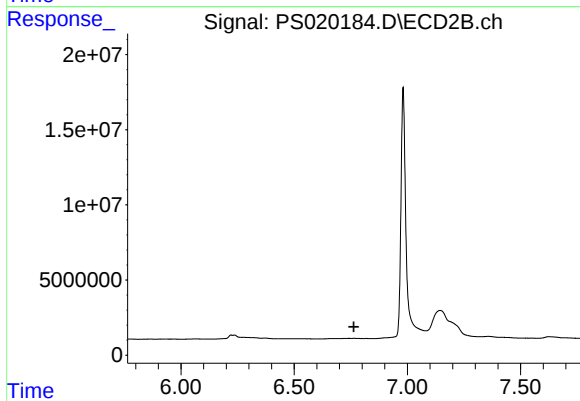

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

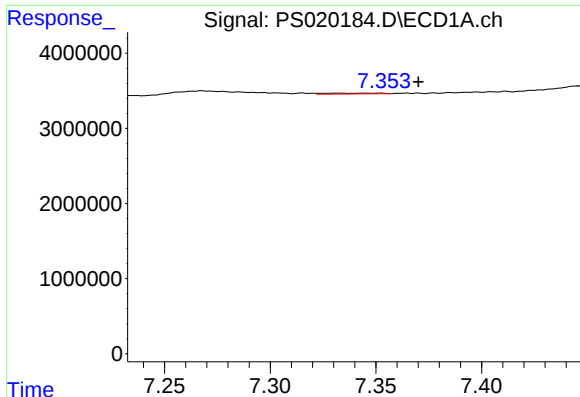

#5 DICAMBA


R.T.: 7.332 min
Delta R.T.: -0.038 min
Response: 197630
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

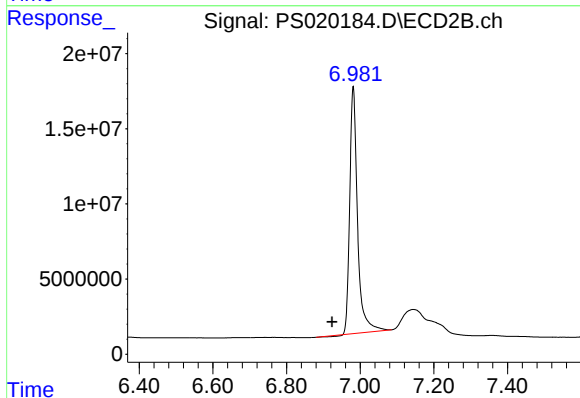


#5 DICAMBA

R.T.: 6.981 min
Delta R.T.: 0.058 min
Response: 241636367
Conc: 67.80 ng/ml

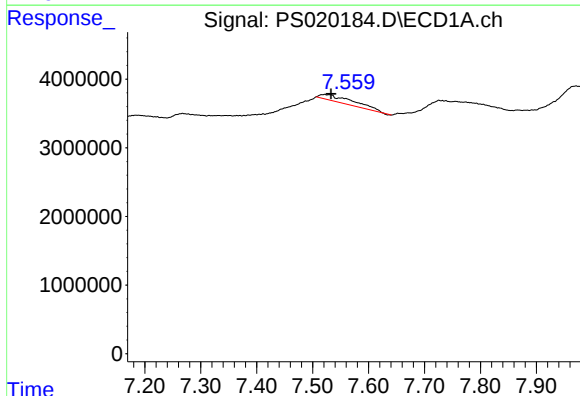


#6 MCP

R.T.: 7.521 min
Delta R.T.: -0.013 min
Response: 3917806
Conc: N.D.

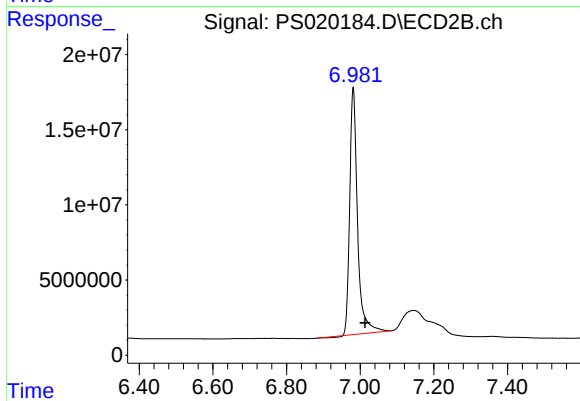

#6 MCP


R.T.: 6.981 min
Delta R.T.: -0.032 min
Response: 241636367
Conc: 88.58 ug/ml

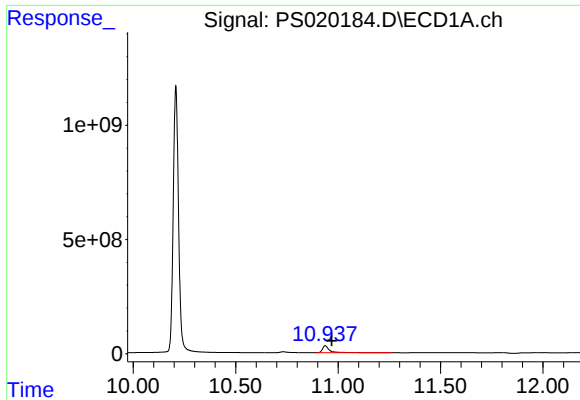

#15 Picloram

R.T.: 10.937 min
Delta R.T.: -0.032 min
Response: 729177935
Conc: 23.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

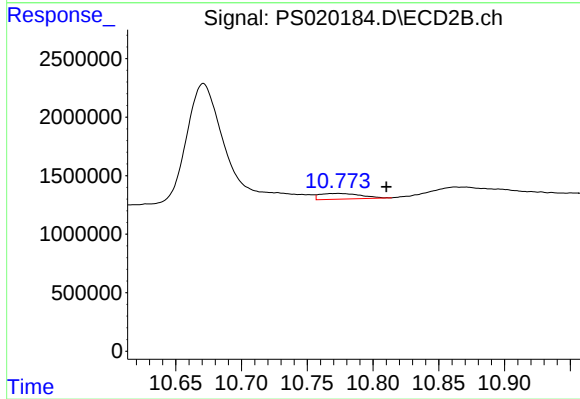

#15 Picloram

R.T.: 10.774 min
Delta R.T.: -0.036 min
Response: 1072911
Conc: N.D.