

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080522\
 Data File : PS020185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2022 10:21
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 07:28:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.184	6.762	1501.9E6	453.2E6	509.354	556.079
Target Compounds							
1) T	Dalapon	3.049f	0.000	1540693	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.449f	0.000	36055900	0	9.269	N.D. #
5) T	DICAMBA	0.000	6.986f	0	8498668	N.D.	2.385
6) T	MCP	7.521	6.986	6018377	8498668	<MDL	3.115 #
7) T	MCPA	7.651	0.000	2460414	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.160	0.000	641836	0	<MDL	N.D. #
12) T	2,4,5-T	9.432	0.000	9082687	0	<MDL	N.D. #
13) T	2,4-DB	9.969	0.000	2400911	0	<MDL	N.D. #
15) T	Picloram	10.947	10.866f	221.9E6	1992771	7.018	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080522\
Data File : PS020185.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2022 10:21
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 07:28:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

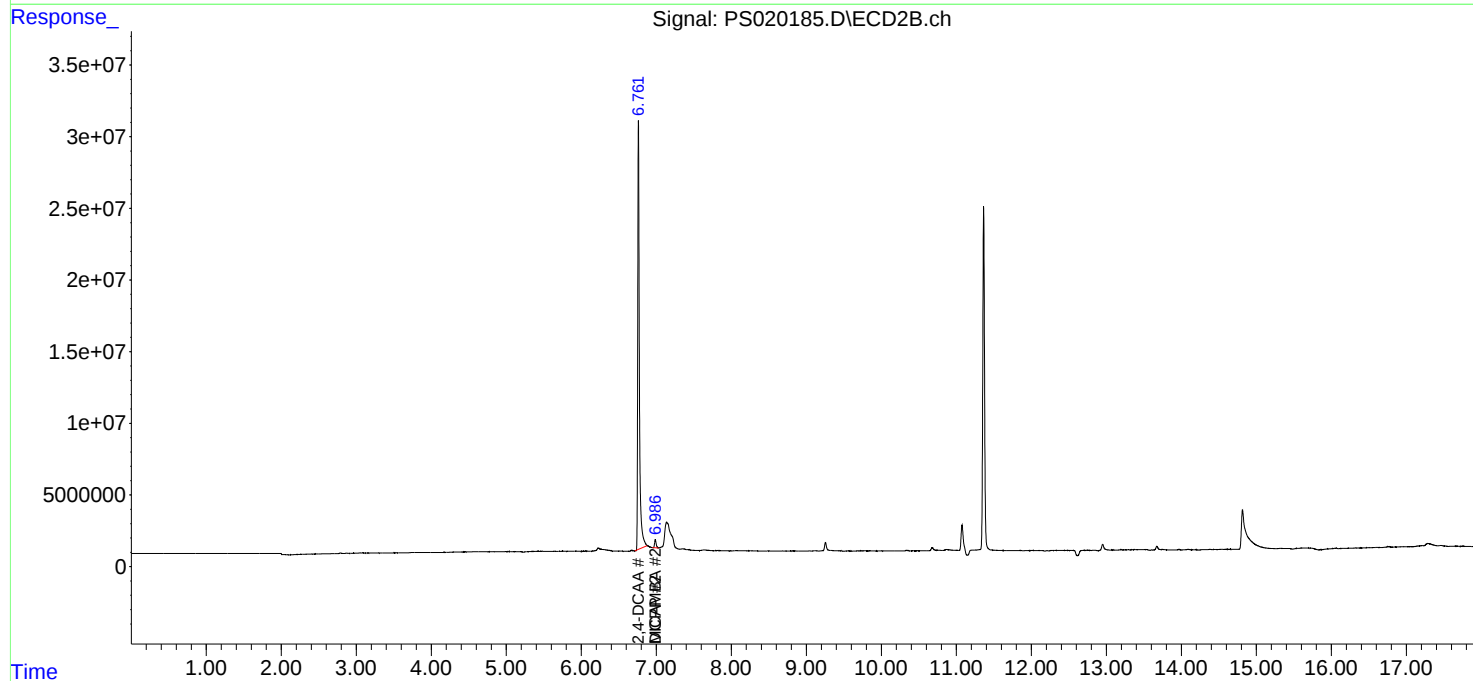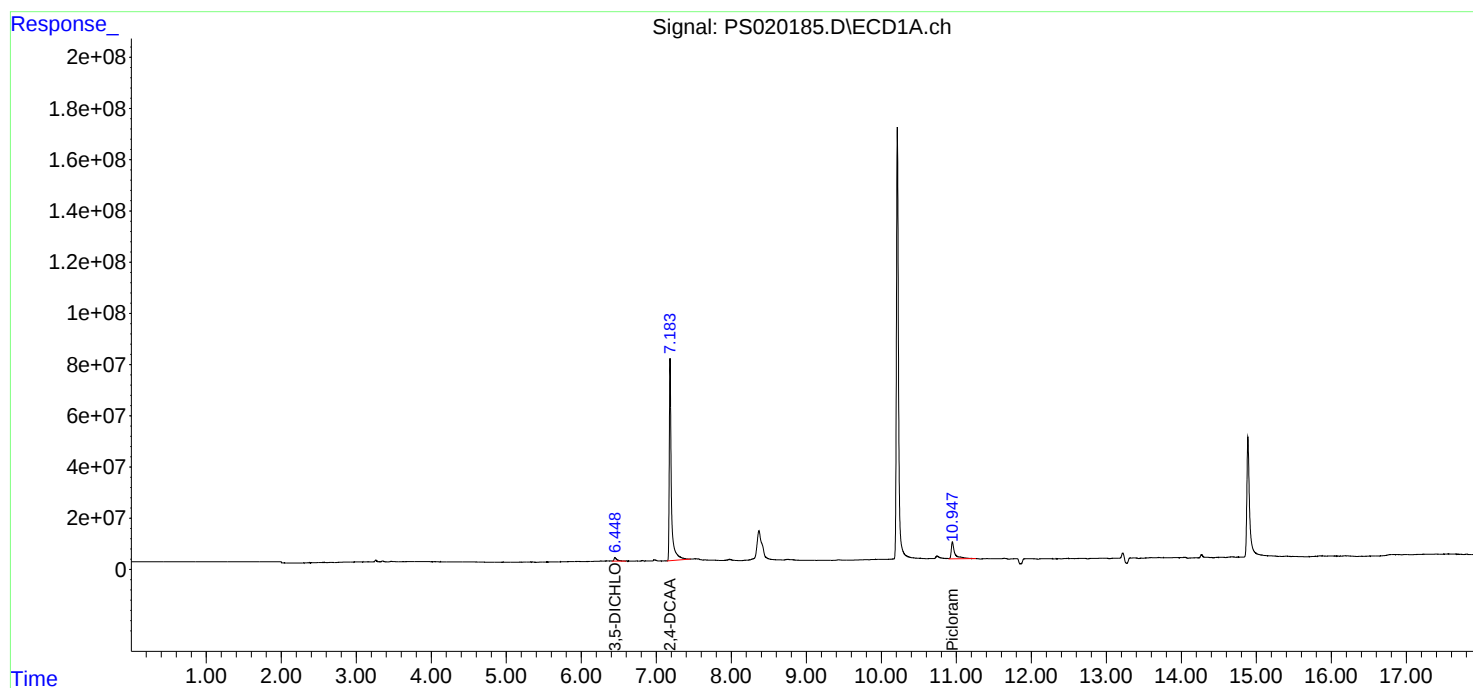


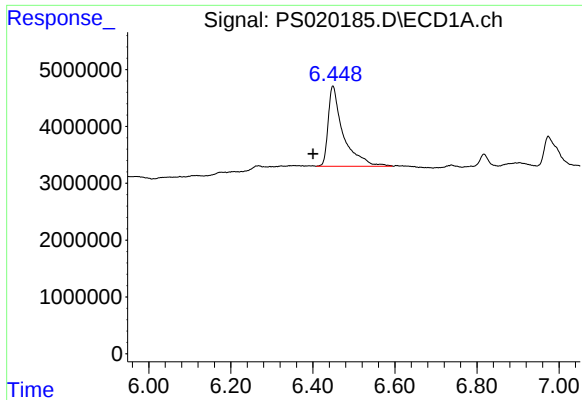

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.449 min
Delta R.T.: 0.048 min
Response: 36055900
Conc: 9.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

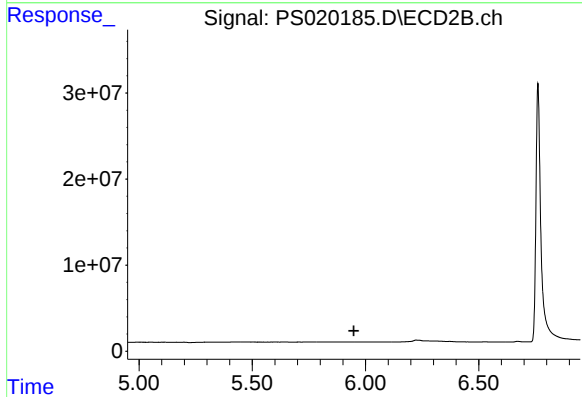


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

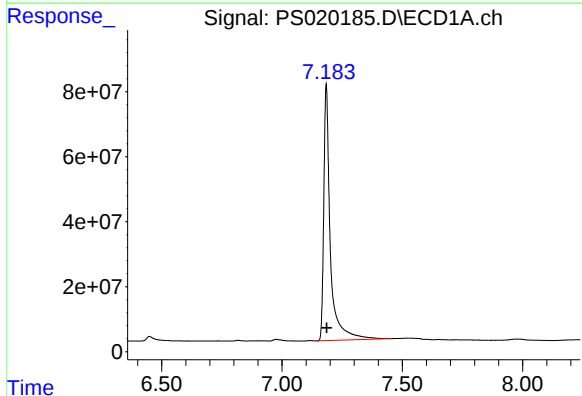


#4 2,4-DCAA

R.T.: 7.184 min
Delta R.T.: -0.002 min
Response: 1501945803
Conc: 509.35 ng/ml

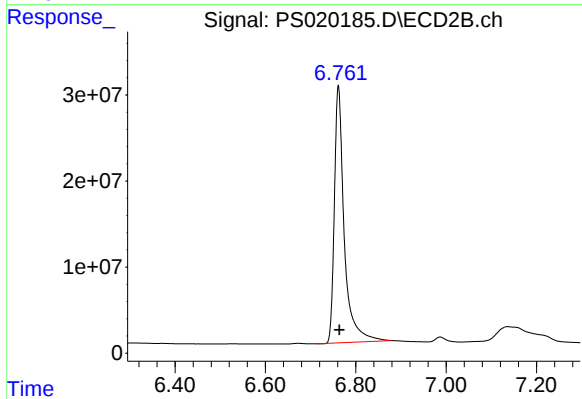

#4 2,4-DCAA


R.T.: 6.762 min
Delta R.T.: -0.002 min
Response: 453179577
Conc: 556.08 ng/ml

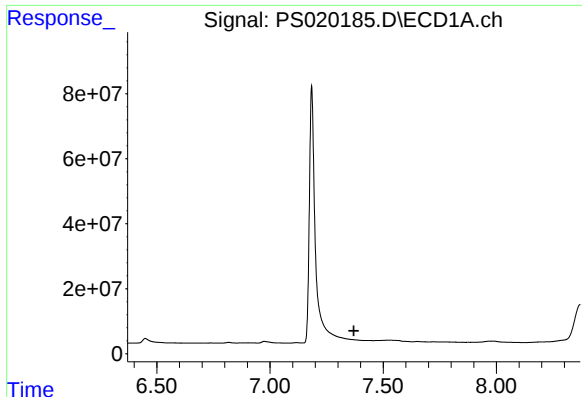

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

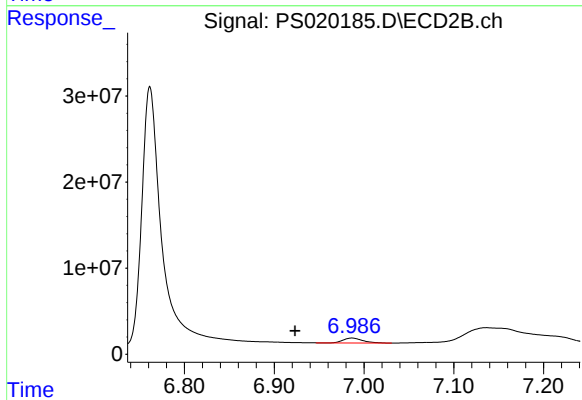


#5 DICAMBA

R.T.: 6.986 min
Delta R.T.: 0.063 min
Response: 8498668
Conc: 2.38 ng/ml

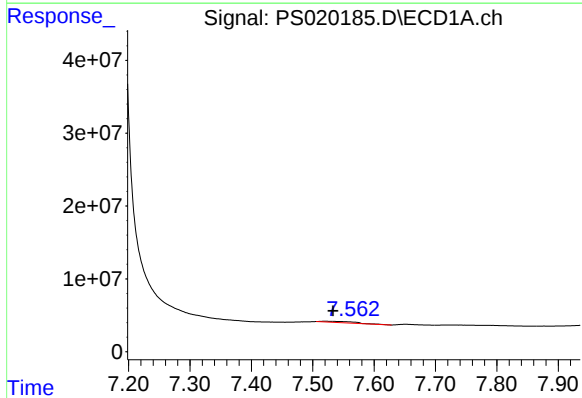


#6 MCP

R.T.: 7.521 min
Delta R.T.: -0.012 min
Response: 6018377
Conc: N.D.

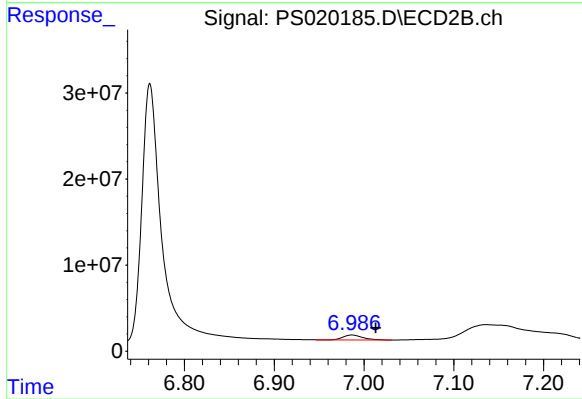

#6 MCP


R.T.: 6.986 min
Delta R.T.: -0.026 min
Response: 8498668
Conc: 3.12 ug/ml

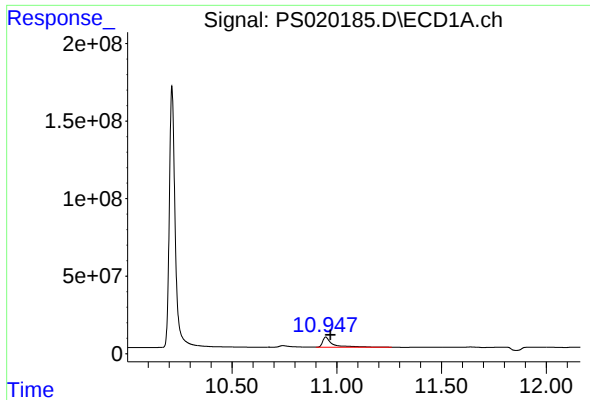

#15 Picloram

R.T.: 10.947 min
Delta R.T.: -0.022 min
Response: 221897247
Conc: 7.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

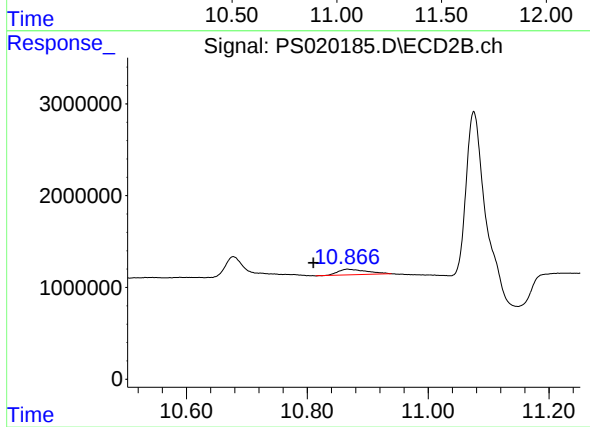

#15 Picloram

R.T.: 10.866 min
Delta R.T.: 0.056 min
Response: 1992771
Conc: N.D.