

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080522\
 Data File : PS020207.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2022 23:24
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 07:37:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.182	6.760	1605.6E6	499.2E6	544.498	612.593
Target Compounds							
1) T	Dalapon	2.985	0.000	439392	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.445f	0.000	28569531	0	7.345	N.D. #
5) T	DICAMBA	0.000	6.984f	0	8398233	N.D.	2.356
6) T	MCP	0.000	6.984	0	8398233	N.D.	3.079
7) T	MCPA	7.676	0.000	8352619	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.599f	0	3670000	N.D.	3.925
10) T	Pentachlo...	8.623	0.000	1934621	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.159	8.586	2047915	740995	<MDL	<MDL #
12) T	2,4,5-T	9.460	0.000	5064764	0	<MDL	N.D. #
13) T	2,4-DB	9.959	9.534	7259249	2547585	1.989	3.746 #
14) T	DINOSEB	11.100	0.000	12003338	0	<MDL	N.D. #
15) T	Picloram	10.935	10.846	248.2E6	1389553	7.850	<MDL #
16) T	DCPA	11.411	10.767	3087279	864174	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080522\
Data File : PS020207.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2022 23:24
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 07:37:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

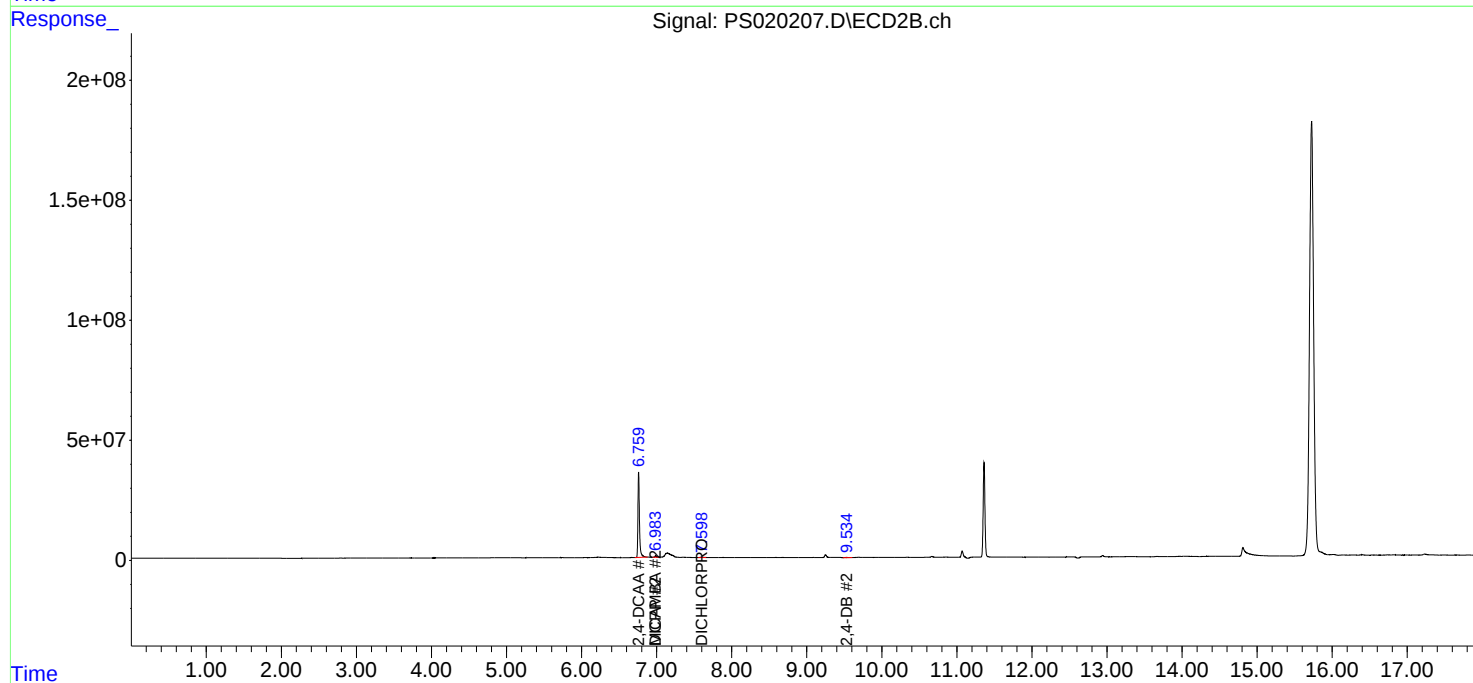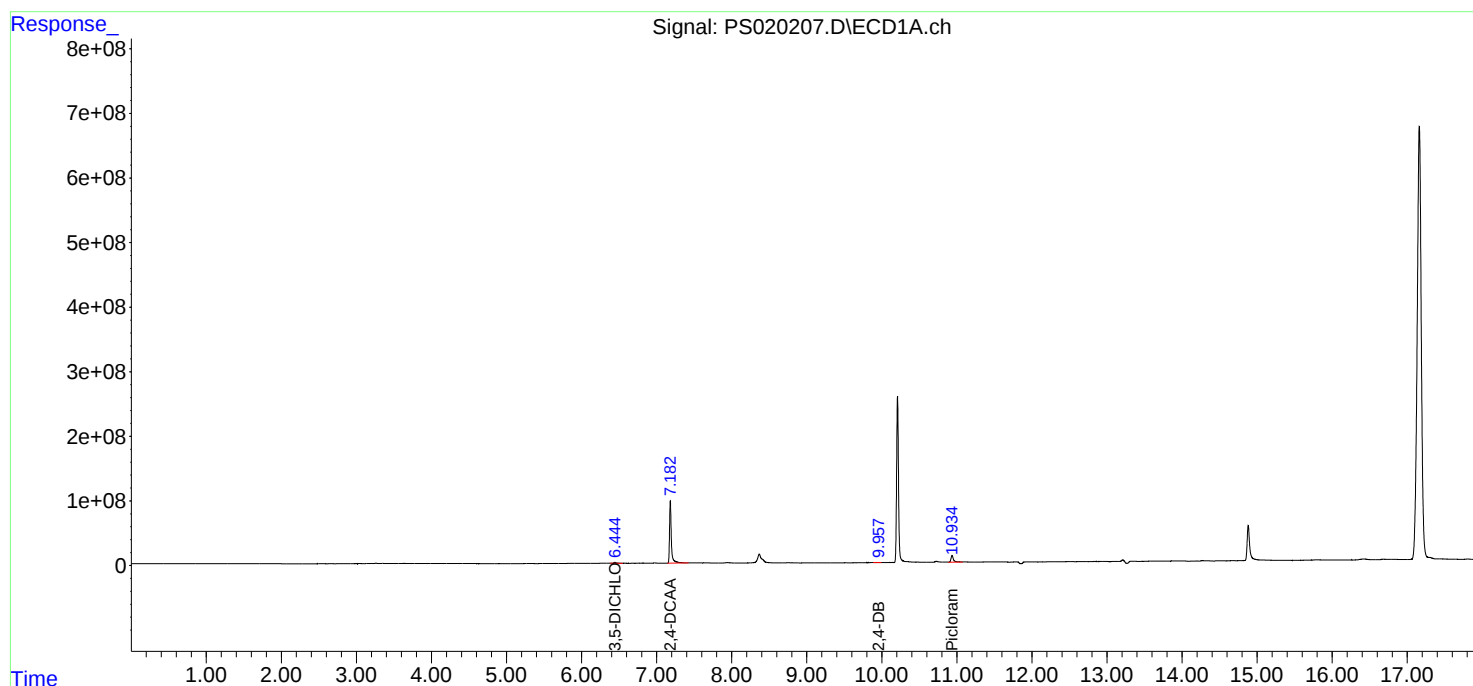


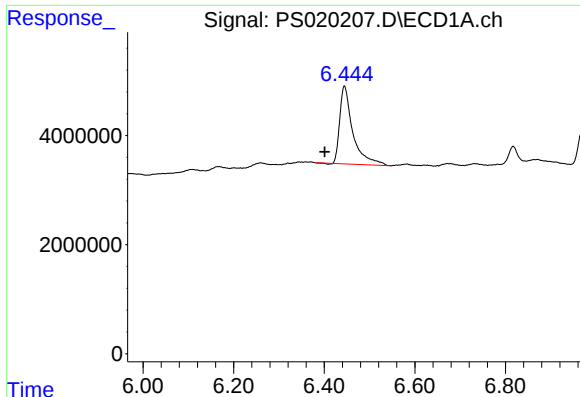

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.445 min
Delta R.T.: 0.044 min
Response: 28569531
Conc: 7.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

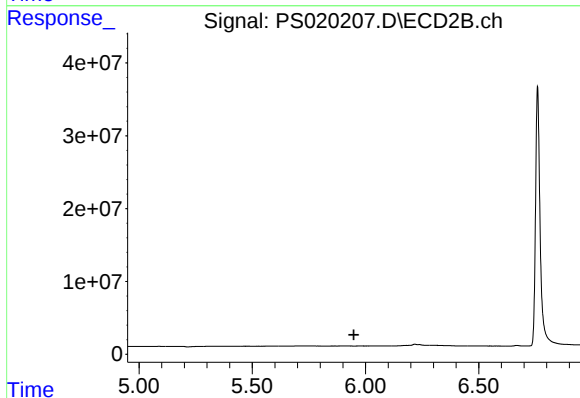


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

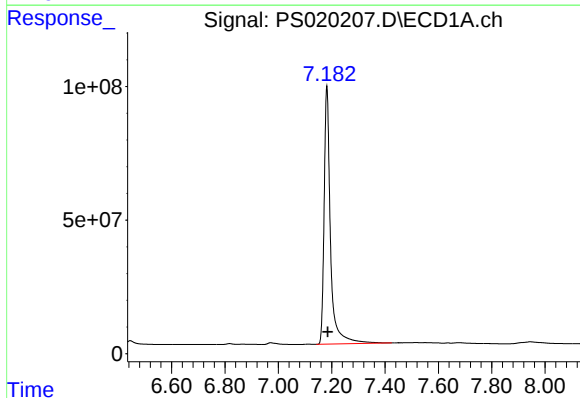


#4 2,4-DCAA

R.T.: 7.182 min
Delta R.T.: -0.004 min
Response: 1605574722
Conc: 544.50 ng/ml

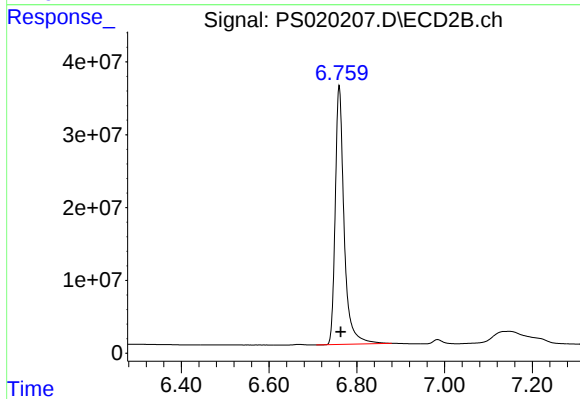

#4 2,4-DCAA


R.T.: 6.760 min
Delta R.T.: -0.004 min
Response: 499236164
Conc: 612.59 ng/ml

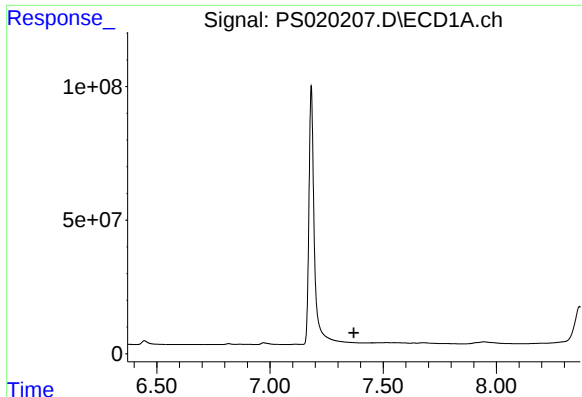

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

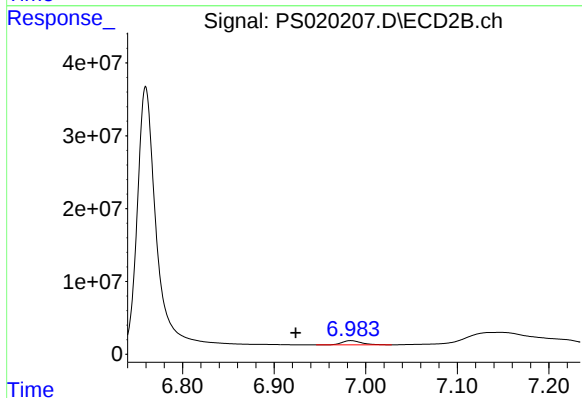


#5 DICAMBA

R.T.: 6.984 min
Delta R.T.: 0.060 min
Response: 8398233
Conc: 2.36 ng/ml

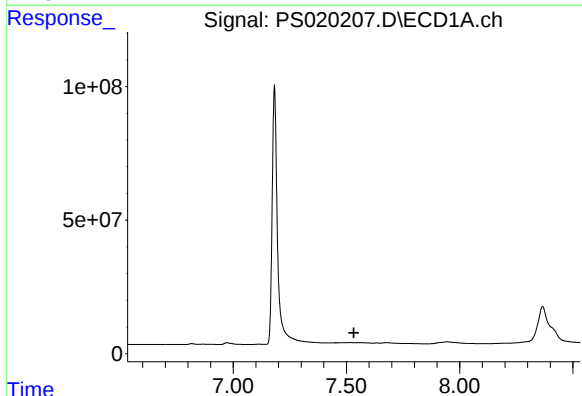


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.533 min
Response: 0
Conc: N.D.

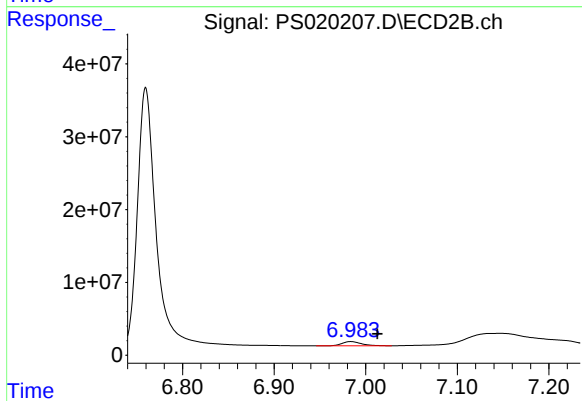

#6 MCP


R.T.: 6.984 min
Delta R.T.: -0.029 min
Response: 8398233
Conc: 3.08 ug/ml

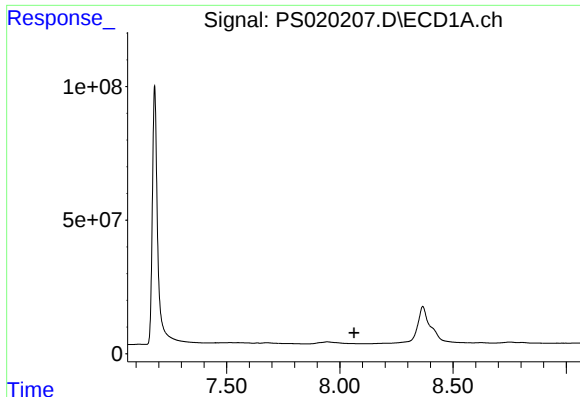

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

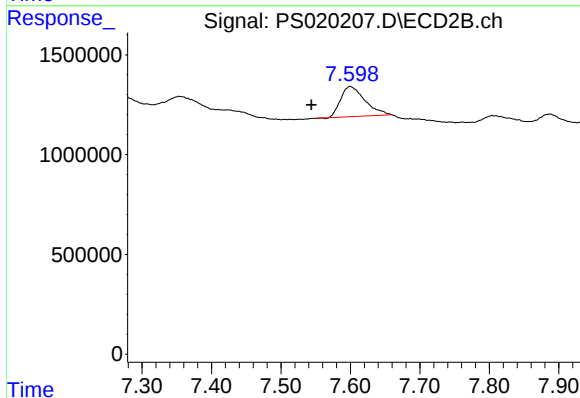


#8 DICHLORPROP

R.T.: 7.599 min
Delta R.T.: 0.055 min
Response: 3670000
Conc: 3.92 ng/ml

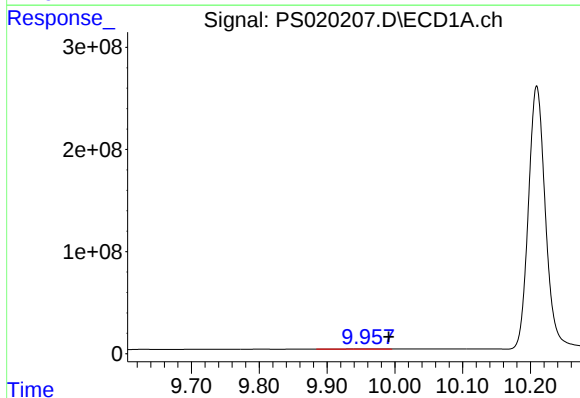


#13 2,4-DB

R.T.: 9.959 min
Delta R.T.: -0.032 min
Response: 7259249
Conc: 1.99 ng/ml

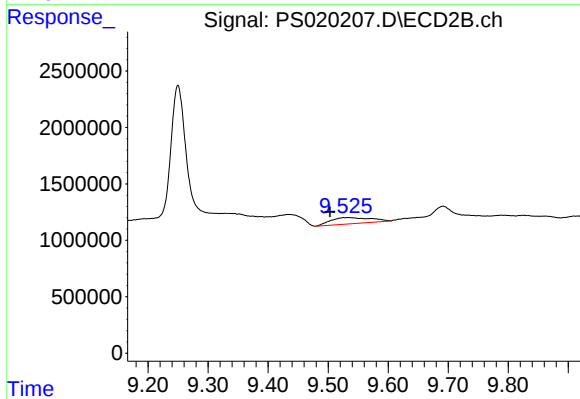

#13 2,4-DB


R.T.: 9.534 min
Delta R.T.: 0.030 min
Response: 2547585
Conc: 3.75 ng/ml

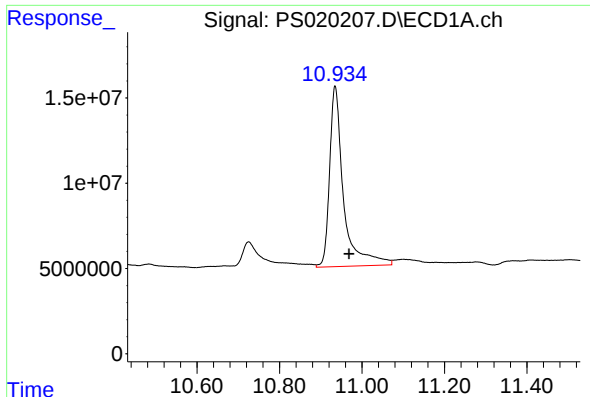

#15 Picloram

R.T.: 10.935 min
Delta R.T.: -0.034 min
Response: 248196262
Conc: 7.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

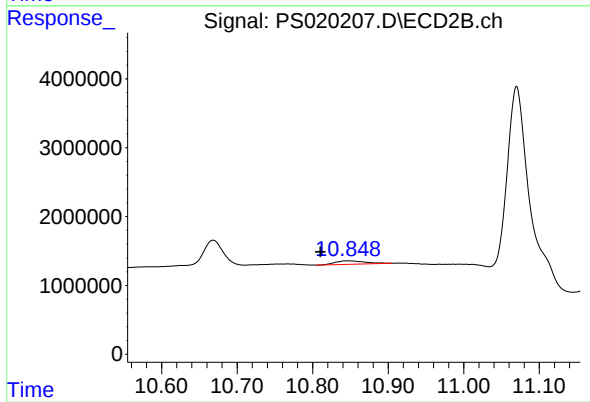

#15 Picloram

R.T.: 10.846 min
Delta R.T.: 0.036 min
Response: 1389553
Conc: N.D.