

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080522\
 Data File : PS020217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2022 03:52
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 07:41:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.180	6.758	1588.1E6	510.5E6	538.573	626.396
Target Compounds							
1) T	Dalapon	3.042	0.000	1133080	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.442f	0.000	37834098	0	9.726	N.D. #
3) T	4-Nitroph...	6.969f	0.000	1610868	0	1.160	N.D. #
5) T	DICAMBA	7.408	6.982f	716814	11717470	<MDL	3.288 #
6) T	MCP	7.550	6.982	-2907873	11717470	N.D.	4.295
7) T	MCPA	7.655	0.000	21423676	0	1.663	N.D. #
8) T	DICHLORPROP	0.000	7.586f	0	6549068	N.D.	7.003
9) T	2,4-D	8.362f	0.000	46654503	0	15.491	N.D. #
10) T	Pentachlo...	8.613	0.000	2825383	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.156	8.581	5493410	1147047	<MDL	<MDL #
12) T	2,4,5-T	9.443	0.000	2052353	0	<MDL	N.D. #
13) T	2,4-DB	10.027	0.000	16309042	0	4.469	N.D. #
14) T	DINOSEB	11.137	0.000	1664905	0	<MDL	N.D. #
15) T	Picloram	10.930	10.848	257.4E6	651049	8.142	<MDL #
16) T	DCPA	11.366	10.759	8876690	1256252	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080522\
Data File : PS020217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2022 03:52
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 07:41:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

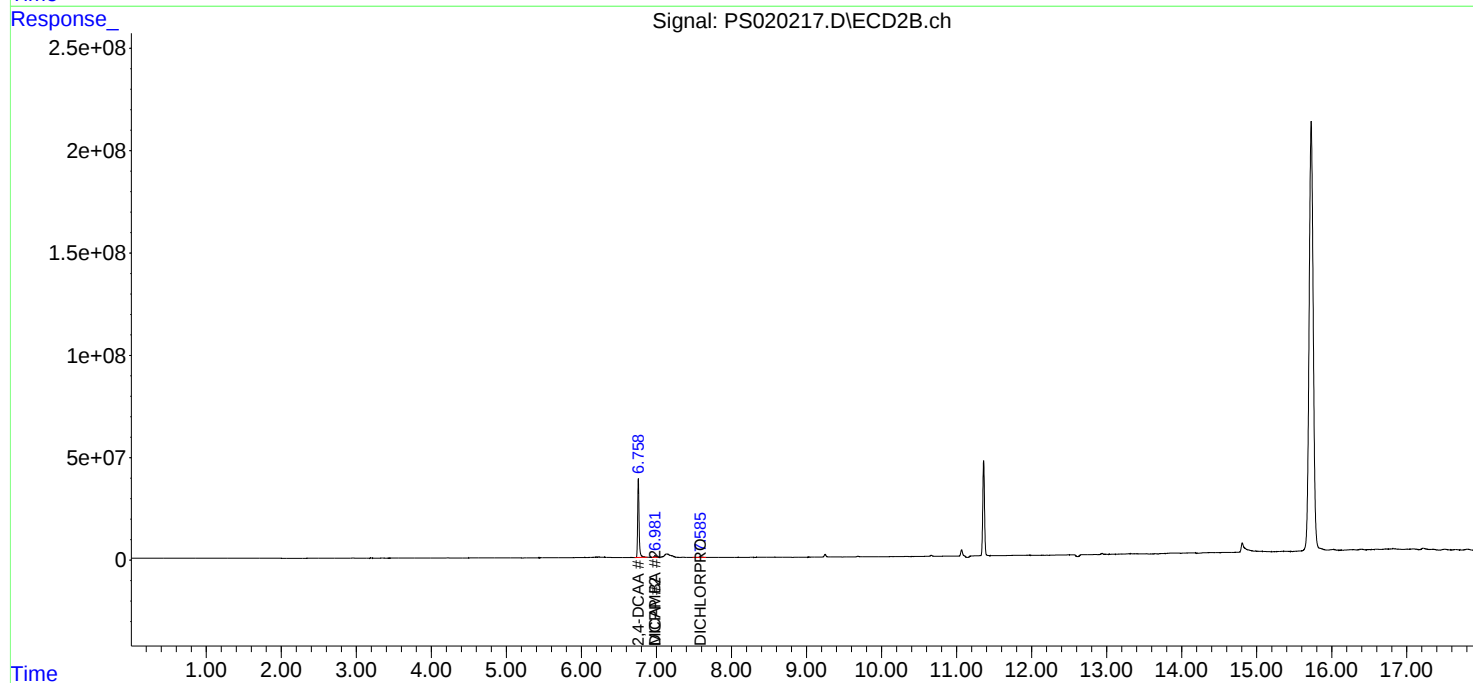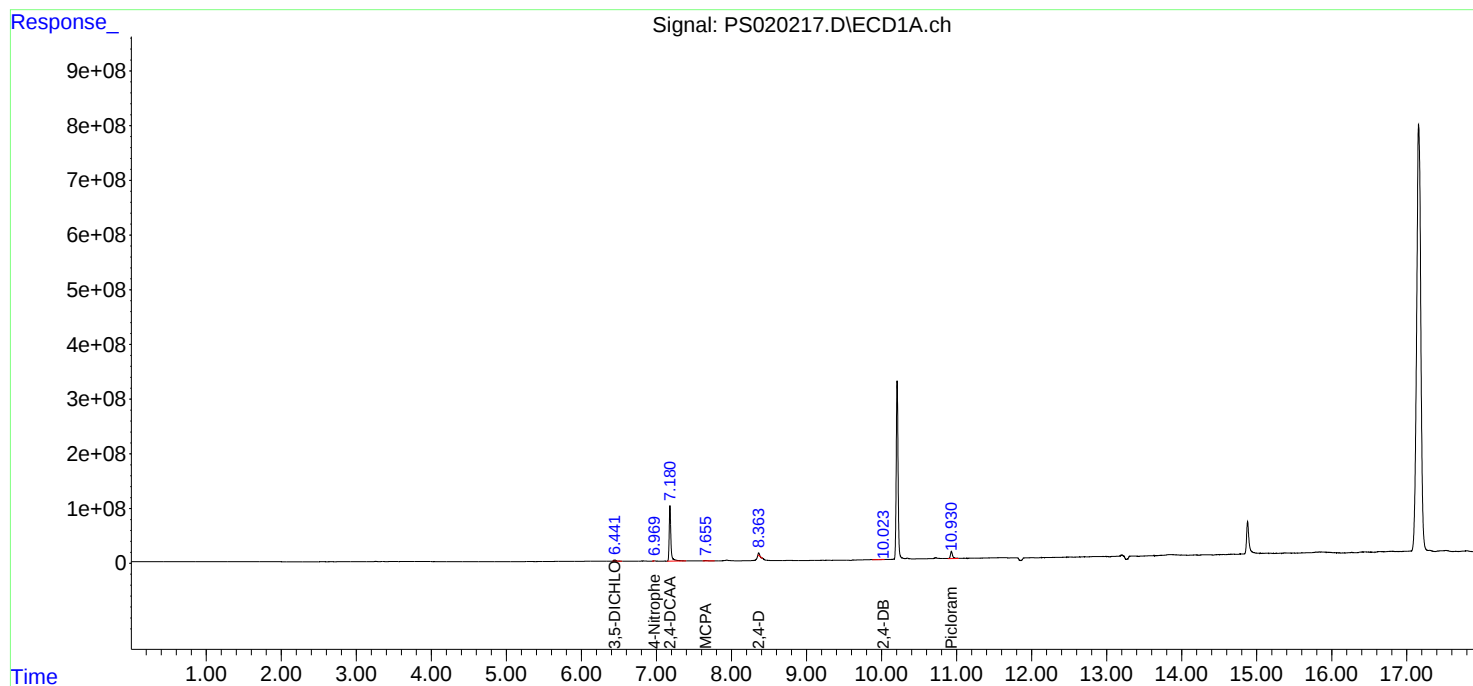


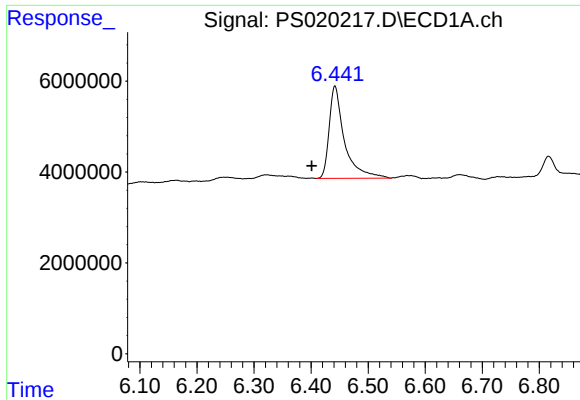

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.442 min
Delta R.T.: 0.041 min
Response: 37834098
Conc: 9.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

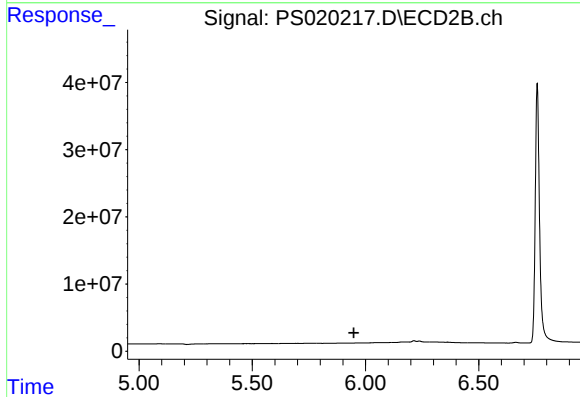


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

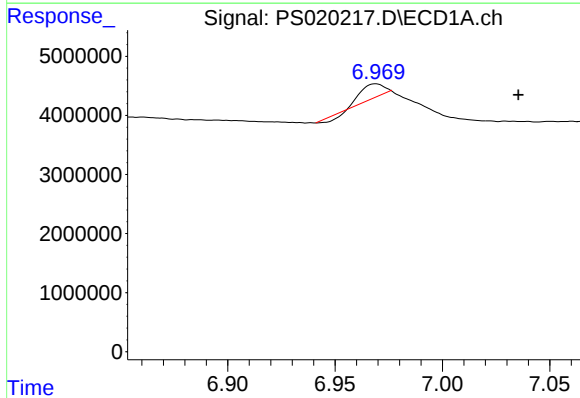


#3 4-Nitrophenol

R.T.: 6.969 min
Delta R.T.: -0.067 min
Response: 1610868
Conc: 1.16 ng/ml

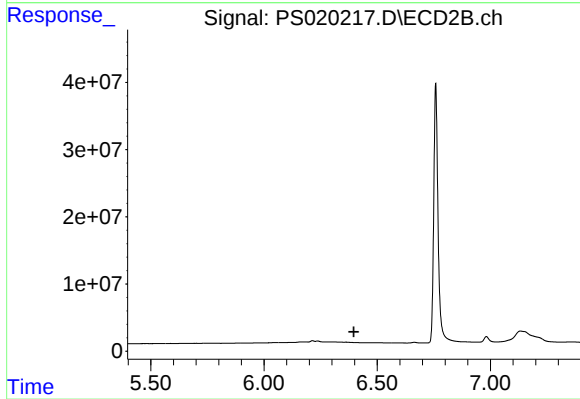

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.397 min
Response: 0
Conc: N.D.

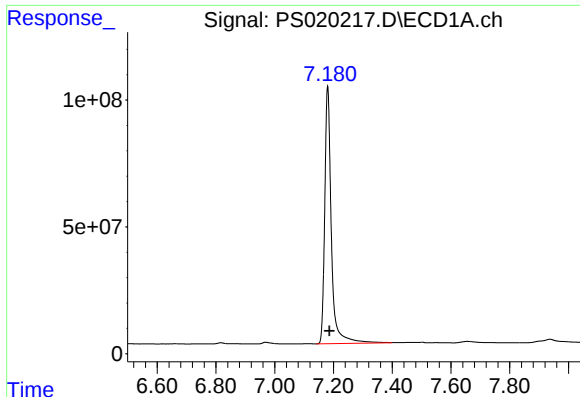

#4 2,4-DCAA


R.T.: 7.180 min
Delta R.T.: -0.005 min
Response: 1588102442
Conc: 538.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

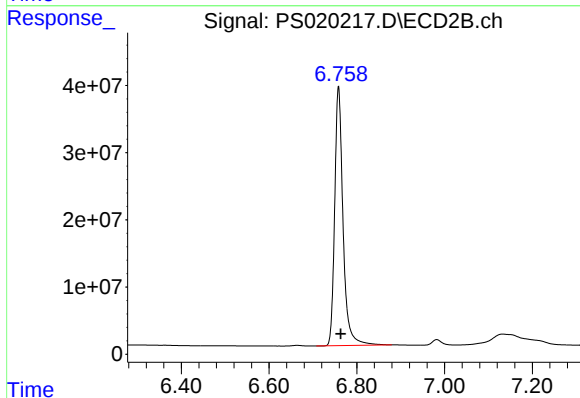


#4 2,4-DCAA

R.T.: 6.758 min
Delta R.T.: -0.005 min
Response: 510485276
Conc: 626.40 ng/ml

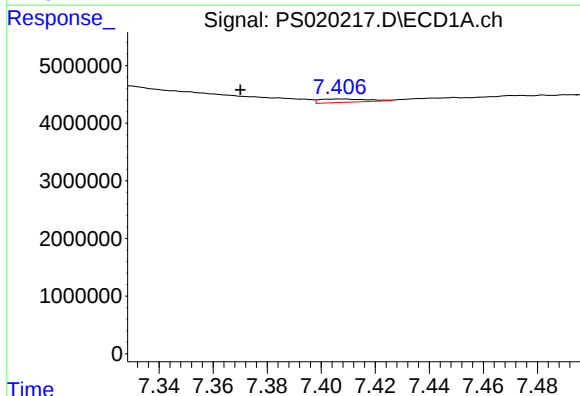


#5 DICAMBA

R.T.: 7.408 min
Delta R.T.: 0.038 min
Response: 716814
Conc: N.D.

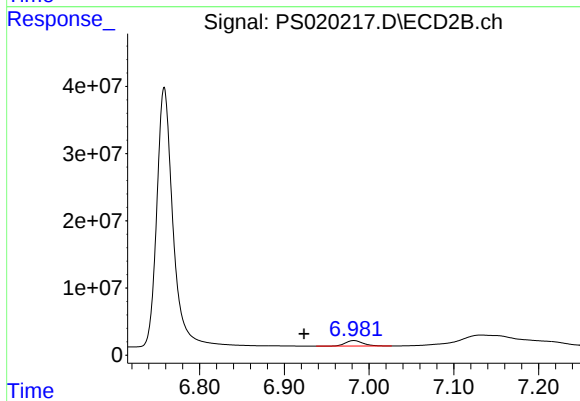

#5 DICAMBA


R.T.: 6.982 min
Delta R.T.: 0.059 min
Response: 11717470
Conc: 3.29 ng/ml

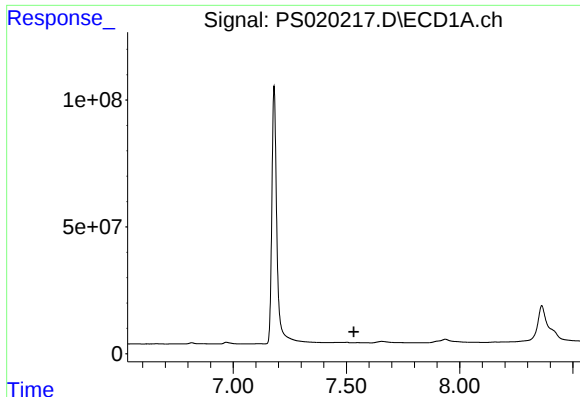

#6 MCPP


R.T.: 7.550 min
Delta R.T.: 0.017 min
Response: -2907873
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

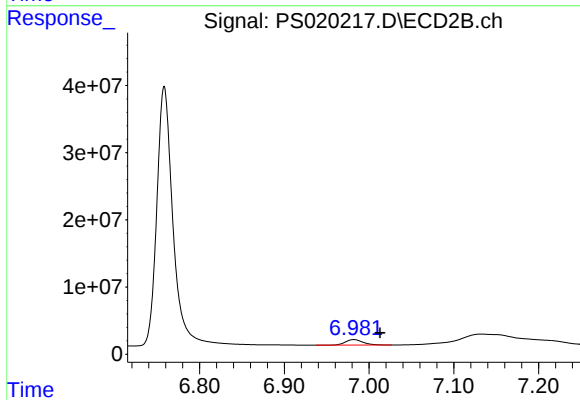


#6 MCPP

R.T.: 6.982 min
Delta R.T.: -0.031 min
Response: 11717470
Conc: 4.30 ug/ml

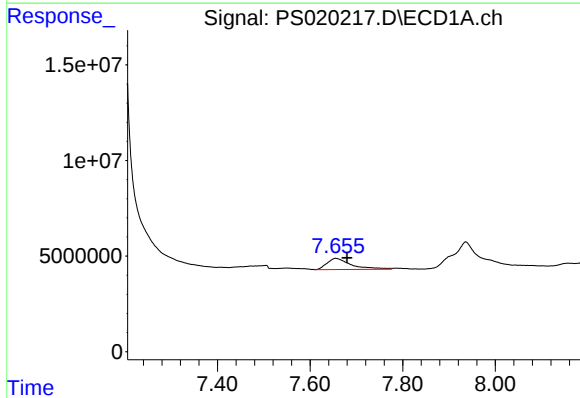


#7 MCPA

R.T.: 7.655 min
Delta R.T.: -0.025 min
Response: 21423676
Conc: 1.66 ug/ml

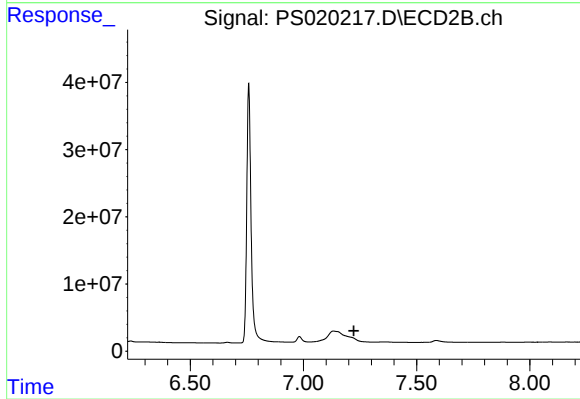

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.223 min
Response: 0
Conc: N.D.

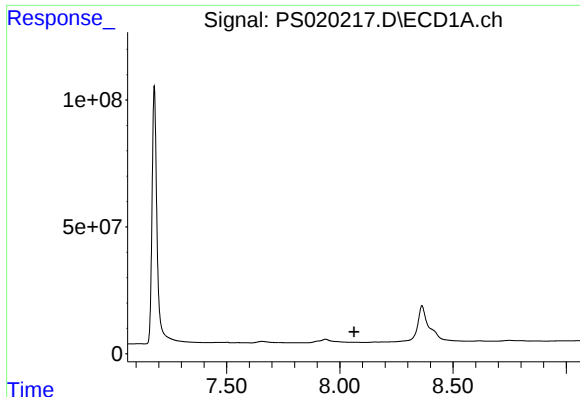

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

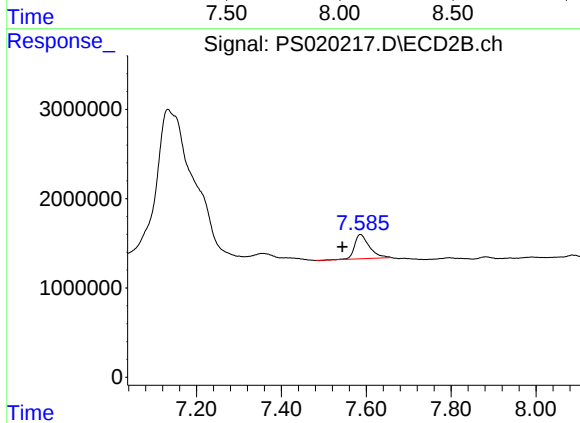


#8 DICHLORPROP

R.T.: 7.586 min
Delta R.T.: 0.042 min
Response: 6549068
Conc: 7.00 ng/ml

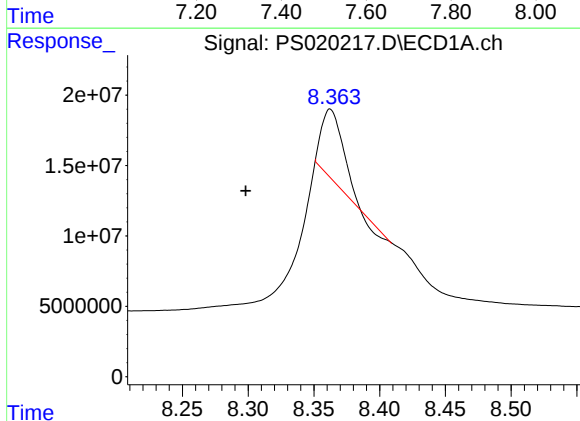


#9 2,4-D

R.T.: 8.362 min
Delta R.T.: 0.064 min
Response: 46654503
Conc: 15.49 ng/ml

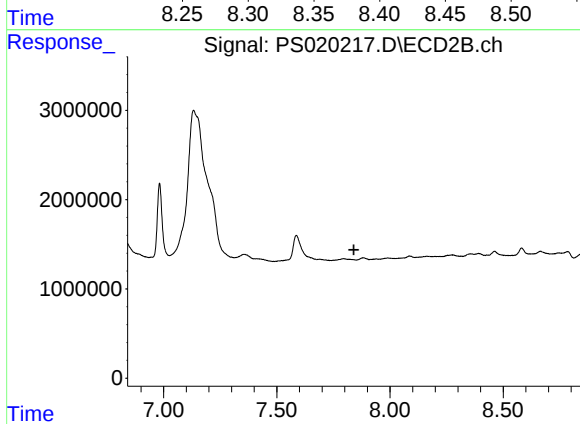

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.840 min
Response: 0
Conc: N.D.

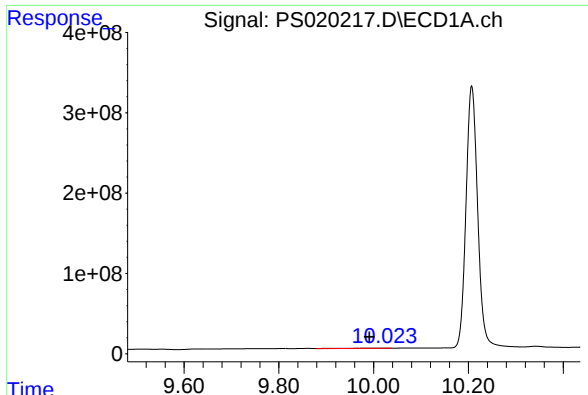

#13 2,4-DB


R.T.: 10.027 min
Delta R.T.: 0.036 min
Response: 16309042
Conc: 4.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

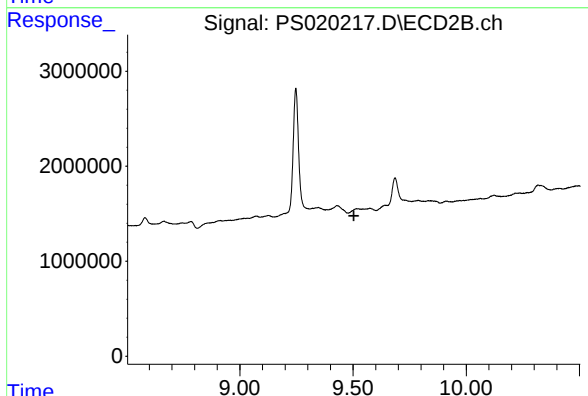


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.503 min
Response: 0
Conc: N.D.

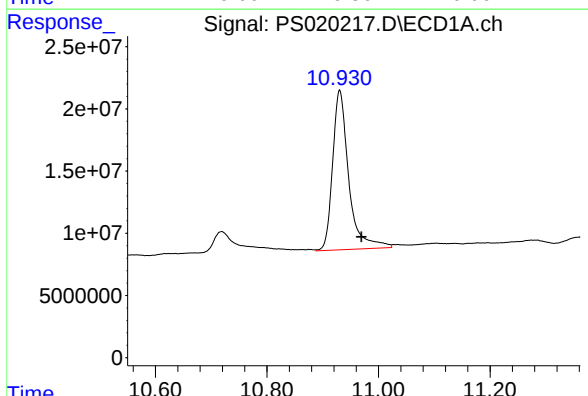

#15 Picloram

R.T.: 10.930 min
Delta R.T.: -0.039 min
Response: 257430529
Conc: 8.14 ng/ml

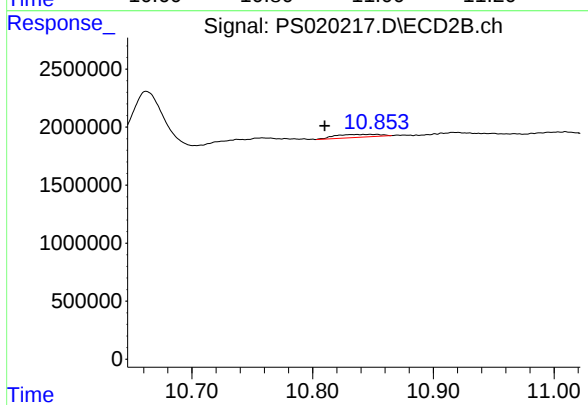

#15 Picloram

R.T.: 10.848 min
Delta R.T.: 0.038 min
Response: 651049
Conc: N.D.