

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080524\
 Data File : PS027301.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2024 20:09
 Operator : AR\AJ
 Sample : HSTDICC200
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC200

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 08:10:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 06 07:56:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.186	7.746	609.0E6	441.9E6	242.153	237.633
Target Compounds							
1) T	Dalapon	2.608	2.696	648.1E6	693.2E6	198.317	207.755
2) T	3,5-DICHL...	6.365	6.700	882.4E6	588.4E6	221.614	214.714
3) T	4-Nitroph...	6.985	7.274	311.9E6	247.1E6	206.302	197.488
5) T	DICAMBA	7.368	7.944	2366.9E6	1815.8E6	214.463	210.810
6) T	MCPD	7.545	8.042	136.3E6	106.1E6	17.907	18.625
7) T	MCPA	7.690	8.285	183.7E6	143.9E6	18.965	19.055
8) T	DICHLORPROP	8.063	8.657	597.5E6	459.2E6	225.820	219.671
9) T	2,4-D	8.291	8.987	642.1E6	512.5E6	225.222	219.970
10) T	Pentachlo...	8.581	9.513	9005.2E6	7090.3E6	227.813	222.775
11) T	2,4,5-TP ...	9.154	9.888	3361.1E6	2817.0E6	221.608	220.577
12) T	2,4,5-T	9.444	10.307	3180.2E6	2770.8E6	217.736	219.745
13) T	2,4-DB	10.012	10.872	438.2E6	338.5E6	213.645	214.117
14) T	DINOSEB	11.202	11.249	2310.1E6	1738.9E6	207.275	204.161
15) T	Picloram	11.020	12.343	4023.5E6	3644.0E6	208.685	201.986
16) T	DCPA	11.498	12.290	3980.1E6	3094.4E6	220.326	222.517



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080524\
Data File : PS027301.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2024 20:09
Operator : AR\AJ
Sample : HSTDICC200
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC200

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 08:10:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
Quant Title : 8080.M
QLast Update : Tue Aug 06 07:56:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

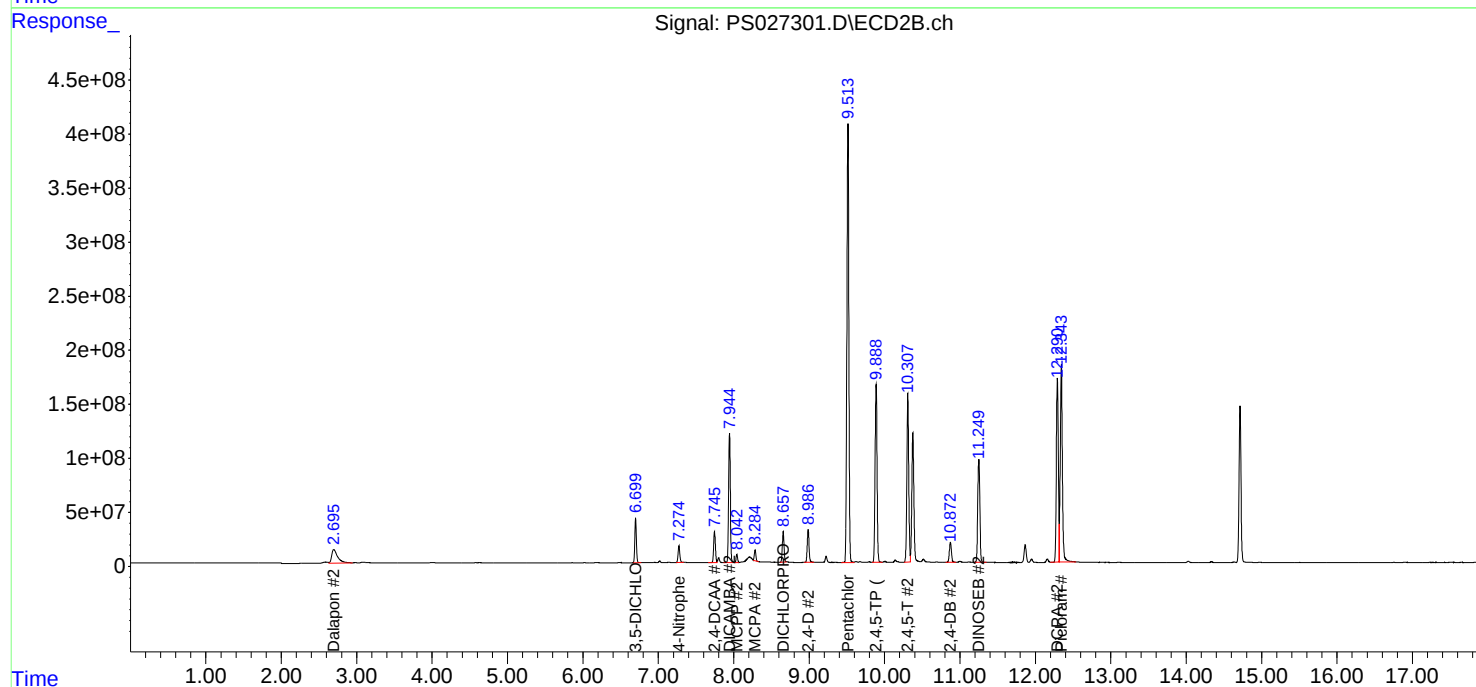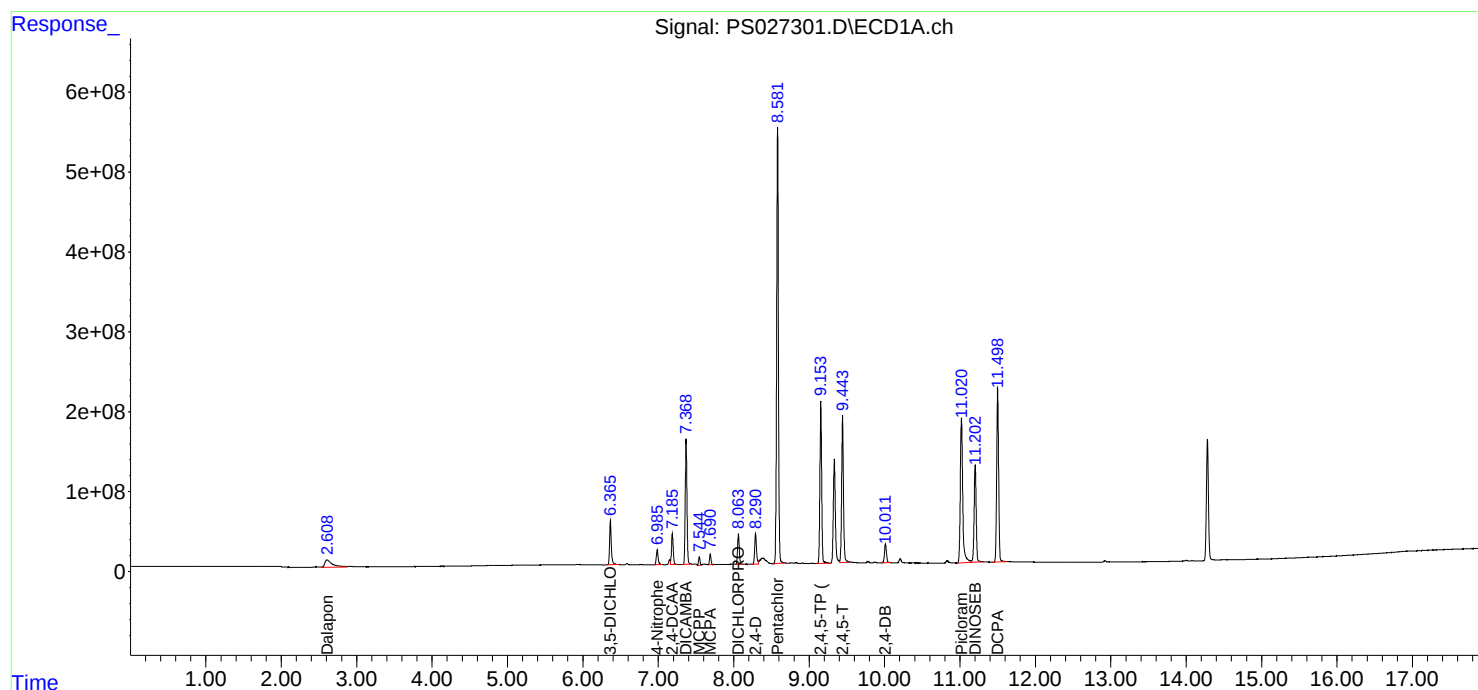


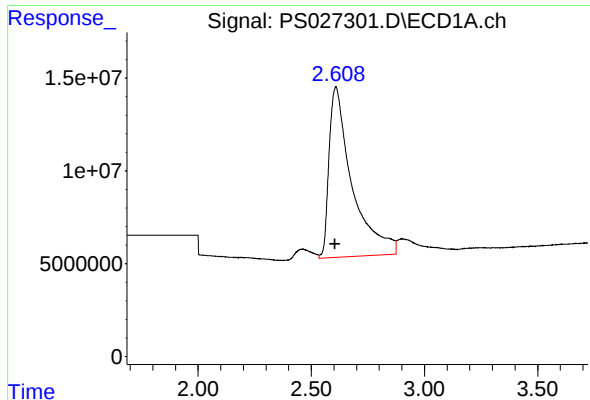

#1 Dalapon


R.T.: 2.608 min
Delta R.T.: 0.003 min
Response: 648103368
Conc: 198.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC200

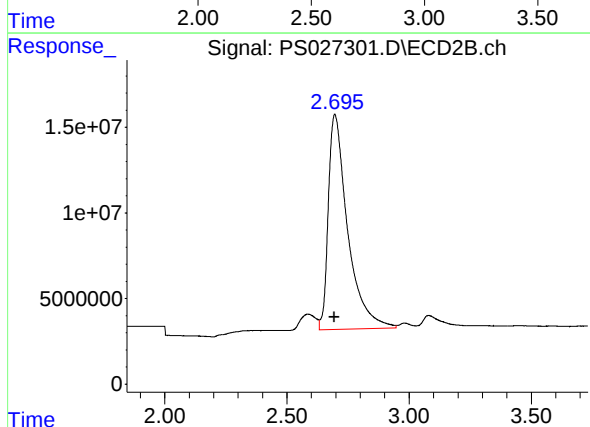


#1 Dalapon

R.T.: 2.696 min
Delta R.T.: 0.000 min
Response: 693213006
Conc: 207.75 ng/ml

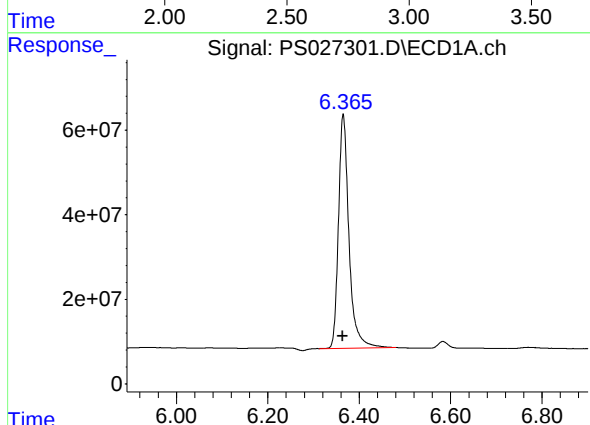


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.365 min
Delta R.T.: 0.000 min
Response: 882405579
Conc: 221.61 ng/ml

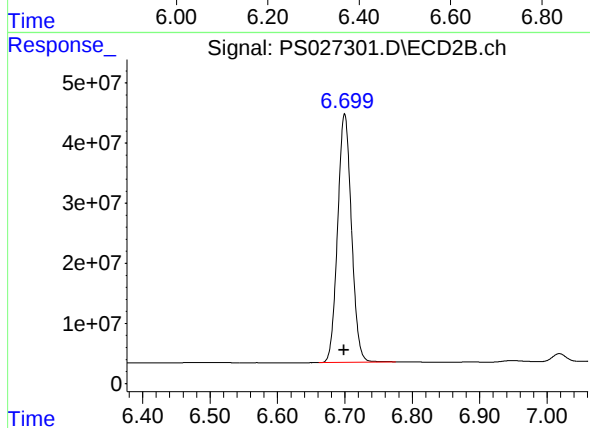

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.700 min
Delta R.T.: 0.000 min
Response: 588428645
Conc: 214.71 ng/ml

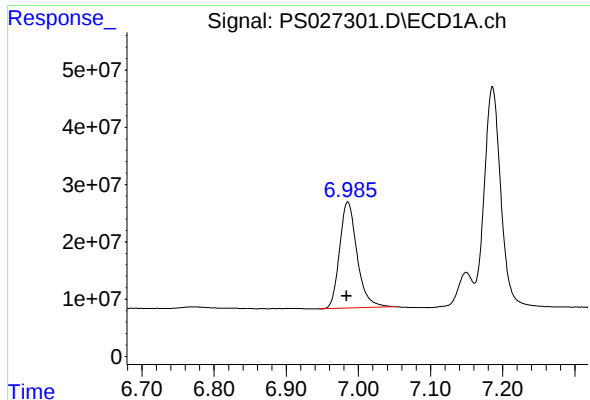

#3 4-Nitrophenol


R.T.: 6.985 min
Delta R.T.: 0.002 min
Response: 311887456
Conc: 206.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC200

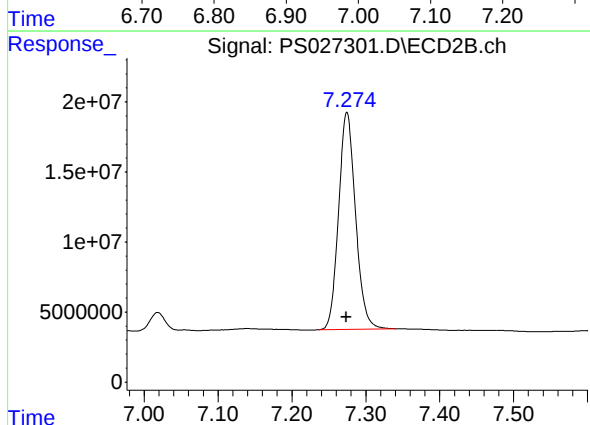


#3 4-Nitrophenol

R.T.: 7.274 min
Delta R.T.: 0.001 min
Response: 247093480
Conc: 197.49 ng/ml

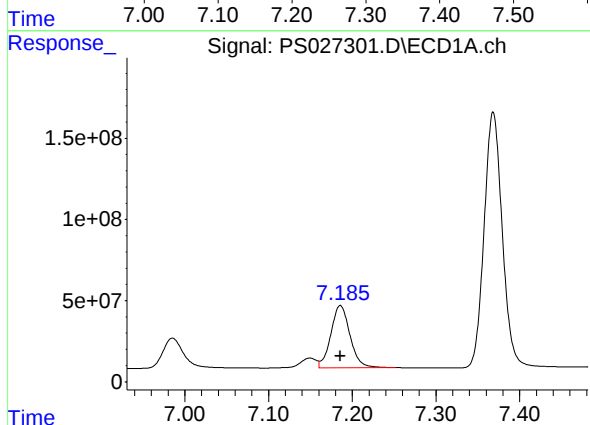


#4 2,4-DCAA

R.T.: 7.186 min
Delta R.T.: 0.000 min
Response: 609044393
Conc: 242.15 ng/ml

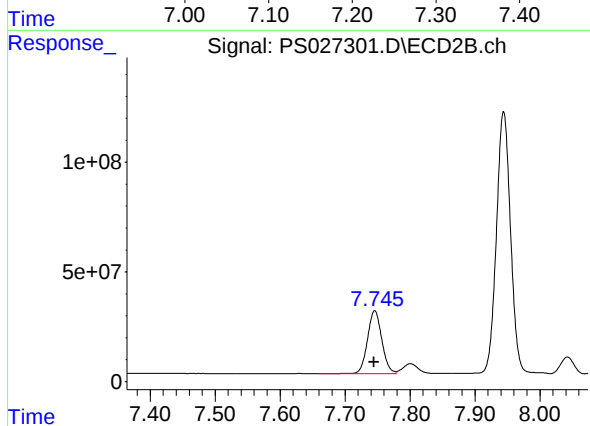

#4 2,4-DCAA


R.T.: 7.746 min
Delta R.T.: 0.000 min
Response: 441942332
Conc: 237.63 ng/ml

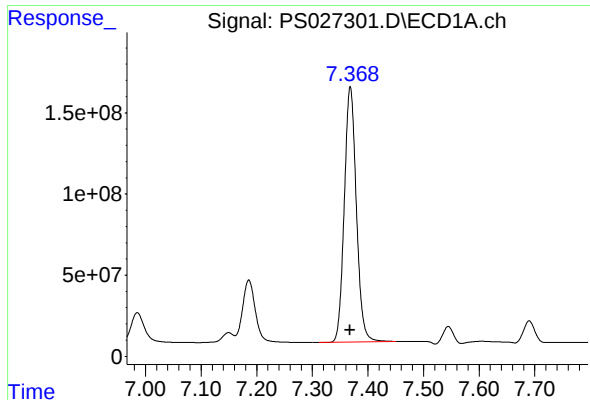

#5 DICAMBA


R.T.: 7.368 min
Delta R.T.: 0.000 min
Response: 2366925711
Conc: 214.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC200

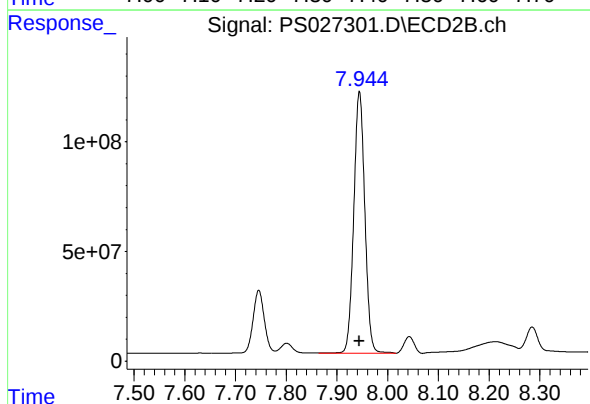


#5 DICAMBA

R.T.: 7.944 min
Delta R.T.: 0.000 min
Response: 1815830963
Conc: 210.81 ng/ml

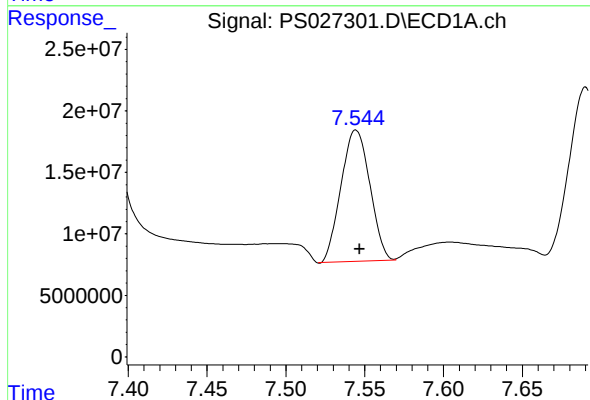


#6 MCPP

R.T.: 7.545 min
Delta R.T.: -0.002 min
Response: 136267382
Conc: 17.91 ug/ml

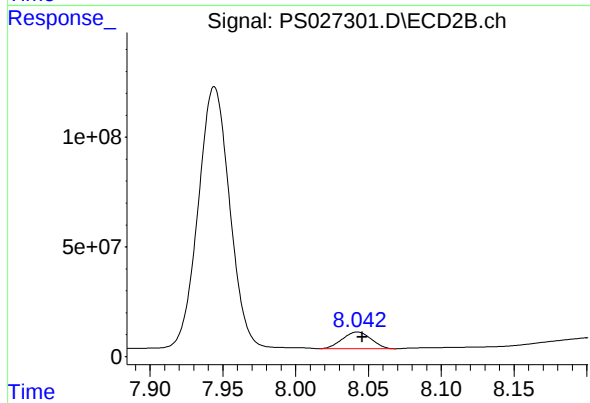

#6 MCPP


R.T.: 8.042 min
Delta R.T.: -0.003 min
Response: 106059808
Conc: 18.63 ug/ml

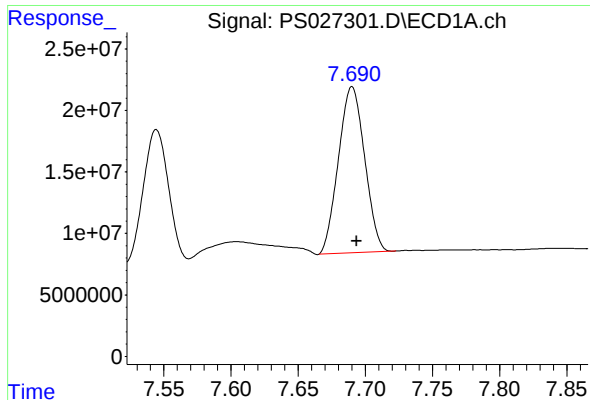

#7 MCPA


R.T.: 7.690 min
Delta R.T.: -0.003 min
Response: 183732965
Conc: 18.96 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC200

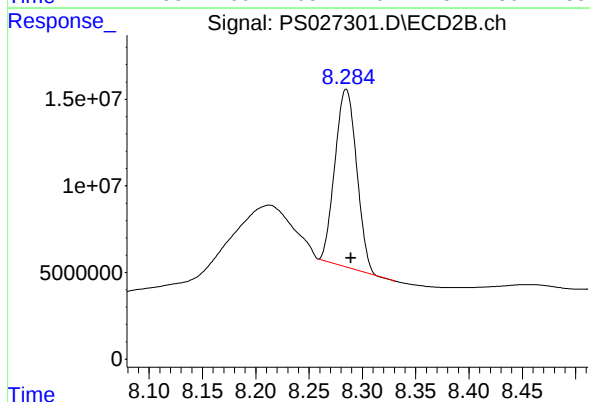


#7 MCPA

R.T.: 8.285 min
Delta R.T.: -0.005 min
Response: 143943308
Conc: 19.06 ug/ml

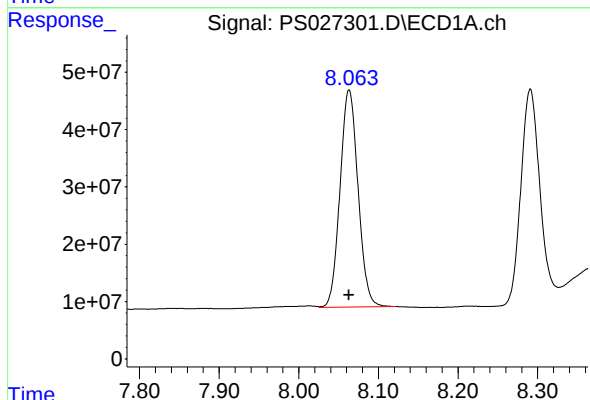


#8 DICHLORPROP

R.T.: 8.063 min
Delta R.T.: 0.000 min
Response: 597495296
Conc: 225.82 ng/ml

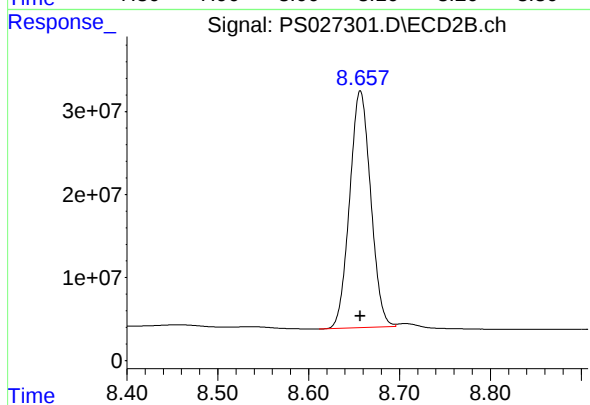

#8 DICHLORPROP


R.T.: 8.657 min
Delta R.T.: 0.000 min
Response: 459218716
Conc: 219.67 ng/ml

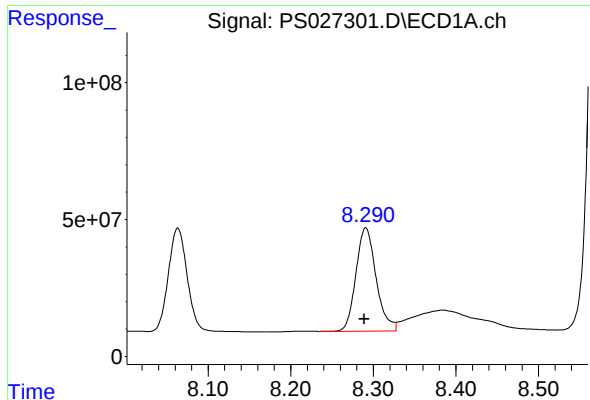

#9 2,4-D


R.T.: 8.291 min
Delta R.T.: 0.002 min
Response: 642137044
Conc: 225.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC200

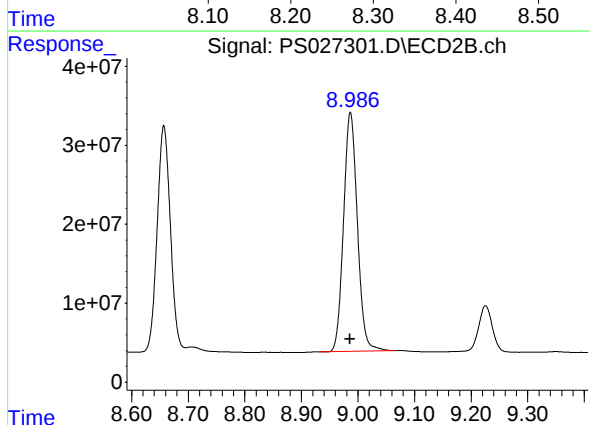


#9 2,4-D

R.T.: 8.987 min
Delta R.T.: 0.000 min
Response: 512464718
Conc: 219.97 ng/ml

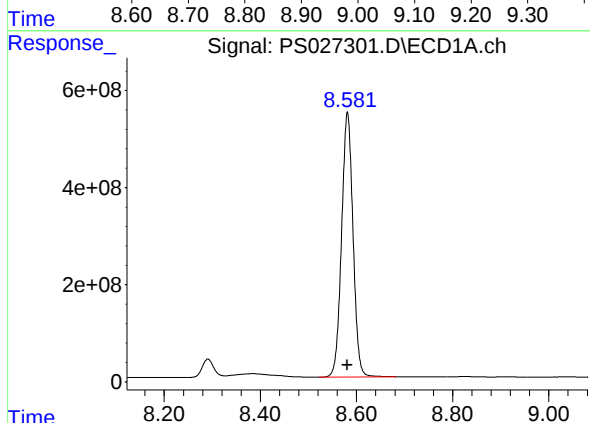


#10 Pentachlorophenol

R.T.: 8.581 min
Delta R.T.: 0.000 min
Response: 9005241575
Conc: 227.81 ng/ml

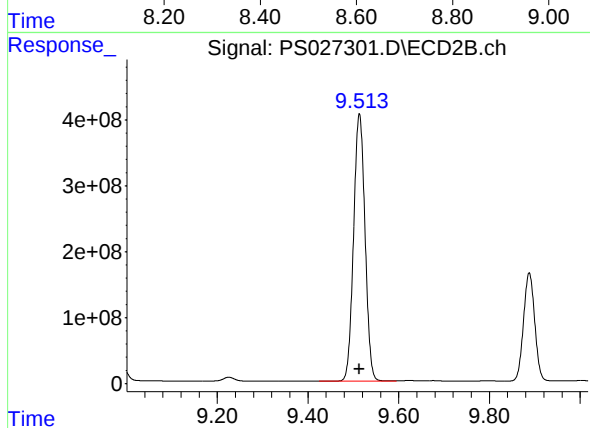

#10 Pentachlorophenol


R.T.: 9.513 min
Delta R.T.: 0.000 min
Response: 7090305529
Conc: 222.78 ng/ml

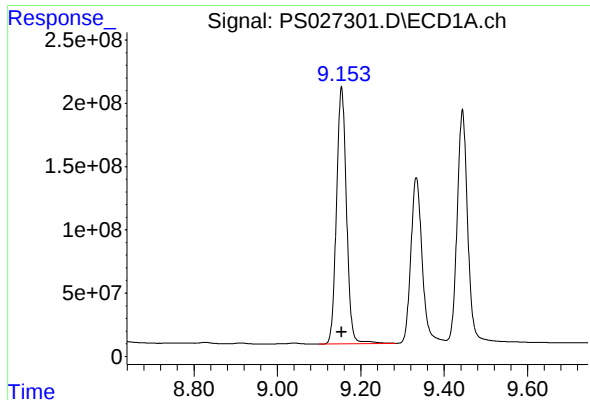

#11 2,4,5-TP (SILVEX)


R.T.: 9.154 min
Delta R.T.: 0.000 min
Response: 3361060313
Conc: 221.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC200

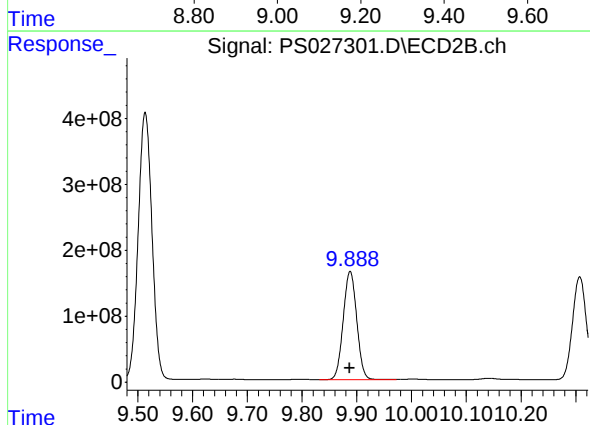


#11 2,4,5-TP (SILVEX)

R.T.: 9.888 min
Delta R.T.: 0.000 min
Response: 2817006236
Conc: 220.58 ng/ml

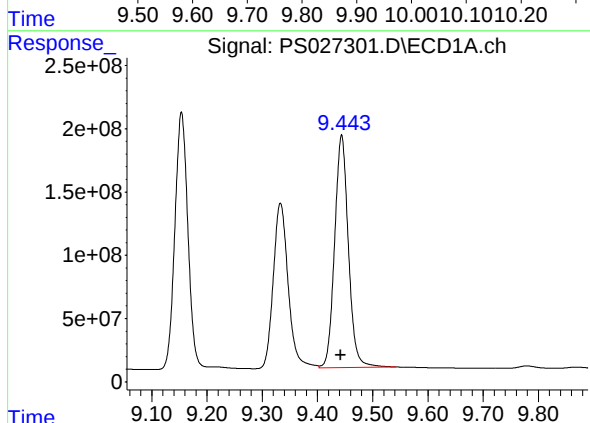


#12 2,4,5-T

R.T.: 9.444 min
Delta R.T.: 0.002 min
Response: 3180172464
Conc: 217.74 ng/ml

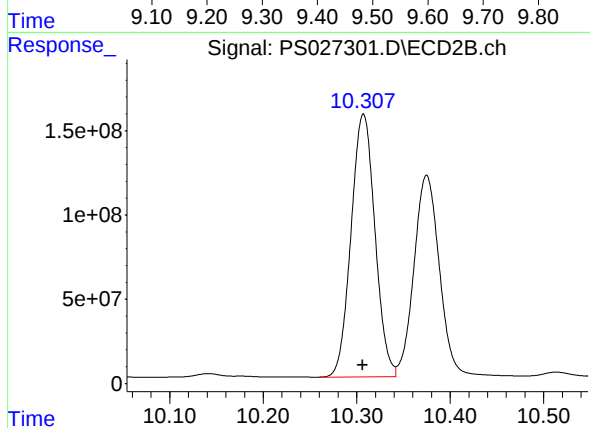

#12 2,4,5-T


R.T.: 10.307 min
Delta R.T.: 0.000 min
Response: 2770807375
Conc: 219.74 ng/ml

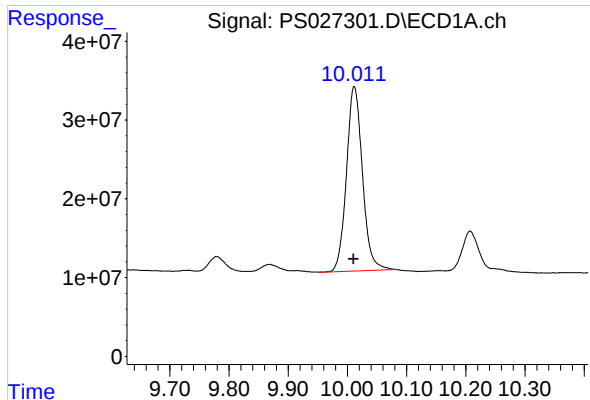

#13 2,4-DB


R.T.: 10.012 min
Delta R.T.: 0.001 min
Response: 438151296
Conc: 213.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC200

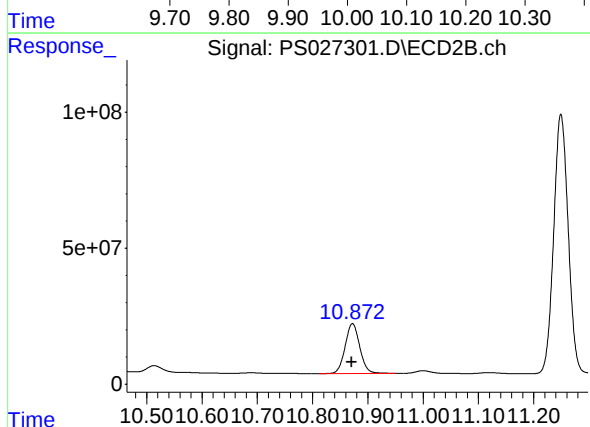


#13 2,4-DB

R.T.: 10.872 min
Delta R.T.: 0.002 min
Response: 338465284
Conc: 214.12 ng/ml

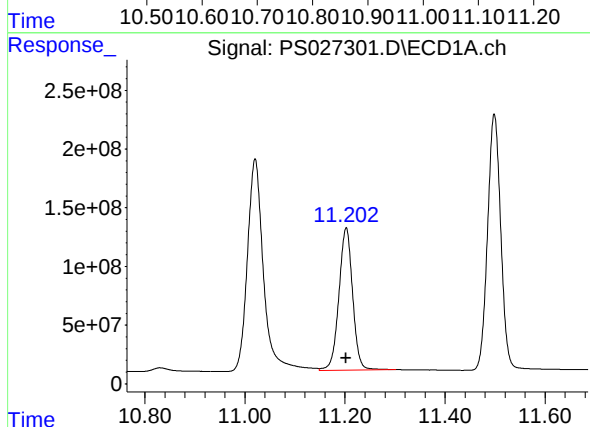


#14 DINOSEB

R.T.: 11.202 min
Delta R.T.: 0.000 min
Response: 2310139278
Conc: 207.28 ng/ml

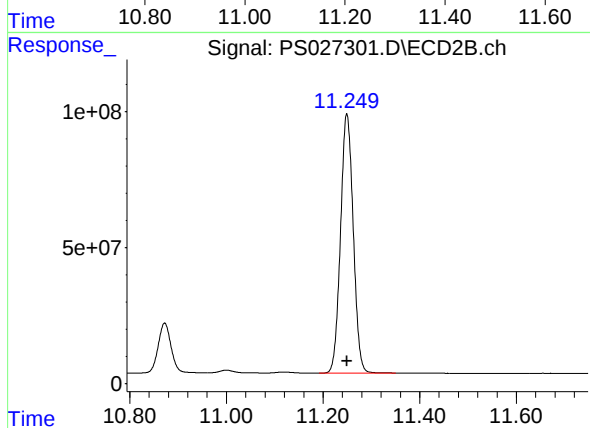

#14 DINOSEB


R.T.: 11.249 min
Delta R.T.: 0.000 min
Response: 1738875163
Conc: 204.16 ng/ml

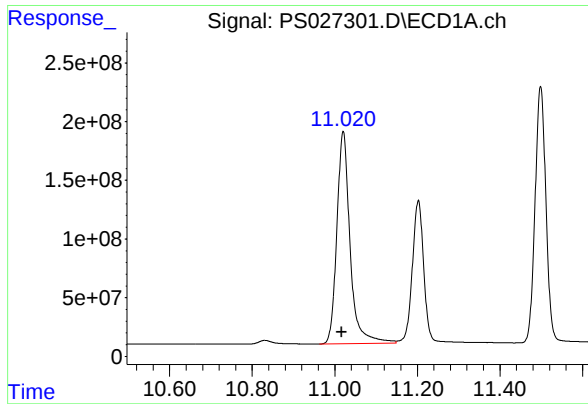

#15 Picloram


R.T.: 11.020 min
Delta R.T.: 0.004 min
Response: 4023530825
Conc: 208.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC200

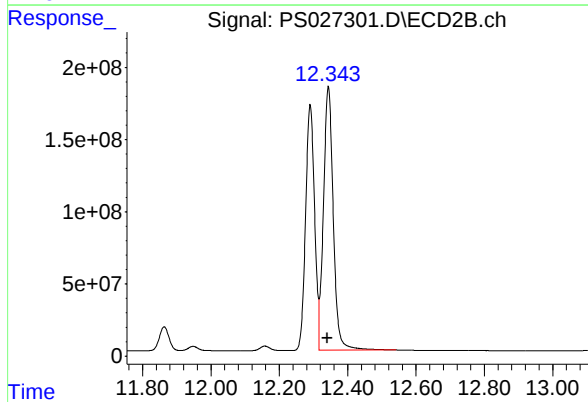


#15 Picloram

R.T.: 12.343 min
Delta R.T.: 0.002 min
Response: 3644046916
Conc: 201.99 ng/ml

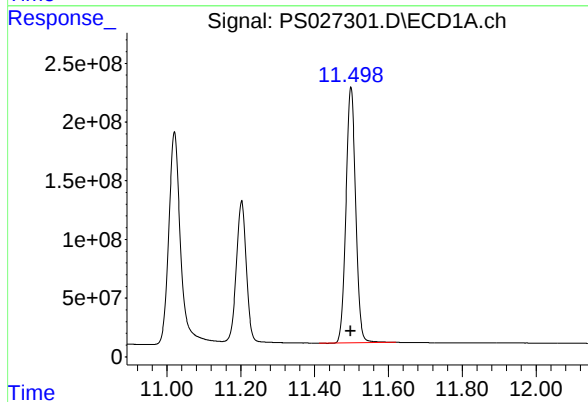

#16 DCPA

R.T.: 11.498 min
Delta R.T.: 0.000 min
Response: 3980145065
Conc: 220.33 ng/ml

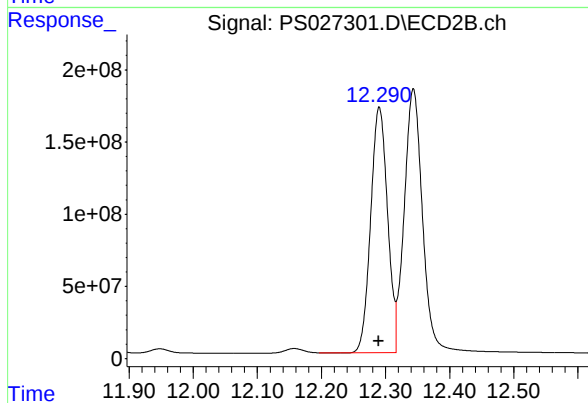

#16 DCPA

R.T.: 12.290 min
Delta R.T.: 0.000 min
Response: 3094400181
Conc: 222.52 ng/ml