

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080525\
 Data File : PS031370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2025 11:00
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 03:48:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072925.M
 Quant Title : 8080.M
 QLast Update : Tue Jul 29 18:38:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.300	7.752	1499.5E6	426.3E6	514.685	510.498
Target Compounds							
1) T	Dalapon	2.734f	2.671f	5186714	38242579	1.075	15.570 #
3) T	4-Nitroph...	7.092	0.000	7245810	0	7.116	N.D. #
5) T	DICAMBA	7.485	0.000	1409878	0	<MDL	N.D. #
6) T	MCP	7.691	0.000	729981	0	<MDL	N.D. #
7) T	MCPA	7.838	0.000	261437	0	<MDL	N.D. #
8) T	DICHLORPROP	8.178f	0.000	2600014	0	<MDL	N.D. #
10) T	Pentachlo...	8.726f	9.522	4697796	7850198	<MDL	<MDL #
11) T	2,4,5-TP ...	9.308	9.912	3274484	5978606	<MDL	<MDL #
12) T	2,4,5-T	9.613	10.375	1703110	8226712	<MDL	<MDL #
13) T	2,4-DB	10.210	0.000	1010851	0	<MDL	N.D. #
14) T	DINOSEB	11.408	0.000	151858	0	<MDL	N.D. #
15) T	Picloram	11.223	12.451f	315307	7561309	<MDL	<MDL #
16) T	DCPA	11.678f	12.332	2847562	4085745	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080525\
Data File : PS031370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2025 11:00
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 03:48:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072925.M
Quant Title : 8080.M
QLast Update : Tue Jul 29 18:38:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

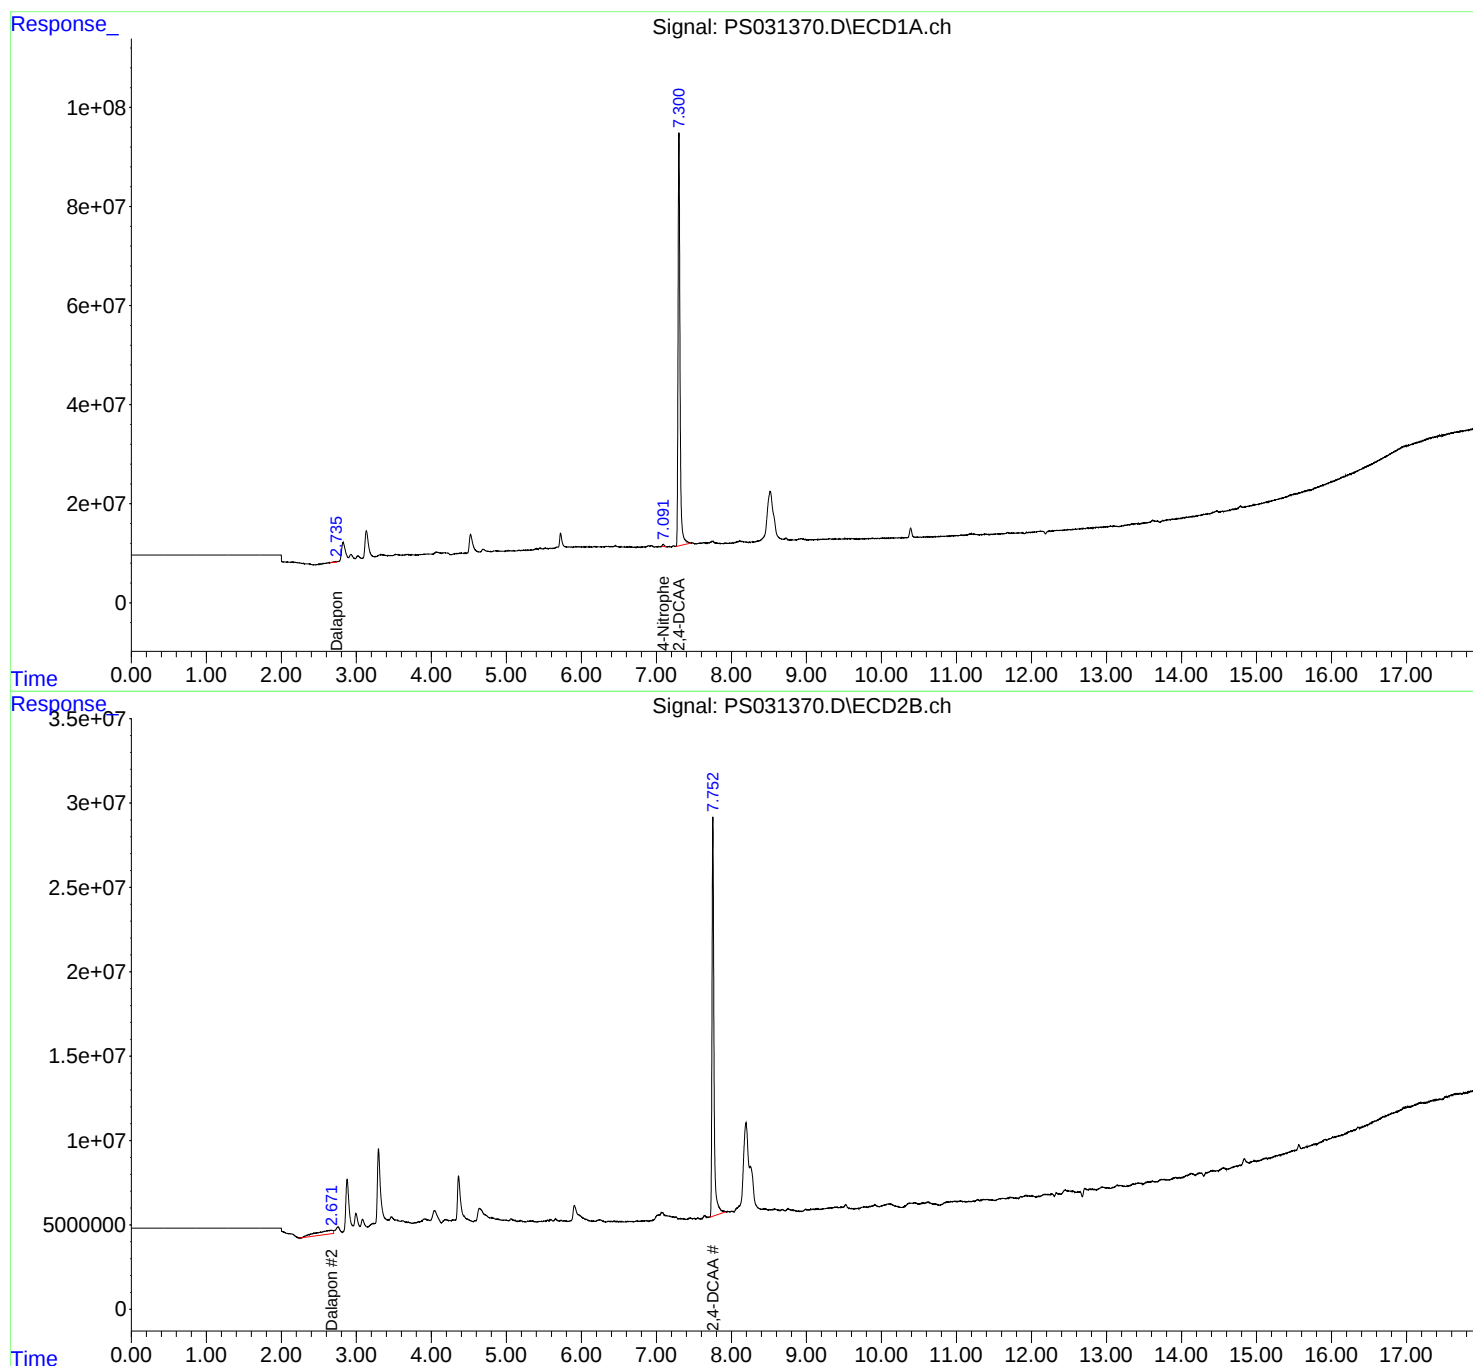


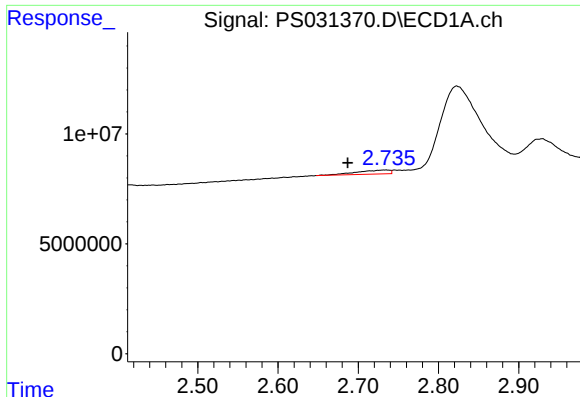

#1 Dalapon


R.T.: 2.734 min
Delta R.T.: 0.047 min
Response: 5186714
Conc: 1.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

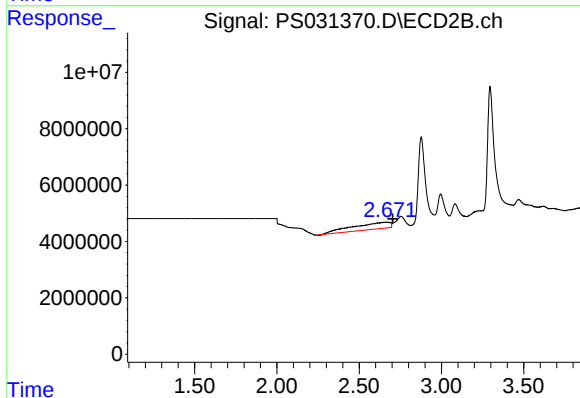


#1 Dalapon

R.T.: 2.671 min
Delta R.T.: -0.032 min
Response: 38242579
Conc: 15.57 ng/ml

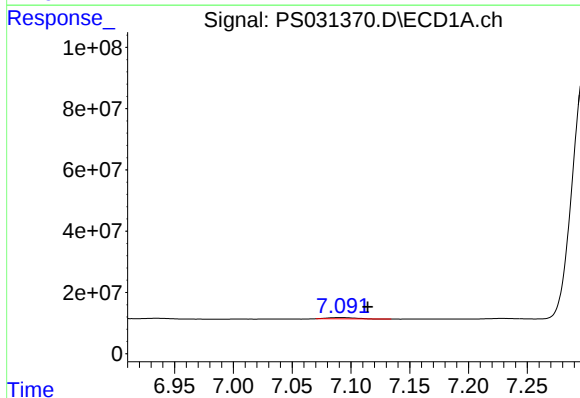


#3 4-Nitrophenol

R.T.: 7.092 min
Delta R.T.: -0.022 min
Response: 7245810
Conc: 7.12 ng/ml

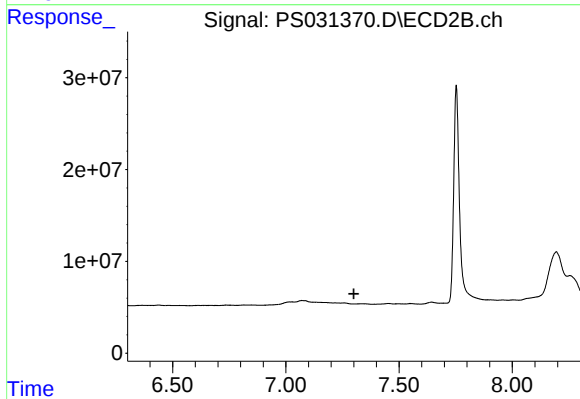

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.300 min
Response: 0
Conc: N.D.

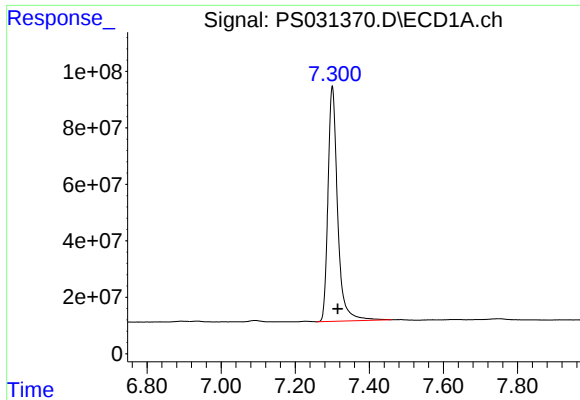

#4 2,4-DCAA

R.T.: 7.300 min
Delta R.T.: -0.014 min
Response: 1499485969
Conc: 514.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

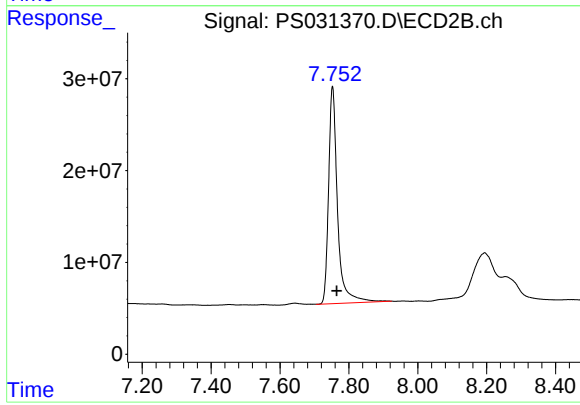

#4 2,4-DCAA

R.T.: 7.752 min
Delta R.T.: -0.012 min
Response: 426307128
Conc: 510.50 ng/ml