

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
 Data File : PS005908.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 17:43
 Operator : SM\AJ
 Sample : K4129-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:38:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.614	5.334	265.2E6	199.5E6	182.763	200.561
Target Compounds							
1) T	Dalapon	2.114	0.000	27734446	0	14.965	N.D. #
3) T	4-Nitroph...	0.000	4.900	0	44101359	N.D.	89.025
5) T	DICAMBA	5.710	0.000	17186099	0	2.878	N.D. #
6) T	MCP	5.835	0.000	34131474	0	7.366	N.D. #
7) T	MCPA	6.010	5.667	76981433	101.3E6	11.797	24.056 #
8) T	DICHLORPROP	0.000	6.022	0	53812004	N.D.	58.268
10) T	Pentachlo...	0.000	6.591	0	24083483	N.D.	1.855
11) T	2,4,5-TP ...	0.000	6.979	0	18334522	N.D.	3.534
12) T	2,4,5-T	7.620	0.000	70996097	0	8.506	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
Data File : PS005908.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 17:43
Operator : SM\AJ
Sample : K4129-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:38:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

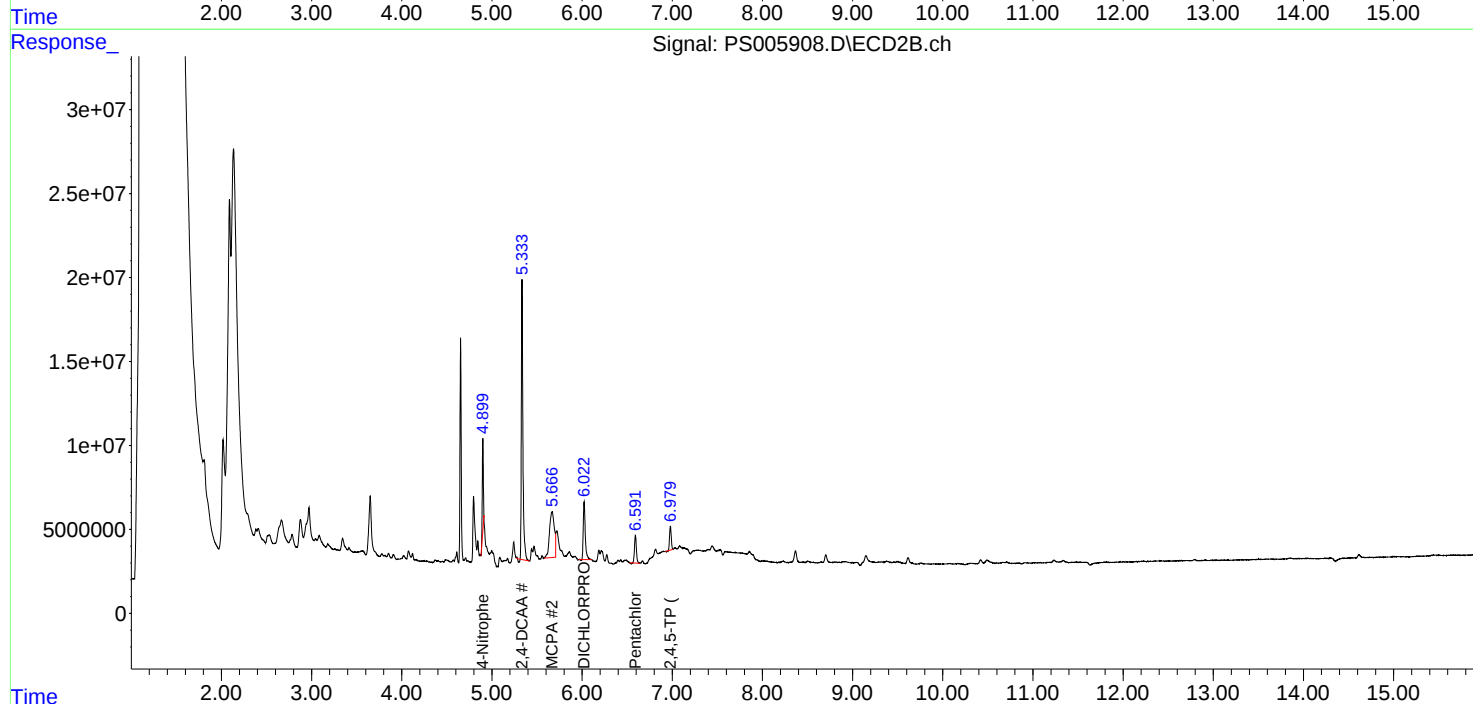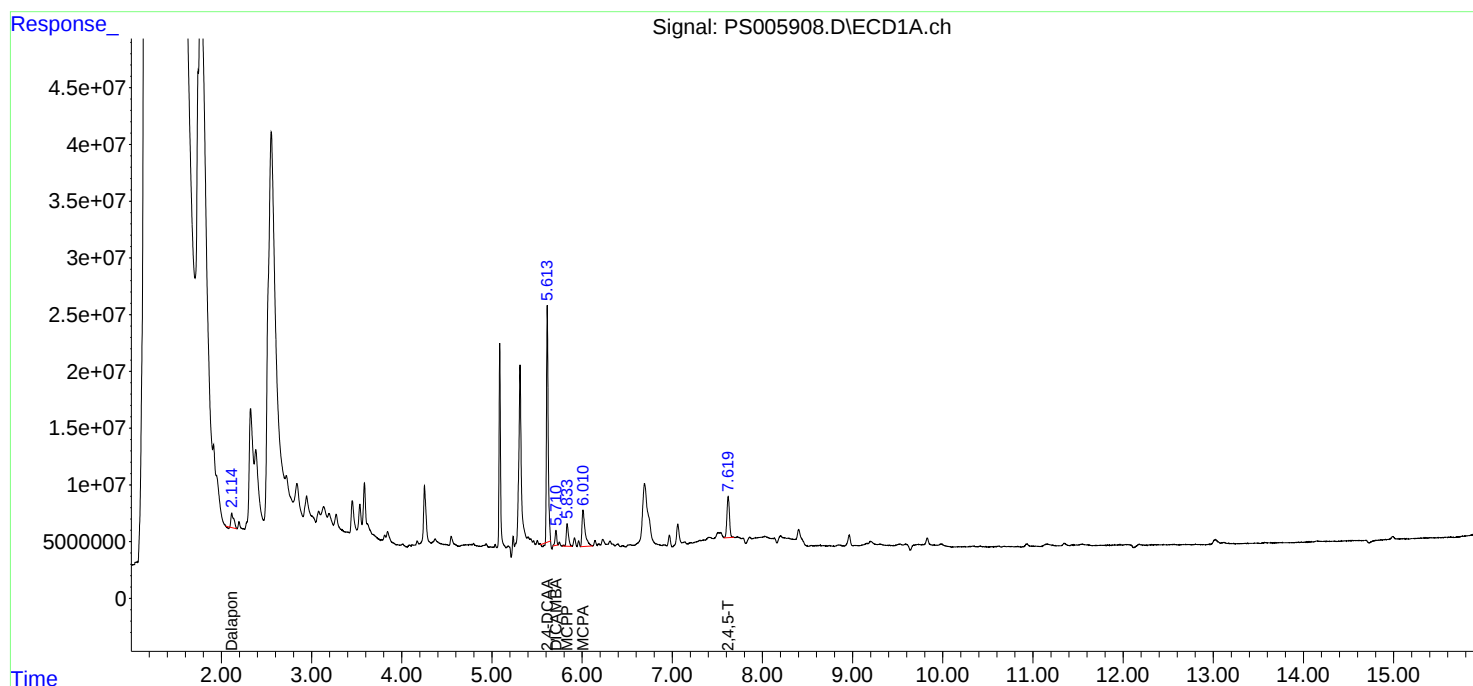


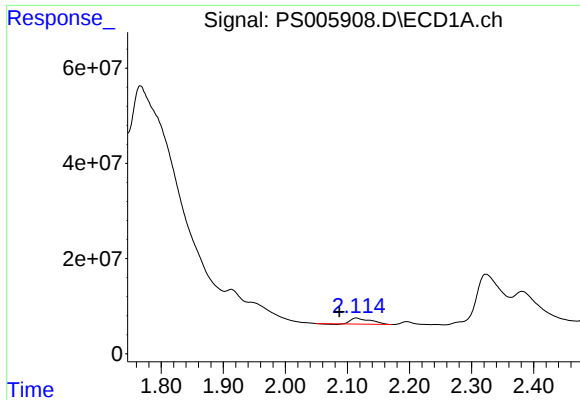

#1 Dalapon


R.T.: 2.114 min
Delta R.T.: 0.027 min
Response: 27734446
Conc: 14.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

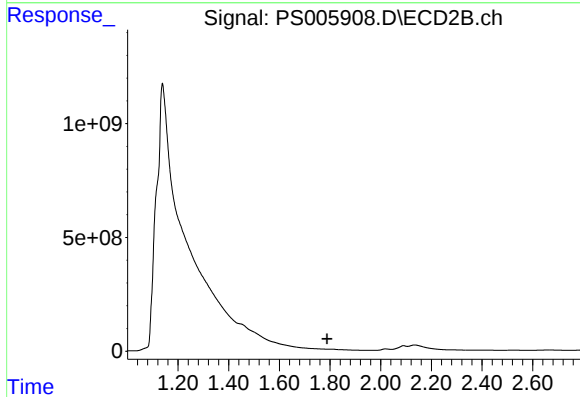


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

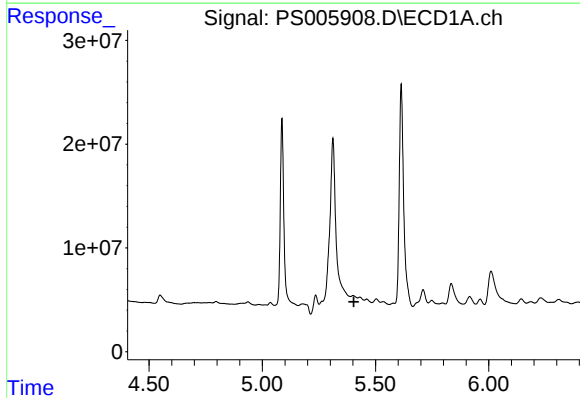


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 5.405 min
Response: 0
Conc: N.D.

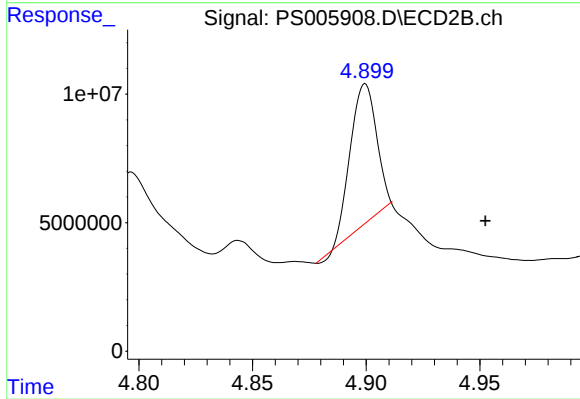

#3 4-Nitrophenol


R.T.: 4.900 min
Delta R.T.: -0.053 min
Response: 44101359
Conc: 89.02 ng/ml

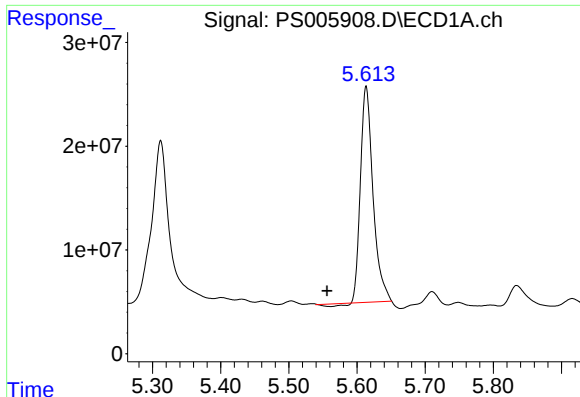

#4 2,4-DCAA


R.T.: 5.614 min
Delta R.T.: 0.057 min
Response: 265155168
Conc: 182.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

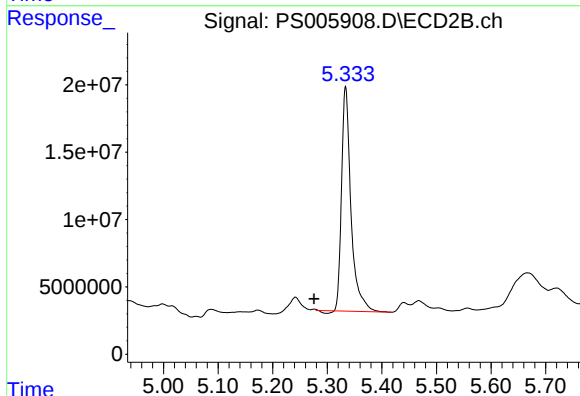


#4 2,4-DCAA

R.T.: 5.334 min
Delta R.T.: 0.058 min
Response: 199493186
Conc: 200.56 ng/ml

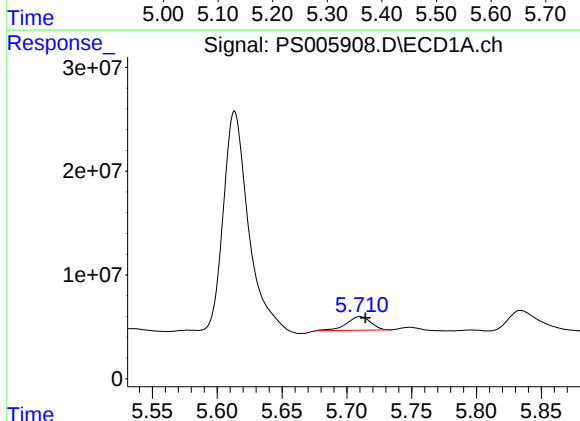


#5 DICAMBA

R.T.: 5.710 min
Delta R.T.: -0.004 min
Response: 17186099
Conc: 2.88 ng/ml

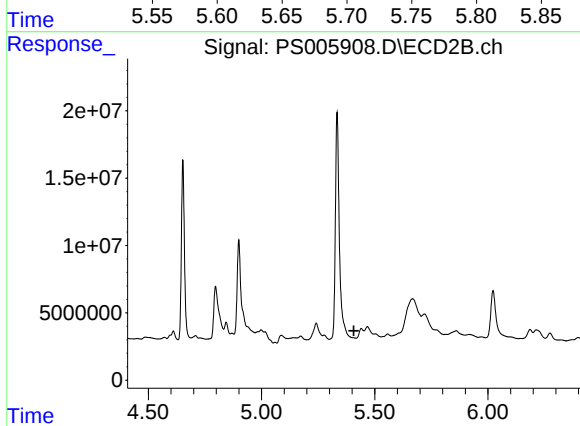

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

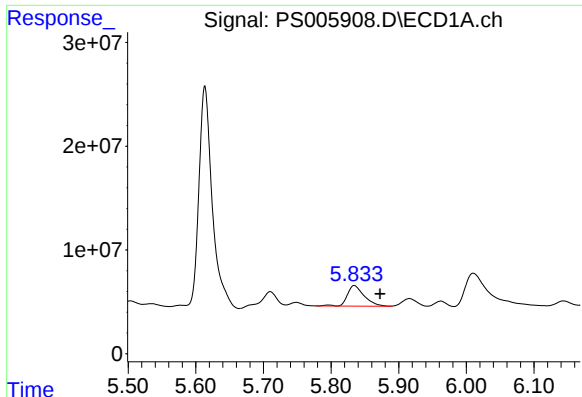

#6 MCPP


R.T.: 5.835 min
Delta R.T.: -0.038 min
Response: 34131474
Conc: 7.37 ug/ml

Instrument :
ECD_S
ClientSampleId :

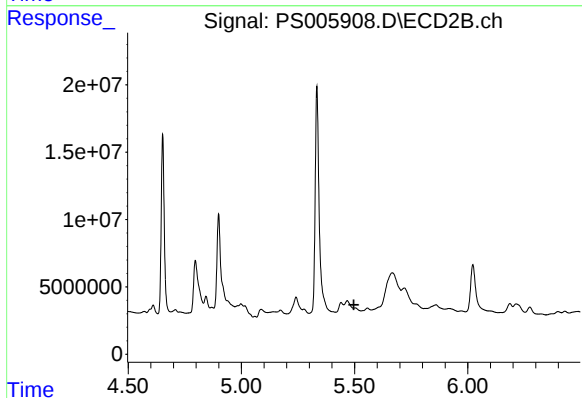


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

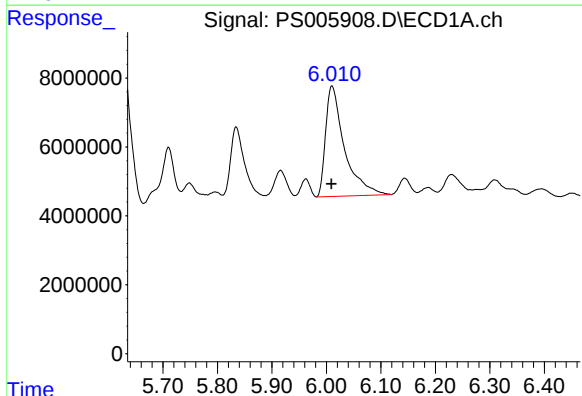


#7 MCPA

R.T.: 6.010 min
Delta R.T.: 0.001 min
Response: 76981433
Conc: 11.80 ug/ml

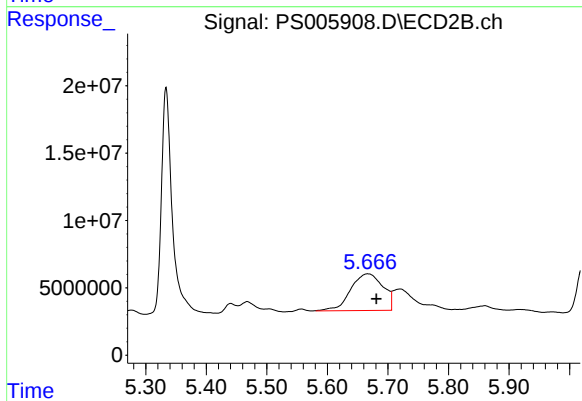

#7 MCPA


R.T.: 5.667 min
Delta R.T.: -0.014 min
Response: 101253105
Conc: 24.06 ug/ml

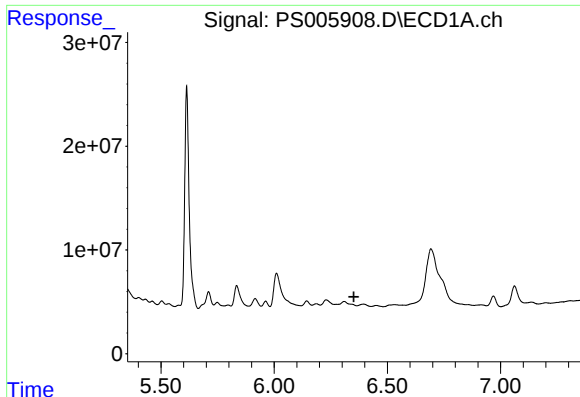

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

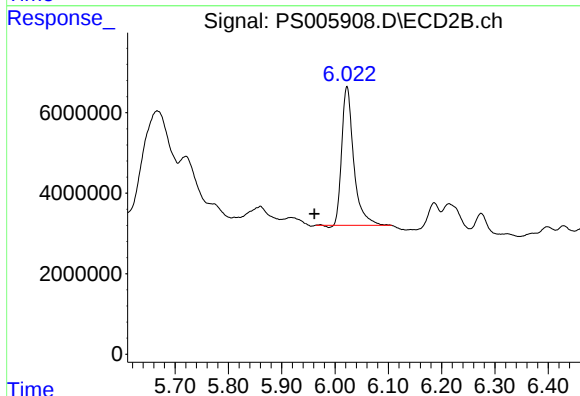


#8 DICHLORPROP

R.T.: 6.022 min
Delta R.T.: 0.061 min
Response: 53812004
Conc: 58.27 ng/ml

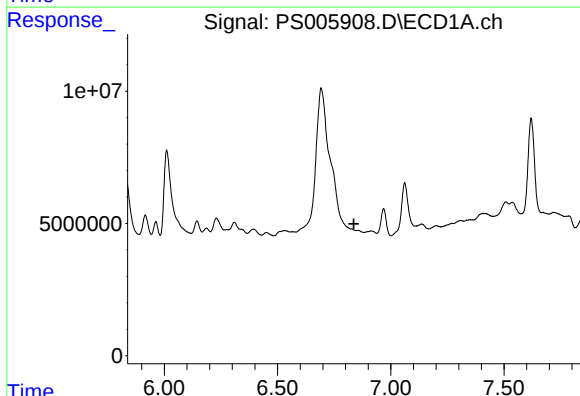


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

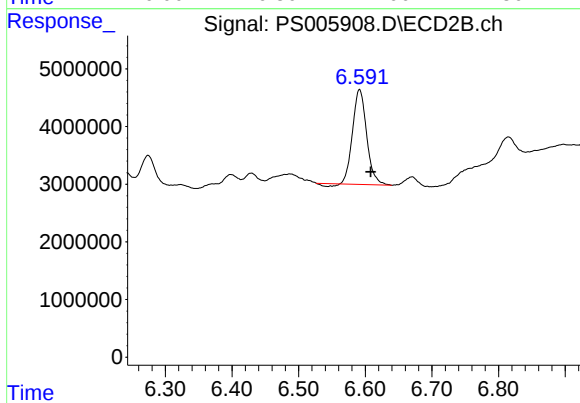

#10 Pentachlorophenol


R.T.: 6.591 min
Delta R.T.: -0.017 min
Response: 24083483
Conc: 1.86 ng/ml

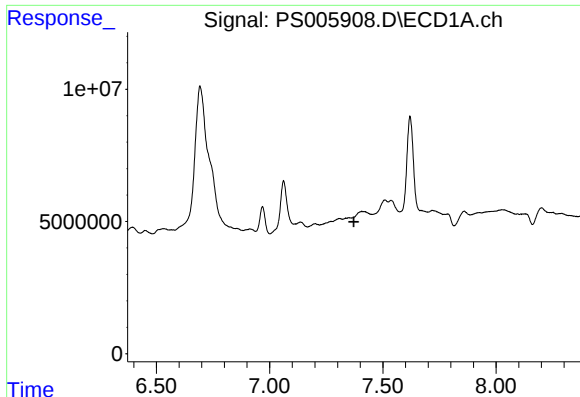

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

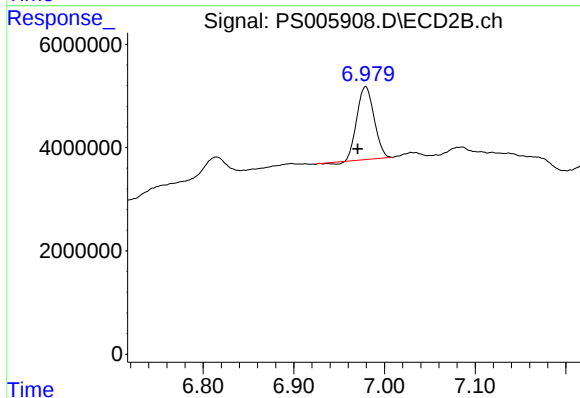


#11 2,4,5-TP (SILVEX)

R.T.: 6.979 min
Delta R.T.: 0.008 min
Response: 18334522
Conc: 3.53 ng/ml

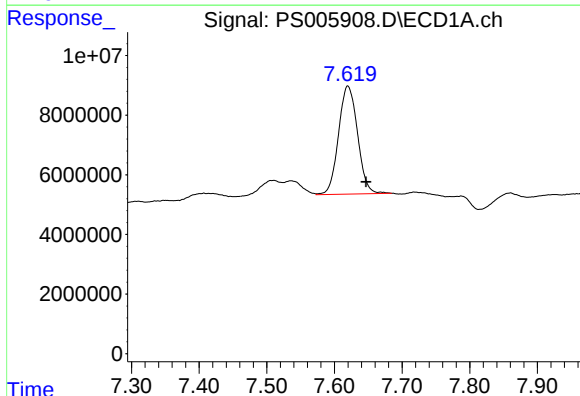

#12 2,4,5-T

R.T.: 7.620 min
Delta R.T.: -0.027 min
Response: 70996097
Conc: 8.51 ng/ml

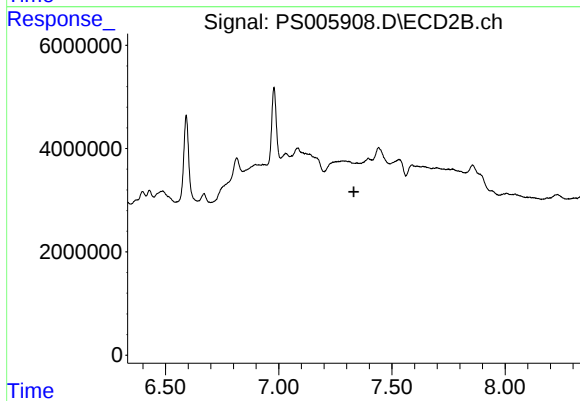

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.