

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
 Data File : PS005911.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 18:50
 Operator : SM\AJ
 Sample : K4129-20
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:40:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.554	5.274	223.5E6	179.5E6	154.064	180.465
Target Compounds							
1) T	Dalapon	2.053	0.000	25862531	0	13.955	N.D. #
2) T	3,5-DICHL...	0.000	4.592	0	111.9E6	N.D.	86.218
3) T	4-Nitroph...	5.340	0.000	7486954	0	12.447	N.D. #
5) T	DICAMBA	5.774	5.378	45533820	6606700	7.624	1.770 #
7) T	MCPA	5.960	0.000	34342740	0	5.263	N.D. #
8) T	DICHLORPROP	0.000	5.967	0	25748315	N.D.	27.881
9) T	2,4-D	6.631	0.000	255.9E6	0	170.752	N.D. #
11) T	2,4,5-TP ...	0.000	6.960	0	1114.3E6	N.D.	214.811
12) T	2,4,5-T	0.000	7.322	0	6986692	N.D.	1.470



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
Data File : PS005911.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 18:50
Operator : SM\AJ
Sample : K4129-20
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:40:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

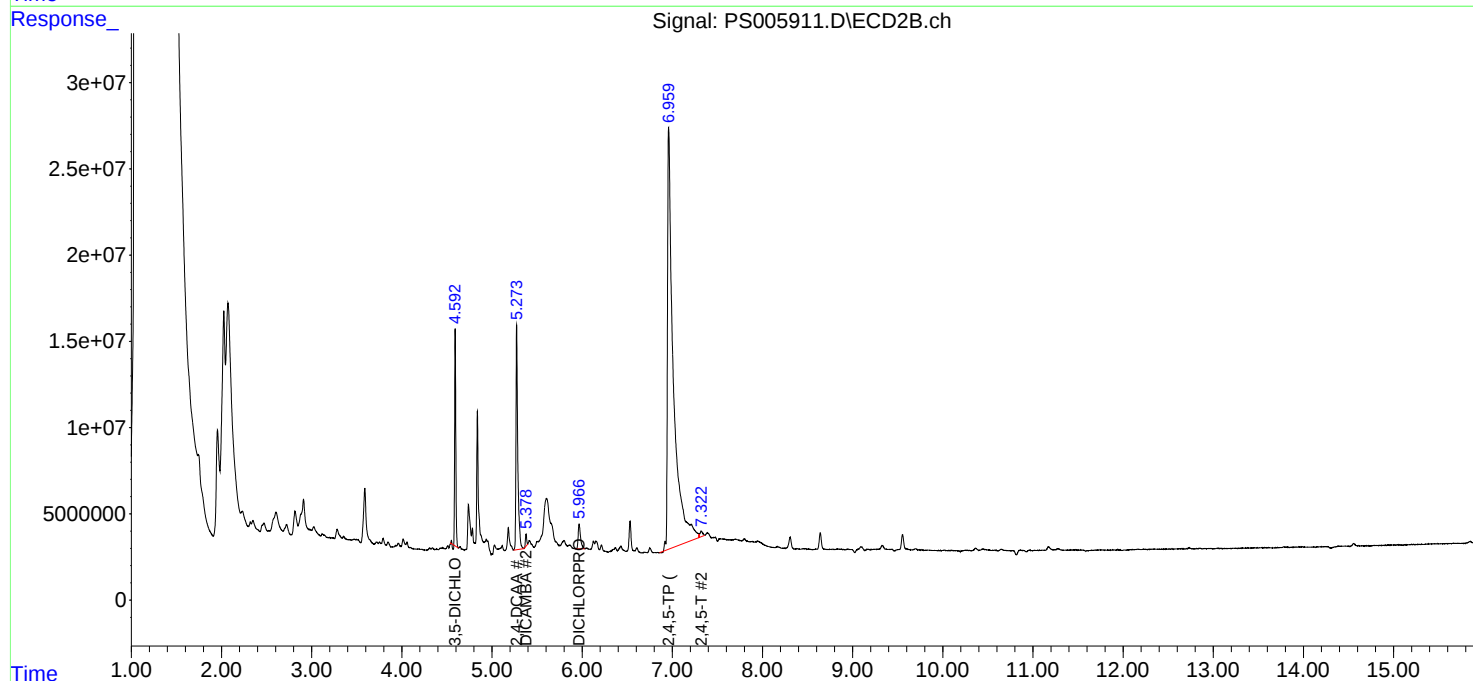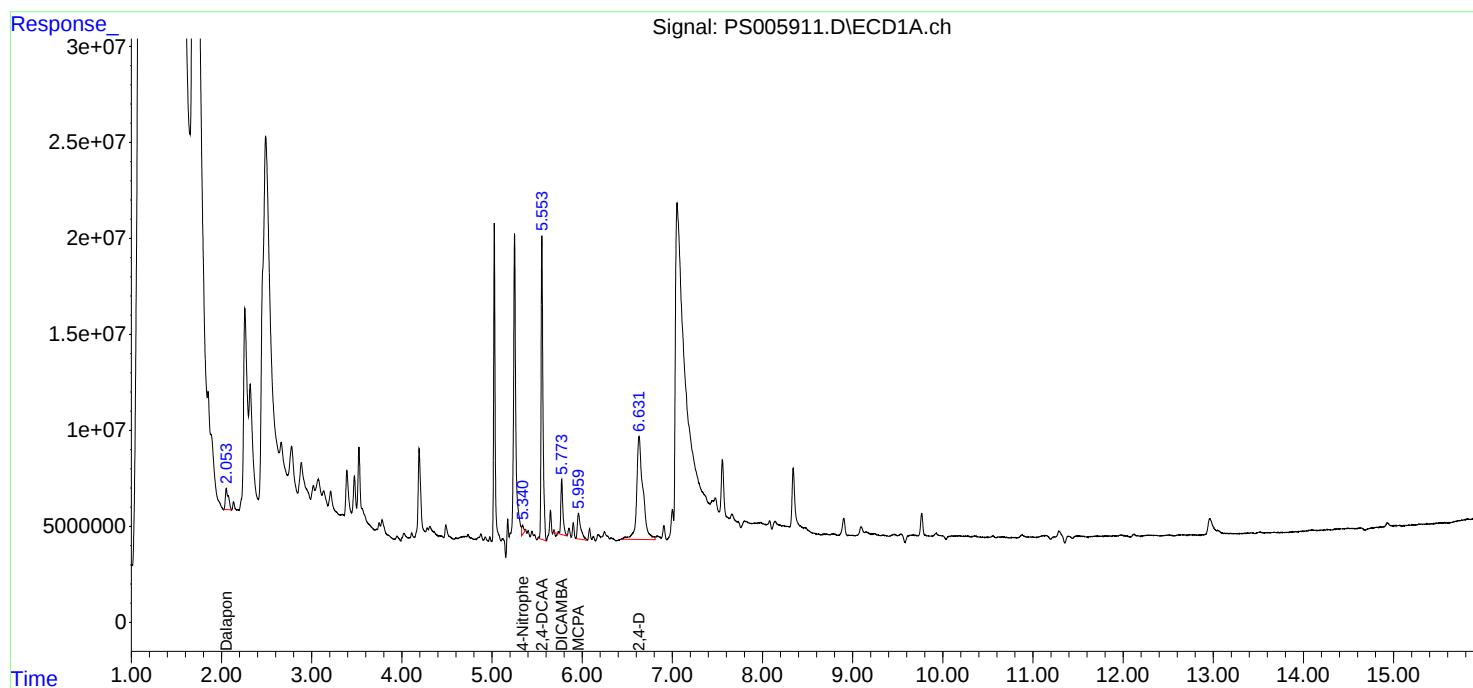


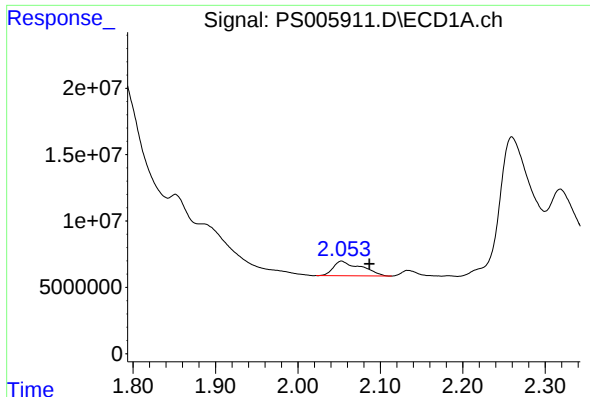

#1 Dalapon


R.T.: 2.053 min
Delta R.T.: -0.034 min
Response: 25862531
Conc: 13.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

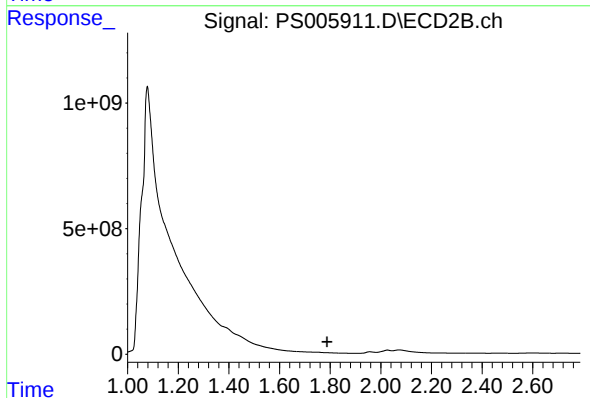


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

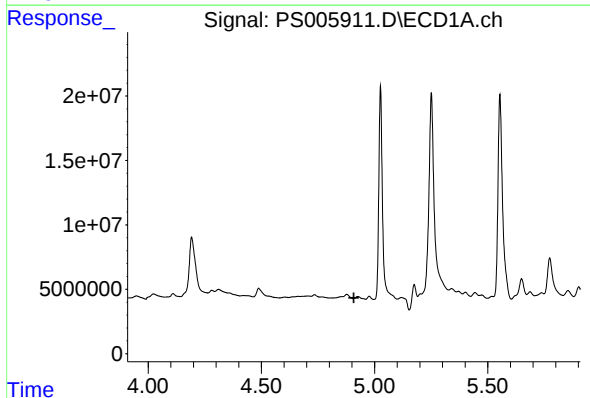


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

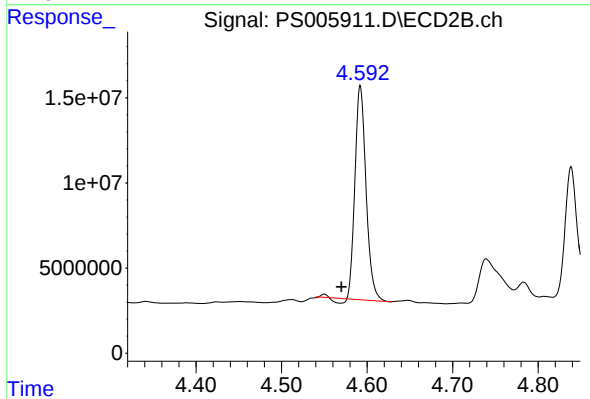

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.592 min
Delta R.T.: 0.022 min
Response: 111851881
Conc: 86.22 ng/ml

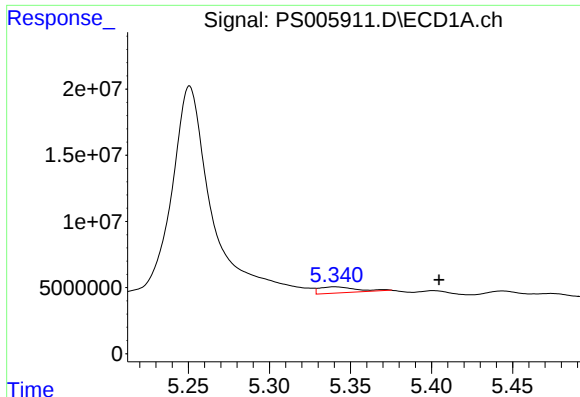

#3 4-Nitrophenol


R.T.: 5.340 min
Delta R.T.: -0.064 min
Response: 7486954
Conc: 12.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

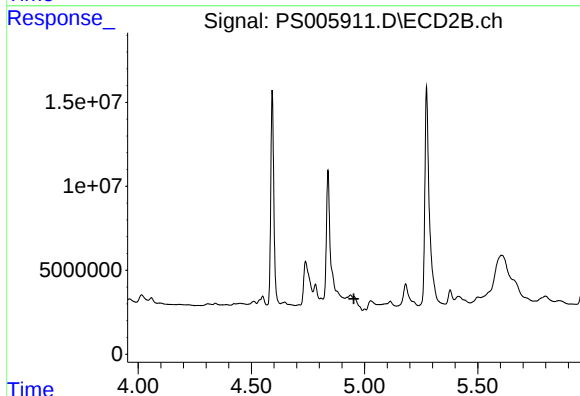


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

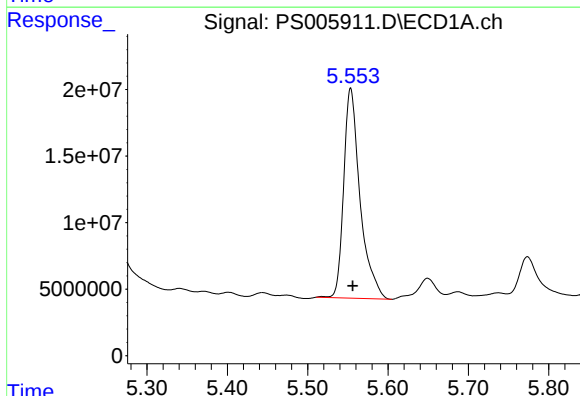


#4 2,4-DCAA

R.T.: 5.554 min
Delta R.T.: -0.002 min
Response: 223518909
Conc: 154.06 ng/ml

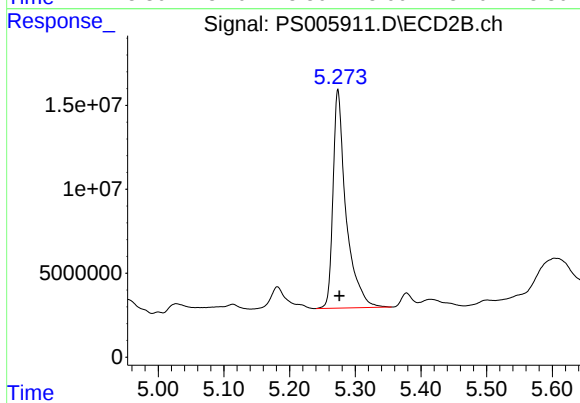

#4 2,4-DCAA


R.T.: 5.274 min
Delta R.T.: -0.002 min
Response: 179504406
Conc: 180.46 ng/ml

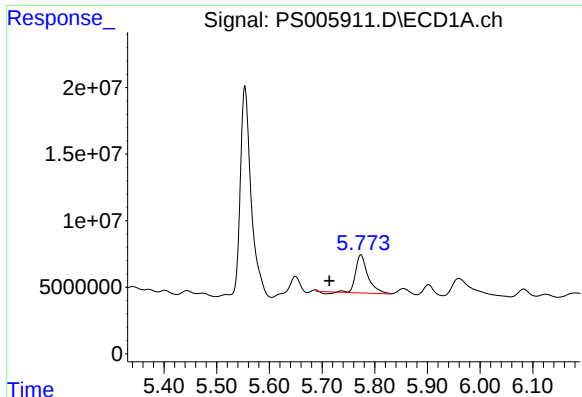

#5 DICAMBA


R.T.: 5.774 min
Delta R.T.: 0.059 min
Response: 45533820
Conc: 7.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

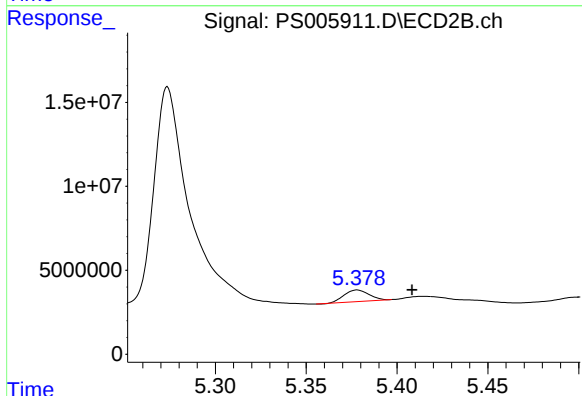


#5 DICAMBA

R.T.: 5.378 min
Delta R.T.: -0.030 min
Response: 6606700
Conc: 1.77 ng/ml

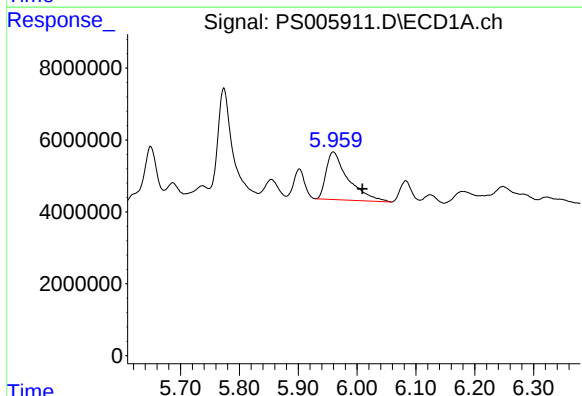


#7 MCPA

R.T.: 5.960 min
Delta R.T.: -0.050 min
Response: 34342740
Conc: 5.26 ug/ml

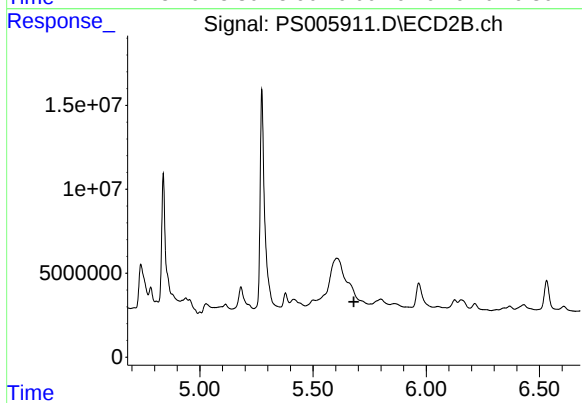

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 5.681 min
Response: 0
Conc: N.D.

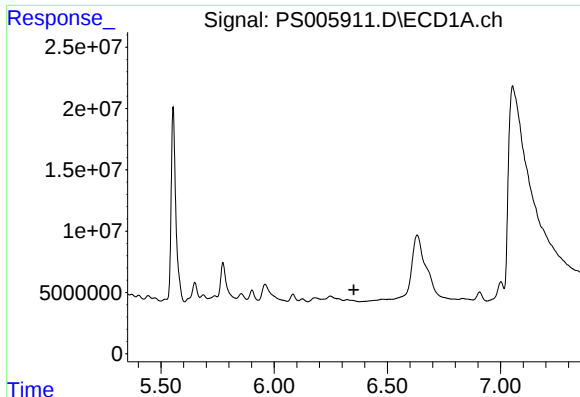

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

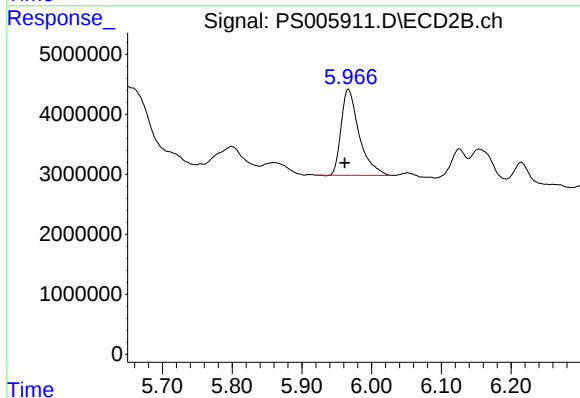


#8 DICHLORPROP

R.T.: 5.967 min
Delta R.T.: 0.006 min
Response: 25748315
Conc: 27.88 ng/ml

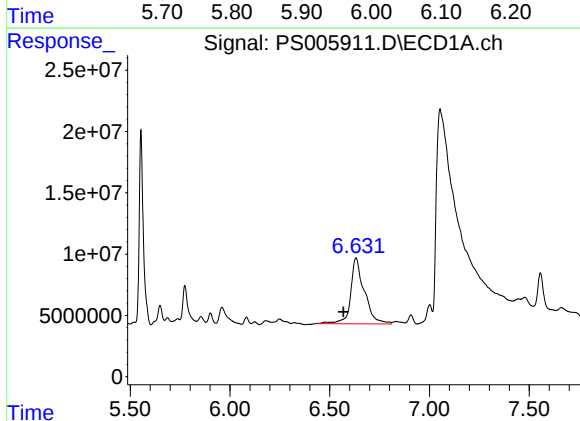


#9 2,4-D

R.T.: 6.631 min
Delta R.T.: 0.062 min
Response: 255900826
Conc: 170.75 ng/ml

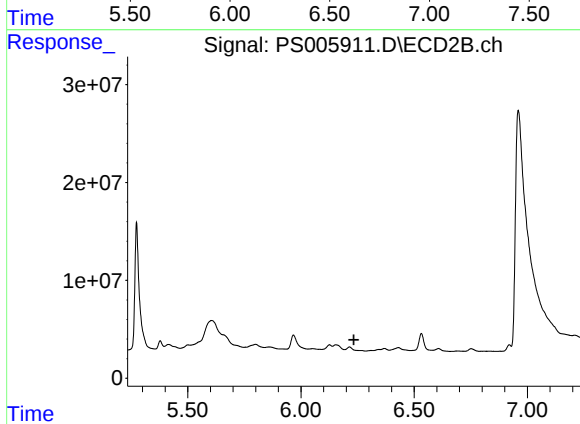

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.234 min
Response: 0
Conc: N.D.

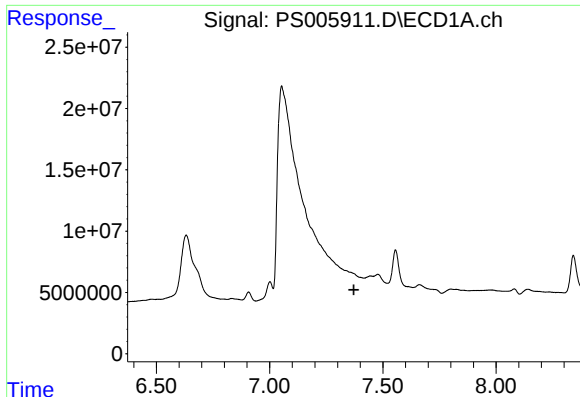

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

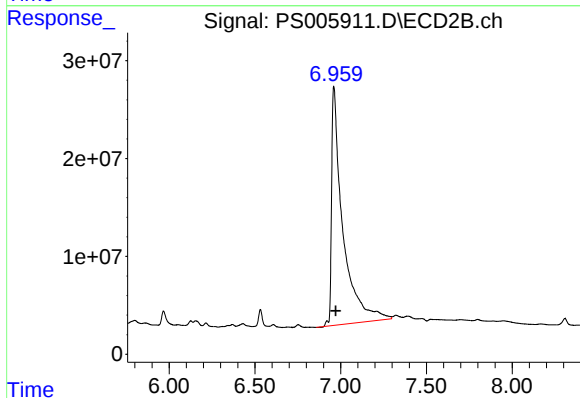


#11 2,4,5-TP (SILVEX)

R.T.: 6.960 min
Delta R.T.: -0.010 min
Response: 1114289138
Conc: 214.81 ng/ml

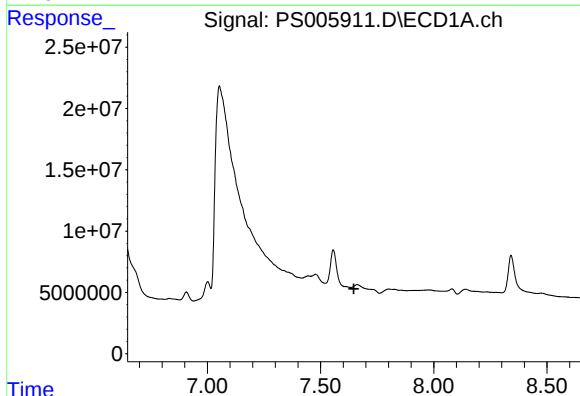

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.647 min
Response: 0
Conc: N.D.

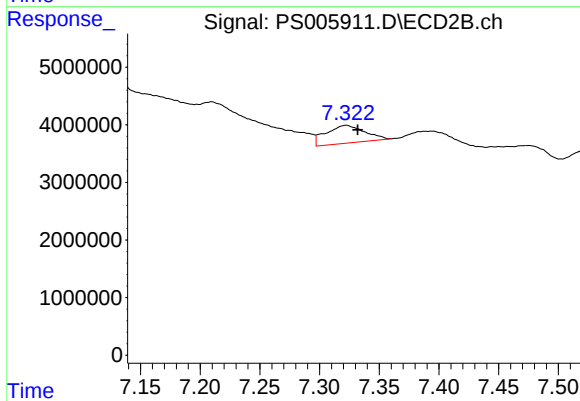

#12 2,4,5-T

R.T.: 7.322 min
Delta R.T.: -0.010 min
Response: 6986692
Conc: 1.47 ng/ml