

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
 Data File : PS005912.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 19:12
 Operator : SM\AJ
 Sample : K4130-21
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:40:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.555	5.275	269.3E6	191.7E6	185.622	192.756
Target Compounds							
1) T	Dalapon	2.053	0.000	31904978	0	17.215	N.D. #
2) T	3,5-DICHL...	0.000	4.593	0	163.6E6	N.D.	126.093
3) T	4-Nitroph...	5.343	0.000	4927714	0	8.192	N.D. #
5) T	DICAMBA	5.776	0.000	21796722	0	3.650	N.D. #
7) T	MCPA	5.959	0.000	59358268	0	9.096	N.D. #
8) T	DICHLORPROP	0.000	5.967	0	40516209	N.D.	43.871
9) T	2,4-D	6.634	0.000	242.7E6	0	161.913	N.D. #
11) T	2,4,5-TP ...	0.000	7.008	0	120.4E6	N.D.	23.214
15) T	Picloram	9.093	0.000	22524705	0	1.924	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
Data File : PS005912.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 19:12
Operator : SM\AJ
Sample : K4130-21
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:40:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

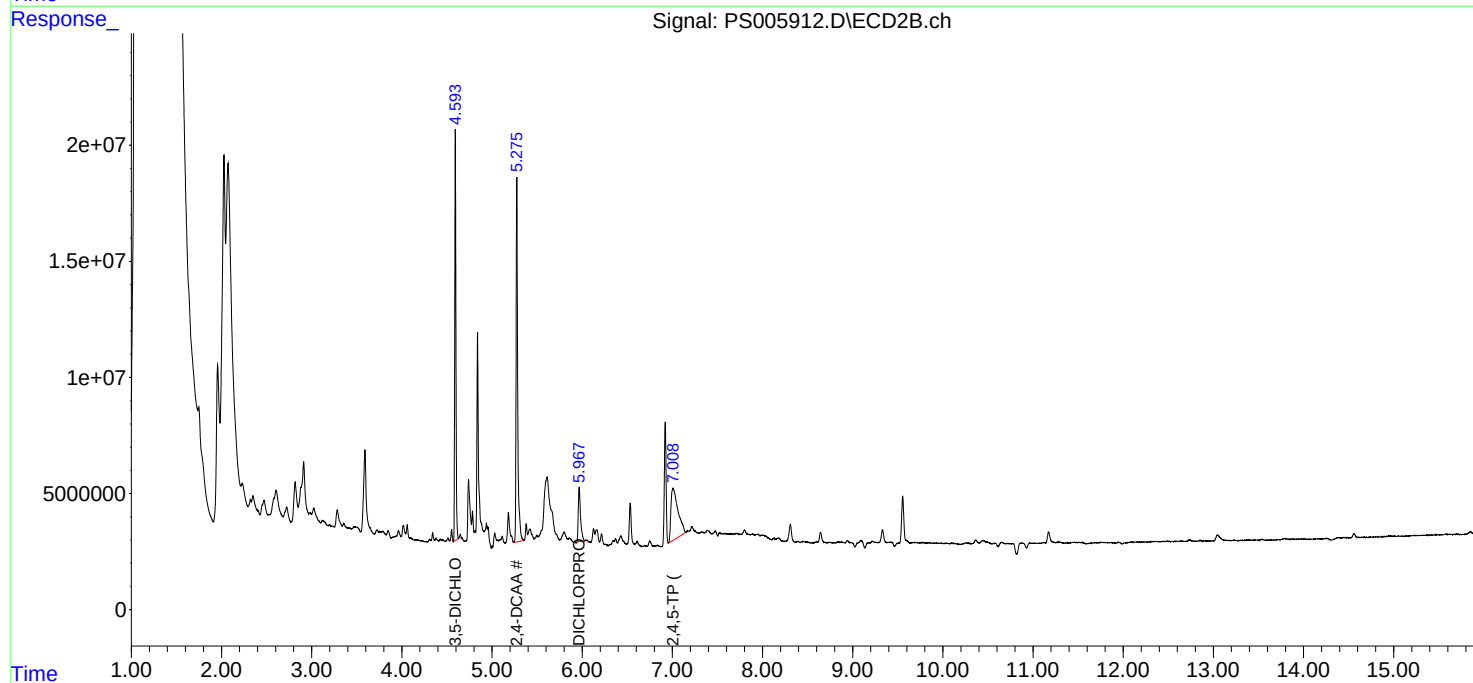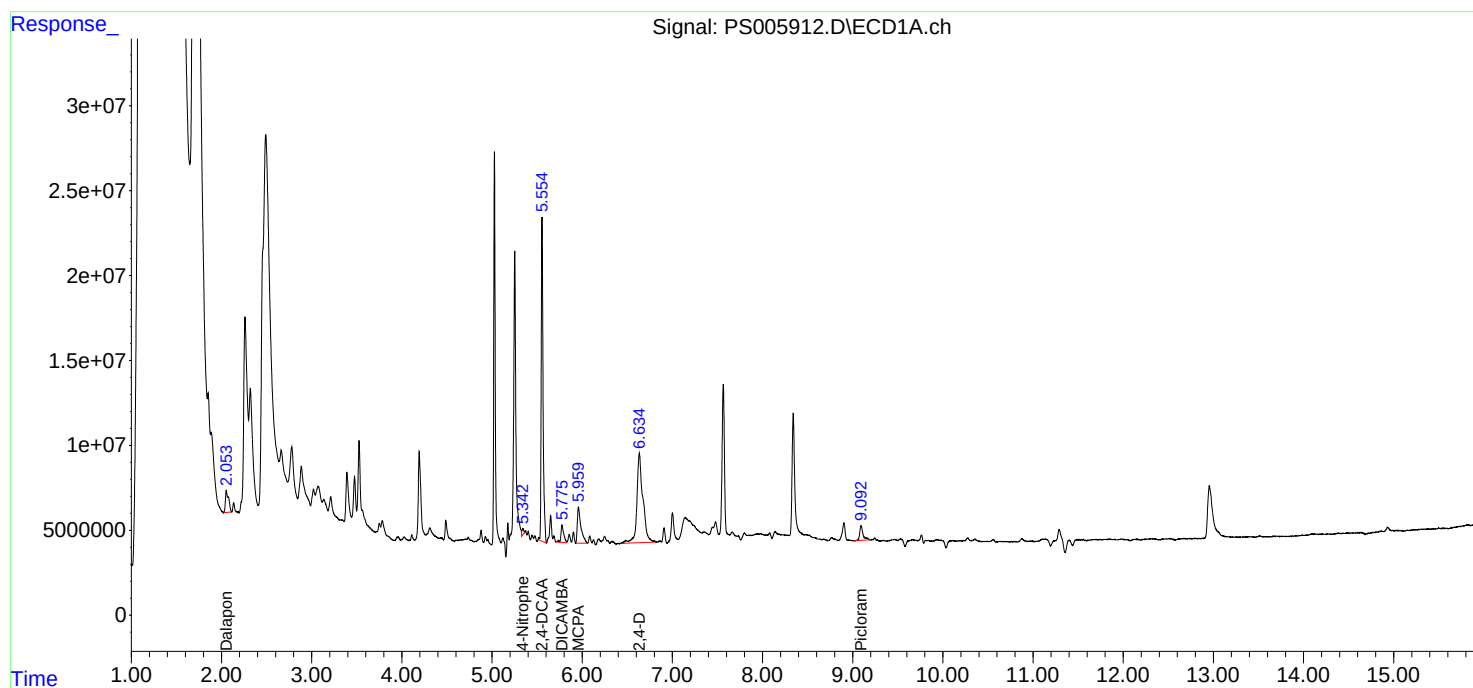


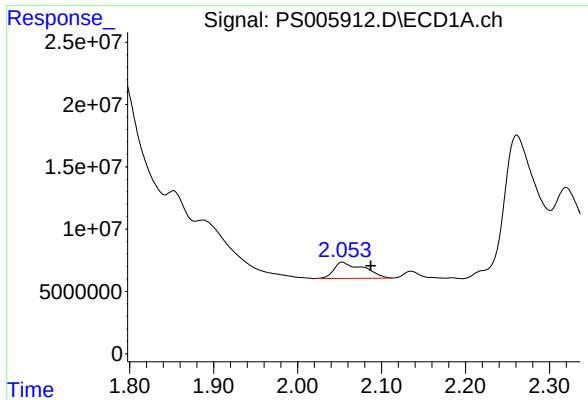

#1 Dalapon


R.T.: 2.053 min
Delta R.T.: -0.034 min
Response: 31904978
Conc: 17.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

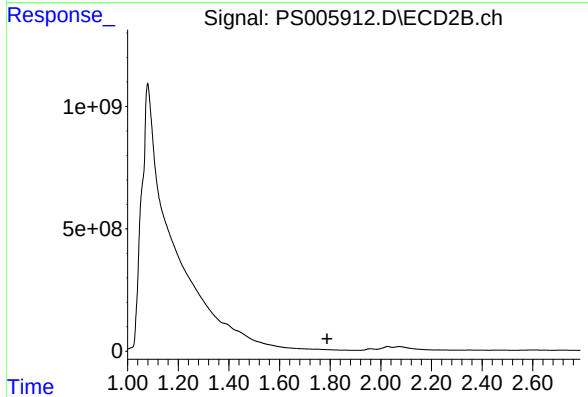


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

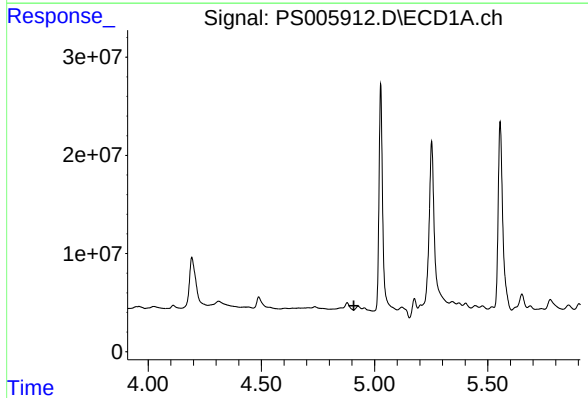


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

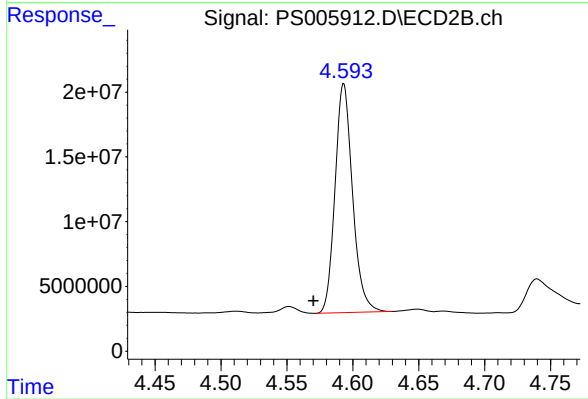

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.593 min
Delta R.T.: 0.023 min
Response: 163582728
Conc: 126.09 ng/ml

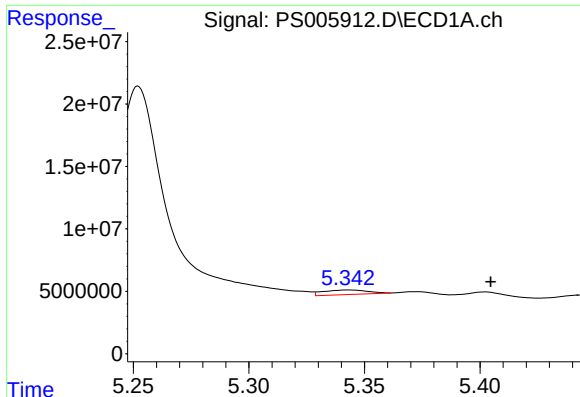

#3 4-Nitrophenol


R.T.: 5.343 min
Delta R.T.: -0.062 min
Response: 4927714
Conc: 8.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

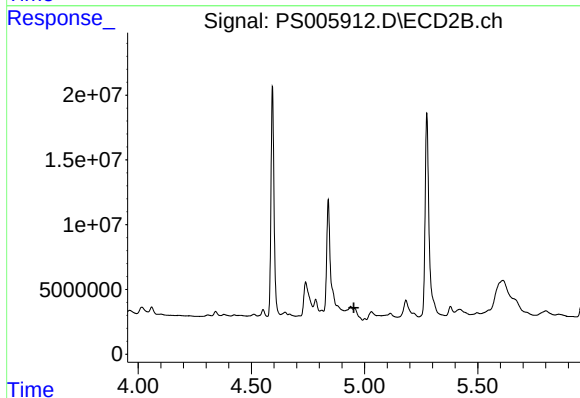


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

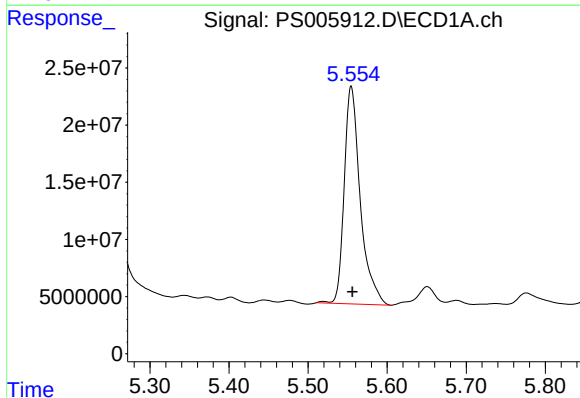


#4 2,4-DCAA

R.T.: 5.555 min
Delta R.T.: -0.001 min
Response: 269303533
Conc: 185.62 ng/ml

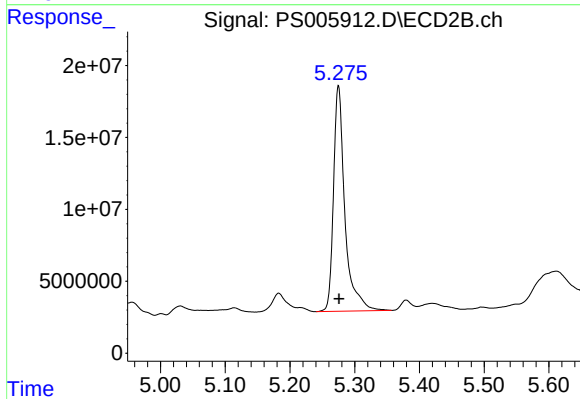

#4 2,4-DCAA


R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 191729914
Conc: 192.76 ng/ml

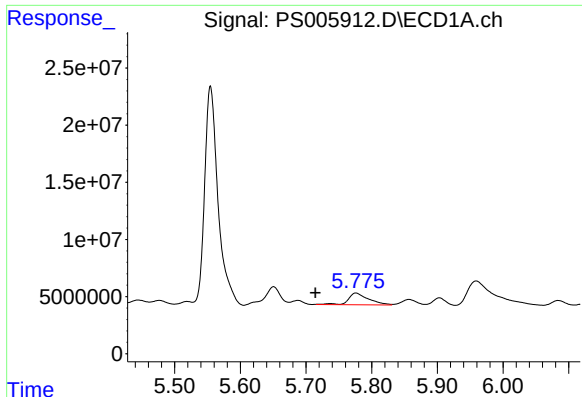

#5 DICAMBA


R.T.: 5.776 min
Delta R.T.: 0.062 min
Response: 21796722
Conc: 3.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

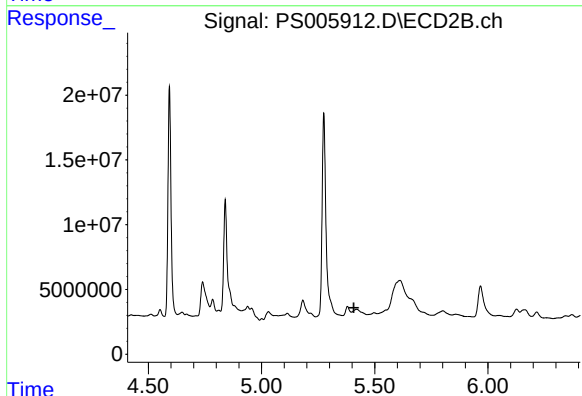


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

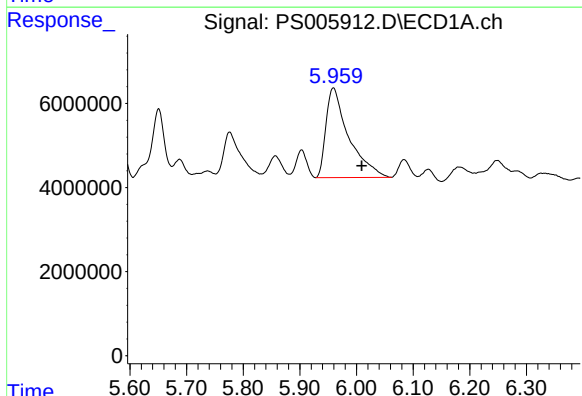


#7 MCPA

R.T.: 5.959 min
Delta R.T.: -0.050 min
Response: 59358268
Conc: 9.10 ug/ml

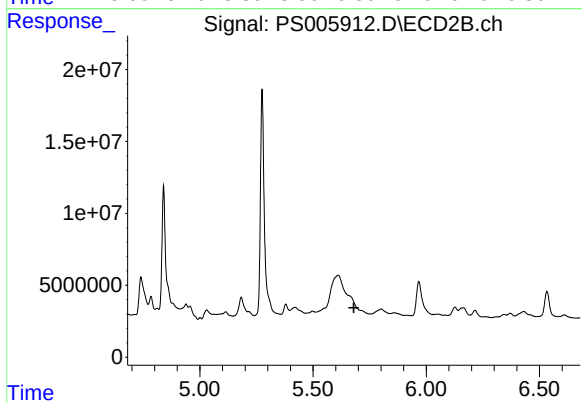

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 5.681 min
Response: 0
Conc: N.D.

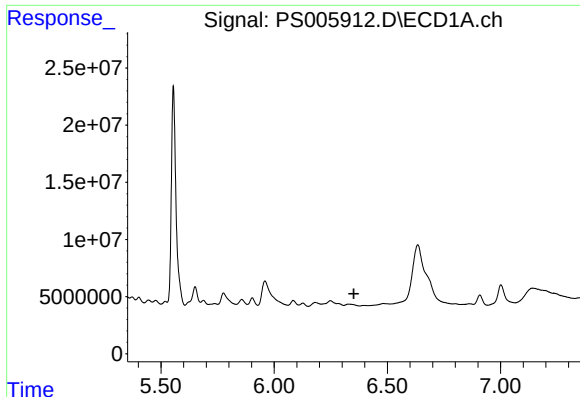

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

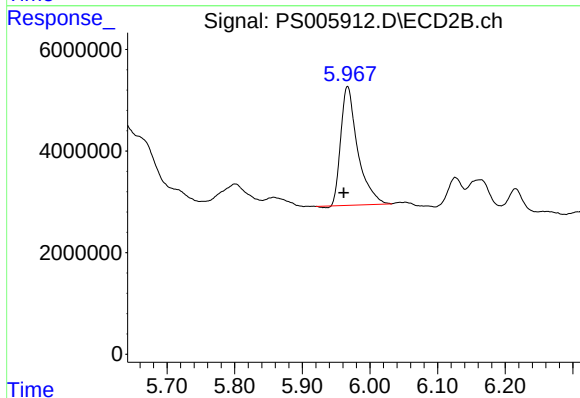


#8 DICHLORPROP

R.T.: 5.967 min
Delta R.T.: 0.006 min
Response: 40516209
Conc: 43.87 ng/ml

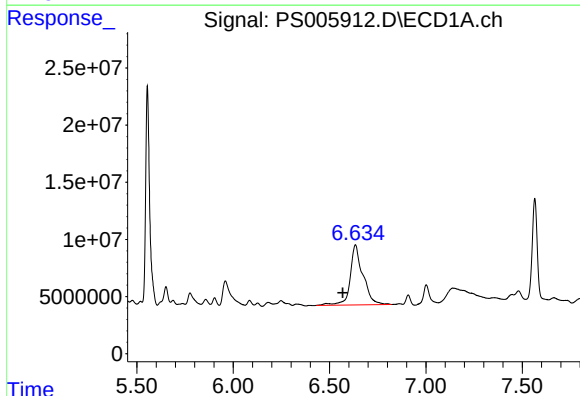


#9 2,4-D

R.T.: 6.634 min
Delta R.T.: 0.065 min
Response: 242653767
Conc: 161.91 ng/ml

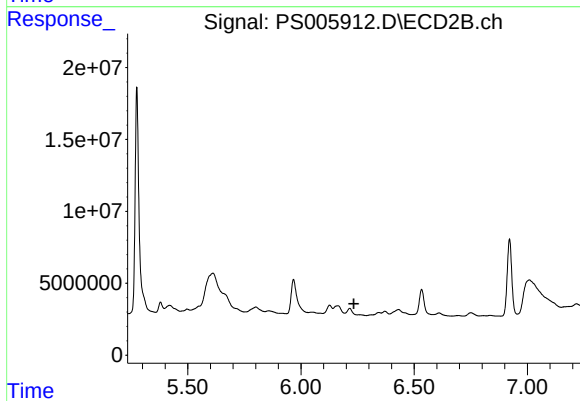

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.234 min
Response: 0
Conc: N.D.

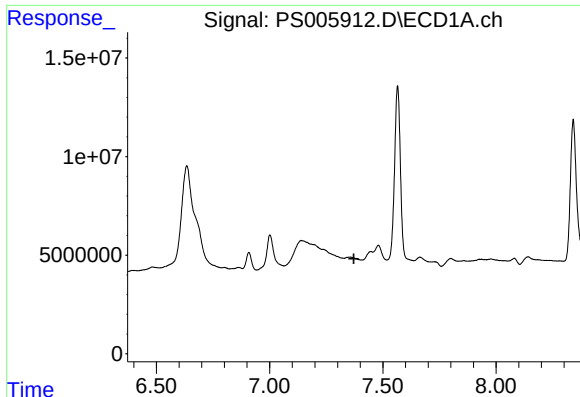

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

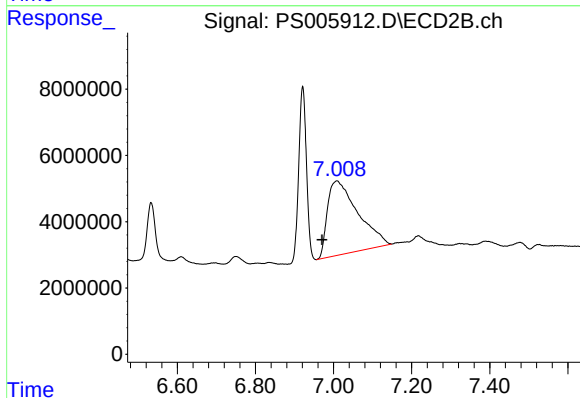


#11 2,4,5-TP (SILVEX)

R.T.: 7.008 min
Delta R.T.: 0.038 min
Response: 120418861
Conc: 23.21 ng/ml

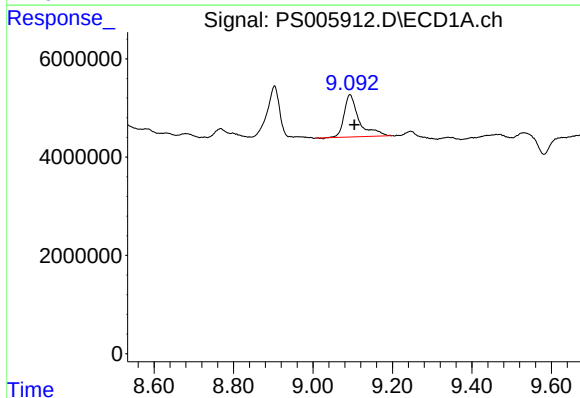

#15 Picloram

R.T.: 9.093 min
Delta R.T.: -0.011 min
Response: 22524705
Conc: 1.92 ng/ml

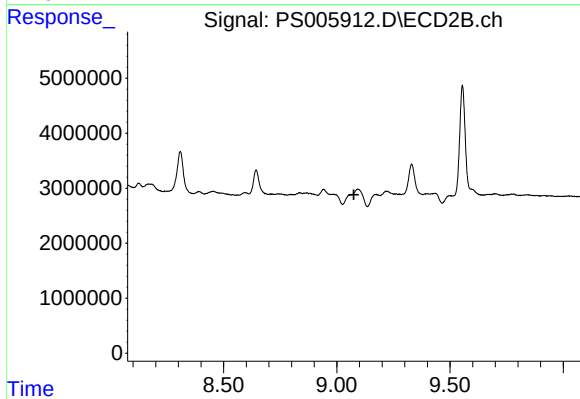

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.075 min
Response: 0
Conc: N.D.