

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
 Data File : PS005915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 20:18
 Operator : SM\AJ
 Sample : K4130-26
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:41:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.588	5.308	239.9E6	168.3E6	165.383	169.179
Target Compounds							
1) T	Dalapon	2.087	0.000	29831525	0	16.096	N.D. #
2) T	3,5-DICHL...	0.000	4.626	0	150.6E6	N.D.	116.051
7) T	MCPA	5.995	5.635	36490227	137.5E6	5.592	32.661 #
8) T	DICHLORPROP	0.000	6.002	0	23789406	N.D.	25.759
10) T	Pentachlo...	0.000	6.566	0	20100483	N.D.	1.548
11) T	2,4,5-TP ...	0.000	6.954	0	68515220	N.D.	13.208
12) T	2,4,5-T	7.599	0.000	147.4E6	0	17.665	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
Data File : PS005915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 20:18
Operator : SM\AJ
Sample : K4130-26
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:41:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

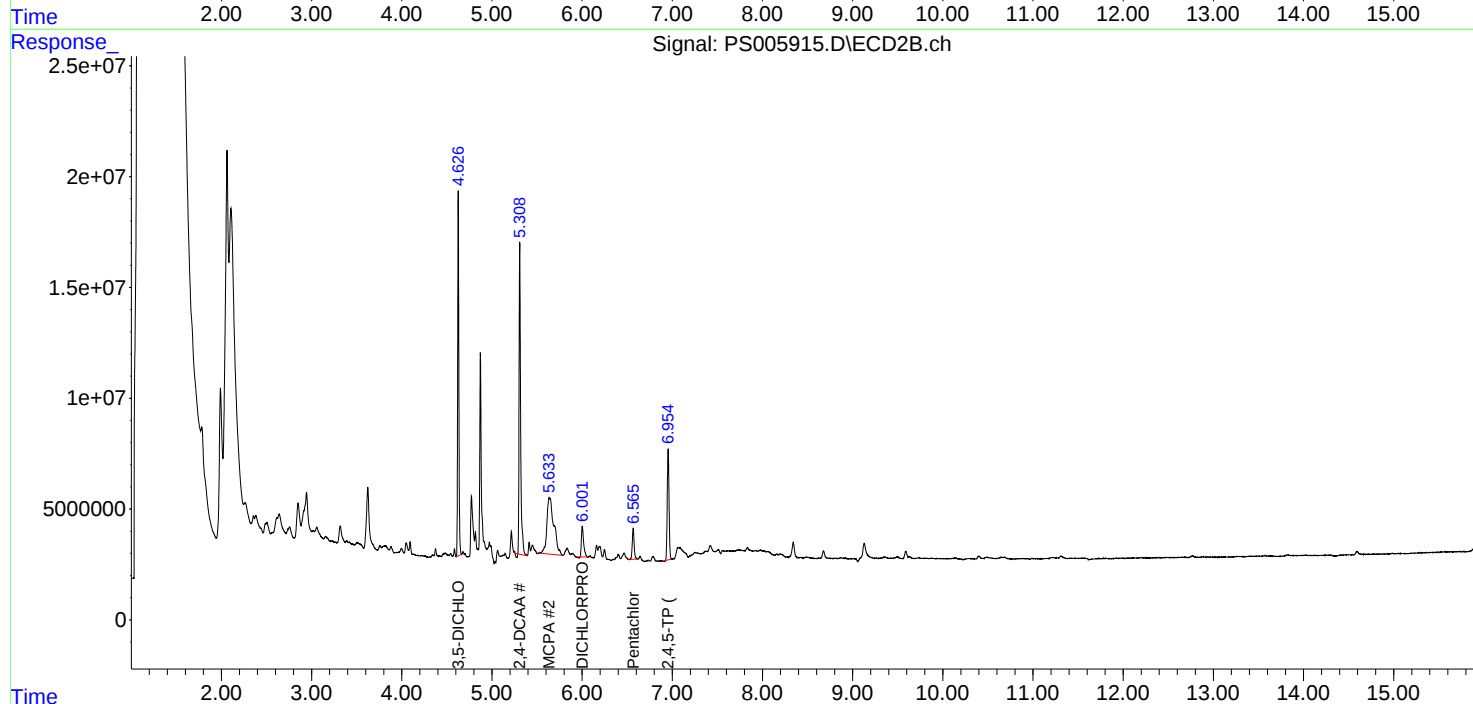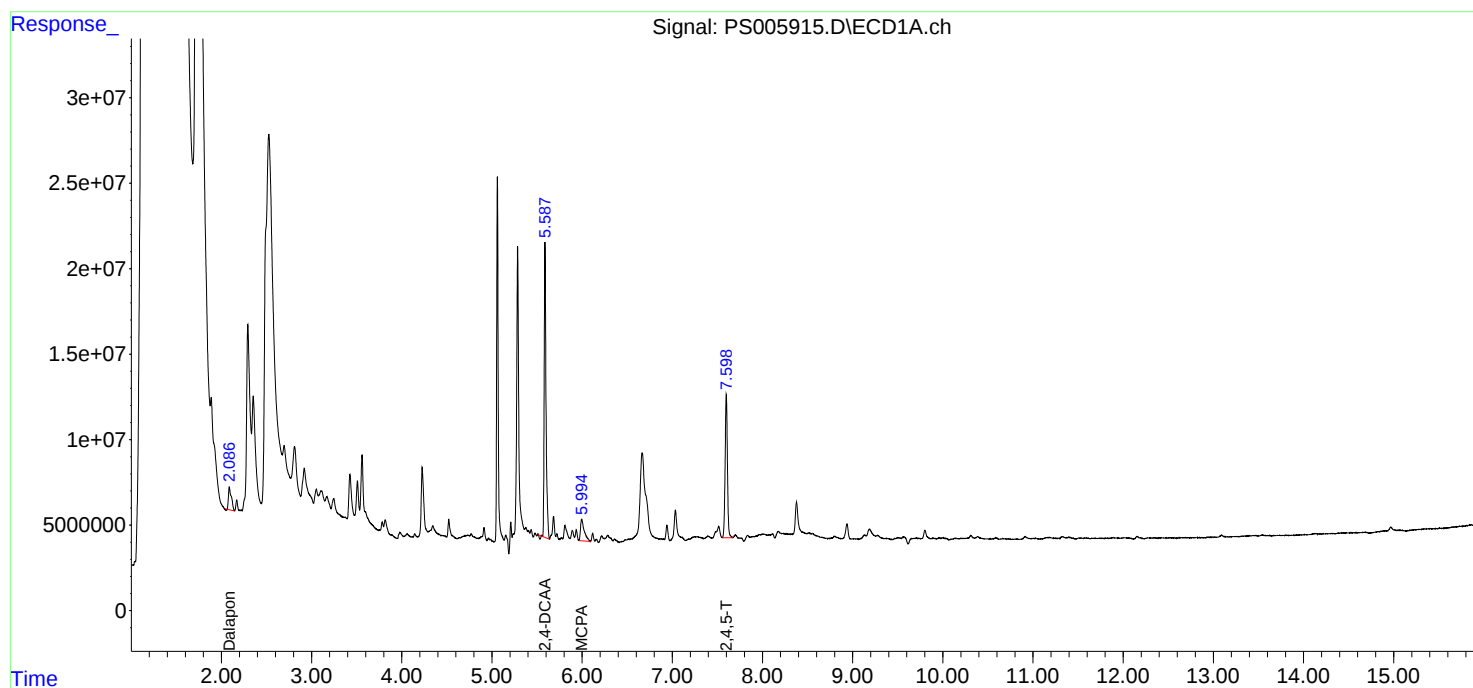


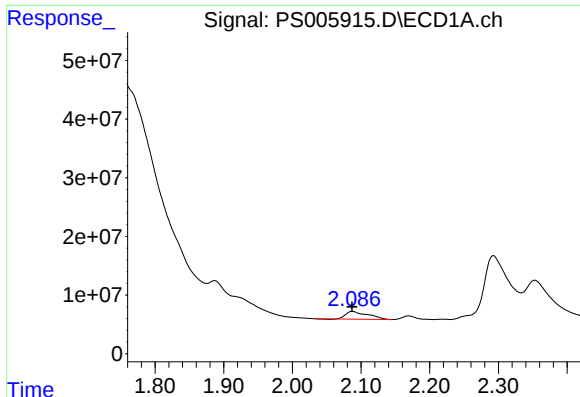

#1 Dalapon


R.T.: 2.087 min
Delta R.T.: 0.000 min
Response: 29831525
Conc: 16.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

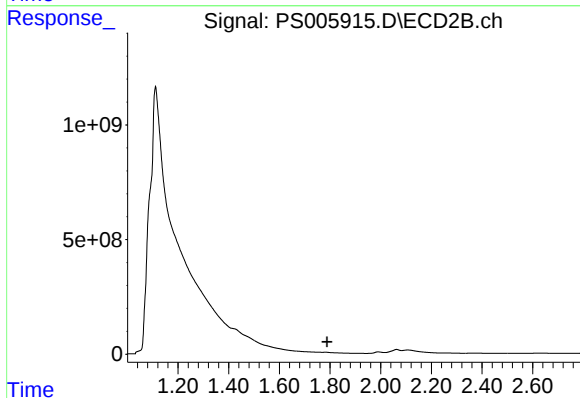


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

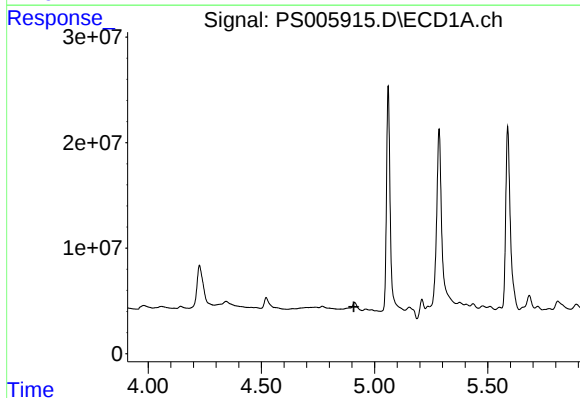


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

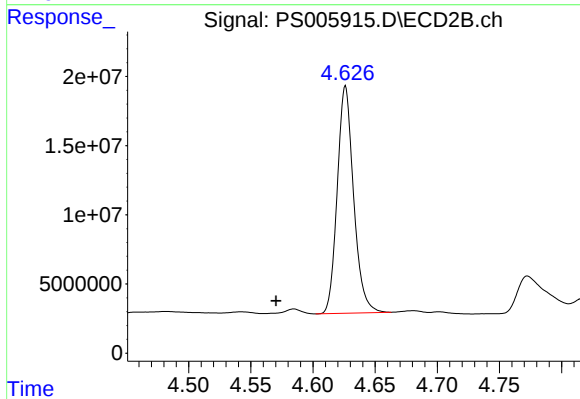

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.626 min
Delta R.T.: 0.056 min
Response: 150554378
Conc: 116.05 ng/ml

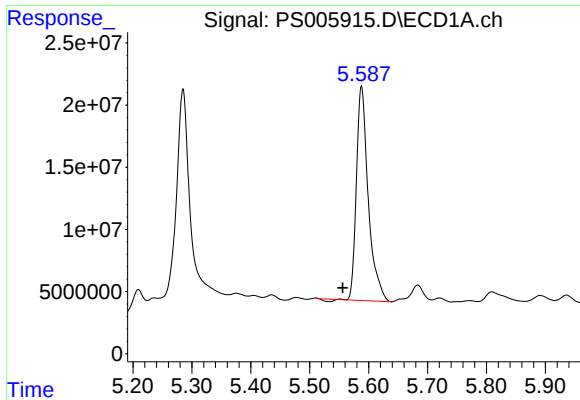

#4 2,4-DCAA


R.T.: 5.588 min
Delta R.T.: 0.032 min
Response: 239941317
Conc: 165.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

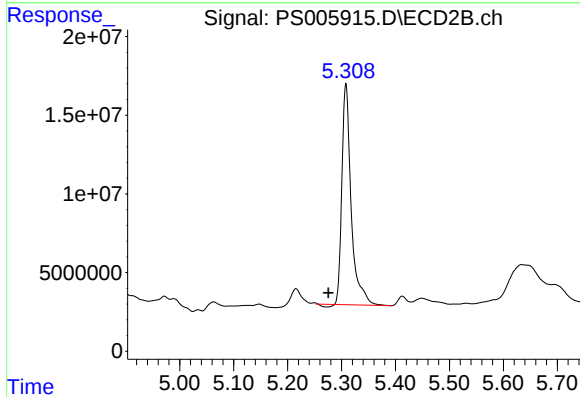


#4 2,4-DCAA

R.T.: 5.308 min
Delta R.T.: 0.032 min
Response: 168279158
Conc: 169.18 ng/ml

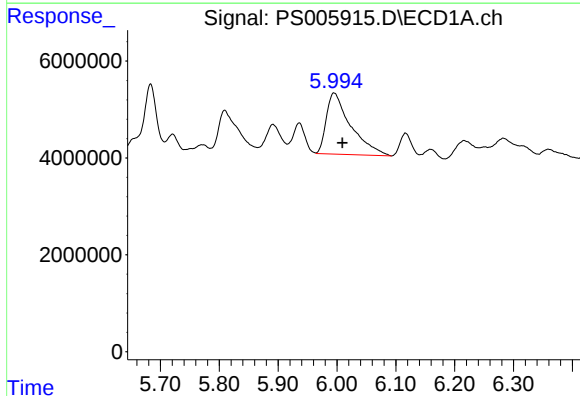


#7 MCPA

R.T.: 5.995 min
Delta R.T.: -0.014 min
Response: 36490227
Conc: 5.59 ug/ml

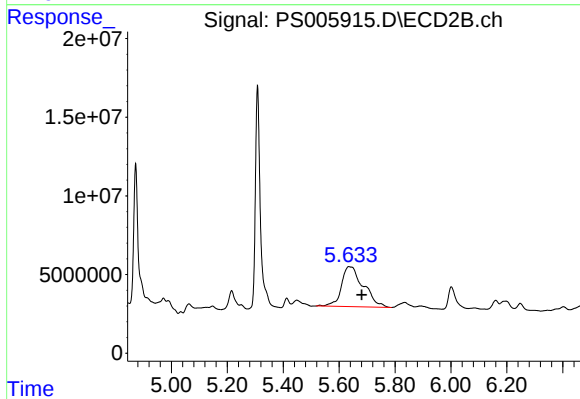

#7 MCPA


R.T.: 5.635 min
Delta R.T.: -0.046 min
Response: 137470222
Conc: 32.66 ug/ml

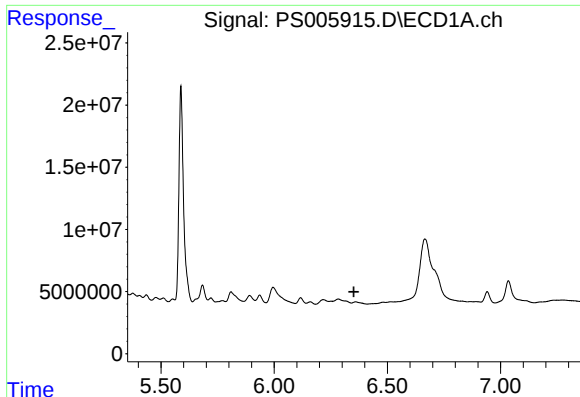

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

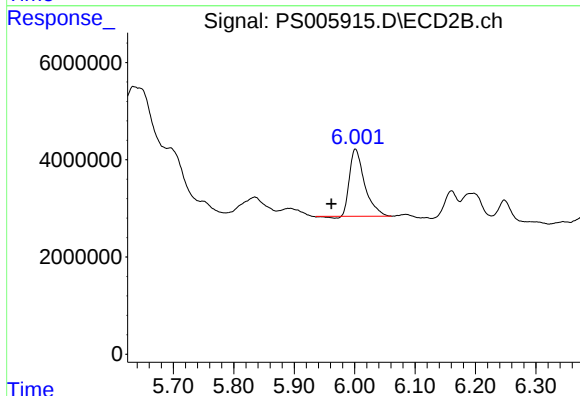


#8 DICHLORPROP

R.T.: 6.002 min
Delta R.T.: 0.040 min
Response: 23789406
Conc: 25.76 ng/ml

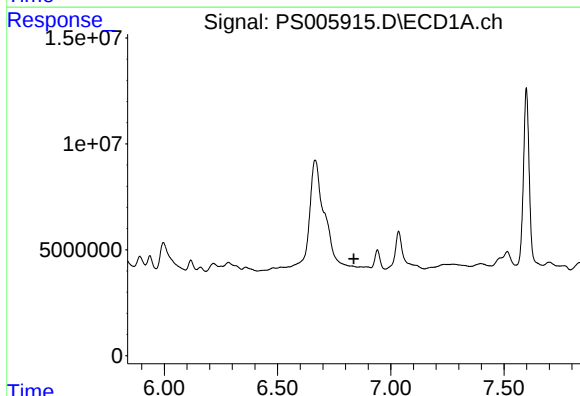


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

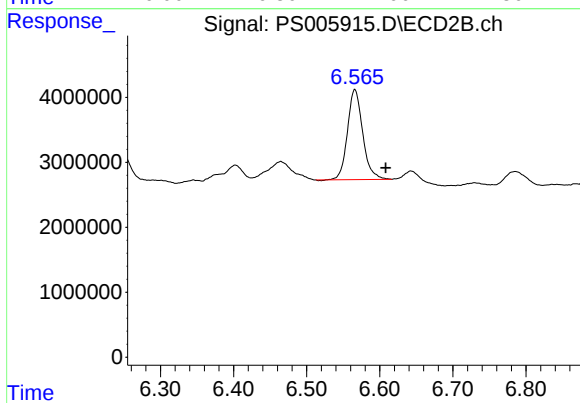

#10 Pentachlorophenol


R.T.: 6.566 min
Delta R.T.: -0.042 min
Response: 20100483
Conc: 1.55 ng/ml

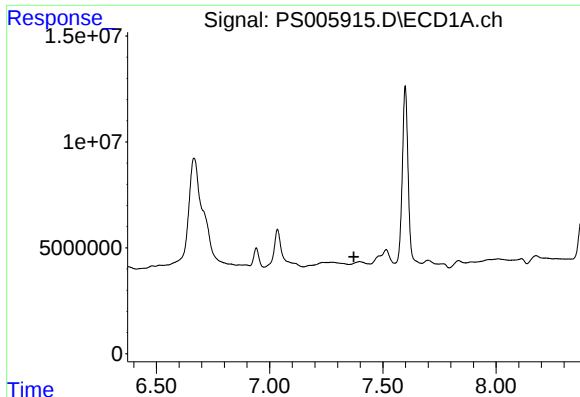

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

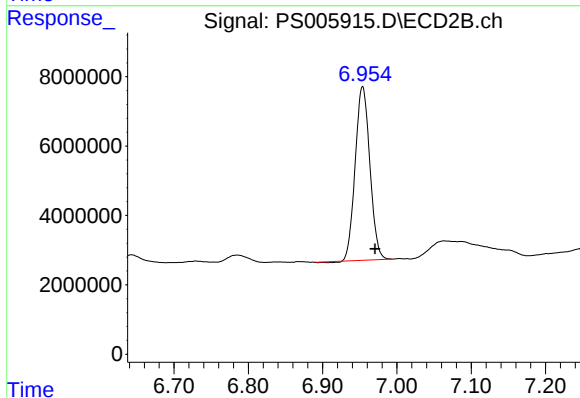


#11 2,4,5-TP (SILVEX)

R.T.: 6.954 min
Delta R.T.: -0.017 min
Response: 68515220
Conc: 13.21 ng/ml

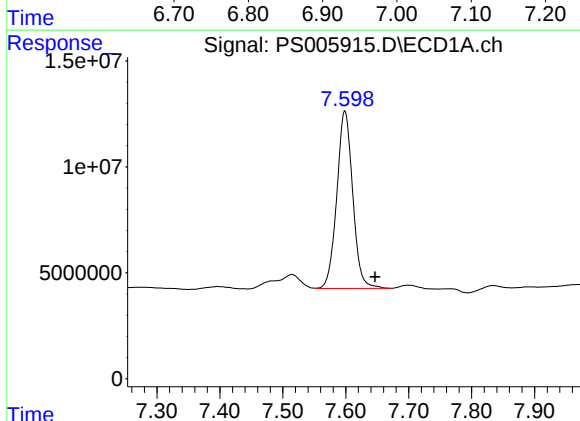

#12 2,4,5-T

R.T.: 7.599 min
Delta R.T.: -0.048 min
Response: 147442776
Conc: 17.66 ng/ml

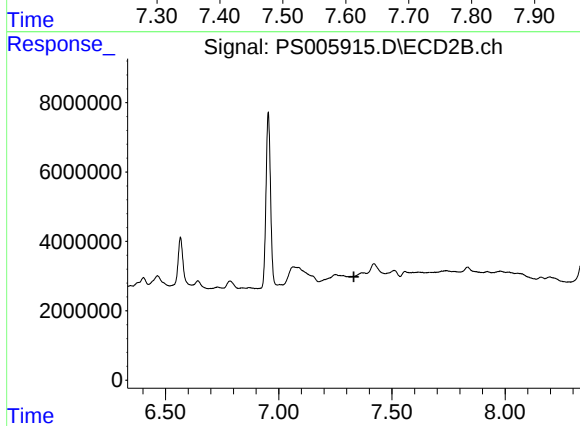

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.