

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
 Data File : PS005916.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 20:40
 Operator : SM\AJ
 Sample : K4130-31
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:42:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.572	5.293	246.6E6	166.0E6	169.992	166.876
Target Compounds							
1) T	Dalapon	2.071	0.000	30957204	0	16.704	N.D. #
2) T	3,5-DICHL...	0.000	4.610	0	167.9E6	N.D.	129.420
3) T	4-Nitroph...	5.360	0.000	4465932	0	7.424	N.D. #
5) T	DICAMBA	5.668	0.000	6044571	0	1.012	N.D. #
7) T	MCPA	5.979	5.627	51988409	133.8E6	7.967	31.798 #
8) T	DICHLORPROP	0.000	5.986	0	33304255	N.D.	36.062
10) T	Pentachlo...	0.000	6.550	0	22584900	N.D.	1.740
11) T	2,4,5-TP ...	0.000	6.938	0	75072188	N.D.	14.472
12) T	2,4,5-T	7.583	0.000	156.7E6	0	18.772	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
Data File : PS005916.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 20:40
Operator : SM\AJ
Sample : K4130-31
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:42:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

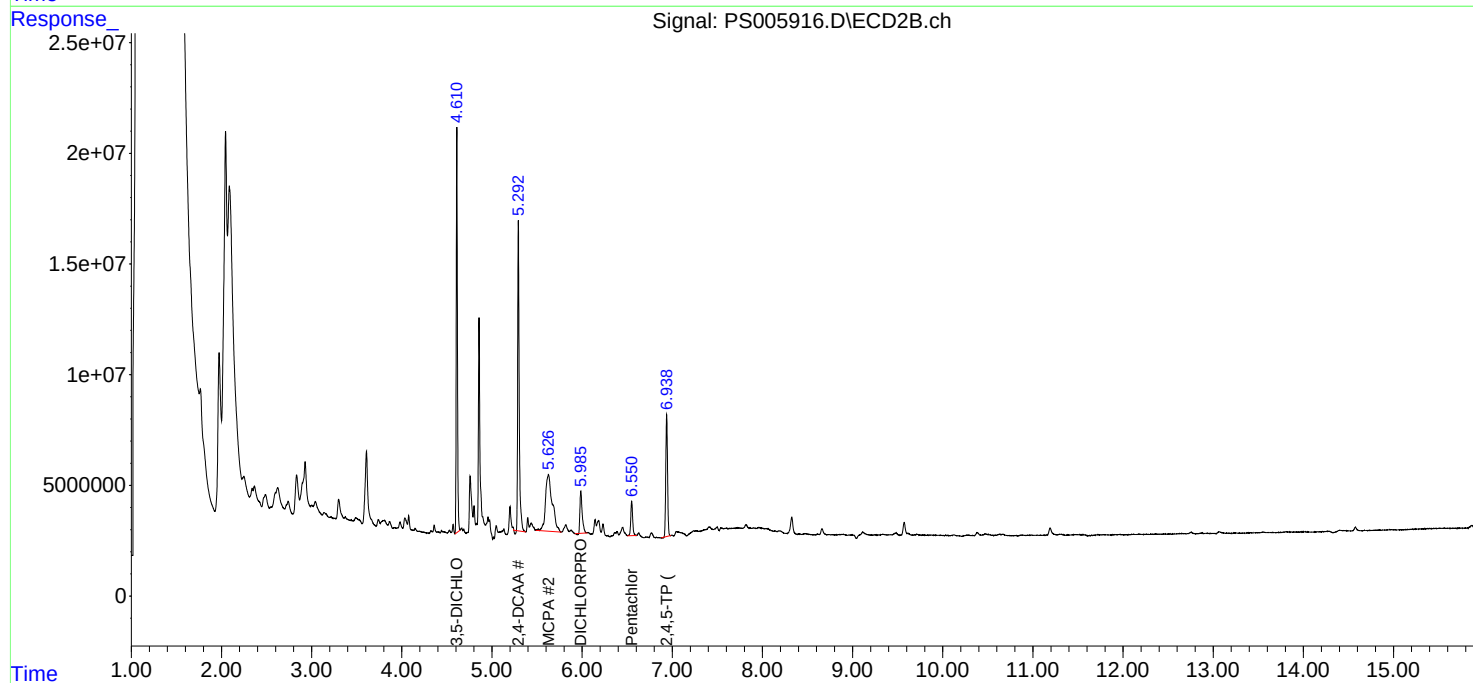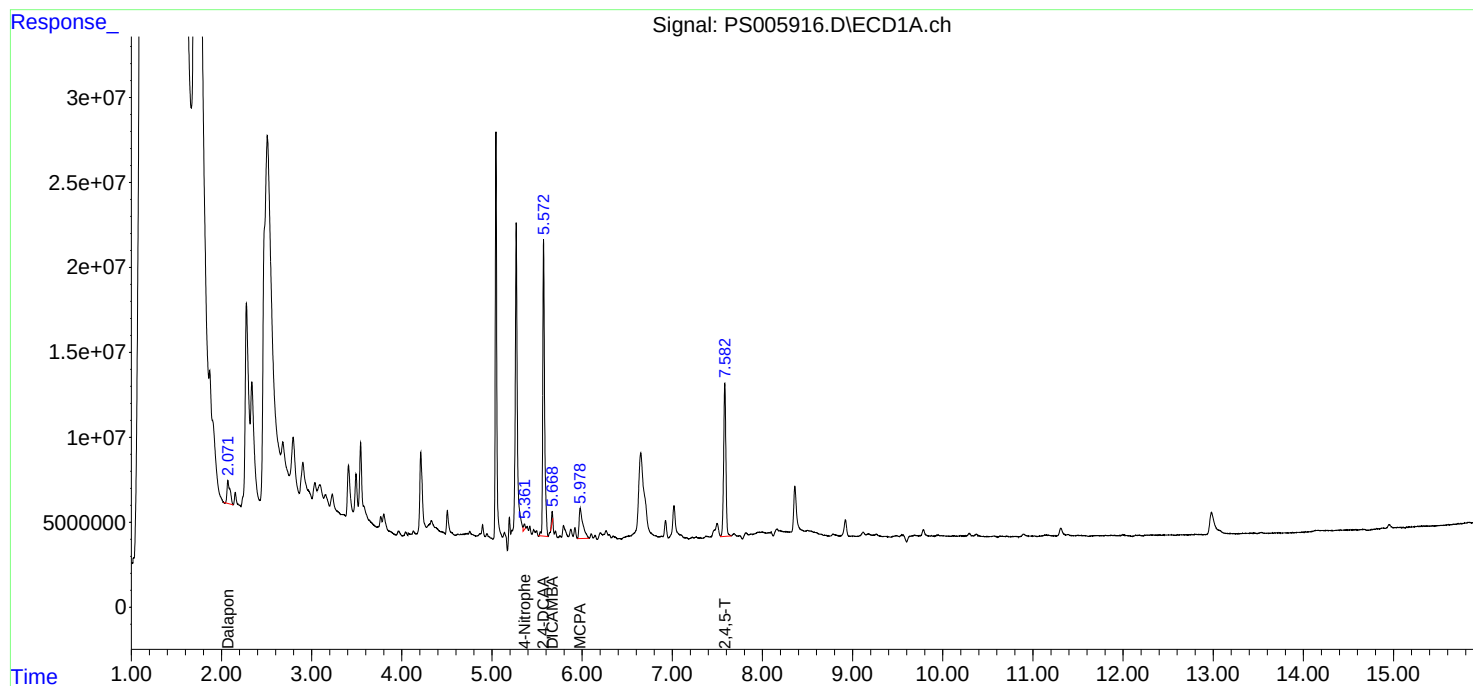


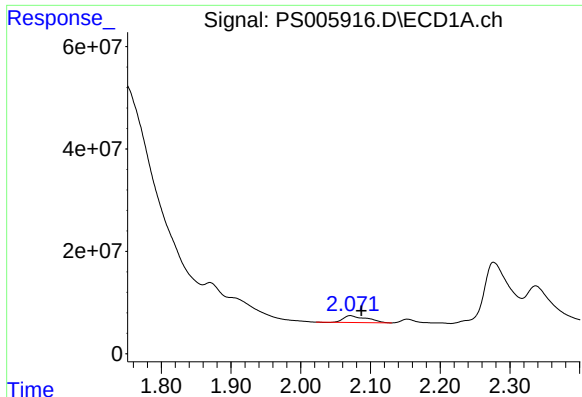

#1 Dalapon


R.T.: 2.071 min
Delta R.T.: -0.016 min
Response: 30957204
Conc: 16.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

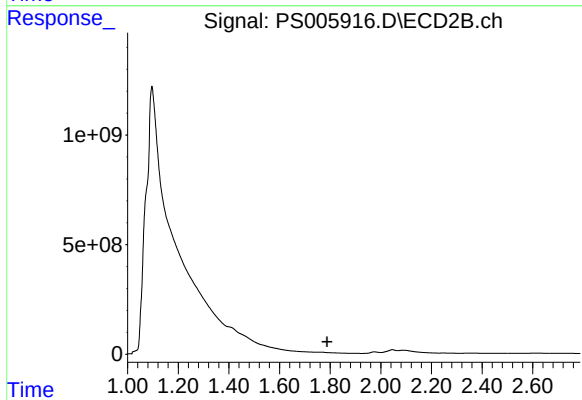


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

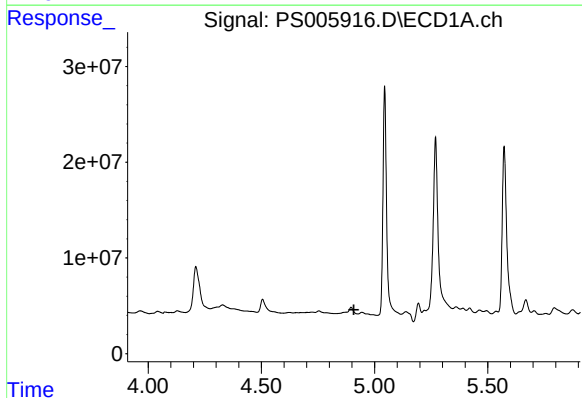


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

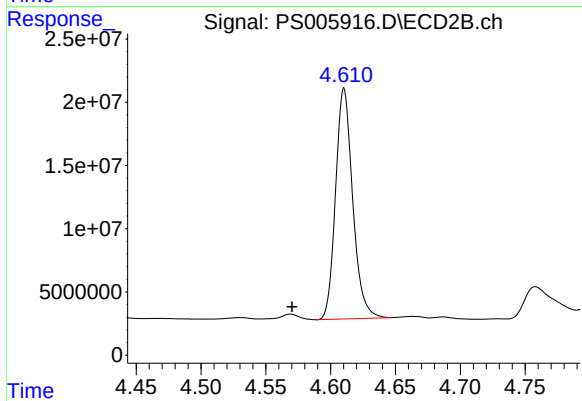

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.610 min
Delta R.T.: 0.040 min
Response: 167898598
Conc: 129.42 ng/ml

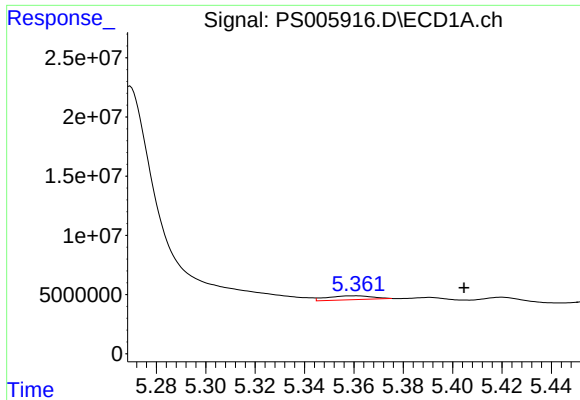

#3 4-Nitrophenol


R.T.: 5.360 min
Delta R.T.: -0.045 min
Response: 4465932
Conc: 7.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

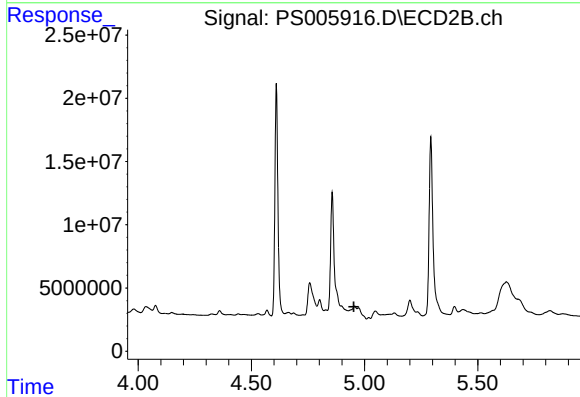


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

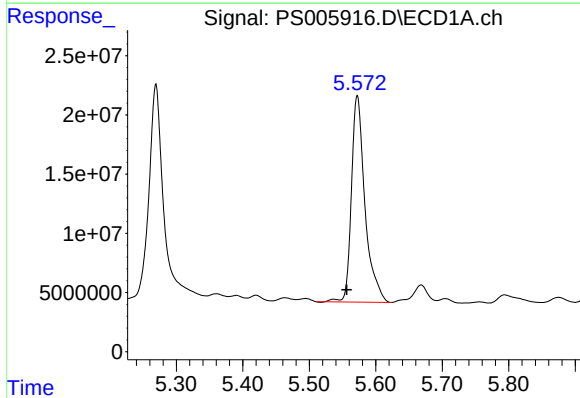


#4 2,4-DCAA

R.T.: 5.572 min
Delta R.T.: 0.016 min
Response: 246627268
Conc: 169.99 ng/ml

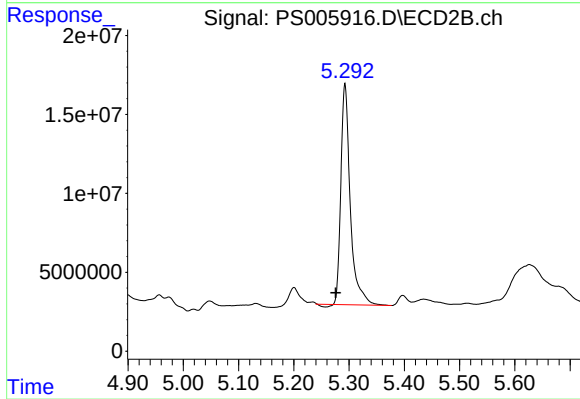

#4 2,4-DCAA


R.T.: 5.293 min
Delta R.T.: 0.017 min
Response: 165988193
Conc: 166.88 ng/ml

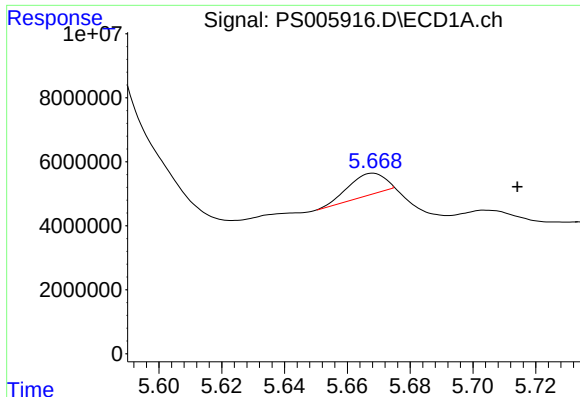

#5 DICAMBA


R.T.: 5.668 min
Delta R.T.: -0.046 min
Response: 6044571
Conc: 1.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

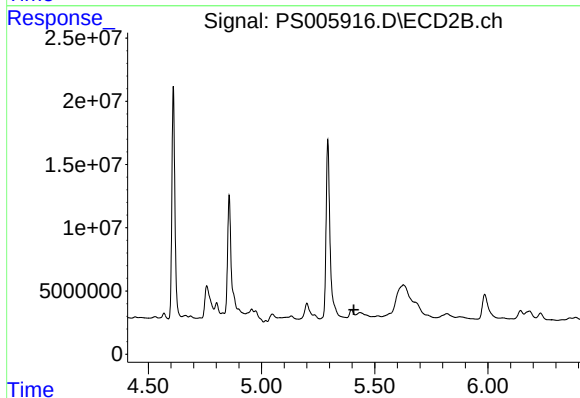


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.408 min
Response: 0
Conc: N.D.

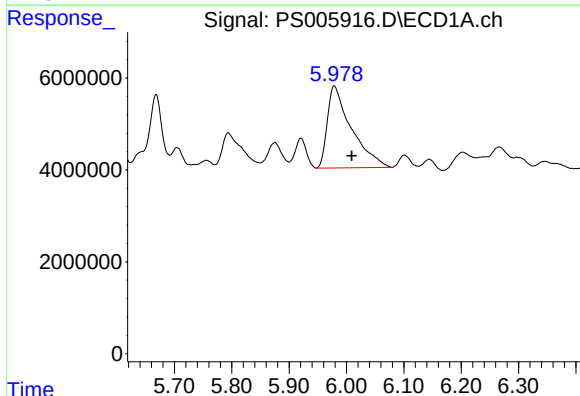


#7 MCPA

R.T.: 5.979 min
Delta R.T.: -0.030 min
Response: 51988409
Conc: 7.97 ug/ml

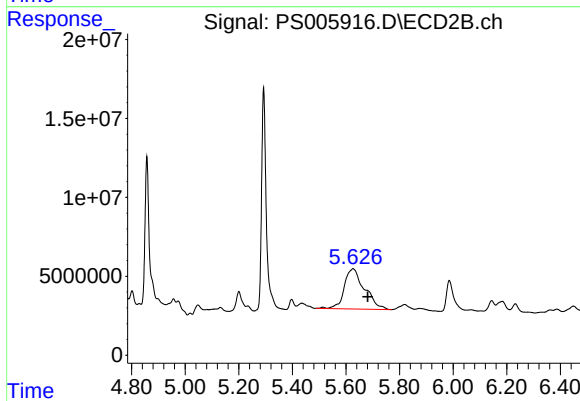

#7 MCPA


R.T.: 5.627 min
Delta R.T.: -0.054 min
Response: 133840064
Conc: 31.80 ug/ml

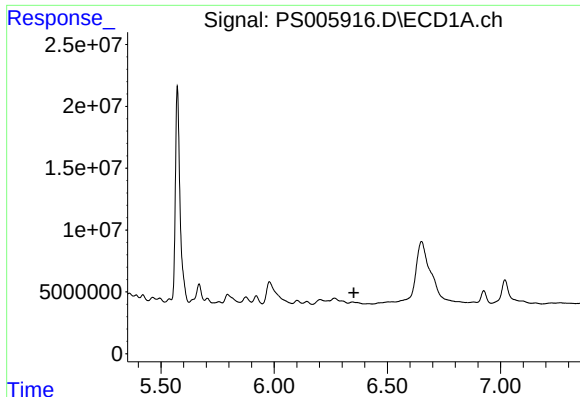

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

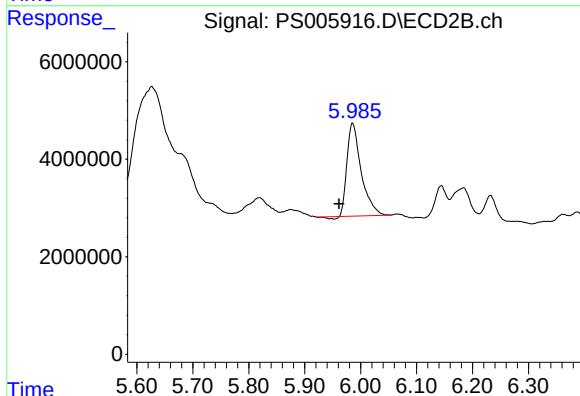


#8 DICHLORPROP

R.T.: 5.986 min
Delta R.T.: 0.024 min
Response: 33304255
Conc: 36.06 ng/ml

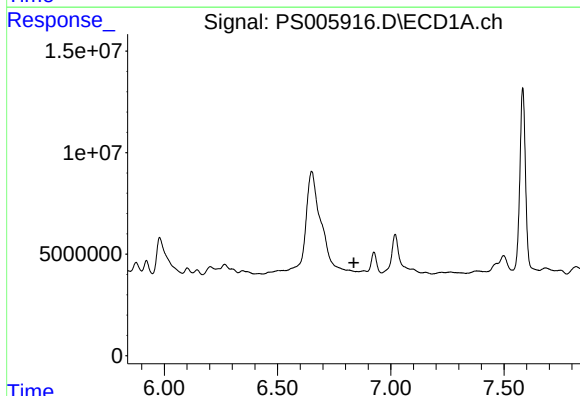


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

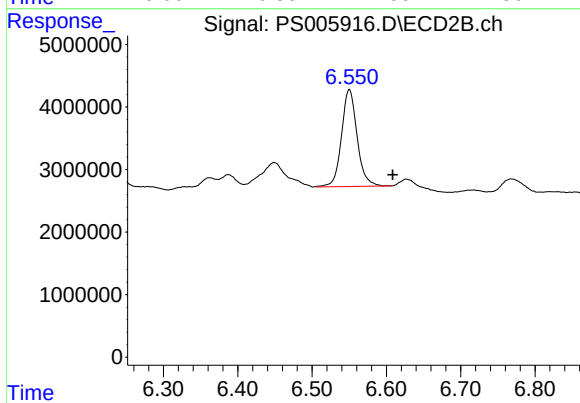

#10 Pentachlorophenol


R.T.: 6.550 min
Delta R.T.: -0.058 min
Response: 22584900
Conc: 1.74 ng/ml

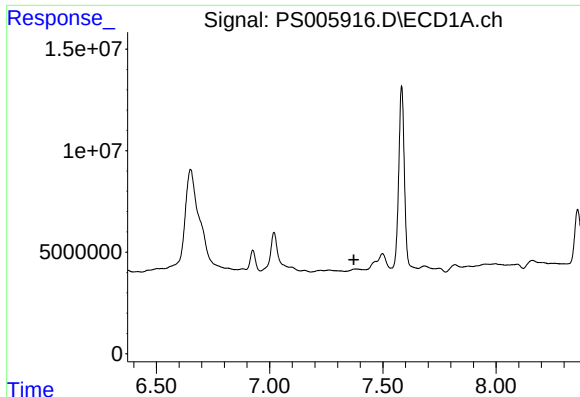

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

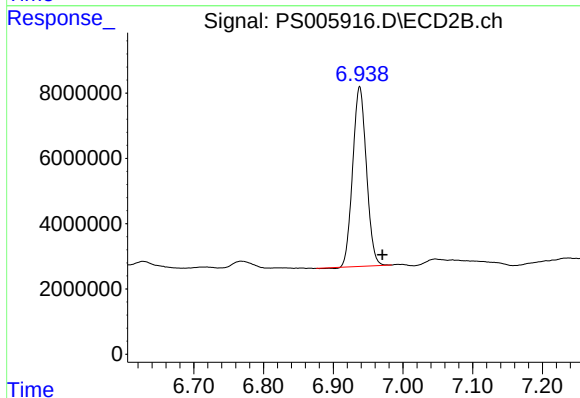


#11 2,4,5-TP (SILVEX)

R.T.: 6.938 min
Delta R.T.: -0.033 min
Response: 75072188
Conc: 14.47 ng/ml

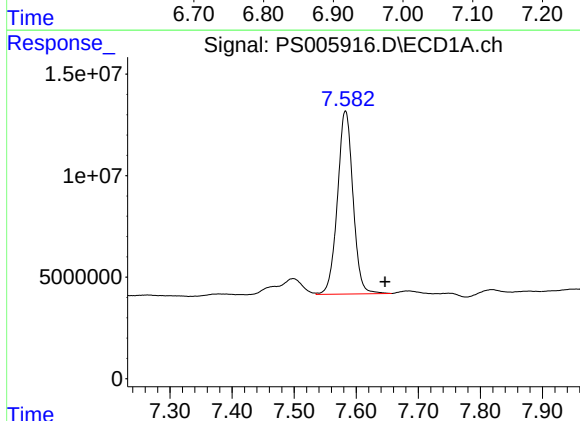

#12 2,4,5-T

R.T.: 7.583 min
Delta R.T.: -0.064 min
Response: 156688259
Conc: 18.77 ng/ml

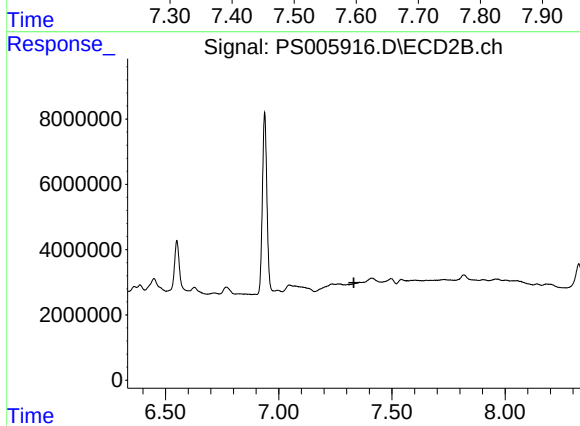

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.332 min
Response: 0
Conc: N.D.