

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
 Data File : PS005918.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2019 21:25
 Operator : SM\AJ
 Sample : K4130-37
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:42:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 27 00:42:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.554	5.275	317.1E6	228.2E6	218.582	229.462
Target Compounds							
1) T	Dalapon	2.054	0.000	50863293	0	27.445	N.D. #
2) T	3,5-DICHL...	0.000	4.593	0	210.5E6	N.D.	162.231
3) T	4-Nitroph...	5.343	0.000	9035506	0	15.021	N.D. #
5) T	DICAMBA	5.776	5.379	11077805	6572010	1.855	1.760
7) T	MCPA	5.963	0.000	32371076	0	4.961	N.D. #
8) T	DICHLORPROP	0.000	5.970	0	18891536	N.D.	20.456
9) T	2,4-D	6.632	6.215	218.5E6	15390549	145.764	14.326 #
11) T	2,4,5-TP ...	0.000	6.920	0	60206397	N.D.	11.606



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS080619\
Data File : PS005918.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2019 21:25
Operator : SM\AJ
Sample : K4130-37
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:42:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072619.M
Quant Title : 8080.M
QLast Update : Sat Jul 27 00:42:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

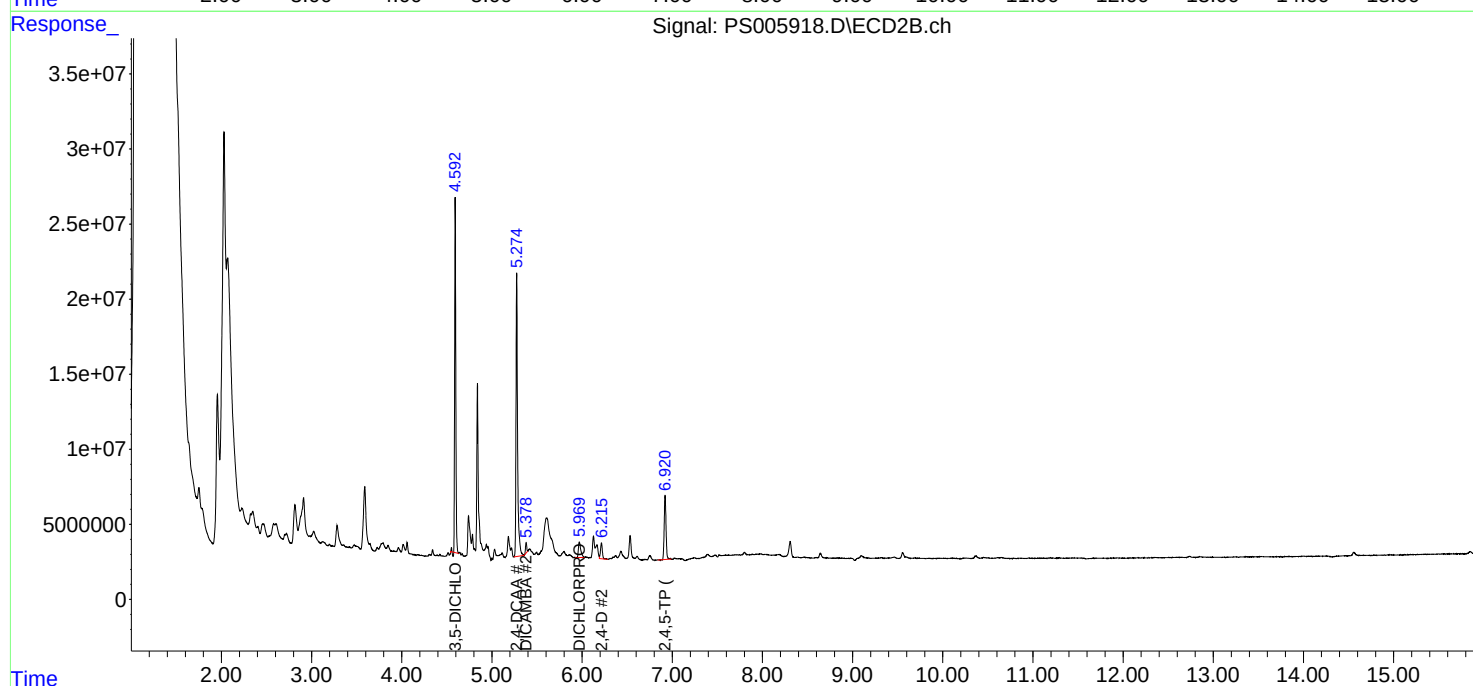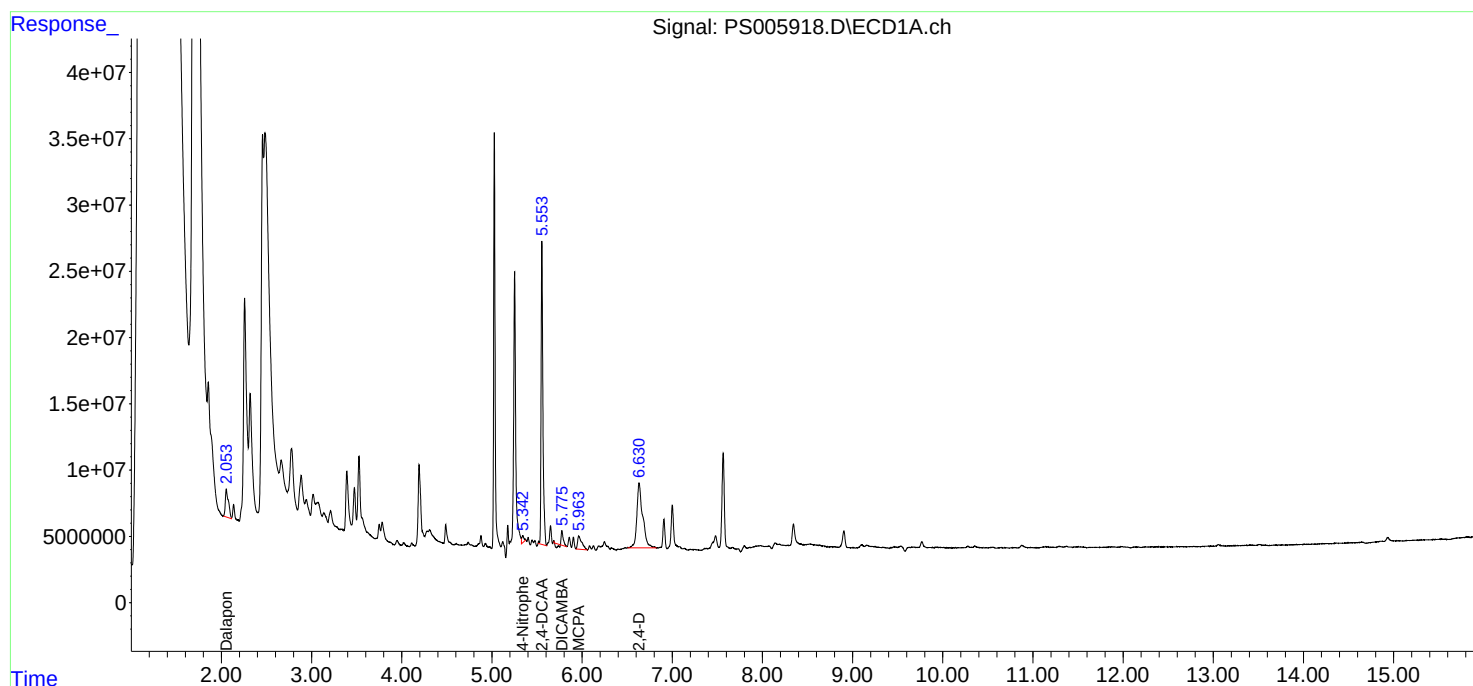


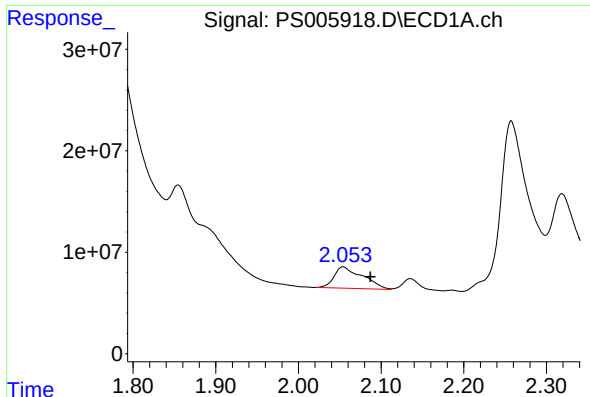

#1 Dalapon


R.T.: 2.054 min
Delta R.T.: -0.033 min
Response: 50863293
Conc: 27.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

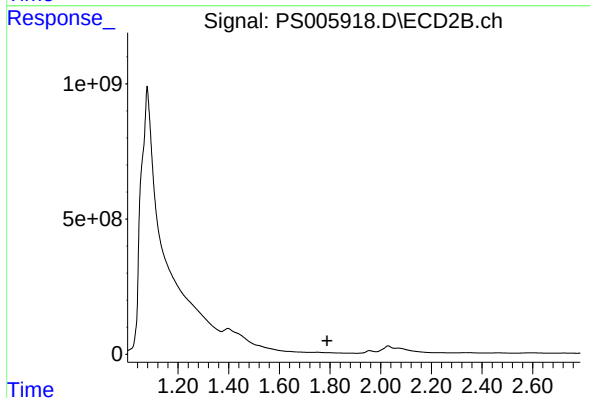


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

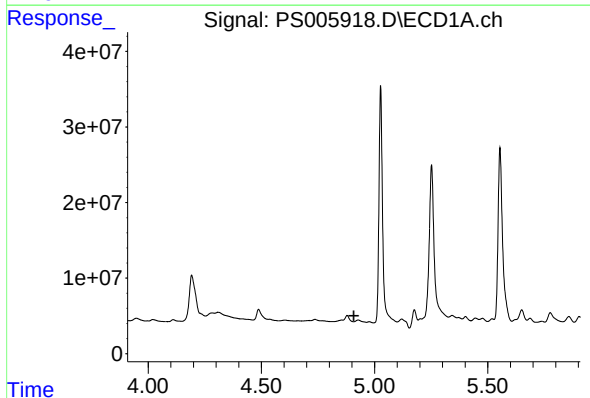


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.909 min
Response: 0
Conc: N.D.

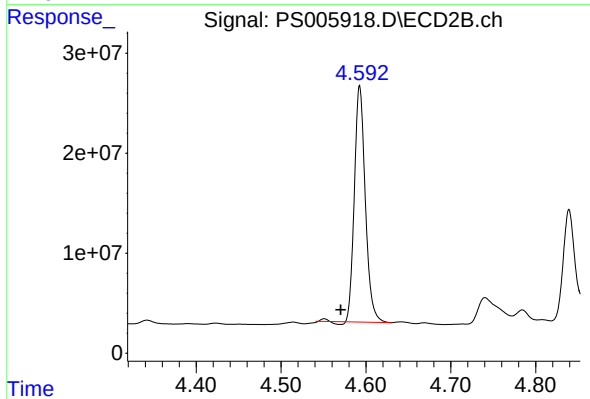

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.593 min
Delta R.T.: 0.023 min
Response: 210465238
Conc: 162.23 ng/ml

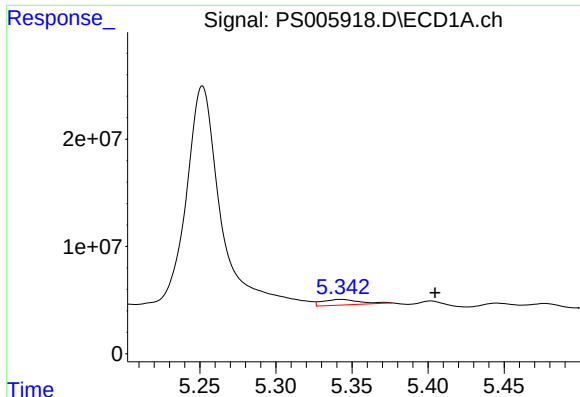

#3 4-Nitrophenol


R.T.: 5.343 min
Delta R.T.: -0.062 min
Response: 9035506
Conc: 15.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

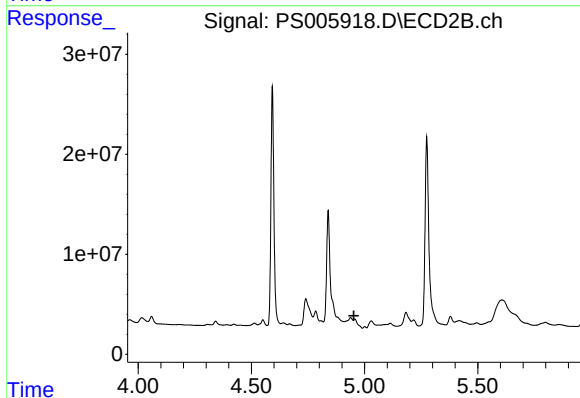


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

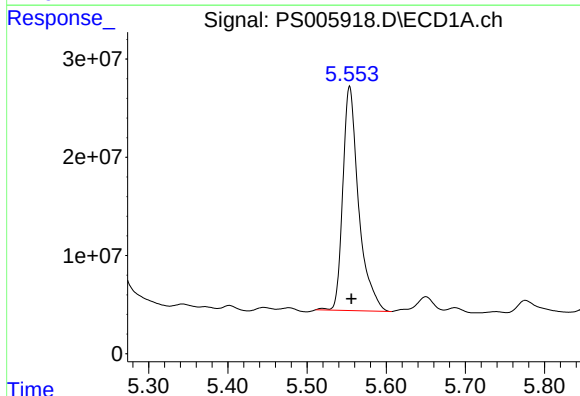


#4 2,4-DCAA

R.T.: 5.554 min
Delta R.T.: -0.002 min
Response: 317121976
Conc: 218.58 ng/ml

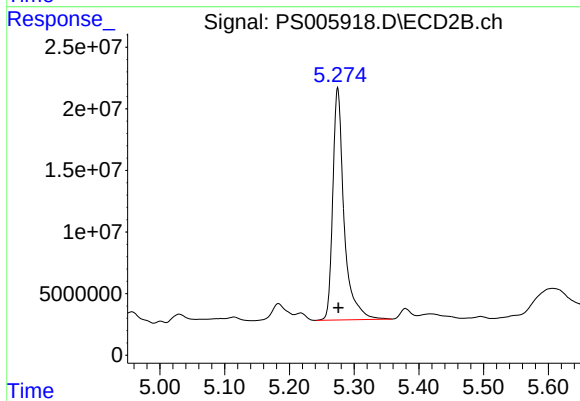

#4 2,4-DCAA


R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 228240538
Conc: 229.46 ng/ml

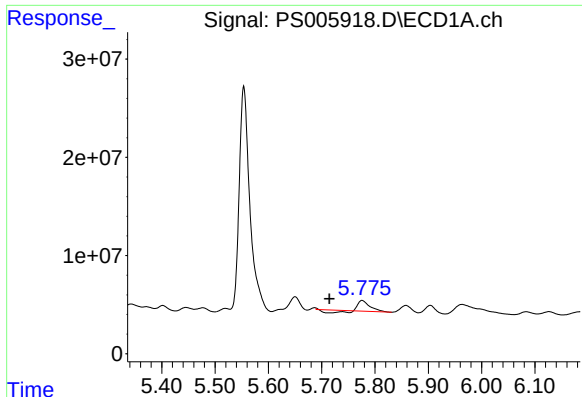

#5 DICAMBA


R.T.: 5.776 min
Delta R.T.: 0.062 min
Response: 11077805
Conc: 1.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

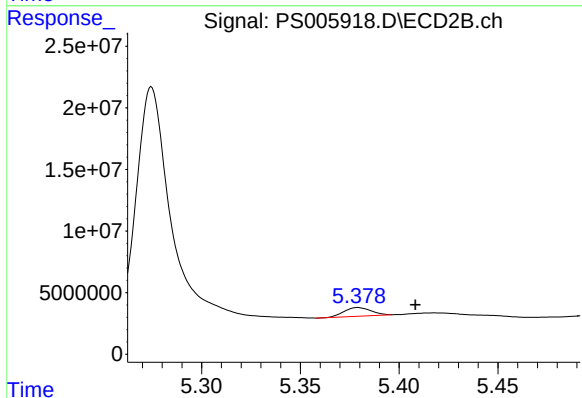


#5 DICAMBA

R.T.: 5.379 min
Delta R.T.: -0.029 min
Response: 6572010
Conc: 1.76 ng/ml

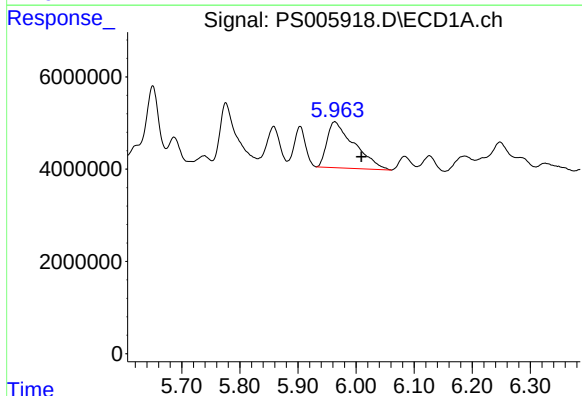


#7 MCPA

R.T.: 5.963 min
Delta R.T.: -0.046 min
Response: 32371076
Conc: 4.96 ug/ml

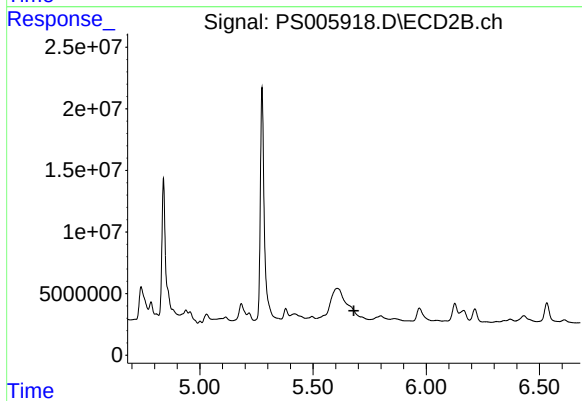

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.681 min
Response: 0
Conc: N.D.

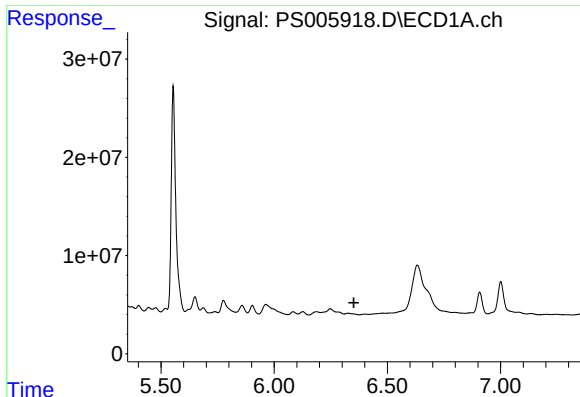

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

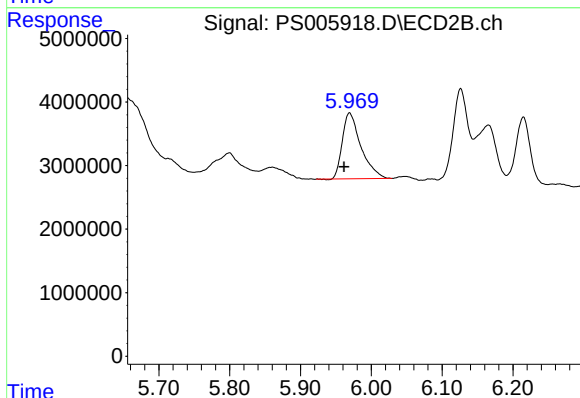


#8 DICHLORPROP

R.T.: 5.970 min
Delta R.T.: 0.008 min
Response: 18891536
Conc: 20.46 ng/ml

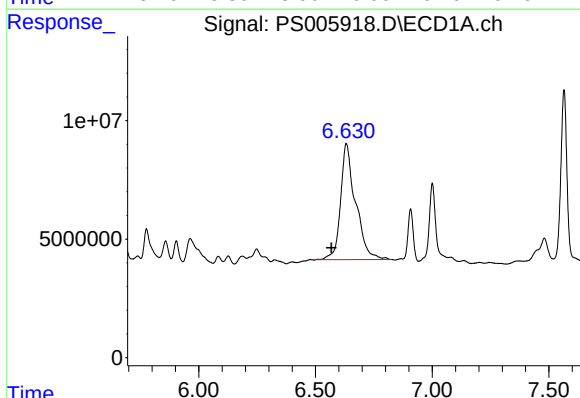


#9 2,4-D

R.T.: 6.632 min
Delta R.T.: 0.063 min
Response: 218451747
Conc: 145.76 ng/ml

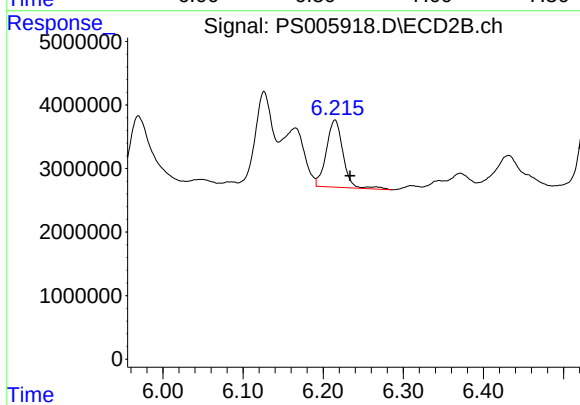

#9 2,4-D


R.T.: 6.215 min
Delta R.T.: -0.019 min
Response: 15390549
Conc: 14.33 ng/ml

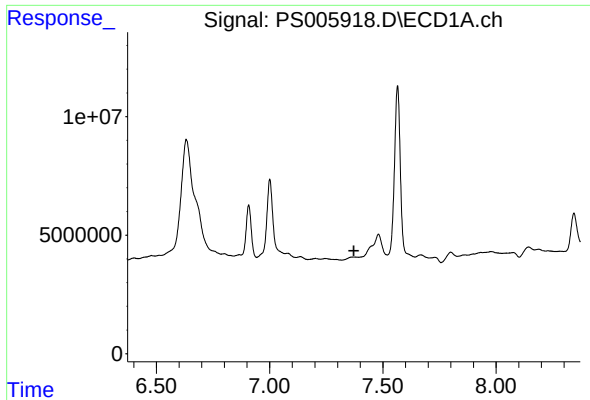

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

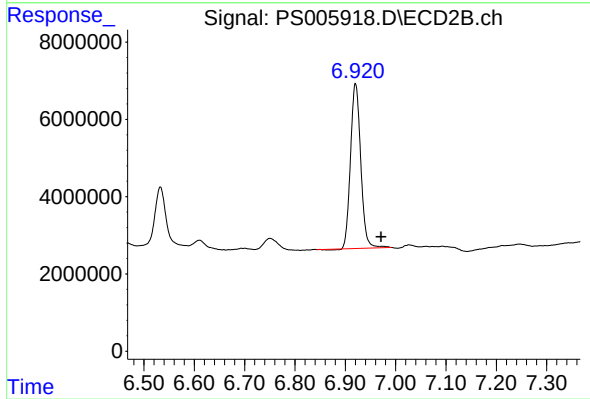

#11 2,4,5-TP (SILVEX)

R.T.: 6.920 min
Delta R.T.: -0.050 min
Response: 60206397
Conc: 11.61 ng/ml